

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0121518\
 Data File : P0052610.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 15 Dec 2018 19:57
 Operator : SM/SJ
 Sample : J6279-09 10X
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 580K-DUP3

Manual Integrations
 APPROVED

Sohil
 12/17/2018 4:46:47 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 16 03:08:10 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0121518.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sun Dec 16 03:01:24 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.259	3.281	642183	300251	0.819m	1.417 #
2) SA Decachlor...	9.815	7.971	516688	203344	1.025	0.922

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO121518\
Data File : PO052610.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 15 Dec 2018 19:57
Operator : SM/SJ
Sample : J6279-09 10X
Misc :
ALS Vial : 28 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
580K-DUP3


Manual Integrations
APPROVED

Sohil
12/17/2018 4:46:47 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 16 03:08:10 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO121518.M
Quant Title : GC EXTRACTABLES
QLast Update : Sun Dec 16 03:01:24 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

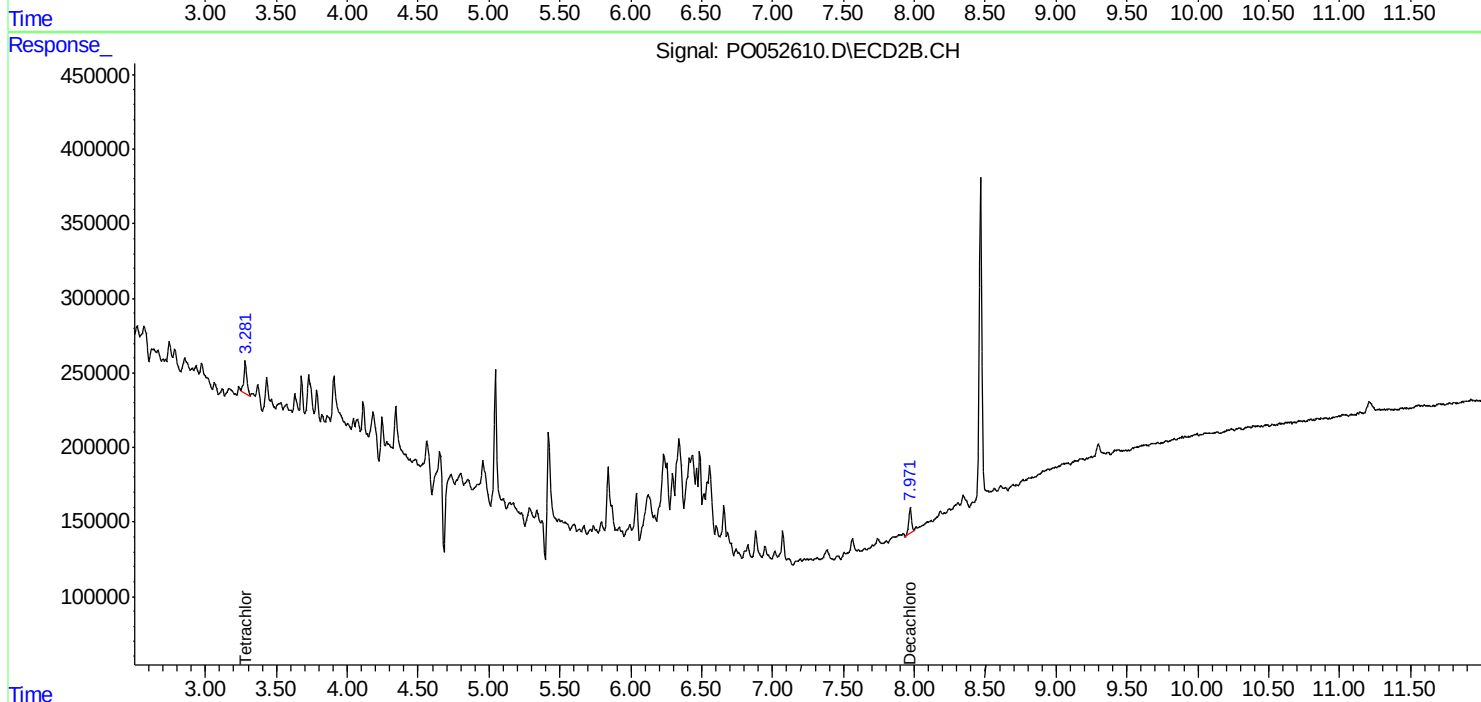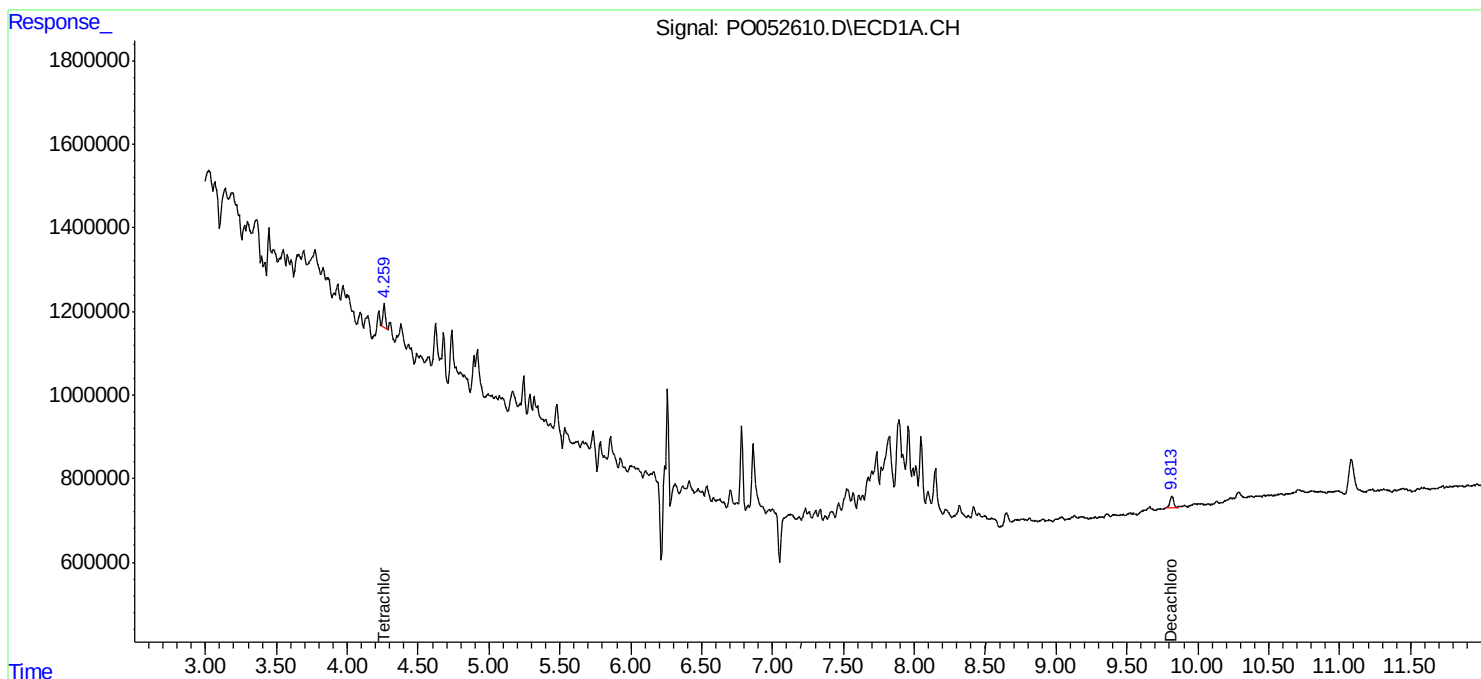

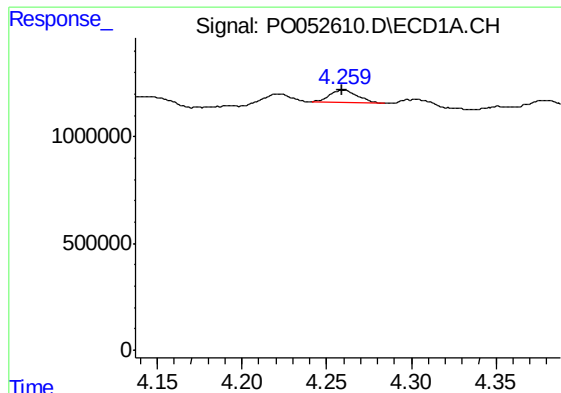


#1 Tetrachloro-m-xylene

R.T.: 4.259 min
Delta R.T.: 0.000 min
Response: 642183
Conc: 0.82 ng/ml m

Instrument :
ECD_O
ClientSampleId :
580K-DUP3


Manual Integrations
APPROVED

Sohil
12/17/2018 4:46:47 PM

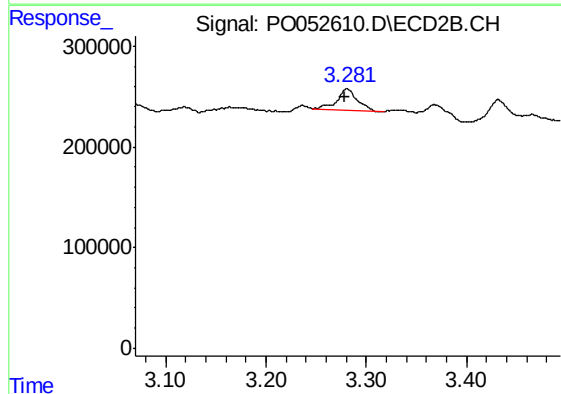


#1 Tetrachloro-m-xylene

R.T.: 3.281 min
Delta R.T.: 0.003 min
Response: 300251
Conc: 1.42 ng/ml

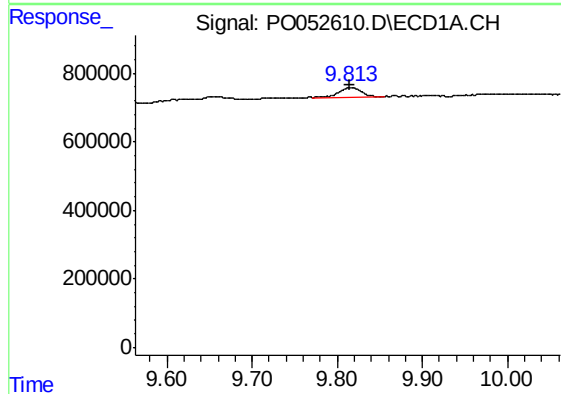

#2 Decachlorobiphenyl

R.T.: 9.815 min
Delta R.T.: 0.000 min
Response: 516688
Conc: 1.03 ng/ml

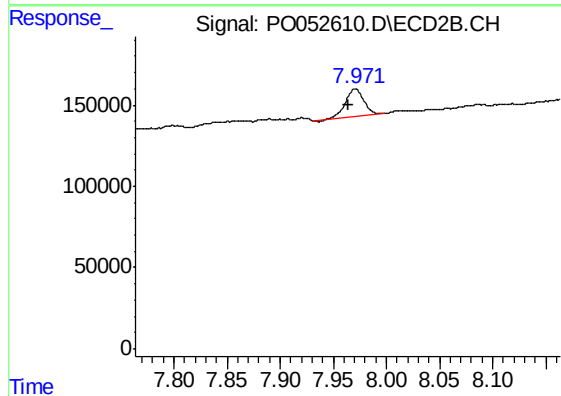

#2 Decachlorobiphenyl

R.T.: 7.971 min
Delta R.T.: 0.006 min
Response: 203344
Conc: 0.92 ng/ml