

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\PO121520\
 Data File : PO073853.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 16 Dec 2020 00:04
 Operator : DD\AJ
 Sample : L5088-01
 Misc :
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 ECD_0
 ClientSampleId :
 TR1-A-D-COMP

Manual Integrations
 APPROVED

Ankita
 12/16/2020 10:58:09 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 16 00:43:13 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\PO121020.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Dec 11 03:58:06 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.937	3.996	1650377	1006550	18.051	18.766
2) SA Decachlor...	10.958	9.258	1589670	942747	19.236	20.148
Target Compounds						
31) L7 AR-1260-1	7.952	6.821	227581	132775	53.847	42.951m
32) L7 AR-1260-2	8.218	7.018	199565	88852	35.524	21.904 #
33) L7 AR-1260-3	8.585	7.171	156827	154804	34.308	44.352 #
34) L7 AR-1260-4	8.814	7.651	204804	115535	43.258	38.260
35) L7 AR-1260-5	9.141	7.898	384496	255316	38.528	34.178

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO121520\
Data File : PO073853.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 16 Dec 2020 00:04
Operator : DD\AJ
Sample : L5088-01
Misc :
ALS Vial : 42 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
TR1-A-D-COMP


Manual Integrations
APPROVED

Ankita
12/16/2020 10:58:09 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 16 00:43:13 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO121020.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Dec 11 03:58:06 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

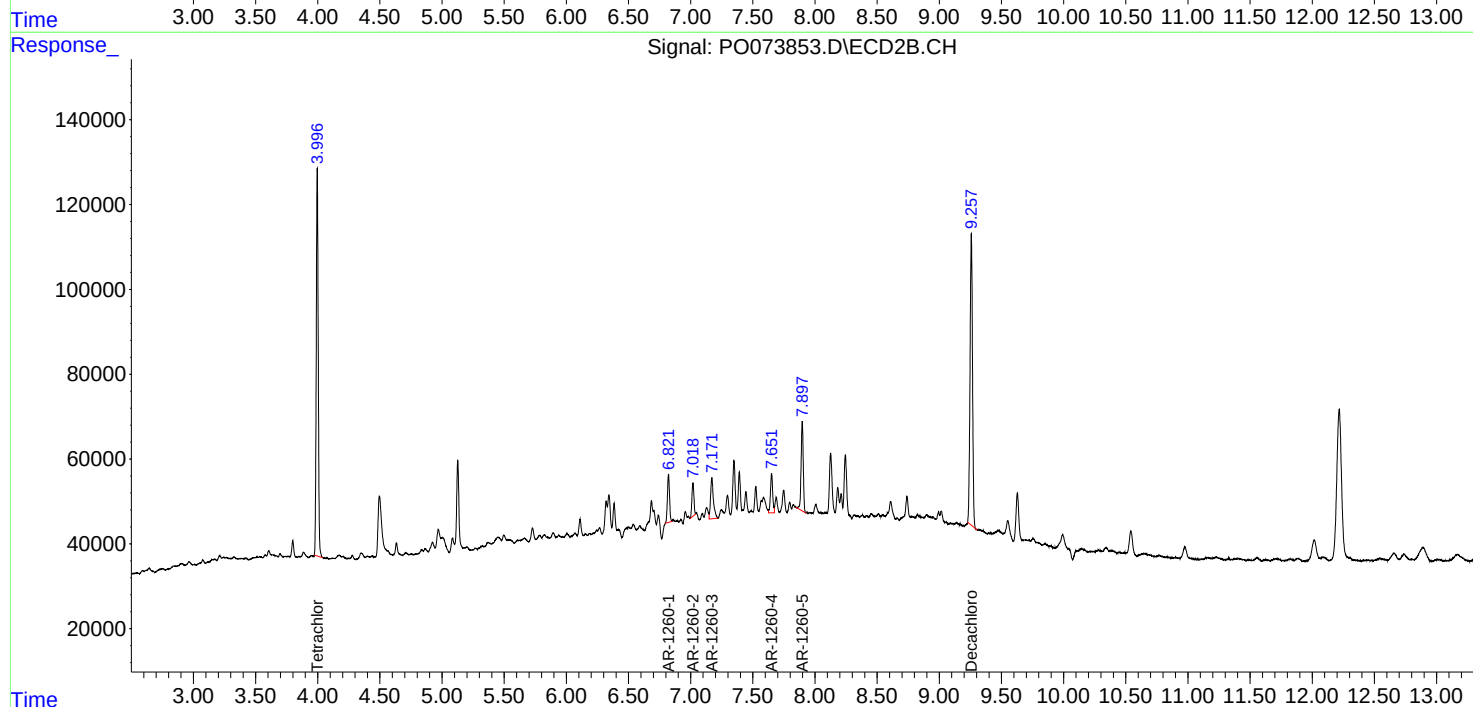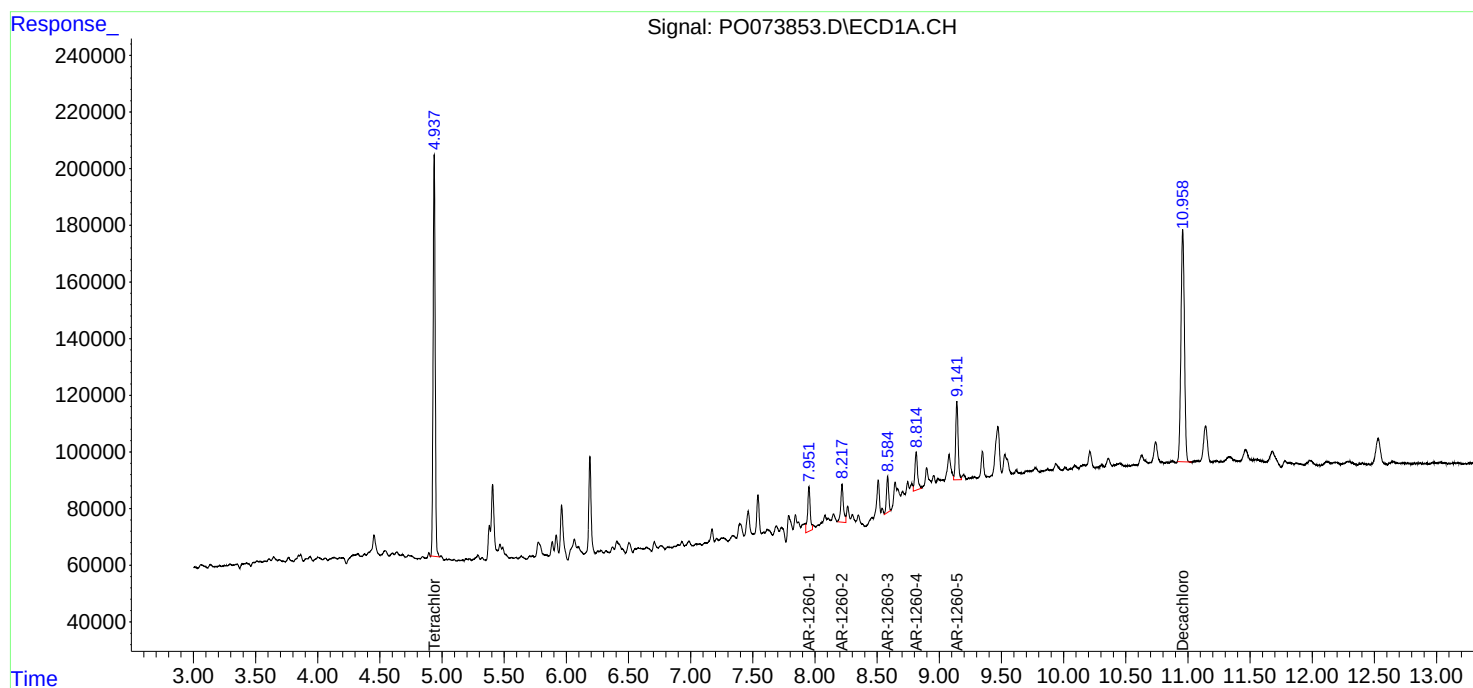

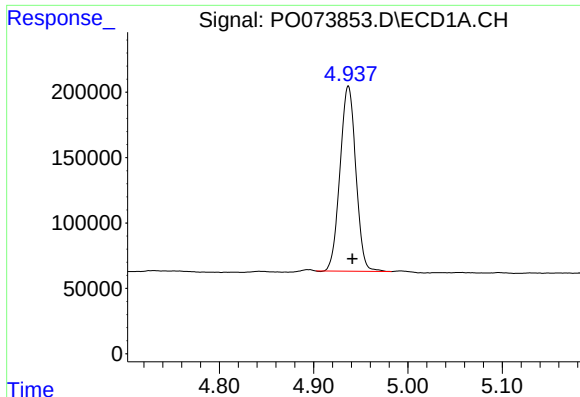


#1 Tetrachloro-m-xylene

R.T.: 4.937 min
Delta R.T.: -0.004 min
Response: 1650377
Conc: 18.05 ng/ml

Instrument :
ECD_O
ClientSampleId :
TR1-A-D-COMP


Manual Integrations
APPROVED

Ankita
12/16/2020 10:58:09 AM

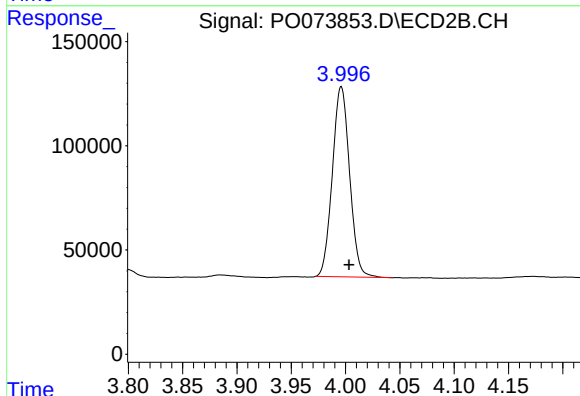


#1 Tetrachloro-m-xylene

R.T.: 3.996 min
Delta R.T.: -0.007 min
Response: 1006550
Conc: 18.77 ng/ml

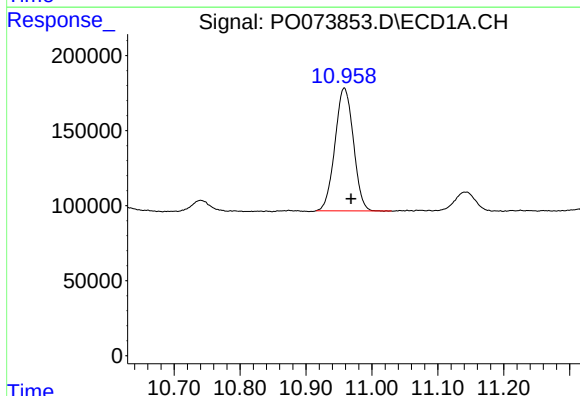


#2 Decachlorobiphenyl

R.T.: 10.958 min
Delta R.T.: -0.010 min
Response: 1589670
Conc: 19.24 ng/ml

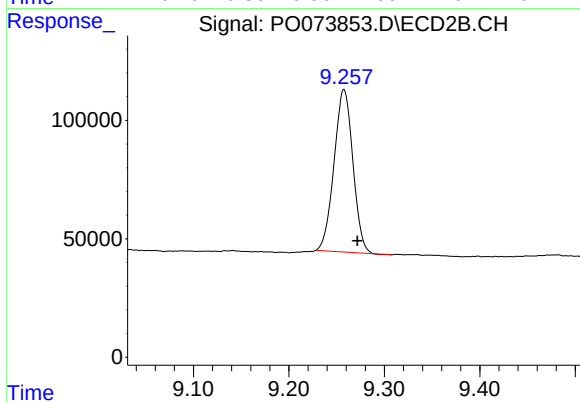

#2 Decachlorobiphenyl

R.T.: 9.258 min
Delta R.T.: -0.014 min
Response: 942747
Conc: 20.15 ng/ml

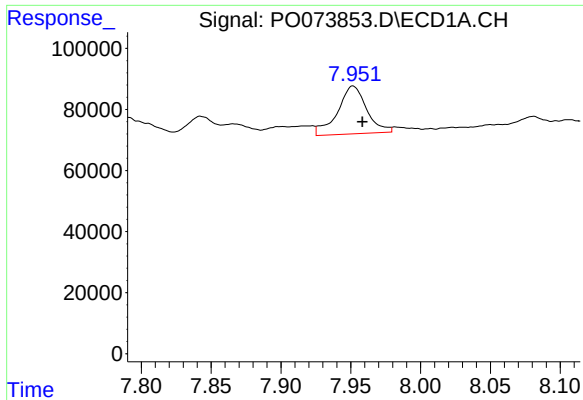


#31 AR-1260-1

R.T.: 7.952 min
Delta R.T.: -0.007 min
Response: 227581
Conc: 53.85 ng/ml

Instrument :
ECD_O
ClientSampleId :
TR1-A-D-COMP


Manual Integrations
APPROVED

Ankita
12/16/2020 10:58:09 AM

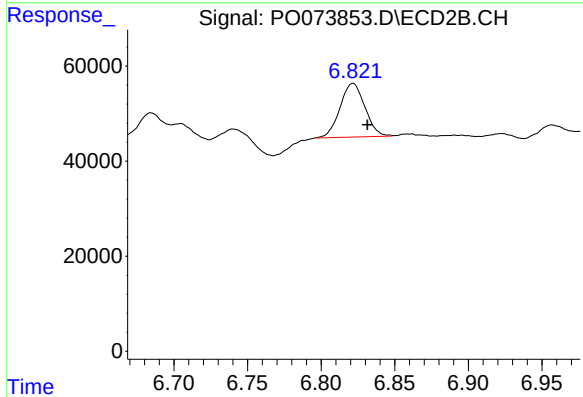


#31 AR-1260-1

R.T.: 6.821 min
Delta R.T.: -0.010 min
Response: 132775
Conc: 42.95 ng/ml m

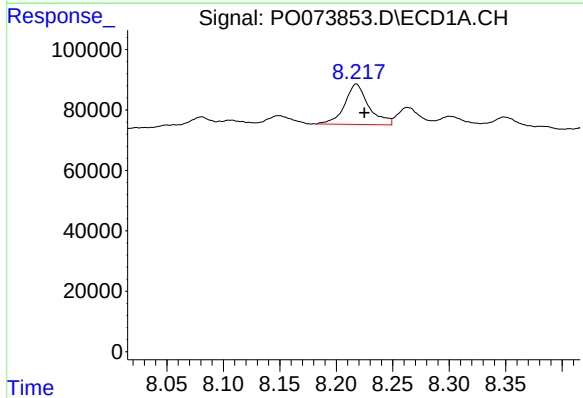


#32 AR-1260-2

R.T.: 8.218 min
Delta R.T.: -0.007 min
Response: 199565
Conc: 35.52 ng/ml

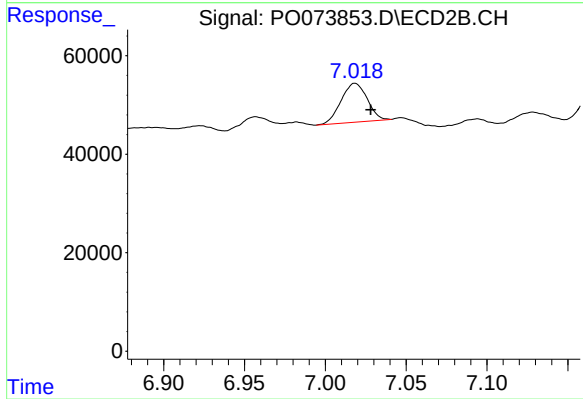

#32 AR-1260-2

R.T.: 7.018 min
Delta R.T.: -0.010 min
Response: 88852
Conc: 21.90 ng/ml

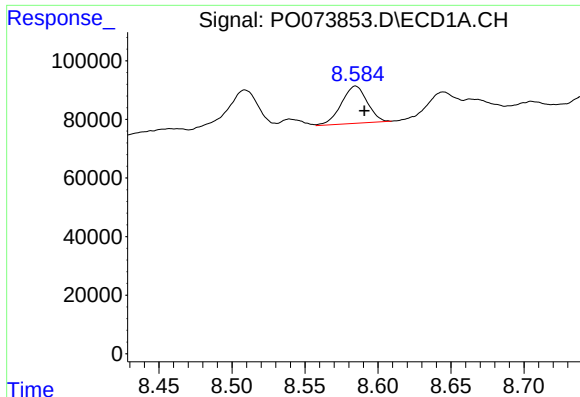


#33 AR-1260-3

R.T.: 8.585 min
Delta R.T.: -0.006 min
Response: 156827
Conc: 34.31 ng/ml

Instrument :
ECD_O
ClientSampleId :
TR1-A-D-COMP


Manual Integrations
APPROVED

Ankita
12/16/2020 10:58:09 AM

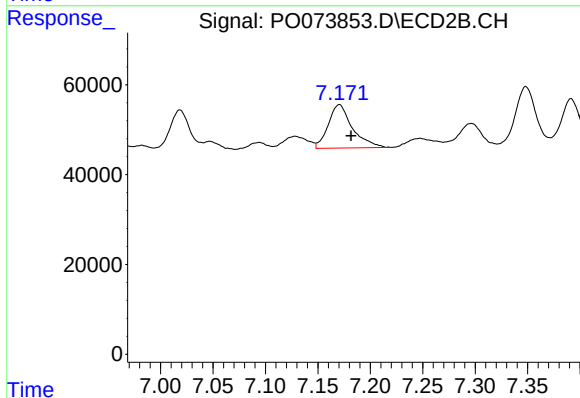


#33 AR-1260-3

R.T.: 7.171 min
Delta R.T.: -0.011 min
Response: 154804
Conc: 44.35 ng/ml

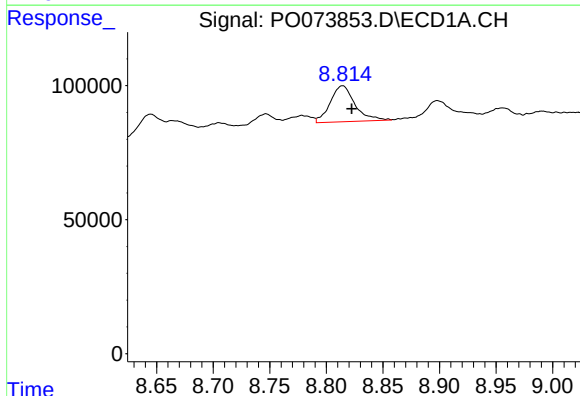


#34 AR-1260-4

R.T.: 8.814 min
Delta R.T.: -0.008 min
Response: 204804
Conc: 43.26 ng/ml

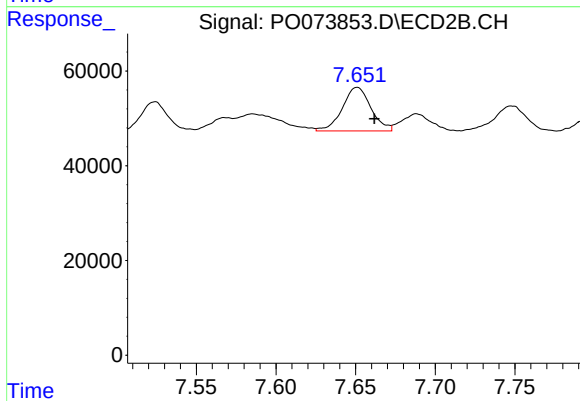

#34 AR-1260-4

R.T.: 7.651 min
Delta R.T.: -0.011 min
Response: 115535
Conc: 38.26 ng/ml

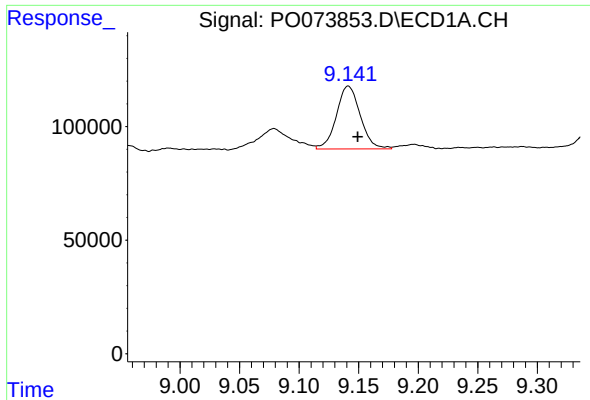


#35 AR-1260-5

R.T.: 9.141 min
Delta R.T.: -0.008 min
Response: 384496
Conc: 38.53 ng/ml

Instrument :
ECD_O
ClientSampleId :
TR1-A-D-COMP

Manual Integrations
APPROVED

Ankita
12/16/2020 10:58:09 AM

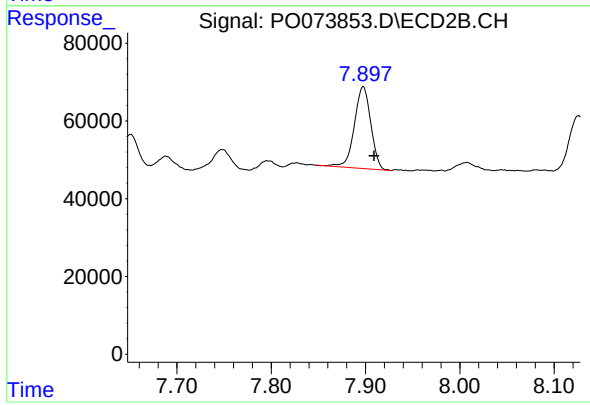

#35 AR-1260-5

R.T.: 7.898 min
Delta R.T.: -0.011 min
Response: 255316
Conc: 34.18 ng/ml