

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0121522\
 Data File : P0091422.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 Dec 2022 00:06
 Operator : YP/AJ
 Sample : N6066-18
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 ORA-1523

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 12/16/2022
 Supervised By :Ankita Jodhani 12/16/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 16 01:50:07 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0112522.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Nov 28 11:25:59 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.295	3.476	3972636	4470929	1.175m	4.260 #
2) SA Decachlor...	10.049	8.479	11539509	611363	4.344	0.630 #

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO121522\
Data File : PO091422.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 Dec 2022 00:06
Operator : YP/AJ
Sample : N6066-18
Misc :
ALS Vial : 28 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
ORA-1523


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 12/16/2022
Supervised By :Ankita Jodhani 12/16/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 16 01:50:07 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO112522.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Nov 28 11:25:59 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

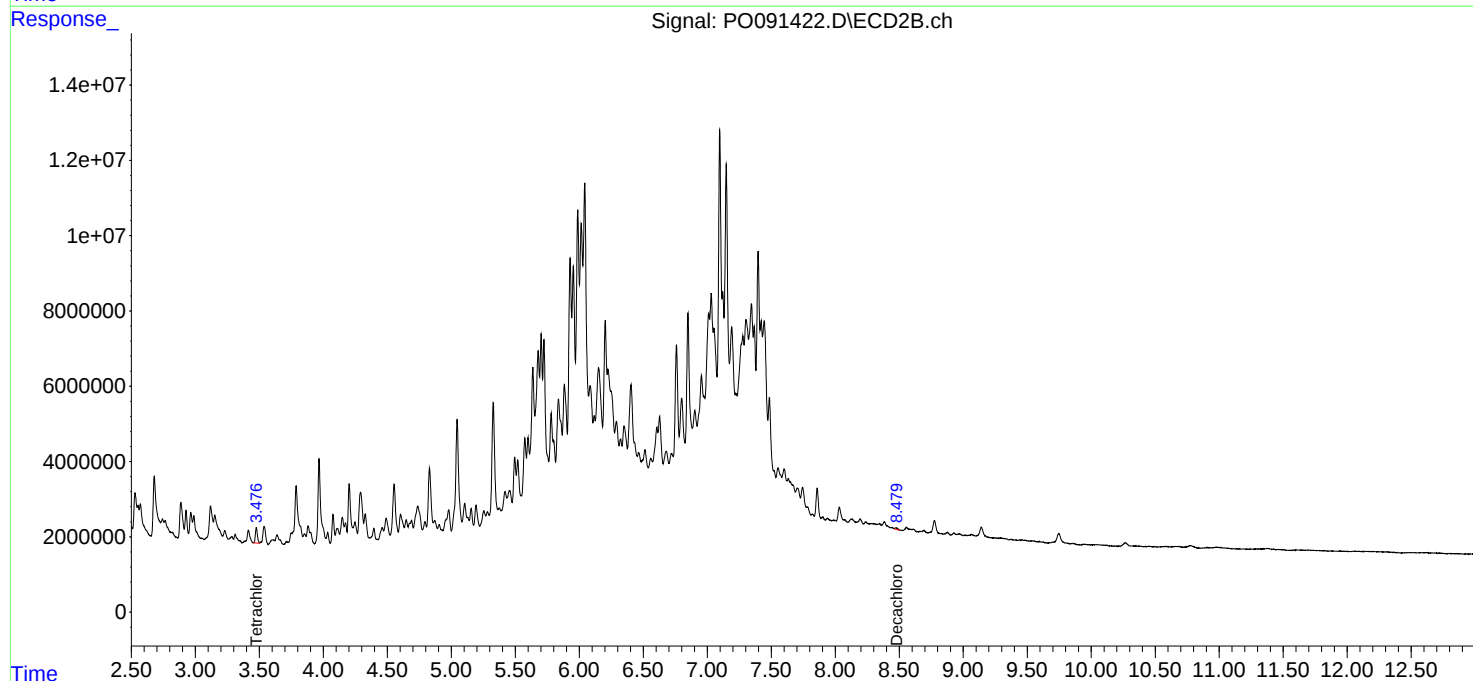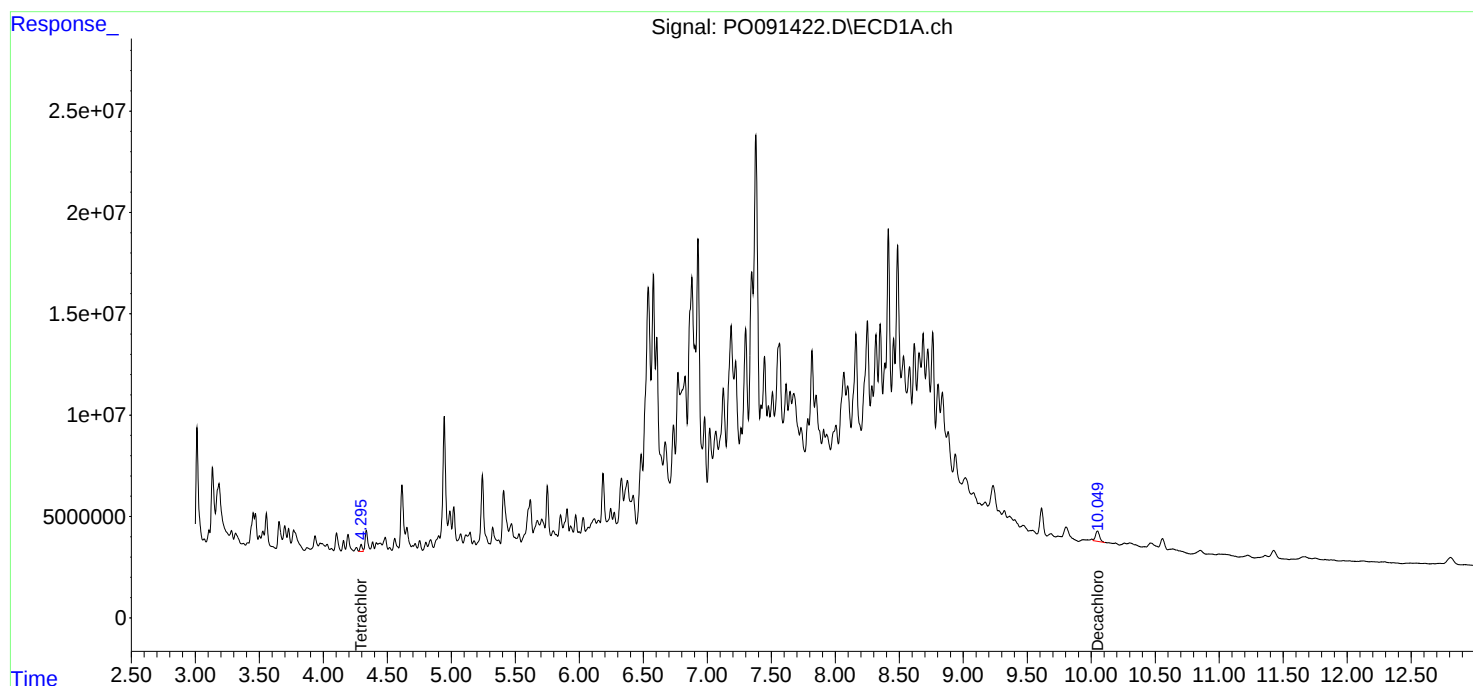

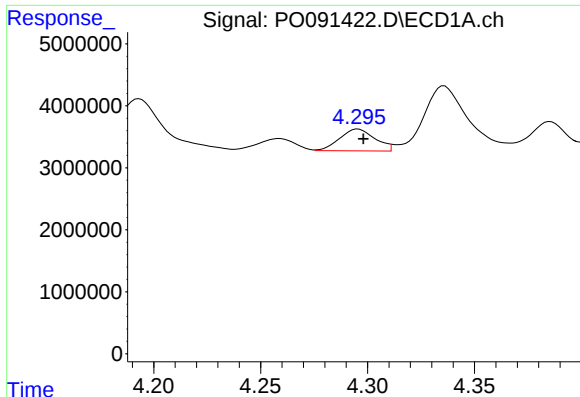


#1 Tetrachloro-m-xylene

R.T.: 4.295 min
Delta R.T.: -0.003 min
Response: 3972636
Conc: 1.17 ng/ml

Instrument :
ECD_O
ClientSampleId :
ORA-1523


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 12/16/2022
Supervised By :Ankita Jodhani 12/16/2022

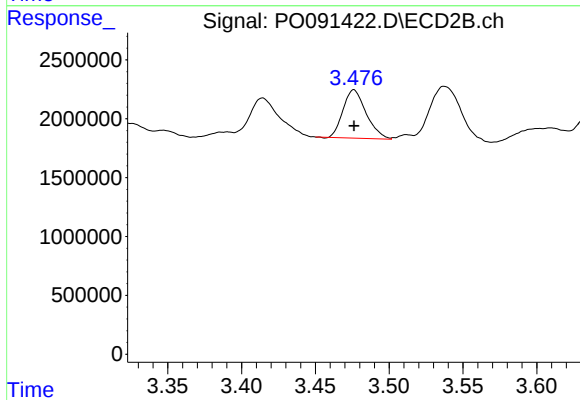


#1 Tetrachloro-m-xylene

R.T.: 3.476 min
Delta R.T.: 0.000 min
Response: 4470929
Conc: 4.26 ng/ml

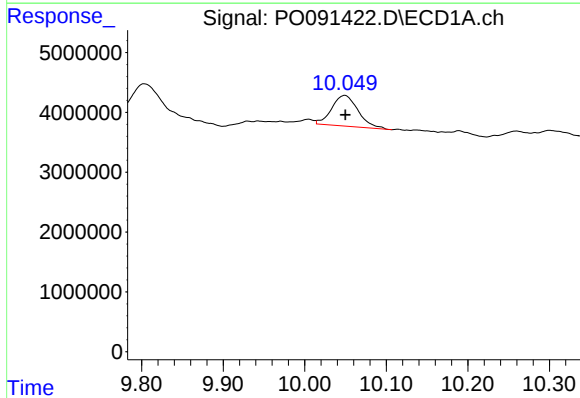

#2 Decachlorobiphenyl

R.T.: 10.049 min
Delta R.T.: 0.000 min
Response: 11539509
Conc: 4.34 ng/ml

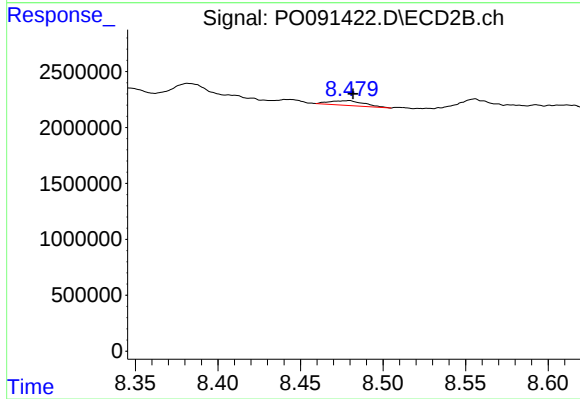

#2 Decachlorobiphenyl

R.T.: 8.479 min
Delta R.T.: -0.003 min
Response: 611363
Conc: 0.63 ng/ml