

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO121620\
 Data File : PO073879.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 16 Dec 2020 14:54
 Operator : DD\AJ
 Sample : L5036-12
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 16 16:20:56 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO121020.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Dec 11 03:58:06 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.937	3.997	1877270	1025673	20.533	19.123
2)	SA Decachlor...	10.958	9.258	915780	543490	11.082	11.615
Target Compounds							
8)	L2 AR-1221-1	5.193	0.000	92125	0	86.949	N.D. #
9)	L2 AR-1221-2	5.290	0.000	27978	0	35.618	N.D. #
12)	L3 AR-1232-2	5.954	0.000	1143	0	1.069	N.D. #
20)	L4 AR-1242-5	7.240	0.000	68442	0	31.340	N.D. #
25)	L5 AR-1248-5	7.240	0.000	68442	0	18.098	N.D. #
32)	L7 AR-1260-2	8.242f	0.000	117122	0	20.848	N.D. #
33)	L7 AR-1260-3	0.000	7.167	0	129749	N.D.	37.174 #
34)	L7 AR-1260-4	8.847f	0.000	22329	0	4.716	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO121620\
Data File : P0073879.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 16 Dec 2020 14:54
Operator : DD\AJ
Sample : L5036-12
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 16 16:20:56 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO121020.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Dec 11 03:58:06 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

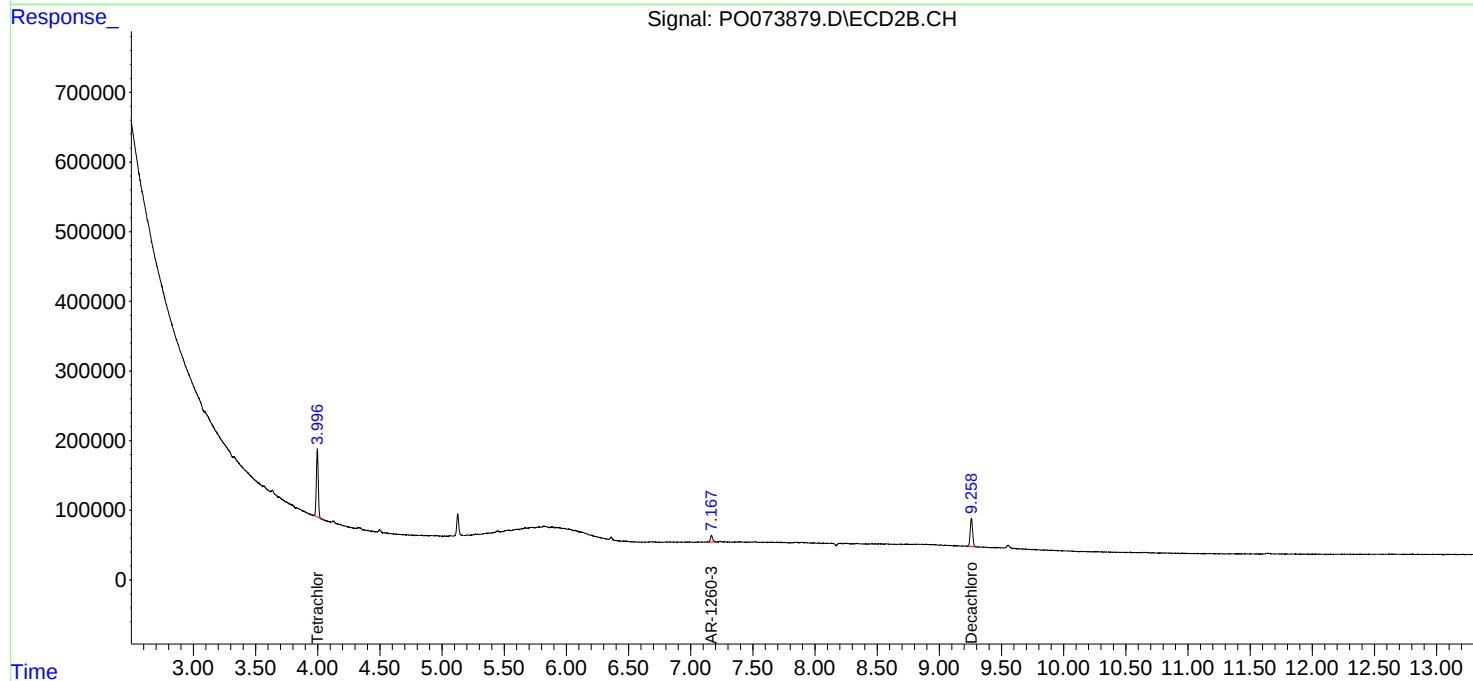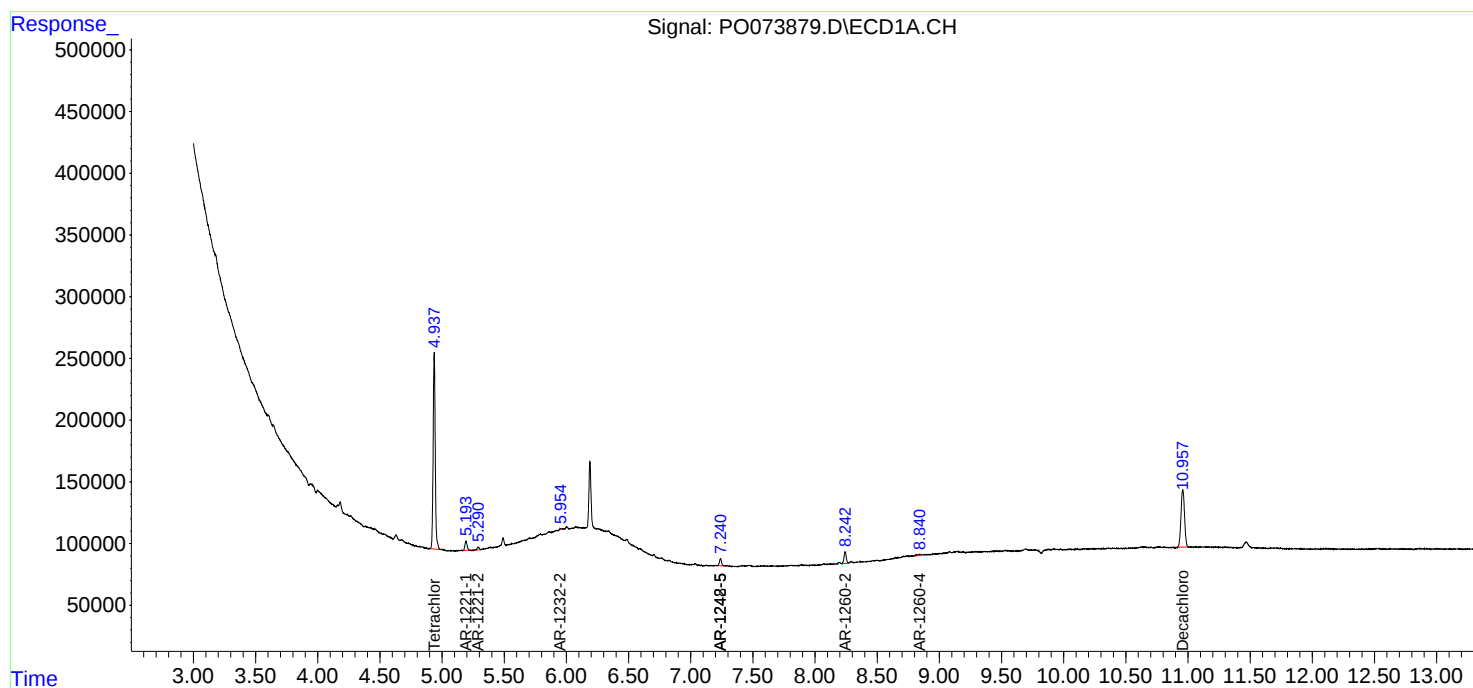


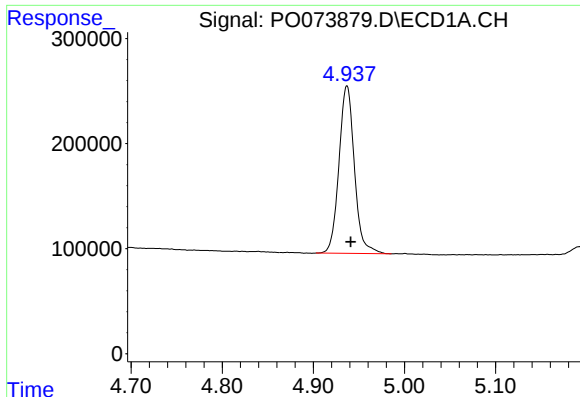

#1 Tetrachloro-m-xylene


R.T.: 4.937 min
Delta R.T.: -0.004 min
Response: 1877270
Conc: 20.53 ng/ml

Instrument :
ECD_O
ClientSampleId :

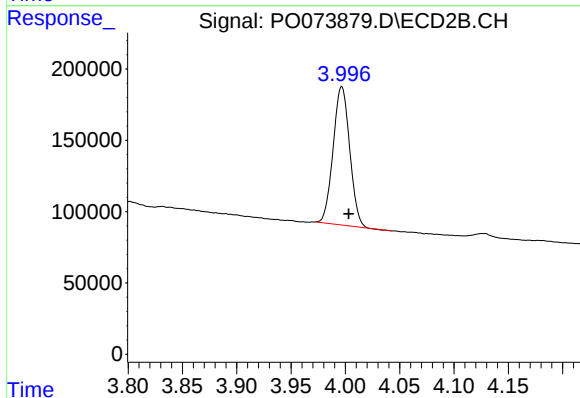


#1 Tetrachloro-m-xylene

R.T.: 3.997 min
Delta R.T.: -0.006 min
Response: 1025673
Conc: 19.12 ng/ml

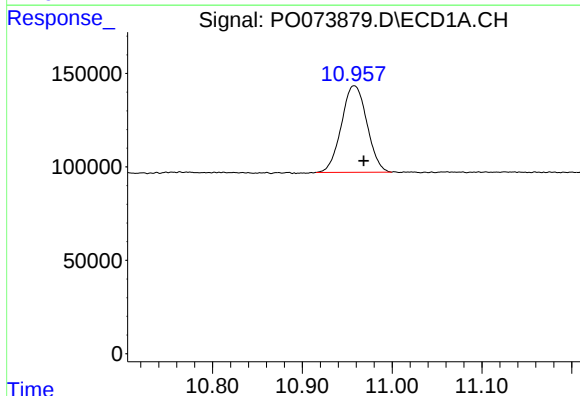


#2 Decachlorobiphenyl

R.T.: 10.958 min
Delta R.T.: -0.011 min
Response: 915780
Conc: 11.08 ng/ml

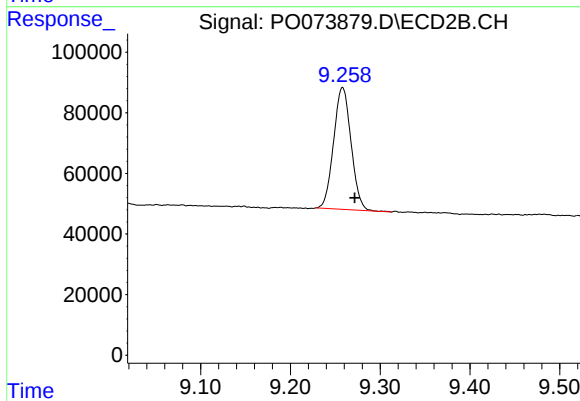

#2 Decachlorobiphenyl


R.T.: 9.258 min
Delta R.T.: -0.014 min
Response: 543490
Conc: 11.62 ng/ml

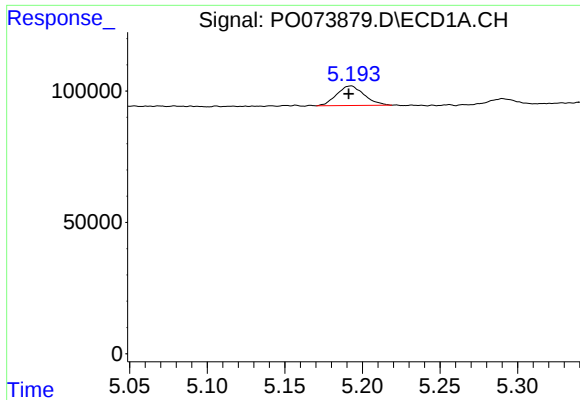

#8 AR-1221-1


R.T.: 5.193 min
Delta R.T.: 0.002 min
Response: 92125
Conc: 86.95 ng/ml

Instrument :
ECD_O
ClientSampleId :

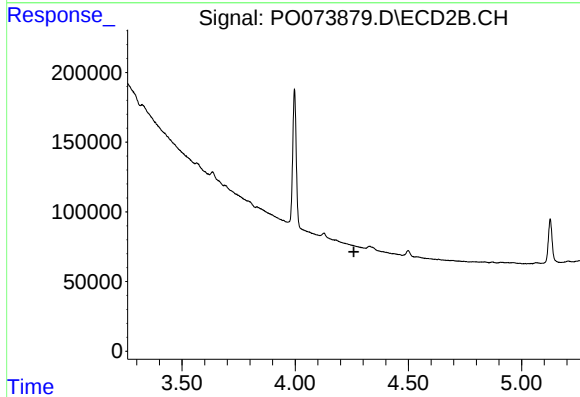


#8 AR-1221-1

R.T.: 0.000 min
Exp R.T. : 4.259 min
Response: 0
Conc: N.D.

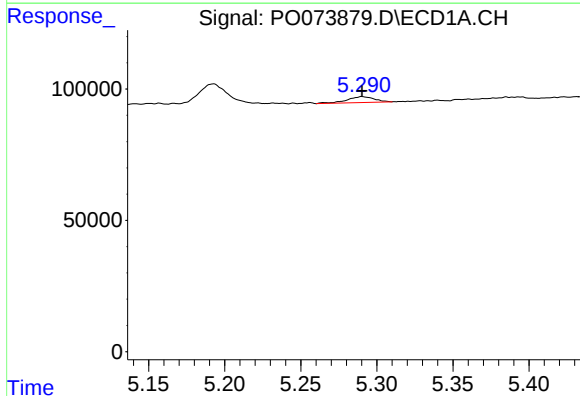


#9 AR-1221-2

R.T.: 5.290 min
Delta R.T.: 0.000 min
Response: 27978
Conc: 35.62 ng/ml

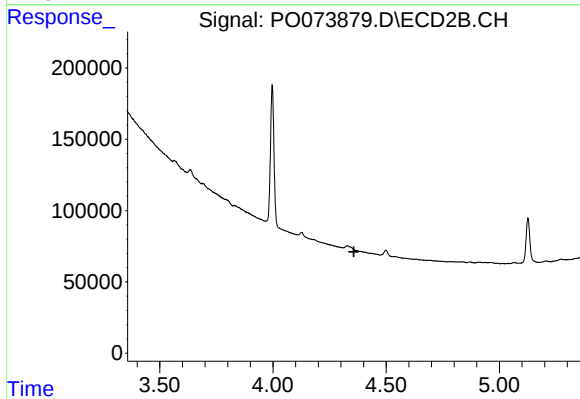

#9 AR-1221-2


R.T.: 0.000 min
Exp R.T. : 4.357 min
Response: 0
Conc: N.D.

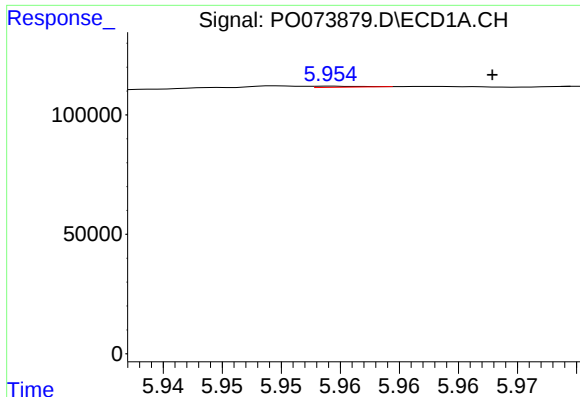

#12 AR-1232-2


R.T.: 5.954 min
Delta R.T.: -0.013 min
Response: 1143
Conc: 1.07 ng/ml

Instrument :
ECD_O
ClientSampleId :

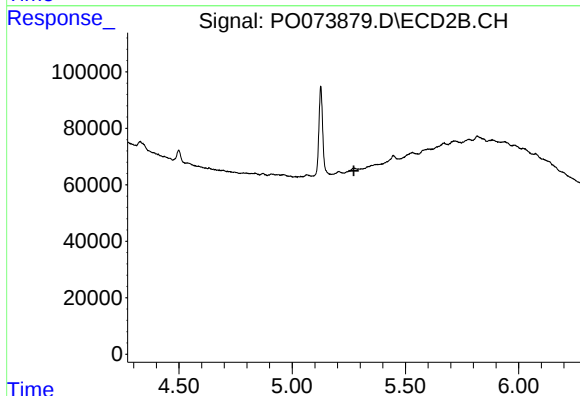


#12 AR-1232-2

R.T.: 0.000 min
Exp R.T. : 5.272 min
Response: 0
Conc: N.D.

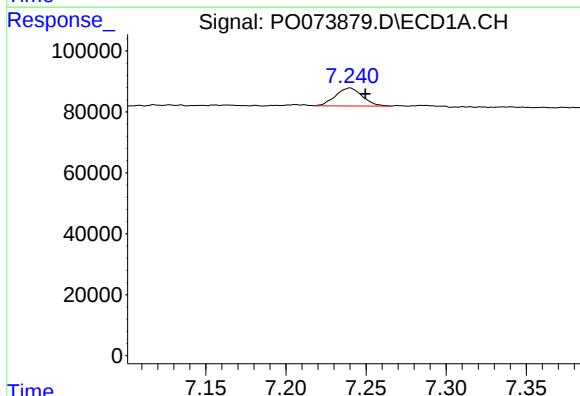


#20 AR-1242-5

R.T.: 7.240 min
Delta R.T.: -0.009 min
Response: 68442
Conc: 31.34 ng/ml

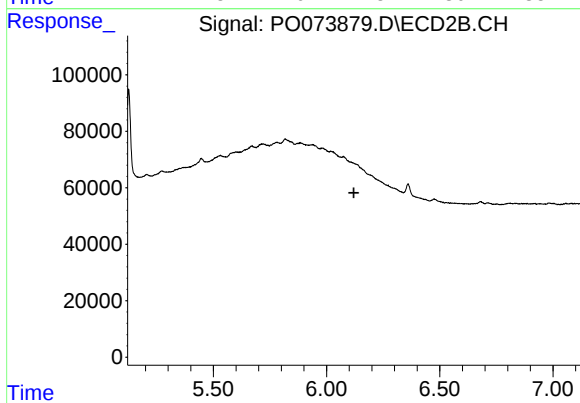

#20 AR-1242-5


R.T.: 0.000 min
Exp R.T. : 6.120 min
Response: 0
Conc: N.D.

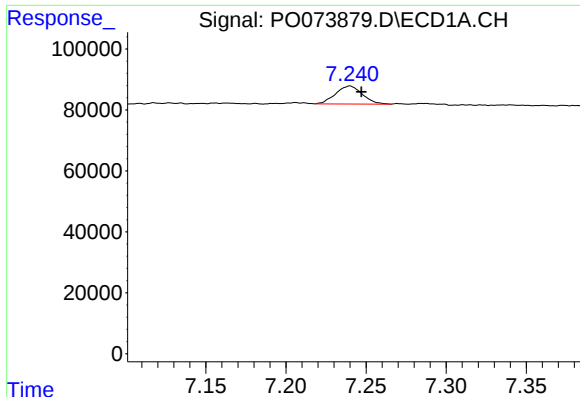

#25 AR-1248-5


R.T.: 7.240 min
Delta R.T.: -0.007 min
Response: 68442
Conc: 18.10 ng/ml

Instrument :
ECD_O
ClientSampleId :

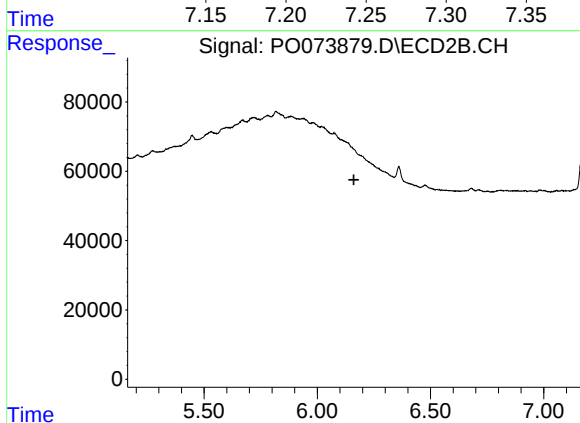


#25 AR-1248-5

R.T.: 0.000 min
Exp R.T. : 6.161 min
Response: 0
Conc: N.D.

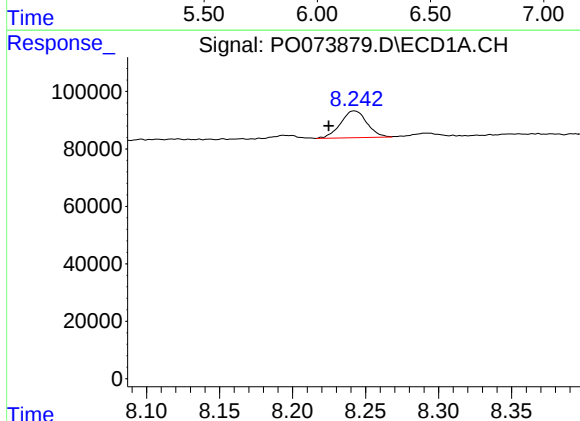


#32 AR-1260-2

R.T.: 8.242 min
Delta R.T.: 0.017 min
Response: 117122
Conc: 20.85 ng/ml

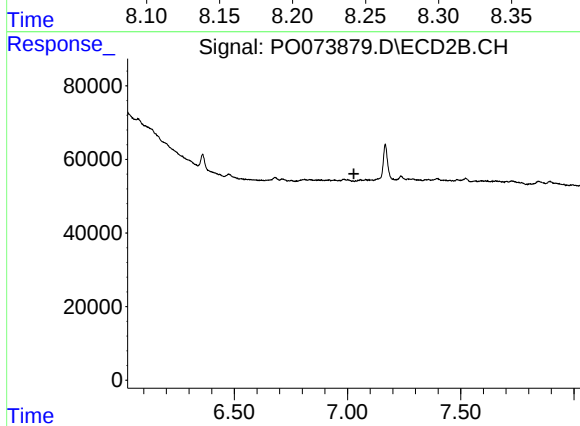

#32 AR-1260-2


R.T.: 0.000 min
Exp R.T. : 7.028 min
Response: 0
Conc: N.D.

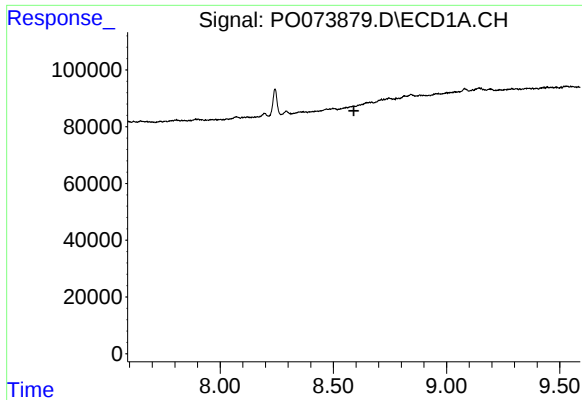

#33 AR-1260-3


R.T.: 0.000 min
Exp R.T.: 8.591 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :

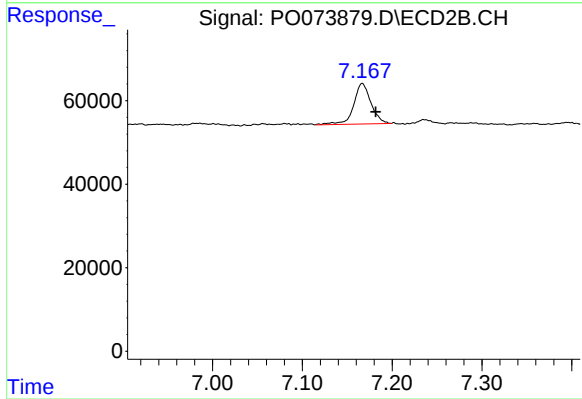


#33 AR-1260-3

R.T.: 7.167 min
Delta R.T.: -0.015 min
Response: 129749
Conc: 37.17 ng/ml

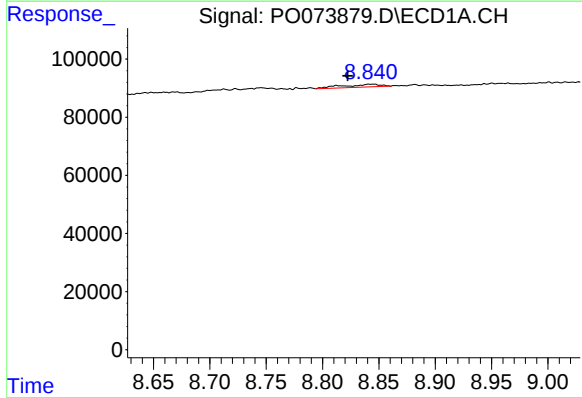

#34 AR-1260-4

R.T.: 8.847 min
Delta R.T.: 0.024 min
Response: 22329
Conc: 4.72 ng/ml

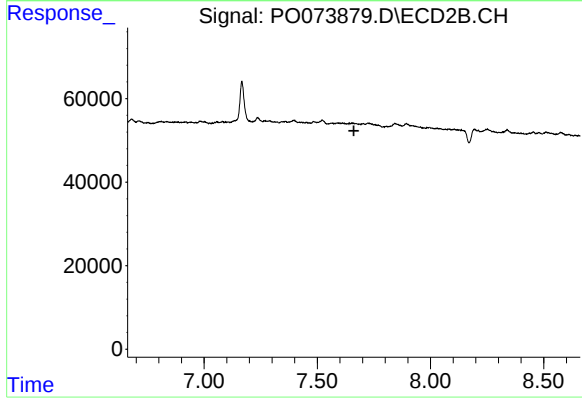

#34 AR-1260-4

R.T.: 0.000 min
Exp R.T.: 7.662 min
Response: 0
Conc: N.D.