

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0121620\
 Data File : P0073897.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 16 Dec 2020 20:02
 Operator : DD\AJ
 Sample : L5120-13
 Misc :
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 K650-6A

Manual Integrations
 APPROVED

Ankita
 12/17/2020 12:41:24 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 17 05:44:51 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0121020.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Dec 11 03:58:06 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.938	3.998	1497965	955255	16.384m	17.810
2) SA Decachlor...	10.963	9.260	1366918	1014604	16.541	21.684 #

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO121620\
Data File : PO073897.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 16 Dec 2020 20:02
Operator : DD\AJ
Sample : L5120-13
Misc :
ALS Vial : 32 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
K650-6A


Manual Integrations
APPROVED

Ankita
12/17/2020 12:41:24 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 17 05:44:51 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO121020.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Dec 11 03:58:06 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

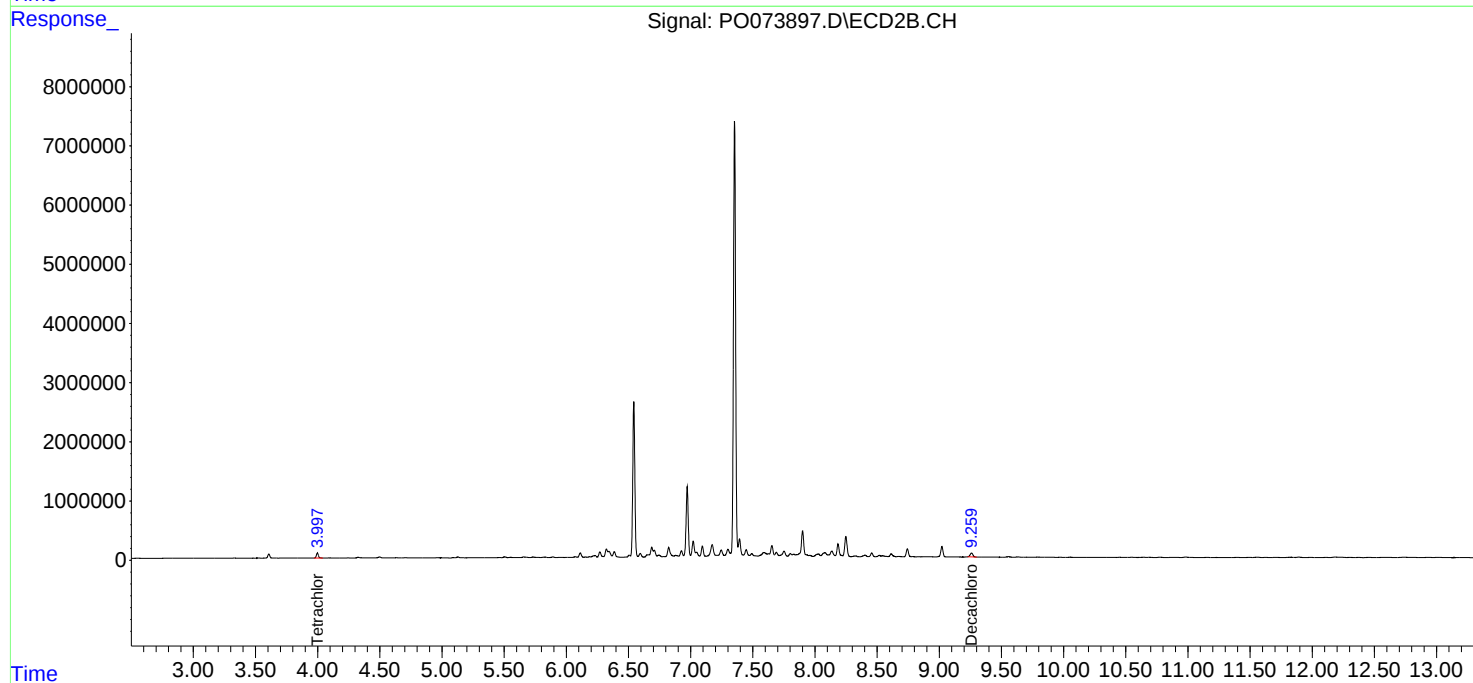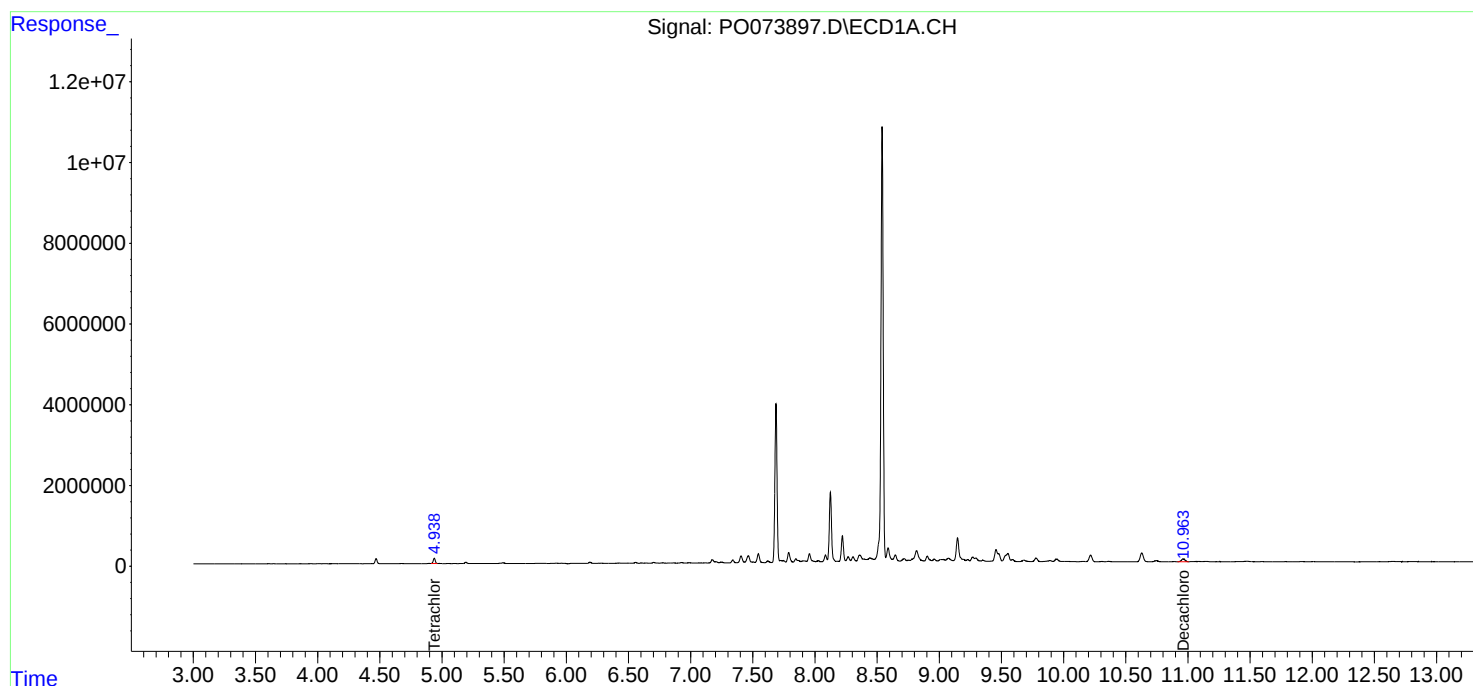

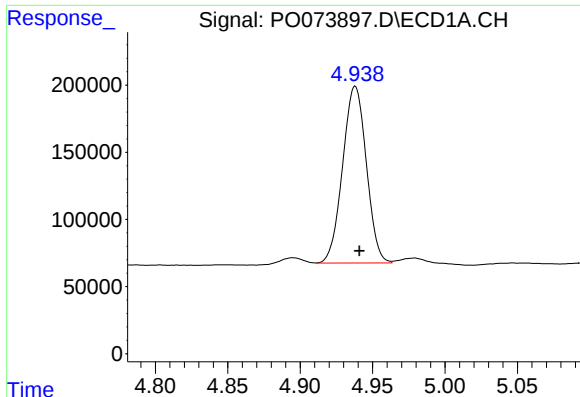


#1 Tetrachloro-m-xylene

R.T.: 4.938 min
Delta R.T.: -0.003 min
Response: 1497965
Conc: 16.38 ng/ml m

Instrument :
ECD_O
ClientSampleId :
K650-6A


Manual Integrations
APPROVED

Ankita
12/17/2020 12:41:24 PM

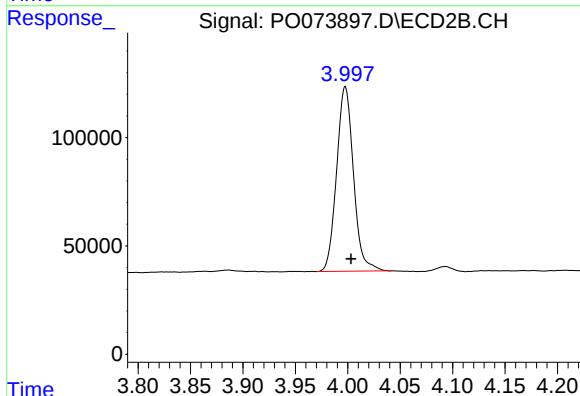


#1 Tetrachloro-m-xylene

R.T.: 3.998 min
Delta R.T.: -0.005 min
Response: 955255
Conc: 17.81 ng/ml

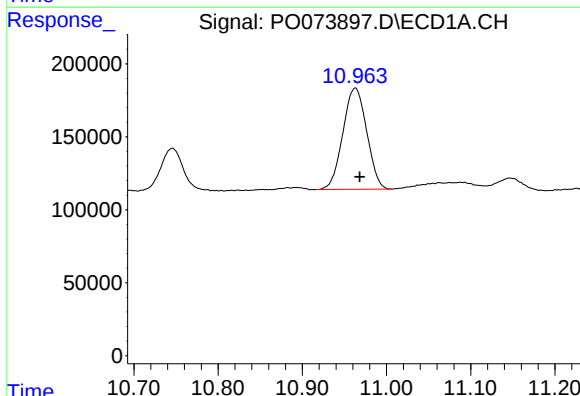

#2 Decachlorobiphenyl

R.T.: 10.963 min
Delta R.T.: -0.005 min
Response: 1366918
Conc: 16.54 ng/ml

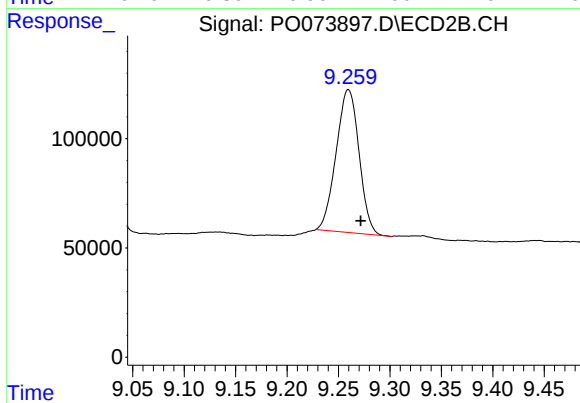

#2 Decachlorobiphenyl

R.T.: 9.260 min
Delta R.T.: -0.012 min
Response: 1014604
Conc: 21.68 ng/ml