

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO121621\
 Data File : PO083769.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 16 Dec 2021 19:25
 Operator : AJ\MA
 Sample : M5070-07 10X
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 CLI-2021-11-B

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 17 01:35:36 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO121521.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Dec 16 04:05:27 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.935	3.940	134066	43541	1.407	1.484
2) SA Decachlor...	11.010	9.238	115686	39327	1.689	1.401
Target Compounds						
30) L6 AR-1254-5	8.537	0.000	6239	0	1.750	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\PO121621\
Data File : PO083769.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 16 Dec 2021 19:25
Operator : AJ\MA
Sample : M5070-07 10X
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
CLI-2021-11-B

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 17 01:35:36 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\PO121521.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Dec 16 04:05:27 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

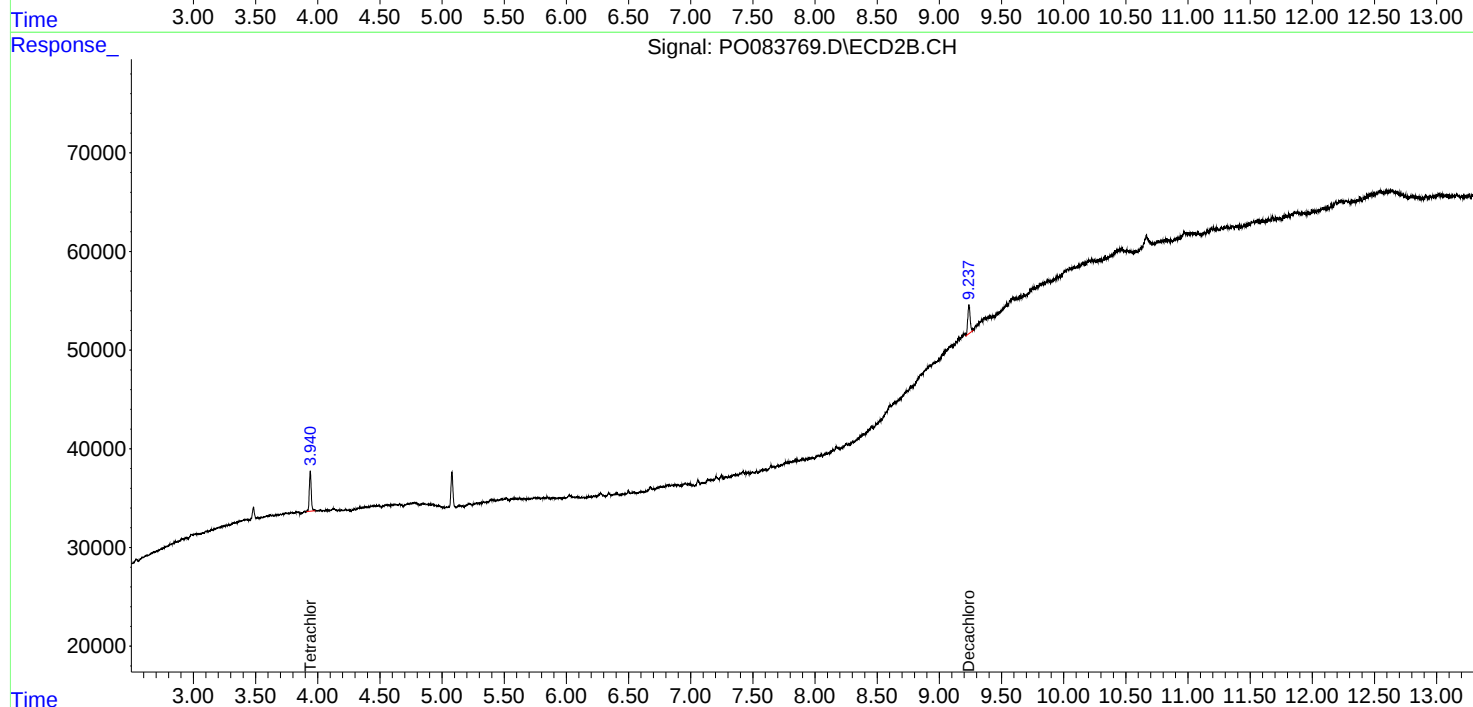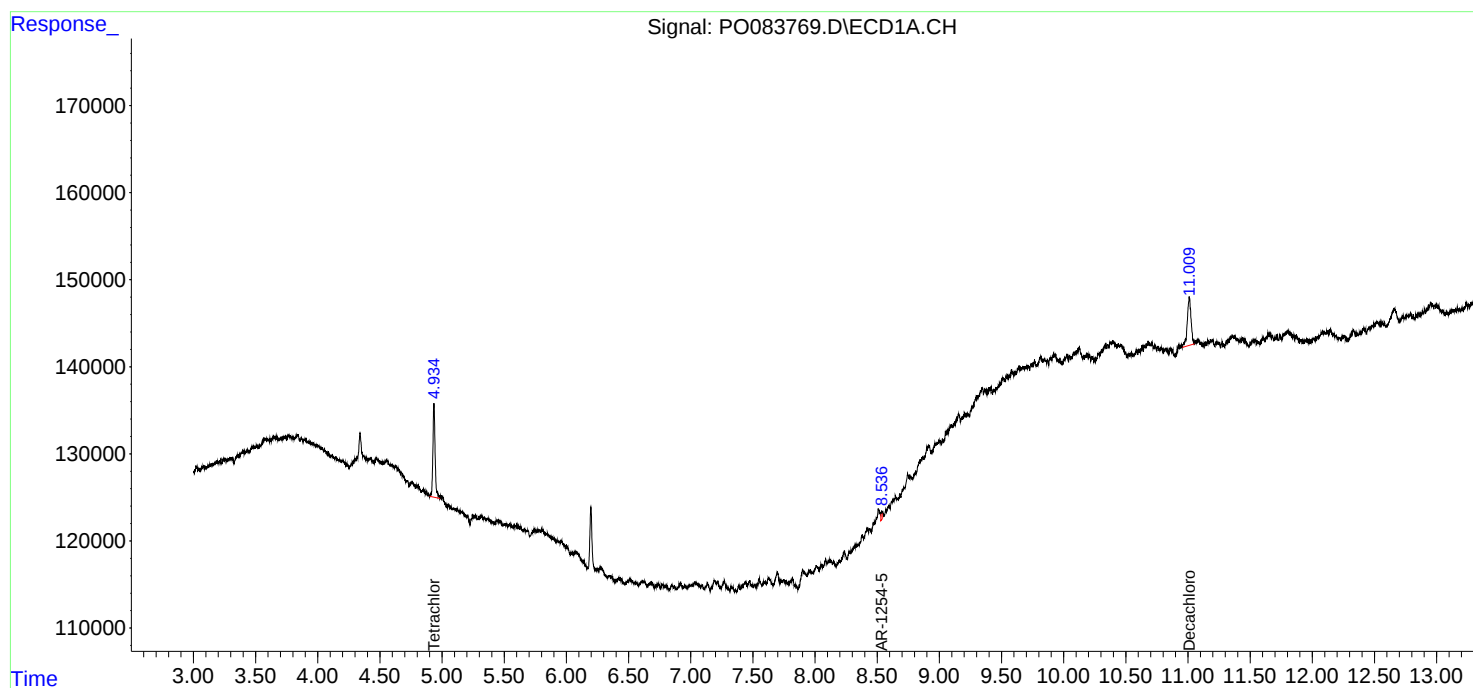


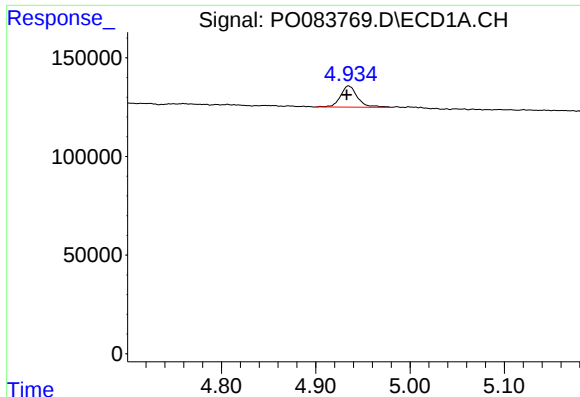

#1 Tetrachloro-m-xylene


R.T.: 4.935 min
Delta R.T.: 0.002 min
Response: 134066
Conc: 1.41 ng/ml

Instrument :
ECD_O
ClientSampleId :
CLI-2021-11-B

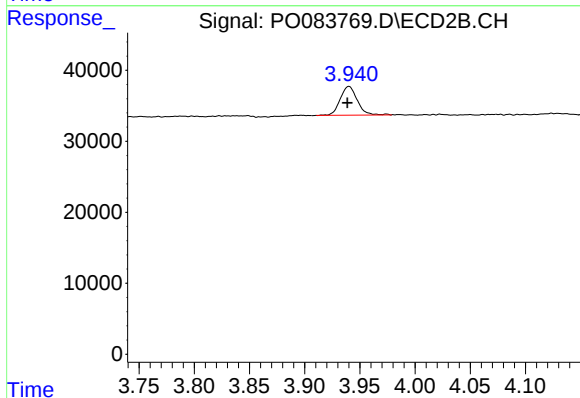


#1 Tetrachloro-m-xylene

R.T.: 3.940 min
Delta R.T.: 0.002 min
Response: 43541
Conc: 1.48 ng/ml

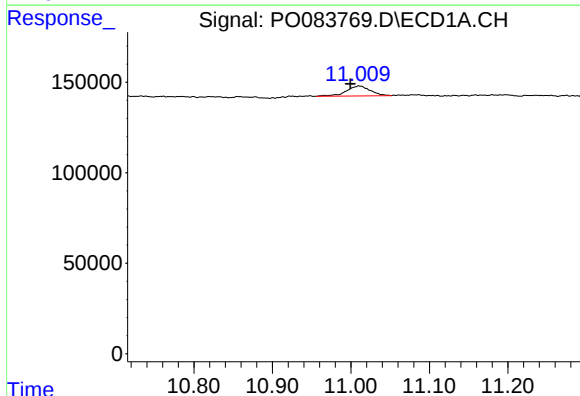


#2 Decachlorobiphenyl

R.T.: 11.010 min
Delta R.T.: 0.010 min
Response: 115686
Conc: 1.69 ng/ml

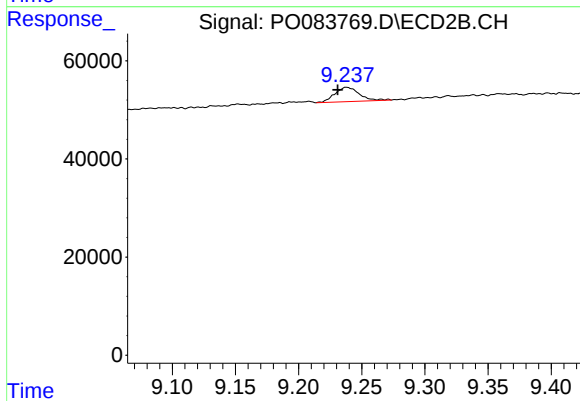

#2 Decachlorobiphenyl


R.T.: 9.238 min
Delta R.T.: 0.007 min
Response: 39327
Conc: 1.40 ng/ml

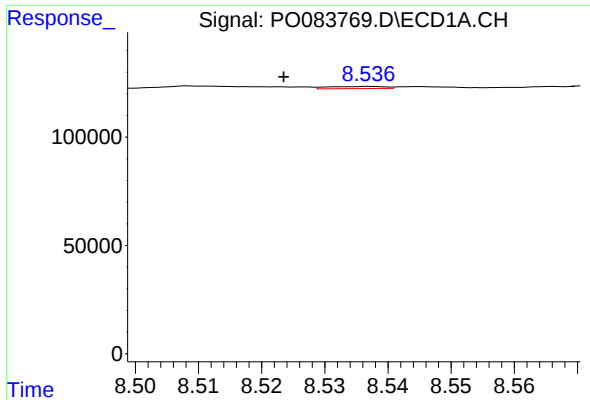

#30 AR-1254-5

R.T.: 8.537 min
Delta R.T.: 0.014 min
Response: 6239
Conc: 1.75 ng/ml

Instrument :
ECD_O
ClientSampleId :
CLI-2021-11-B

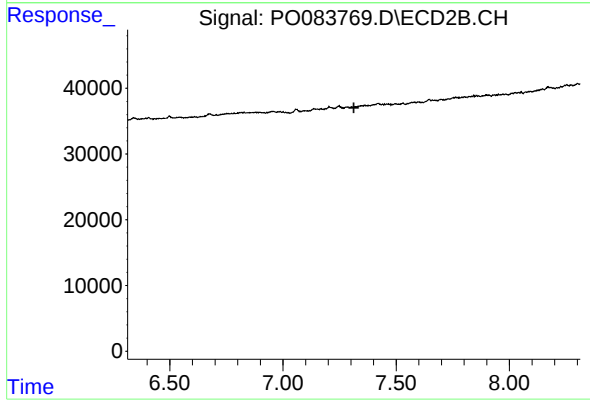

#30 AR-1254-5

R.T.: 0.000 min
Exp R.T. : 7.313 min
Response: 0
Conc: N.D.