

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO121621\
 Data File : PO083776.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 16 Dec 2021 22:01
 Operator : AJ\MA
 Sample : M5070-09 10X
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 CLI-2021-12-B

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 17 01:37:53 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO121521.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Dec 16 04:05:27 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.935	3.941	121218	44540	1.272	1.518
2) SA Decachlor...	11.011	9.237	115049	44944	1.680	1.601
Target Compounds						
24) L5 AR-1248-4	7.188f	0.000	27193	0	9.235	N.D. #
26) L6 AR-1254-1	7.188	0.000	27193	0	8.829	N.D. #
29) L6 AR-1254-4	8.110f	0.000	11737	0	3.434	N.D. #
30) L6 AR-1254-5	8.511	0.000	29510	0	8.278	N.D. #
32) L7 AR-1260-2	8.234	0.000	15896	0	4.104	N.D. #
33) L7 AR-1260-3	8.587	0.000	9212	0	3.110	N.D. #
34) L7 AR-1260-4	8.851f	0.000	16891	0	4.938	N.D. #
36) L8 AR-1262-1	8.587	0.000	9212	0	2.284	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO121621\
Data File : P0083776.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 16 Dec 2021 22:01
Operator : AJ\MA
Sample : M5070-09 10X
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
CLI-2021-12-B

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 17 01:37:53 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO121521.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Dec 16 04:05:27 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

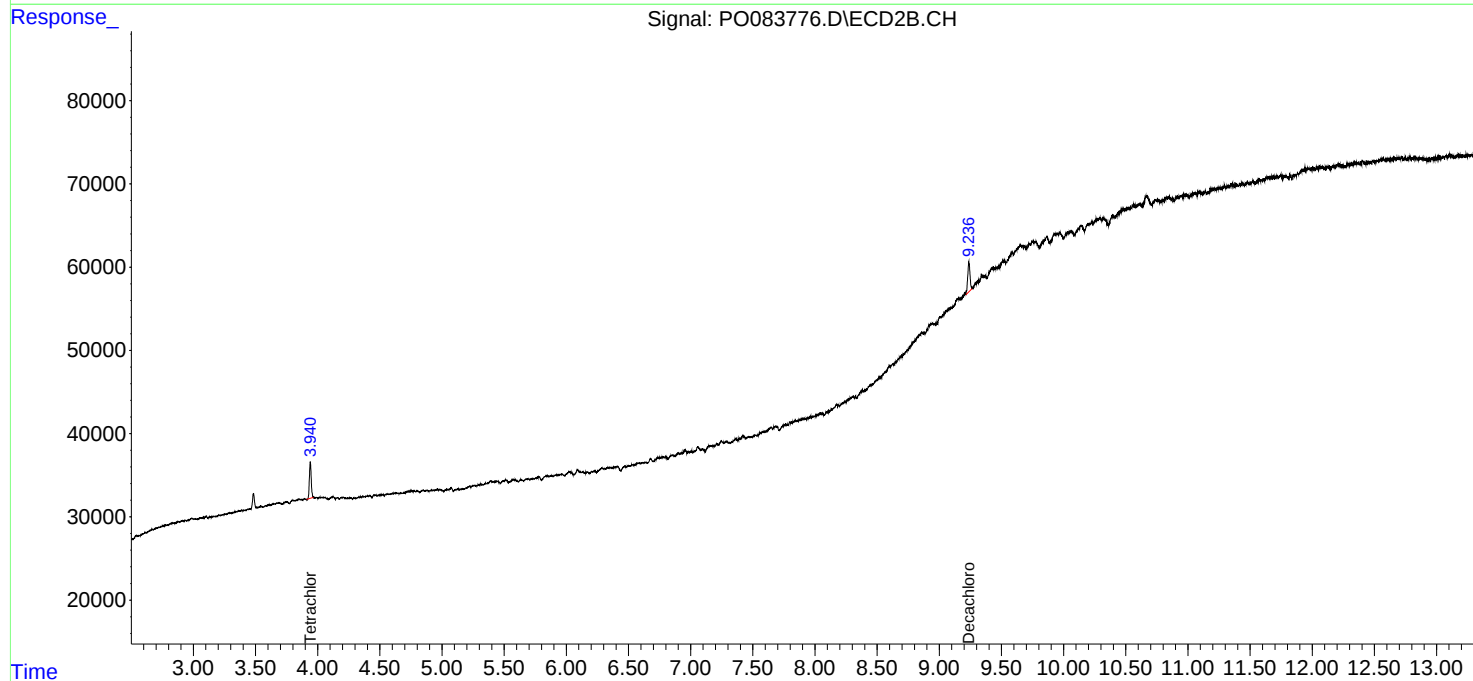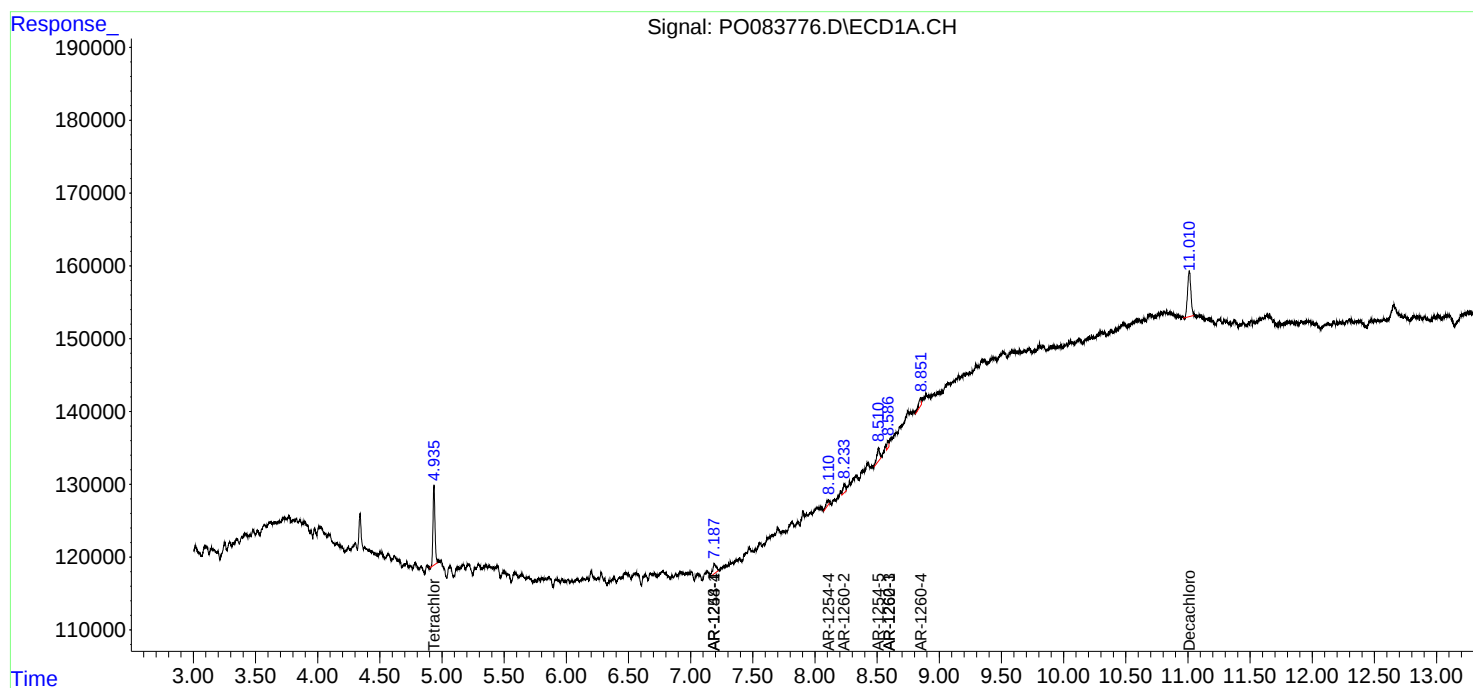


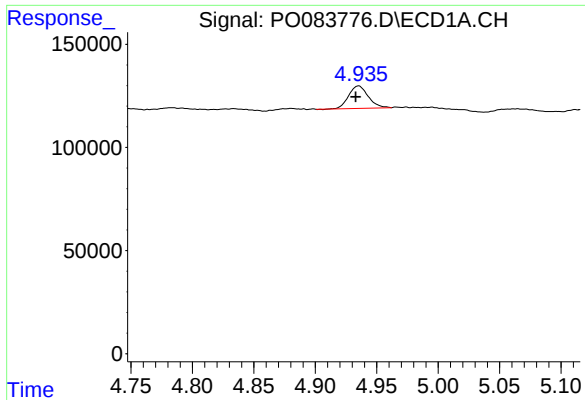

#1 Tetrachloro-m-xylene


R.T.: 4.935 min
Delta R.T.: 0.002 min
Response: 121218
Conc: 1.27 ng/ml

Instrument :
ECD_O
ClientSampleId :
CLI-2021-12-B

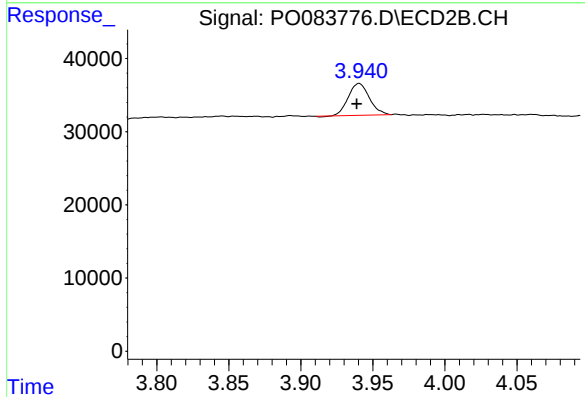


#1 Tetrachloro-m-xylene

R.T.: 3.941 min
Delta R.T.: 0.002 min
Response: 44540
Conc: 1.52 ng/ml

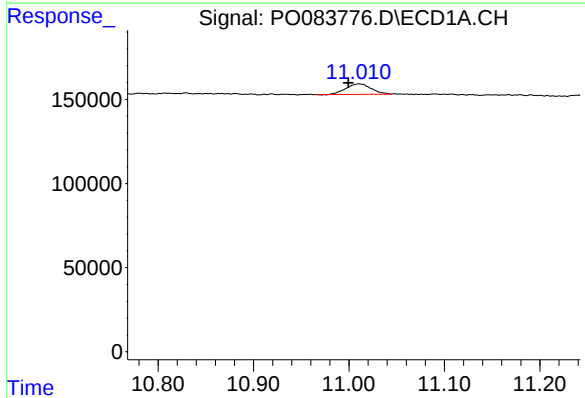


#2 Decachlorobiphenyl

R.T.: 11.011 min
Delta R.T.: 0.011 min
Response: 115049
Conc: 1.68 ng/ml

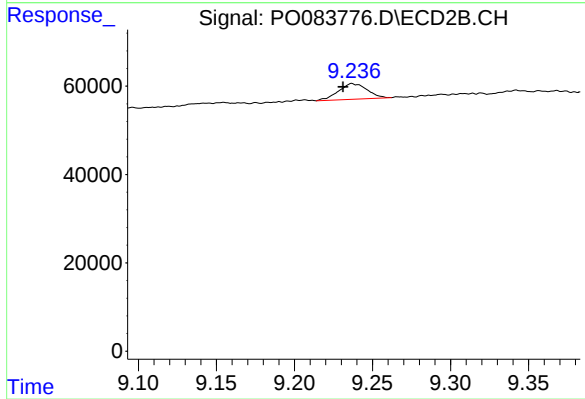

#2 Decachlorobiphenyl


R.T.: 9.237 min
Delta R.T.: 0.006 min
Response: 44944
Conc: 1.60 ng/ml

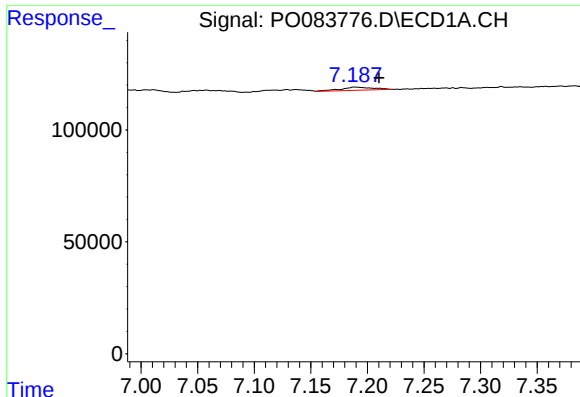

#24 AR-1248-4


R.T.: 7.188 min
Delta R.T.: -0.022 min
Response: 27193
Conc: 9.24 ng/ml

Instrument :
ECD_O
ClientSampleId :
CLI-2021-12-B

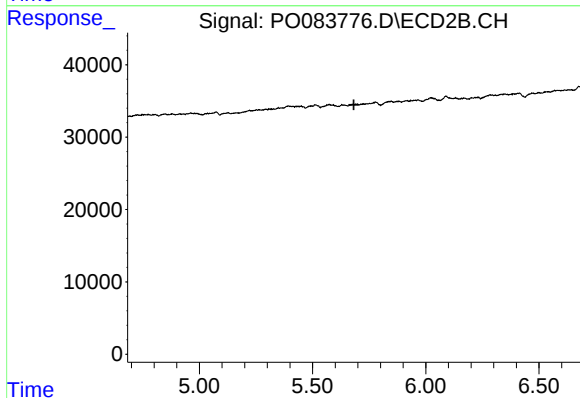


#24 AR-1248-4

R.T.: 0.000 min
Exp R.T. : 5.683 min
Response: 0
Conc: N.D.

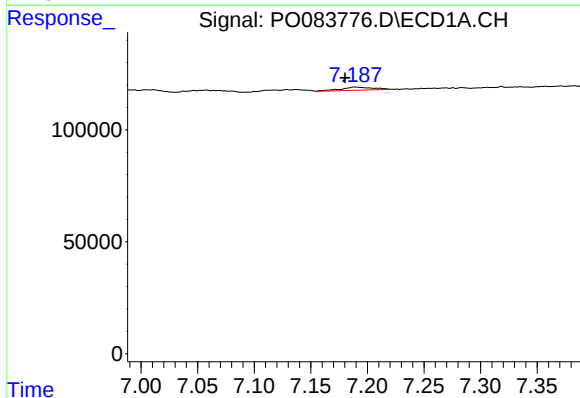


#26 AR-1254-1

R.T.: 7.188 min
Delta R.T.: 0.008 min
Response: 27193
Conc: 8.83 ng/ml

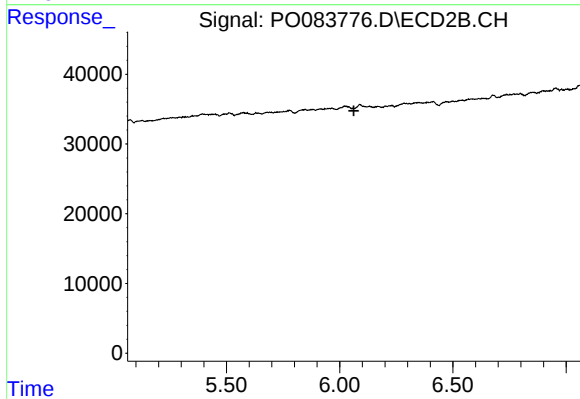

#26 AR-1254-1


R.T.: 0.000 min
Exp R.T. : 6.063 min
Response: 0
Conc: N.D.

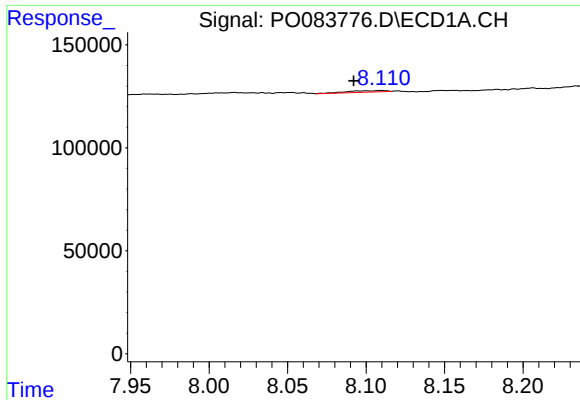

#29 AR-1254-4


R.T.: 8.110 min
Delta R.T.: 0.018 min
Response: 11737
Conc: 3.43 ng/ml

Instrument :
ECD_O
ClientSampleId :
CLI-2021-12-B

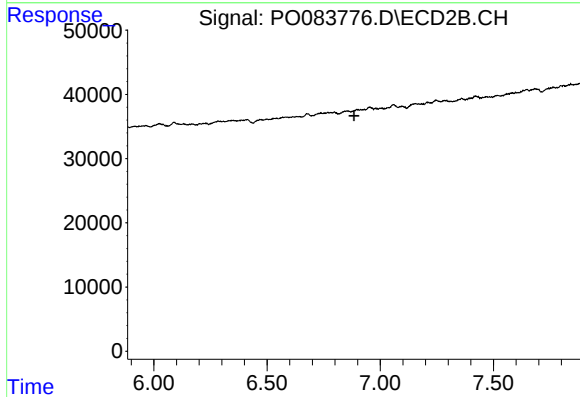


#29 AR-1254-4

R.T.: 0.000 min
Exp R.T. : 6.884 min
Response: 0
Conc: N.D.

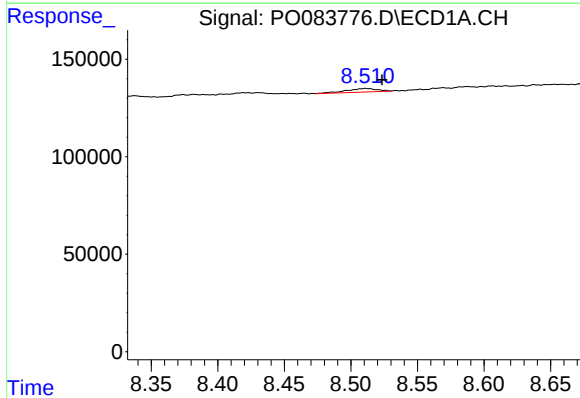


#30 AR-1254-5

R.T.: 8.511 min
Delta R.T.: -0.013 min
Response: 29510
Conc: 8.28 ng/ml

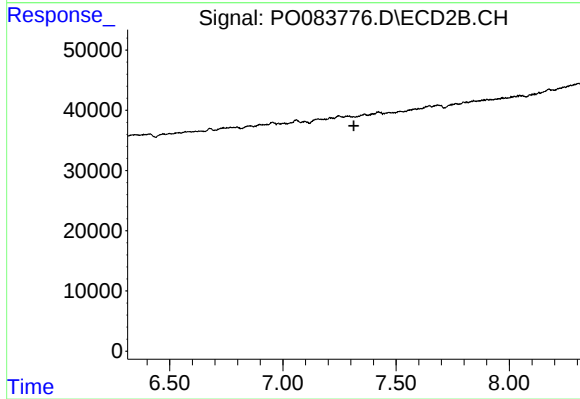

#30 AR-1254-5


R.T.: 0.000 min
Exp R.T. : 7.313 min
Response: 0
Conc: N.D.

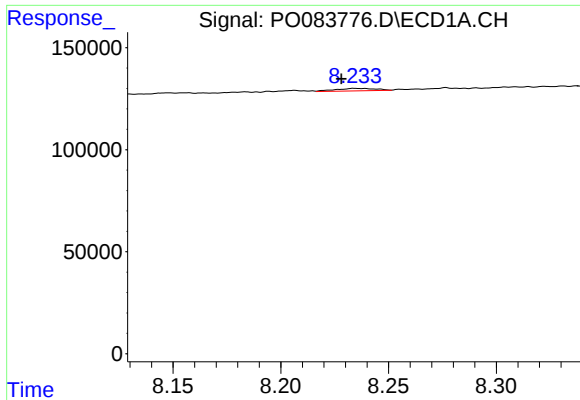

#32 AR-1260-2


R.T.: 8.234 min
Delta R.T.: 0.006 min
Response: 15896
Conc: 4.10 ng/ml

Instrument :
ECD_O
ClientSampleId :
CLI-2021-12-B

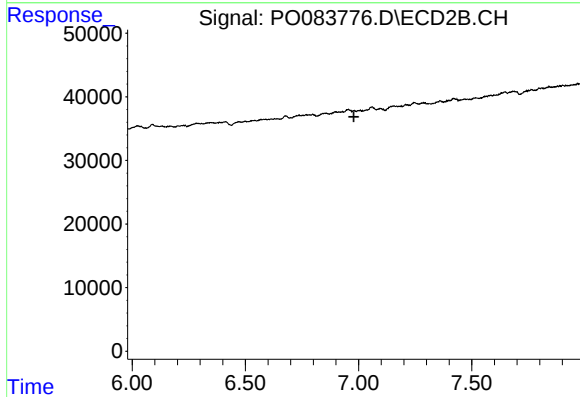


#32 AR-1260-2

R.T.: 0.000 min
Exp R.T. : 6.979 min
Response: 0
Conc: N.D.

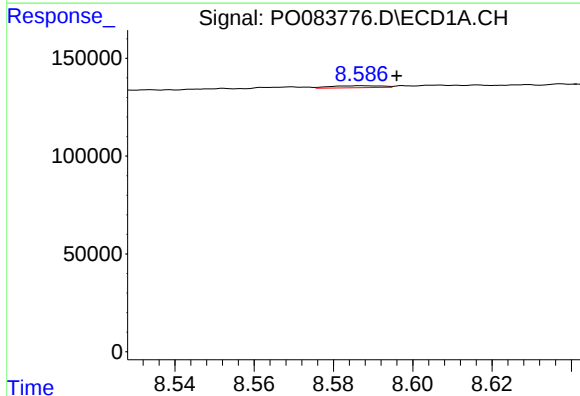


#33 AR-1260-3

R.T.: 8.587 min
Delta R.T.: -0.009 min
Response: 9212
Conc: 3.11 ng/ml

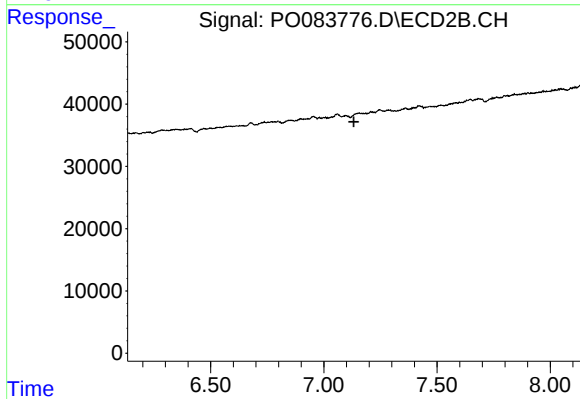

#33 AR-1260-3


R.T.: 0.000 min
Exp R.T. : 7.133 min
Response: 0
Conc: N.D.

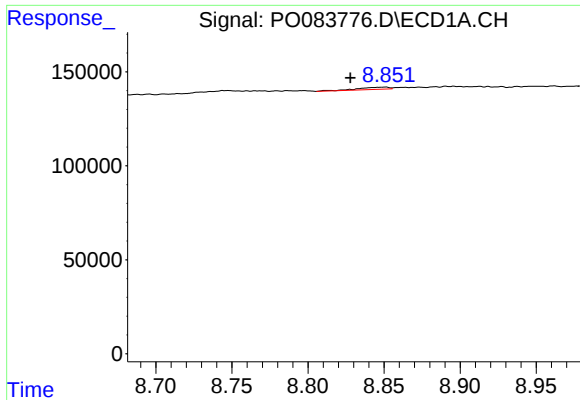

#34 AR-1260-4


R.T.: 8.851 min
Delta R.T.: 0.023 min
Response: 16891
Conc: 4.94 ng/ml

Instrument :
ECD_O
ClientSampleId :
CLI-2021-12-B

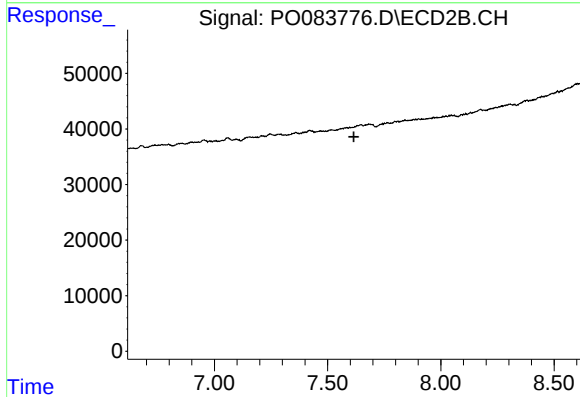


#34 AR-1260-4

R.T.: 0.000 min
Exp R.T. : 7.616 min
Response: 0
Conc: N.D.

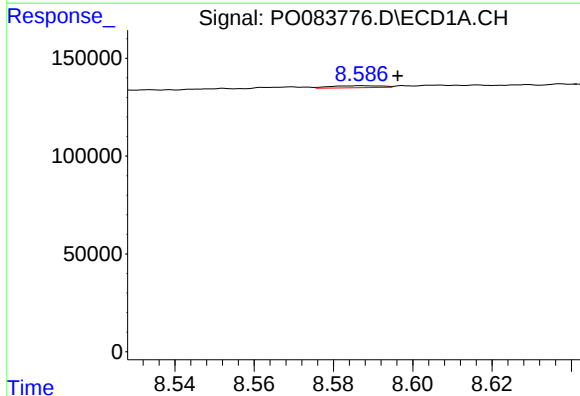

#36 AR-1262-1

R.T.: 8.587 min
Delta R.T.: -0.009 min
Response: 9212
Conc: 2.28 ng/ml

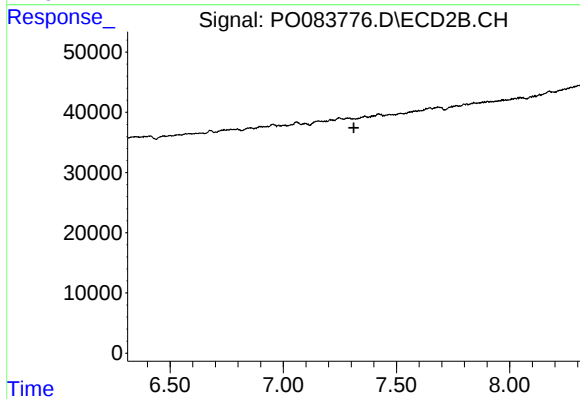

#36 AR-1262-1

R.T.: 0.000 min
Exp R.T. : 7.312 min
Response: 0
Conc: N.D.