

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO121621\
 Data File : PO083784.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 17 Dec 2021 00:19
 Operator : AJ\MA
 Sample : M5070-17 10X
 Misc :
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 CLI-2021-16-B

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 17 01:39:46 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO121521.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Dec 16 04:05:27 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.936	3.941	144190	46633	1.514	1.590
2) SA Decachlor...	11.013	9.238	113475	42930	1.657	1.529
Target Compounds						
30) L6 AR-1254-5	8.511	0.000	10666	0	2.992	N.D. #
32) L7 AR-1260-2	8.239	0.000	14104	0	3.641	N.D. #
33) L7 AR-1260-3	8.596	0.000	11684	0	3.944	N.D. #
34) L7 AR-1260-4	8.845f	0.000	13930	0	4.072	N.D. #
35) L7 AR-1260-5	9.157	0.000	21836	0	3.241	N.D. #
36) L8 AR-1262-1	8.596	0.000	11684	0	2.897	N.D. #
37) L8 AR-1262-2	9.157	0.000	21836	0	3.121	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\PO121621\
Data File : PO083784.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 17 Dec 2021 00:19
Operator : AJ\MA
Sample : M5070-17 10X
Misc :
ALS Vial : 41 Sample Multiplier: 1

Instrument :
ECD_0
ClientSampleId :
CLI-2021-16-B

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 17 01:39:46 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\PO121521.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Dec 16 04:05:27 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

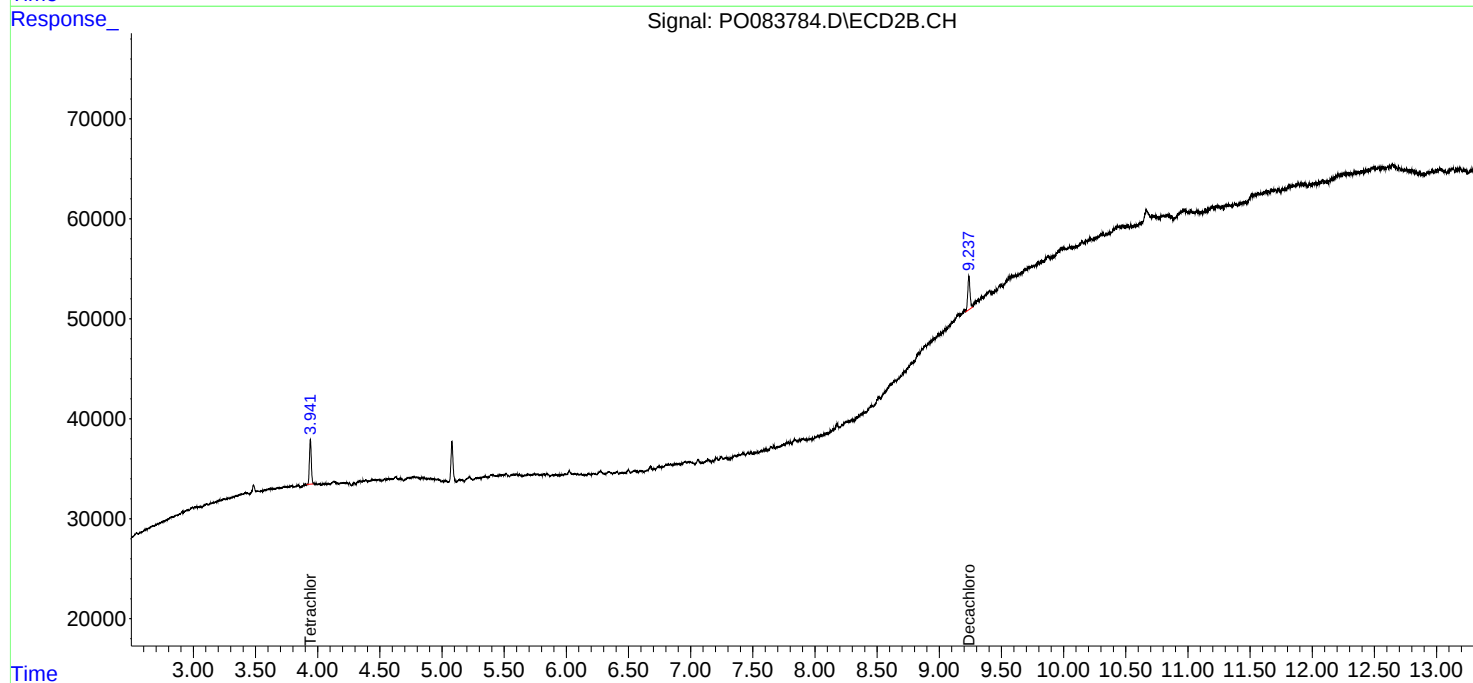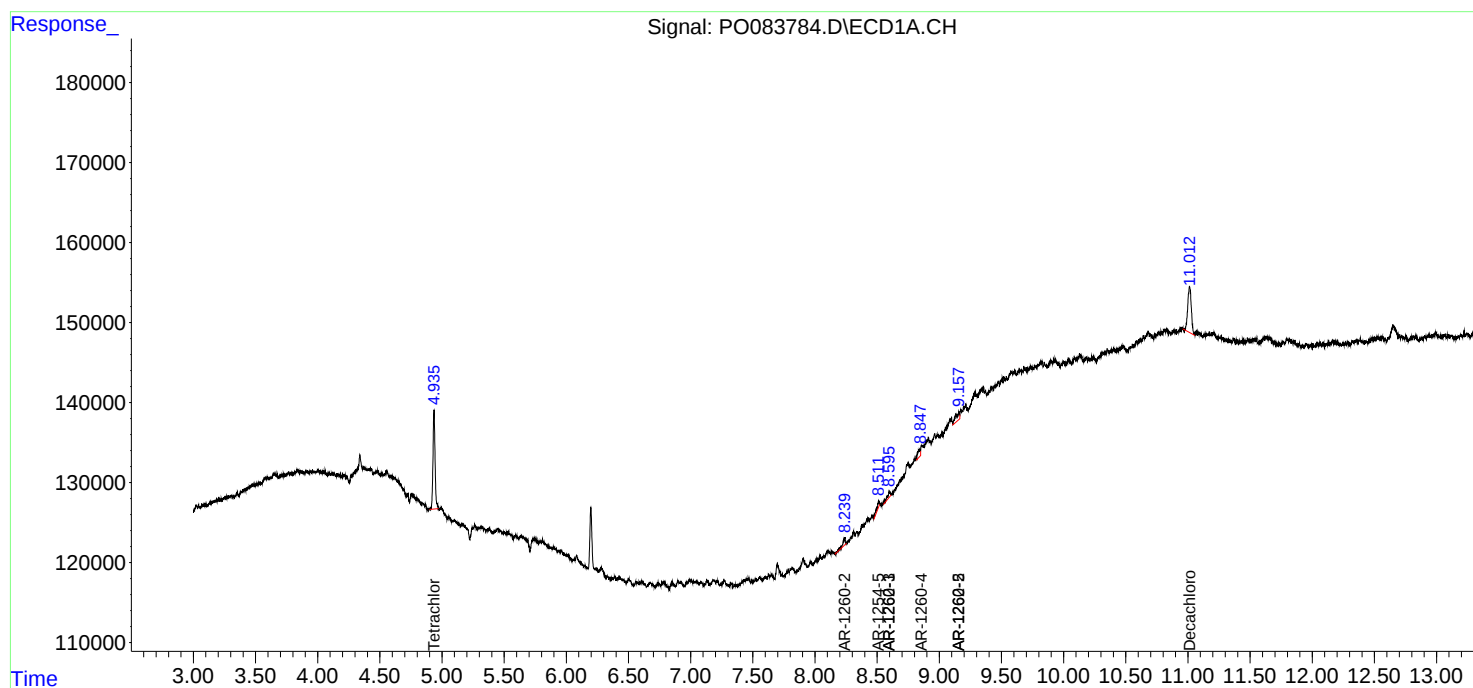


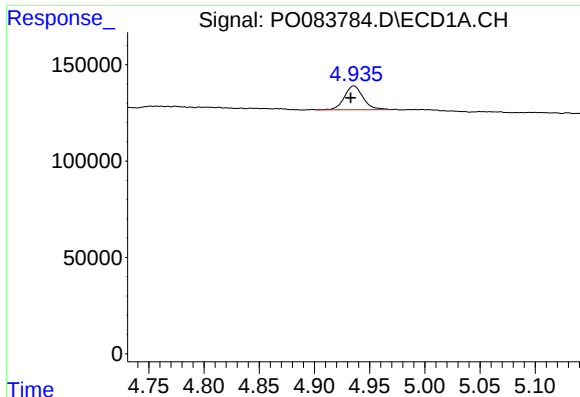

#1 Tetrachloro-m-xylene


R.T.: 4.936 min
Delta R.T.: 0.003 min
Response: 144190
Conc: 1.51 ng/ml

Instrument :
ECD_O
ClientSampleId :
CLI-2021-16-B

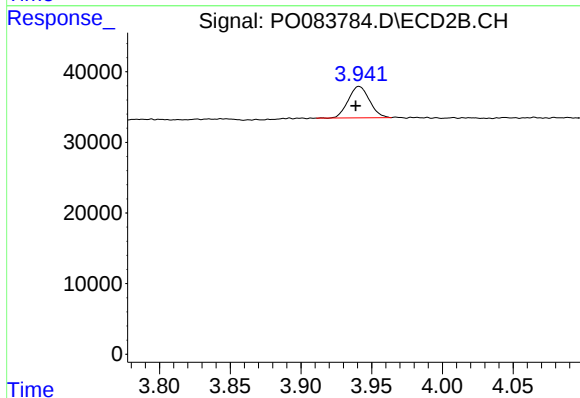


#1 Tetrachloro-m-xylene

R.T.: 3.941 min
Delta R.T.: 0.002 min
Response: 46633
Conc: 1.59 ng/ml

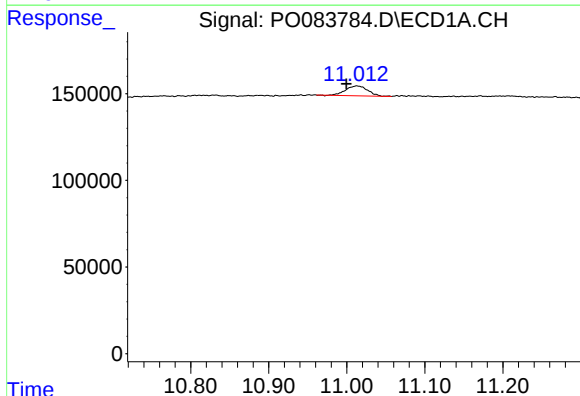


#2 Decachlorobiphenyl

R.T.: 11.013 min
Delta R.T.: 0.013 min
Response: 113475
Conc: 1.66 ng/ml

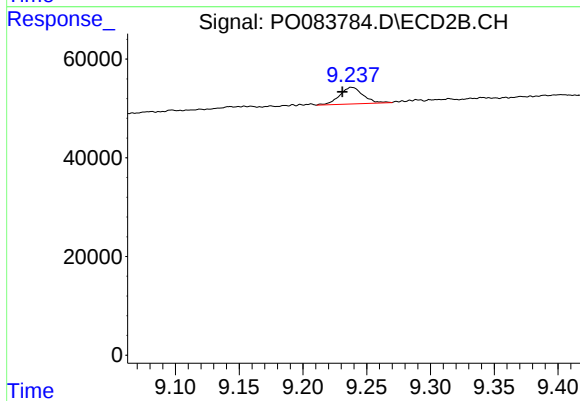

#2 Decachlorobiphenyl


R.T.: 9.238 min
Delta R.T.: 0.007 min
Response: 42930
Conc: 1.53 ng/ml

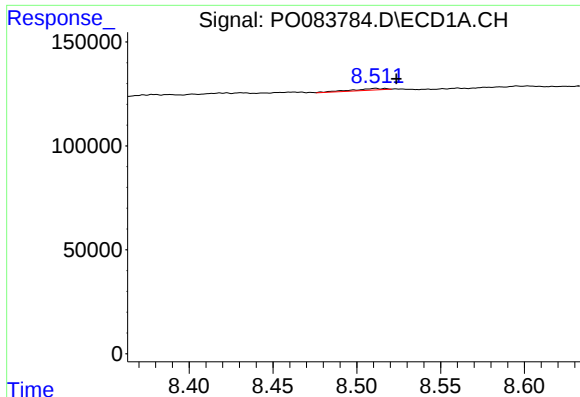

#30 AR-1254-5


R.T.: 8.511 min
Delta R.T.: -0.012 min
Response: 10666
Conc: 2.99 ng/ml

Instrument :
ECD_O
ClientSampleId :
CLI-2021-16-B

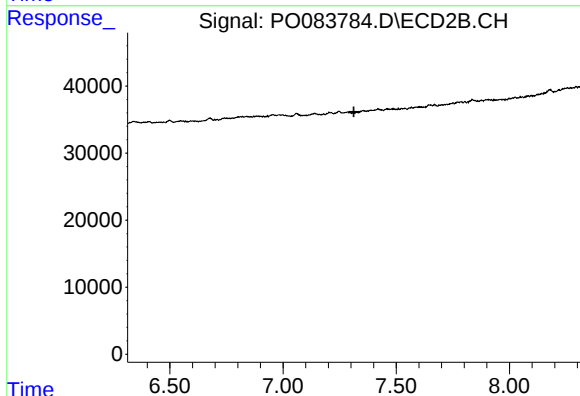


#30 AR-1254-5

R.T.: 0.000 min
Exp R.T. : 7.313 min
Response: 0
Conc: N.D.

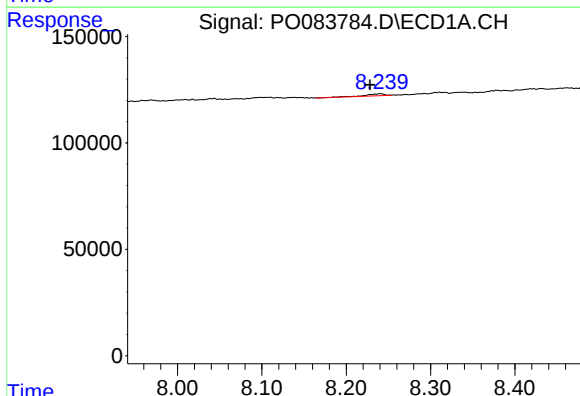


#32 AR-1260-2

R.T.: 8.239 min
Delta R.T.: 0.011 min
Response: 14104
Conc: 3.64 ng/ml

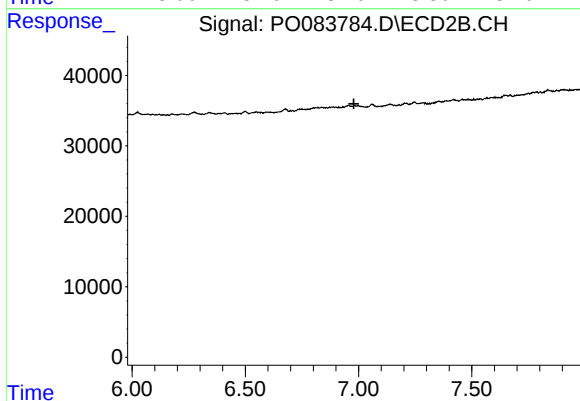

#32 AR-1260-2


R.T.: 0.000 min
Exp R.T. : 6.979 min
Response: 0
Conc: N.D.

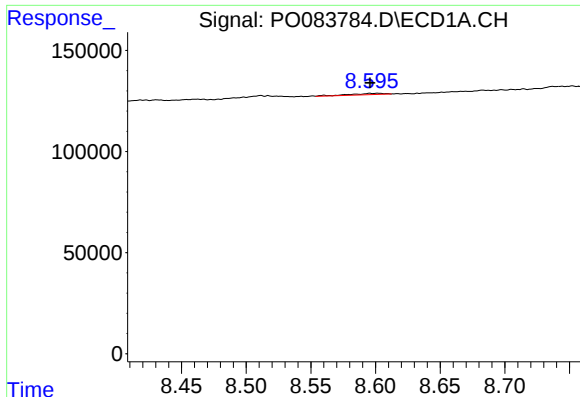

#33 AR-1260-3


R.T.: 8.596 min
Delta R.T.: 0.000 min
Response: 11684
Conc: 3.94 ng/ml

Instrument :
ECD_O
ClientSampleId :
CLI-2021-16-B

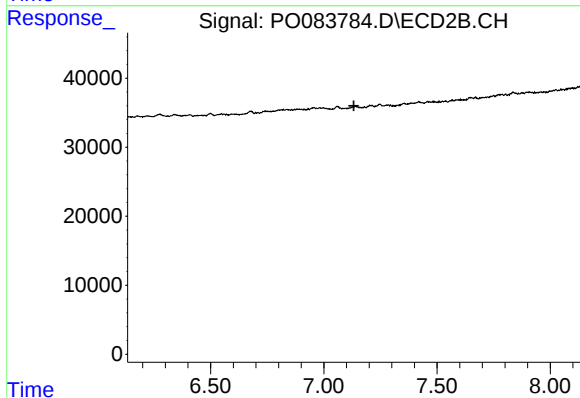


#33 AR-1260-3

R.T.: 0.000 min
Exp R.T. : 7.133 min
Response: 0
Conc: N.D.

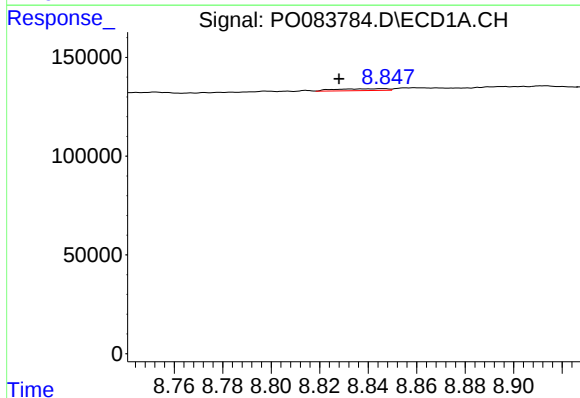


#34 AR-1260-4

R.T.: 8.845 min
Delta R.T.: 0.017 min
Response: 13930
Conc: 4.07 ng/ml

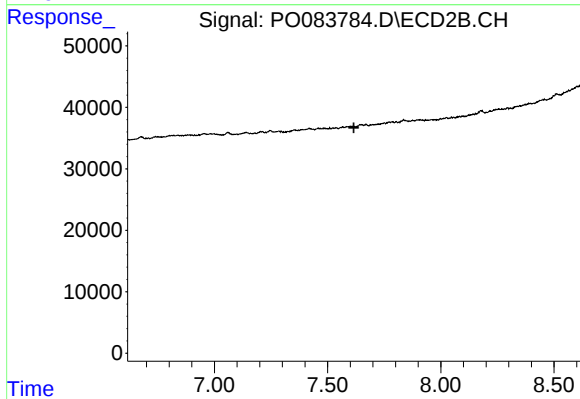

#34 AR-1260-4


R.T.: 0.000 min
Exp R.T. : 7.616 min
Response: 0
Conc: N.D.

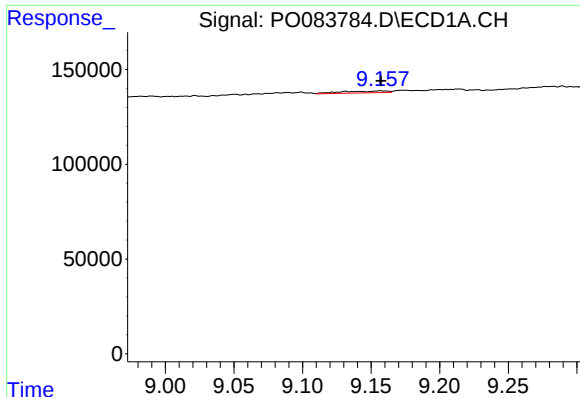

#35 AR-1260-5


R.T.: 9.157 min
Delta R.T.: 0.000 min
Response: 21836
Conc: 3.24 ng/ml

Instrument :
ECD_O
ClientSampleId :
CLI-2021-16-B

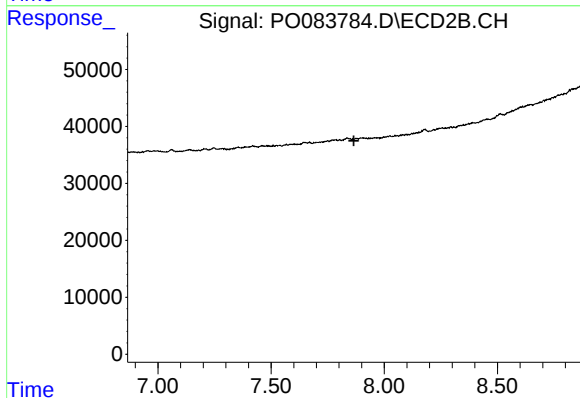


#35 AR-1260-5

R.T.: 0.000 min
Exp R.T. : 7.866 min
Response: 0
Conc: N.D.

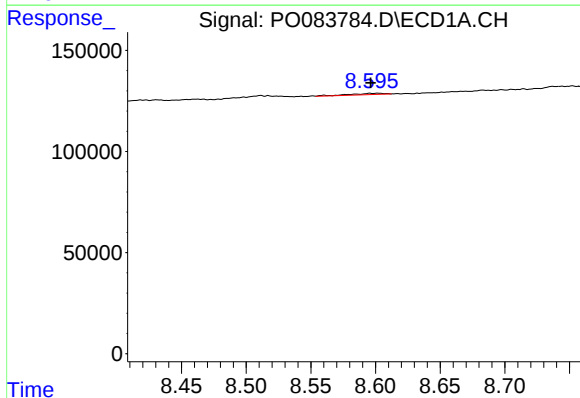


#36 AR-1262-1

R.T.: 8.596 min
Delta R.T.: 0.000 min
Response: 11684
Conc: 2.90 ng/ml

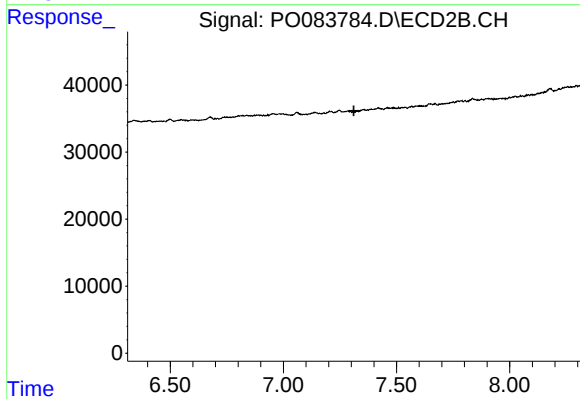

#36 AR-1262-1


R.T.: 0.000 min
Exp R.T. : 7.312 min
Response: 0
Conc: N.D.

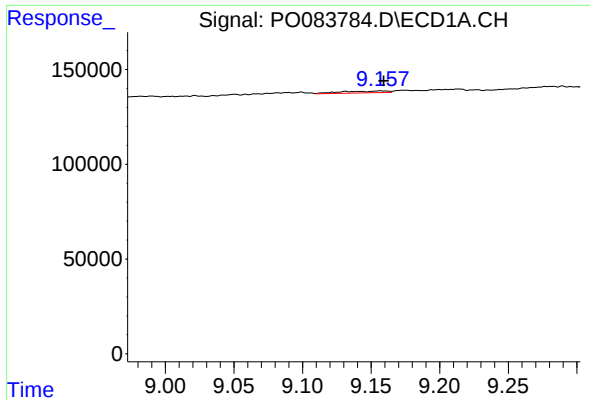

#37 AR-1262-2

R.T.: 9.157 min
Delta R.T.: -0.002 min
Response: 21836
Conc: 3.12 ng/ml

Instrument :
ECD_O
ClientSampleId :
CLI-2021-16-B

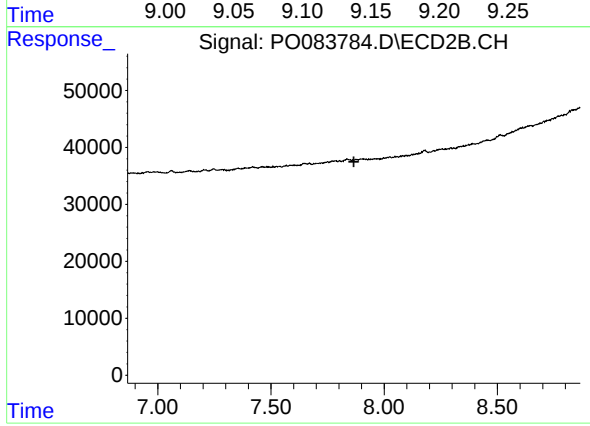

#37 AR-1262-2

R.T.: 0.000 min
Exp R.T. : 7.866 min
Response: 0
Conc: N.D.