

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO121621\
 Data File : P0083792.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 17 Dec 2021 3:12
 Operator : AJ\MA
 Sample : M5070-20 10X
 Misc :
 ALS Vial : 44 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 CLI-2021-18-A

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 17 03:35:37 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO121521.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Dec 16 04:05:27 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.938	3.944	135358	44265	1.421	1.509
2)	SA Decachlor...	11.014	9.241	139113	36205	2.031	1.289 #
Target Compounds							
27)	L6 AR-1254-2	7.413	0.000	9750	0	2.101	N.D. #
28)	L6 AR-1254-3	7.789	0.000	12628	0	2.708	N.D. #
29)	L6 AR-1254-4	8.117f	0.000	11914	0	3.485	N.D. #
30)	L6 AR-1254-5	8.515	0.000	34898	0	9.789	N.D. #
33)	L7 AR-1260-3	8.598	0.000	4182	0	1.412	N.D. #
34)	L7 AR-1260-4	8.845f	0.000	16474	0	4.816	N.D. #
35)	L7 AR-1260-5	9.138f	0.000	7749	0	1.150	N.D. #
36)	L8 AR-1262-1	8.598	0.000	4182	0	1.037	N.D. #
37)	L8 AR-1262-2	9.138f	0.000	7749	0	1.108	N.D. #
43)	L9 AR-1268-3	9.817f	0.000	11010	0	1.535	N.D. #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO121621\
Data File : P0083792.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 17 Dec 2021 3:12
Operator : AJ\MA
Sample : M5070-20 10X
Misc :
ALS Vial : 44 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
CLI-2021-18-A

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 17 03:35:37 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO121521.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Dec 16 04:05:27 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

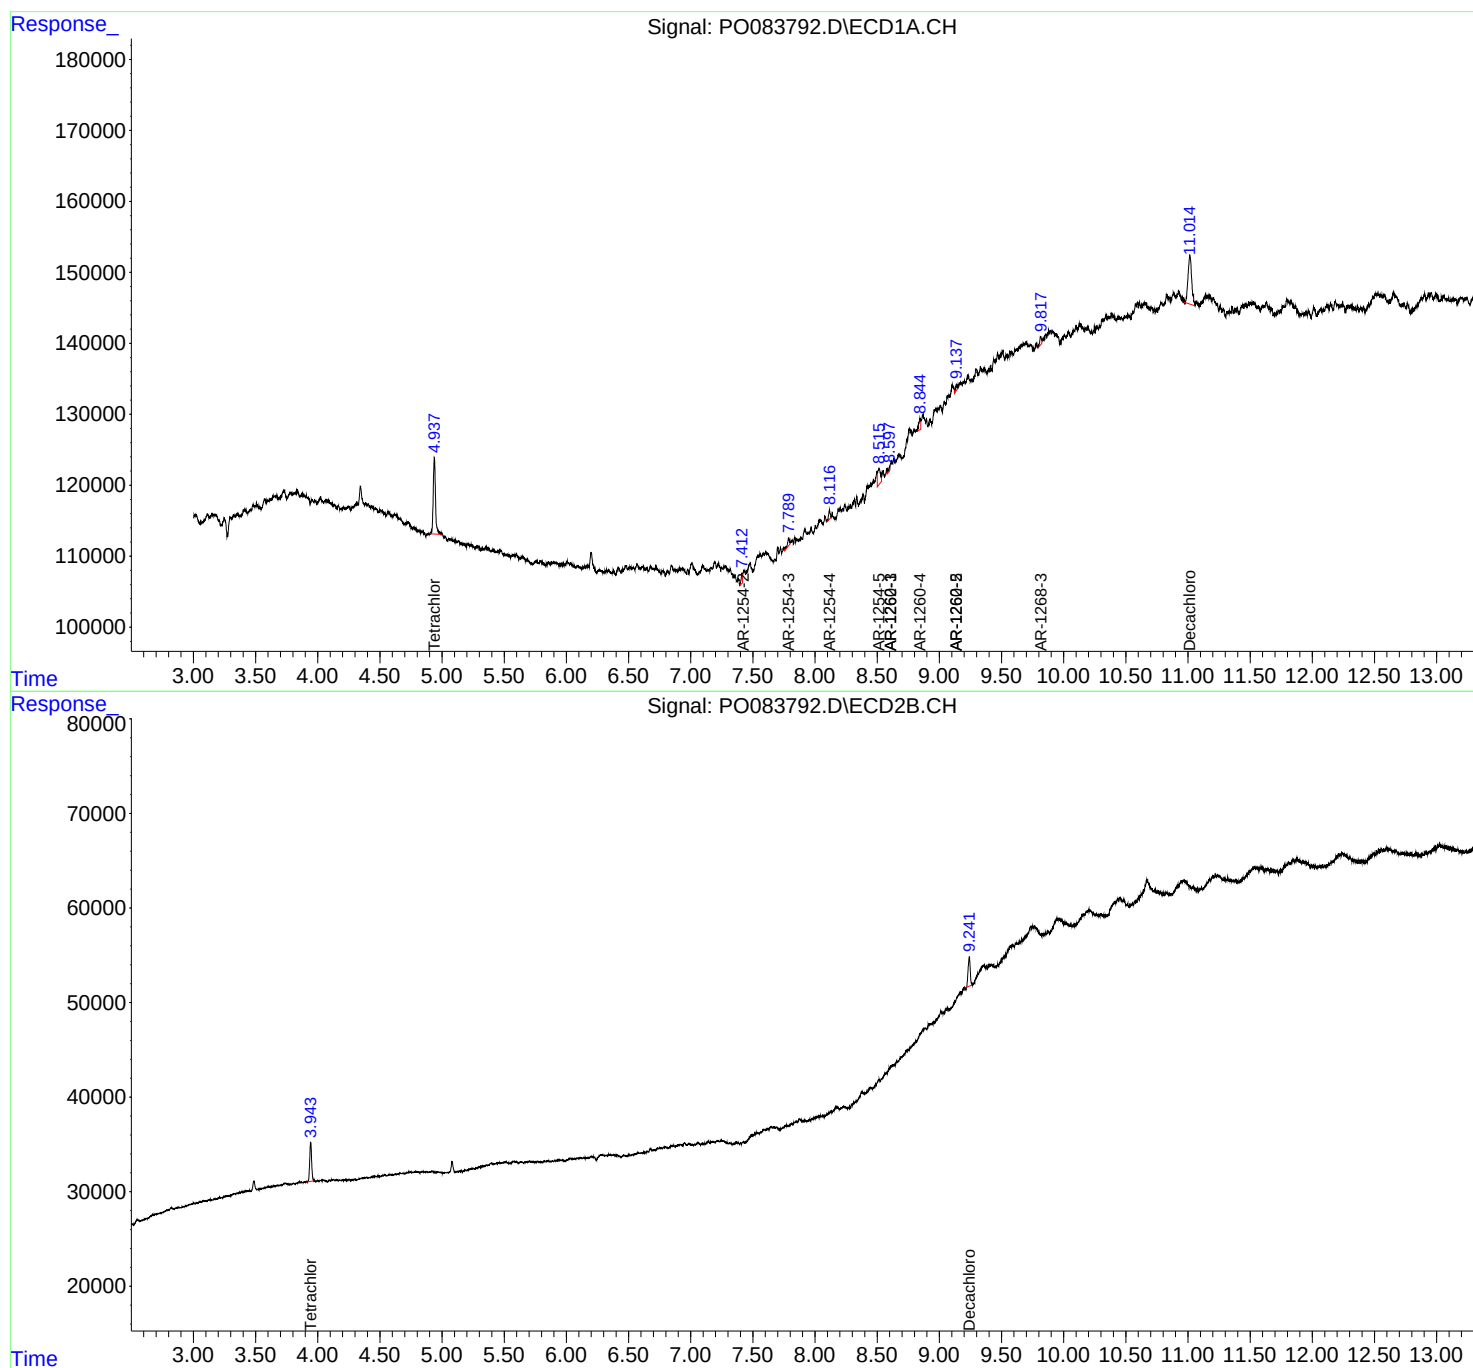


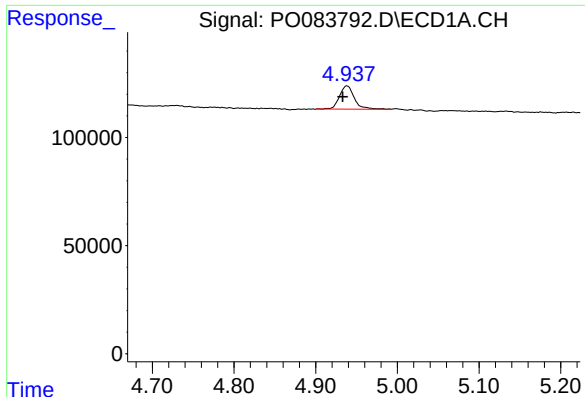

#1 Tetrachloro-m-xylene


R.T.: 4.938 min
Delta R.T.: 0.005 min
Response: 135358
Conc: 1.42 ng/ml

Instrument :
ECD_O
ClientSampleId :
CLI-2021-18-A

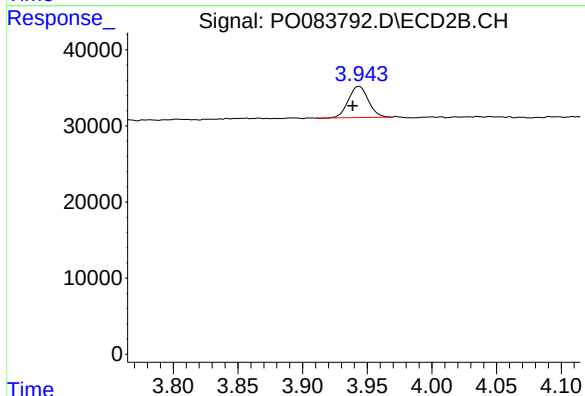


#1 Tetrachloro-m-xylene

R.T.: 3.944 min
Delta R.T.: 0.005 min
Response: 44265
Conc: 1.51 ng/ml

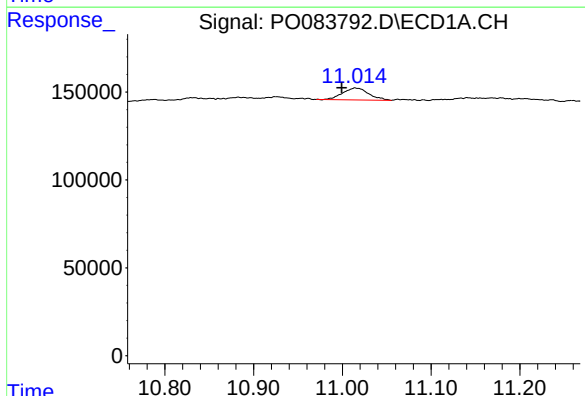


#2 Decachlorobiphenyl

R.T.: 11.014 min
Delta R.T.: 0.015 min
Response: 139113
Conc: 2.03 ng/ml

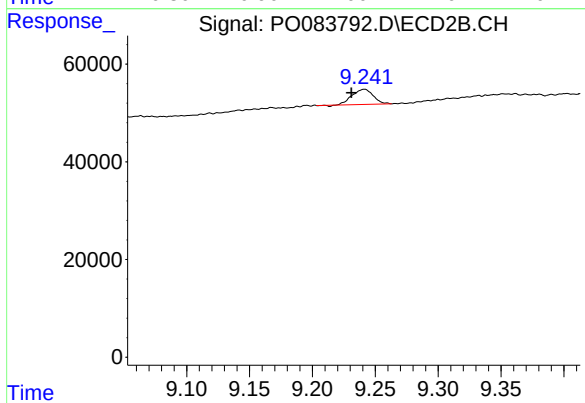

#2 Decachlorobiphenyl


R.T.: 9.241 min
Delta R.T.: 0.010 min
Response: 36205
Conc: 1.29 ng/ml

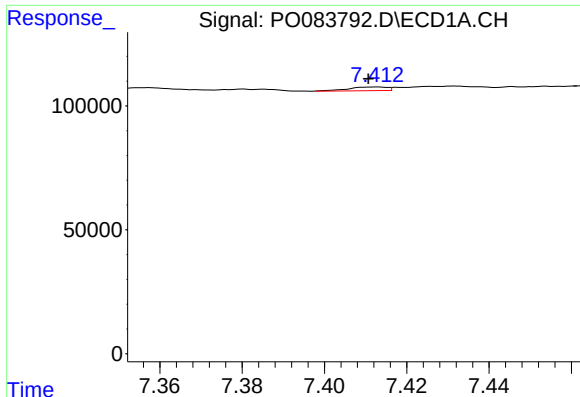

#27 AR-1254-2


R.T.: 7.413 min
Delta R.T.: 0.002 min
Response: 9750
Conc: 2.10 ng/ml

Instrument :
ECD_O
ClientSampleId :
CLI-2021-18-A

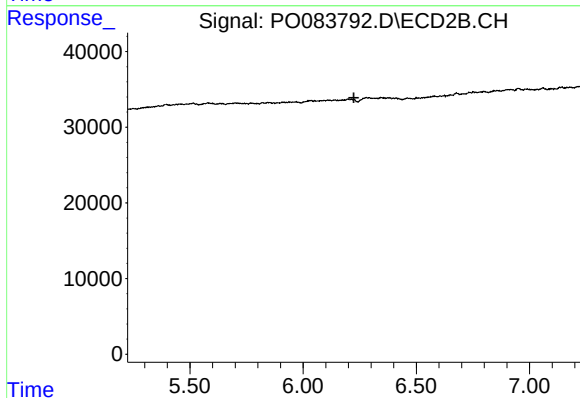


#27 AR-1254-2

R.T.: 0.000 min
Exp R.T. : 6.224 min
Response: 0
Conc: N.D.

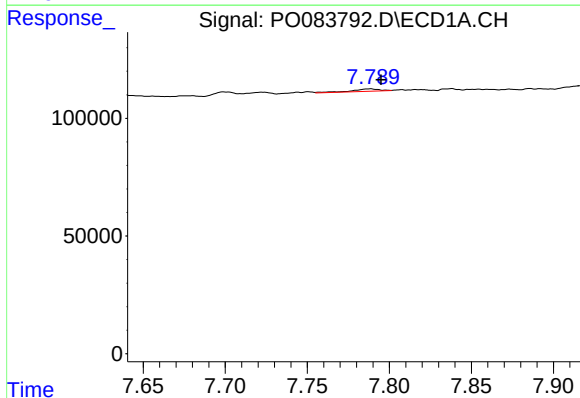


#28 AR-1254-3

R.T.: 7.789 min
Delta R.T.: -0.006 min
Response: 12628
Conc: 2.71 ng/ml

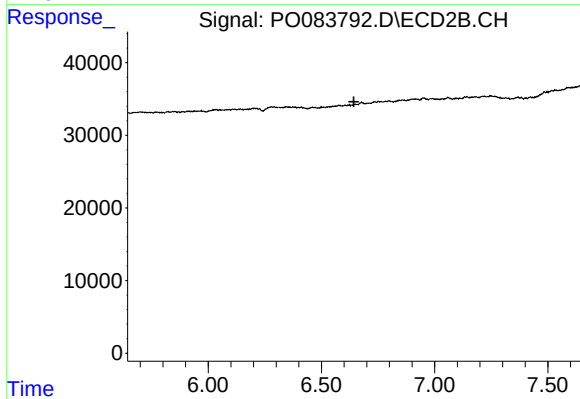

#28 AR-1254-3


R.T.: 0.000 min
Exp R.T. : 6.643 min
Response: 0
Conc: N.D.

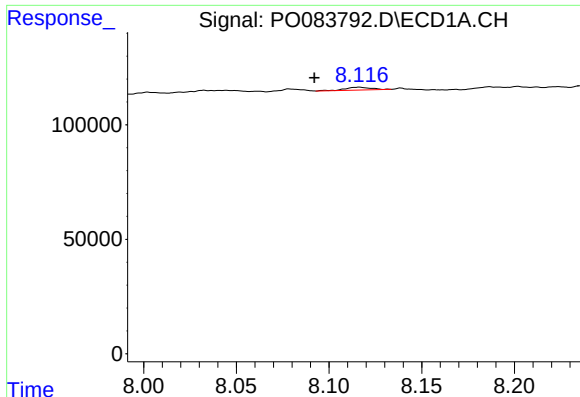

#29 AR-1254-4


R.T.: 8.117 min
Delta R.T.: 0.024 min
Response: 11914
Conc: 3.49 ng/ml

Instrument :
ECD_O
ClientSampleId :
CLI-2021-18-A

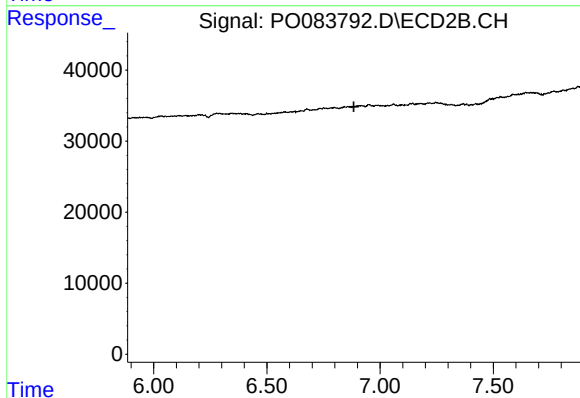


#29 AR-1254-4

R.T.: 0.000 min
Exp R.T. : 6.884 min
Response: 0
Conc: N.D.

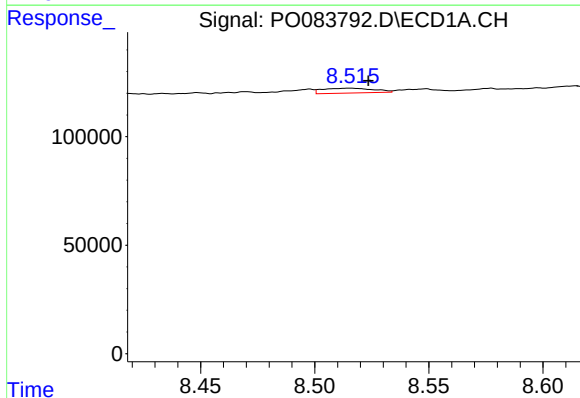


#30 AR-1254-5

R.T.: 8.515 min
Delta R.T.: -0.008 min
Response: 34898
Conc: 9.79 ng/ml

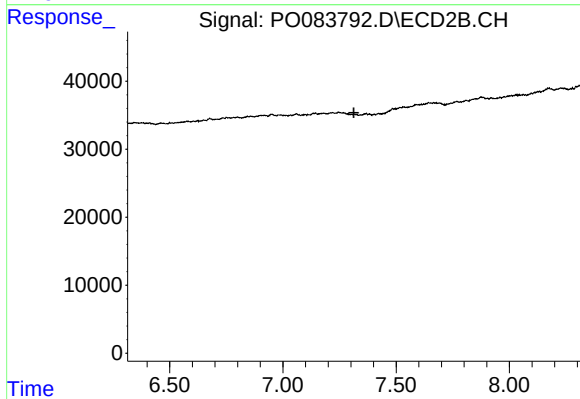

#30 AR-1254-5


R.T.: 0.000 min
Exp R.T. : 7.313 min
Response: 0
Conc: N.D.

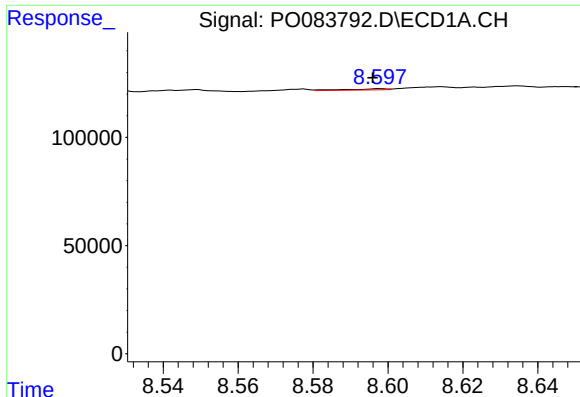

#33 AR-1260-3


R.T.: 8.598 min
Delta R.T.: 0.002 min
Response: 4182
Conc: 1.41 ng/ml

Instrument :
ECD_O
ClientSampleId :
CLI-2021-18-A

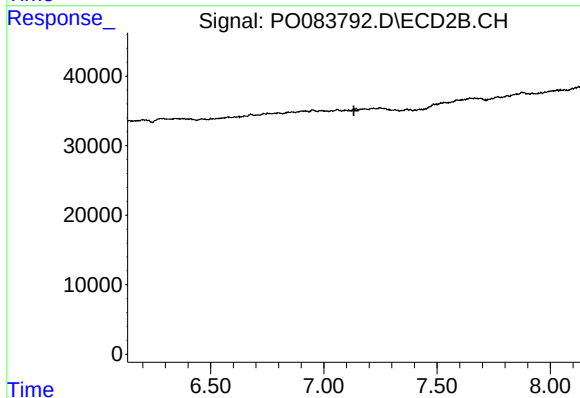


#33 AR-1260-3

R.T.: 0.000 min
Exp R.T. : 7.133 min
Response: 0
Conc: N.D.

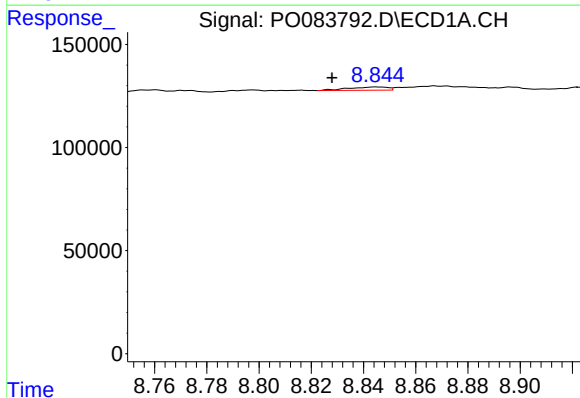


#34 AR-1260-4

R.T.: 8.845 min
Delta R.T.: 0.017 min
Response: 16474
Conc: 4.82 ng/ml

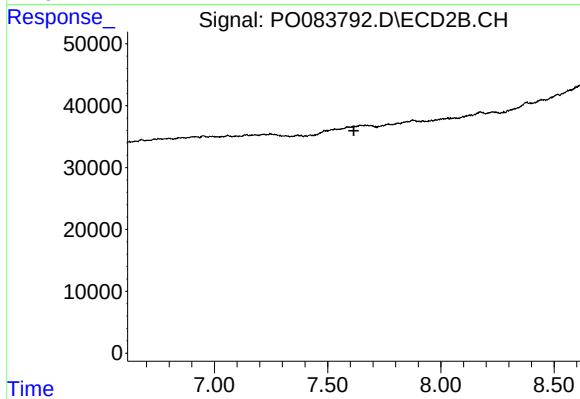

#34 AR-1260-4


R.T.: 0.000 min
Exp R.T. : 7.616 min
Response: 0
Conc: N.D.

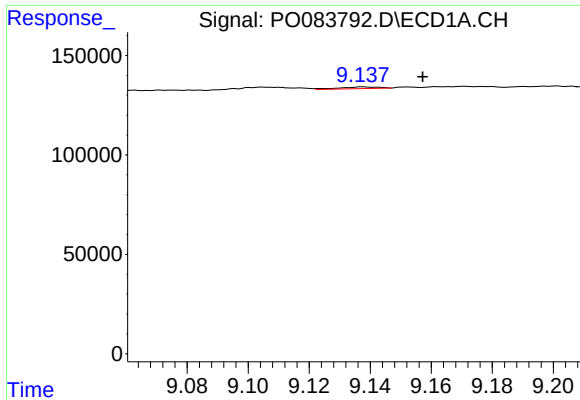

#35 AR-1260-5


R.T.: 9.138 min
Delta R.T.: -0.020 min
Response: 7749
Conc: 1.15 ng/ml

Instrument :
ECD_O
ClientSampleId :
CLI-2021-18-A

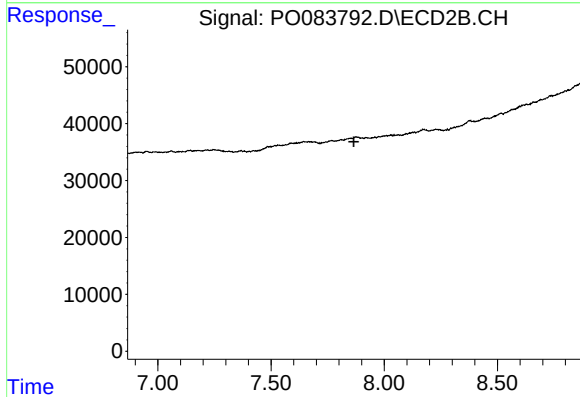


#35 AR-1260-5

R.T.: 0.000 min
Exp R.T. : 7.866 min
Response: 0
Conc: N.D.

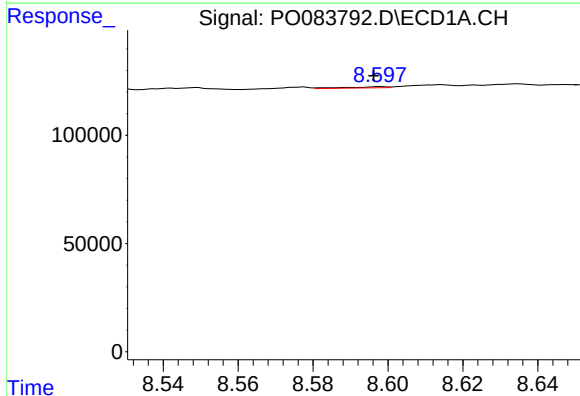


#36 AR-1262-1

R.T.: 8.598 min
Delta R.T.: 0.002 min
Response: 4182
Conc: 1.04 ng/ml

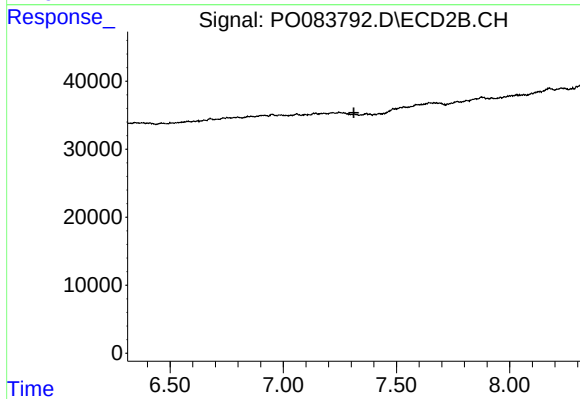

#36 AR-1262-1


R.T.: 0.000 min
Exp R.T. : 7.312 min
Response: 0
Conc: N.D.

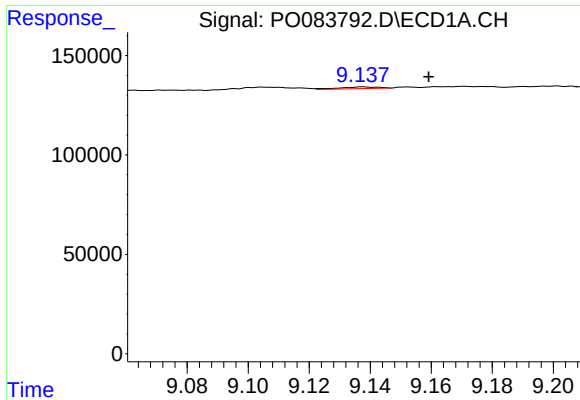

#37 AR-1262-2


R.T.: 9.138 min
Delta R.T.: -0.022 min
Response: 7749
Conc: 1.11 ng/ml

Instrument :
ECD_O
ClientSampleId :
CLI-2021-18-A

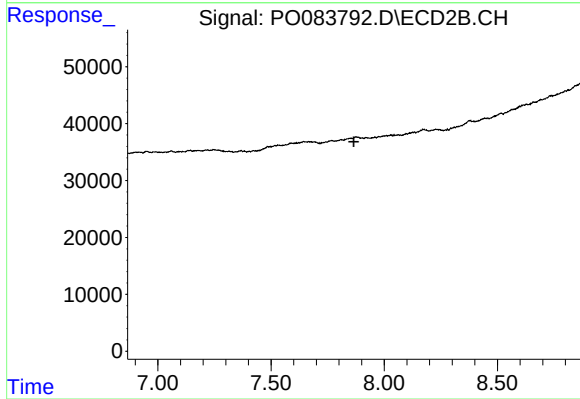


#37 AR-1262-2

R.T.: 0.000 min
Exp R.T. : 7.866 min
Response: 0
Conc: N.D.

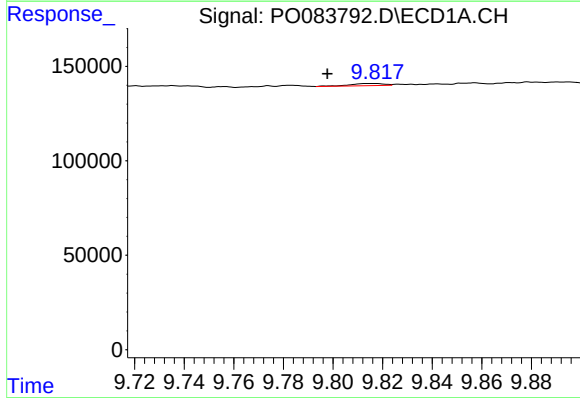

#43 AR-1268-3

R.T.: 9.817 min
Delta R.T.: 0.019 min
Response: 11010
Conc: 1.53 ng/ml

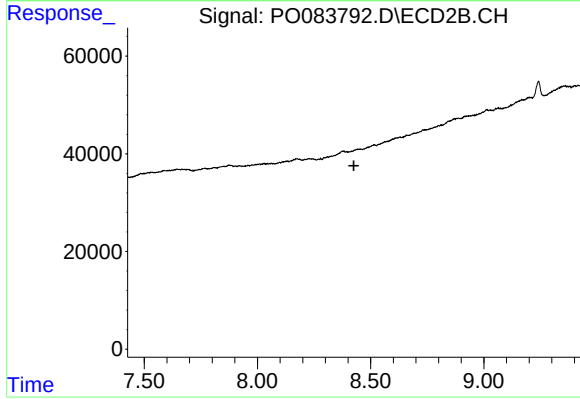

#43 AR-1268-3

R.T.: 0.000 min
Exp R.T. : 8.426 min
Response: 0
Conc: N.D.