

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO121621\
 Data File : P0083793.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 17 Dec 2021 3:30
 Operator : AJ\MA
 Sample : M5070-21 10X
 Misc :
 ALS Vial : 45 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 CLI-2021-19-A

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 17 04:45:29 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO121521.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Dec 16 04:05:27 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.936	3.941	146035	51340	1.533	1.750
2)	SA Decachlor...	11.014	9.239	167768	48394	2.449	1.723 #
Target Compounds							
28)	L6 AR-1254-3	7.812f	0.000	74357	0	15.947	N.D. #
29)	L6 AR-1254-4	8.120f	0.000	53369	0	15.613	N.D. #
30)	L6 AR-1254-5	8.511	0.000	41365	0	11.603	N.D. #
31)	L7 AR-1260-1	7.978f	0.000	11161	0	3.445	N.D. #
32)	L7 AR-1260-2	8.237	0.000	19493	0	5.032	N.D. #
33)	L7 AR-1260-3	8.592	0.000	8672	0	2.927	N.D. #
35)	L7 AR-1260-5	9.144	0.000	33845	0	5.023	N.D. #
36)	L8 AR-1262-1	8.592	0.000	8672	0	2.150	N.D. #
37)	L8 AR-1262-2	9.144	0.000	33845	0	4.837	N.D. #
39)	L8 AR-1262-4	9.580	0.000	26263	0	13.204	N.D. #
42)	L9 AR-1268-2	9.580	0.000	26263	0	3.129	N.D. #
45)	L9 AR-1268-5	10.681	0.000	17508	0	0.707	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO121621\
Data File : P0083793.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 17 Dec 2021 3:30
Operator : AJ\MA
Sample : M5070-21 10X
Misc :
ALS Vial : 45 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
CLI-2021-19-A

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 17 04:45:29 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO121521.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Dec 16 04:05:27 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

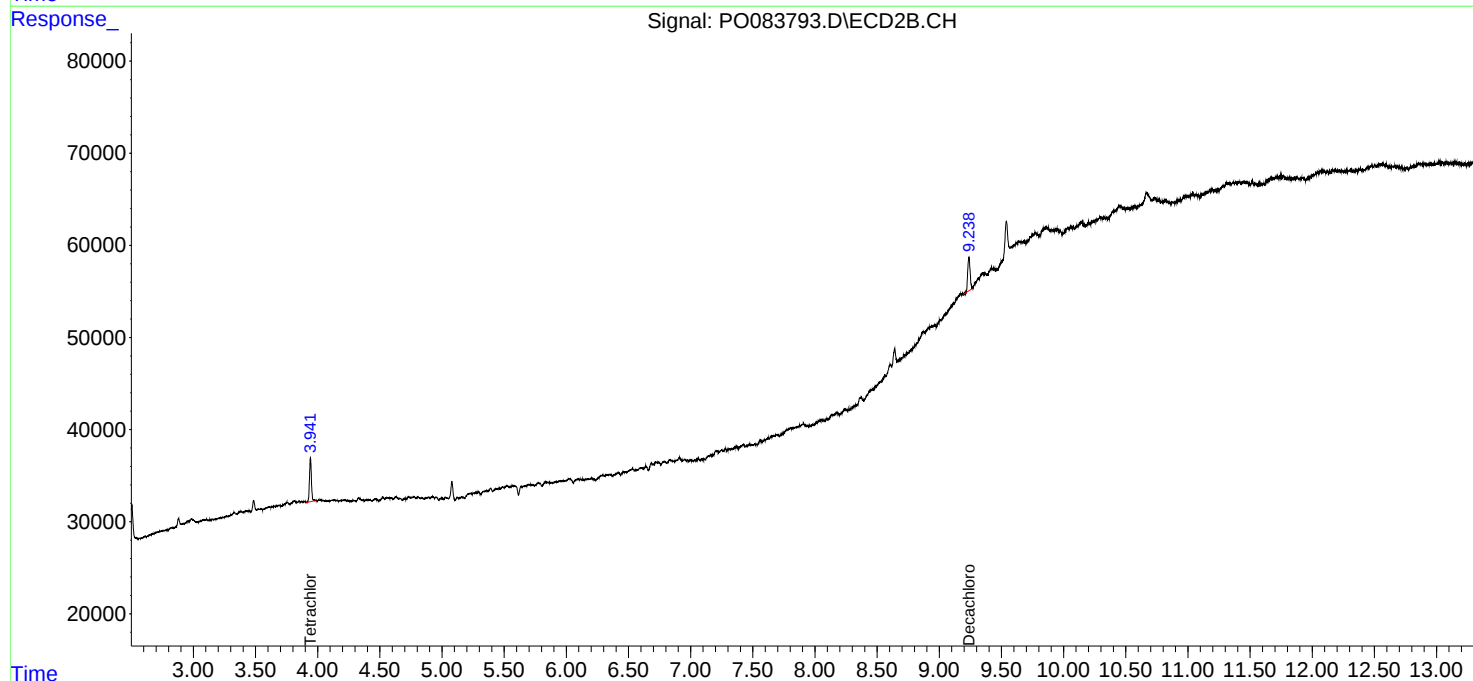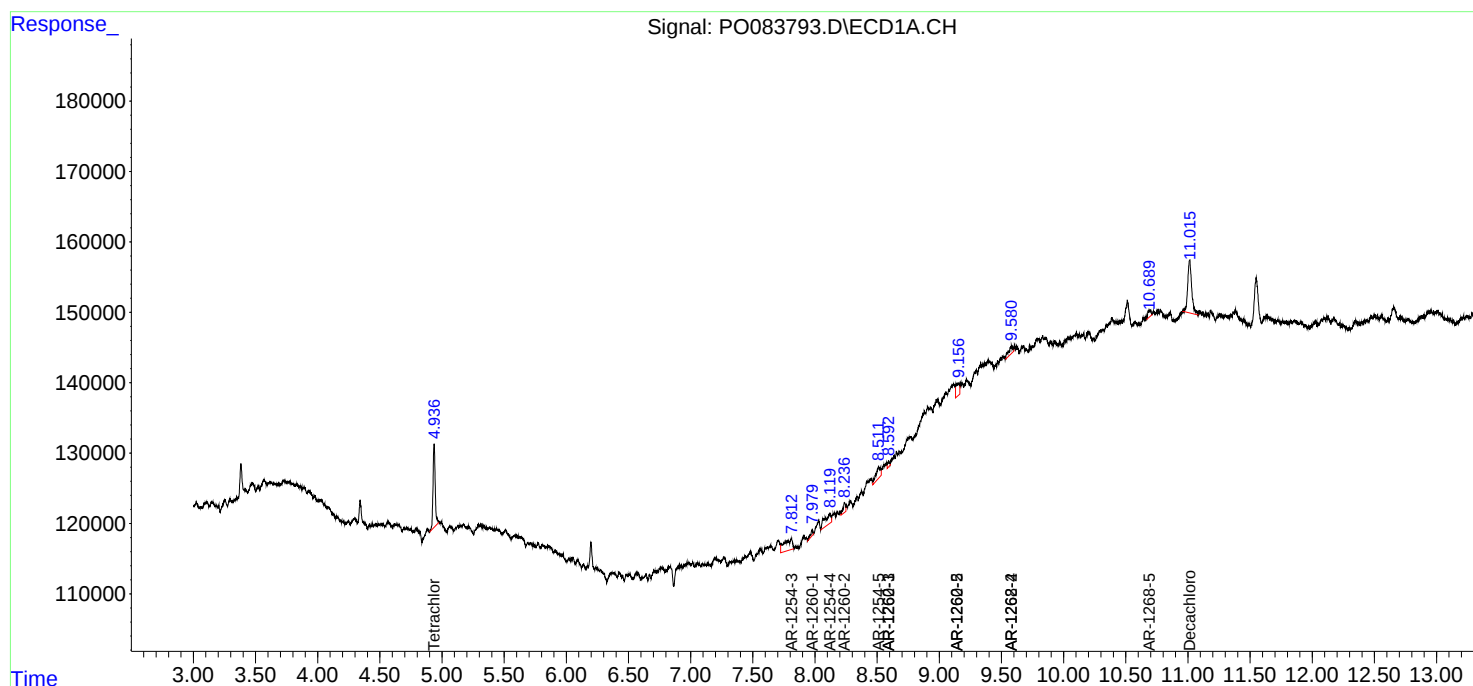


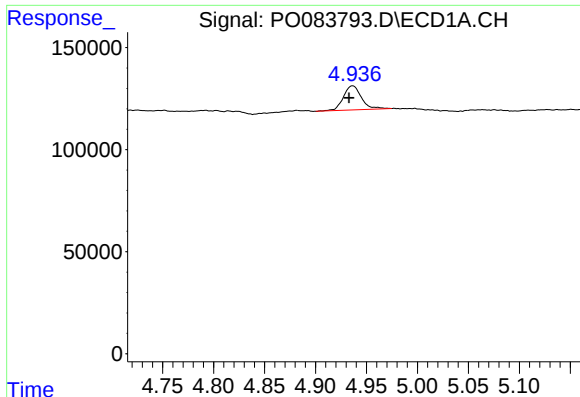

#1 Tetrachloro-m-xylene


R.T.: 4.936 min
Delta R.T.: 0.003 min
Response: 146035
Conc: 1.53 ng/ml

Instrument :
ECD_O
ClientSampleId :
CLI-2021-19-A

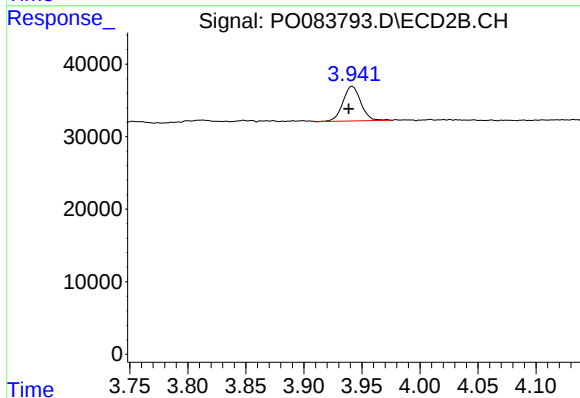


#1 Tetrachloro-m-xylene

R.T.: 3.941 min
Delta R.T.: 0.003 min
Response: 51340
Conc: 1.75 ng/ml

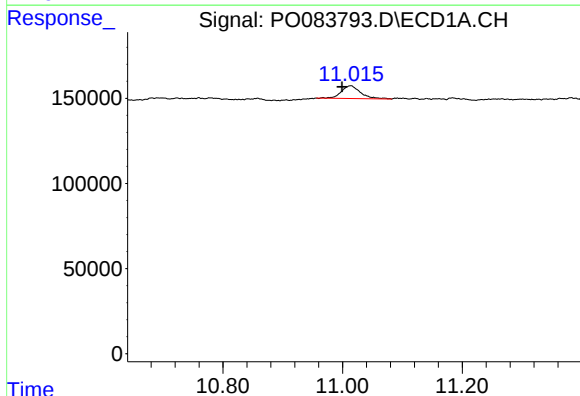


#2 Decachlorobiphenyl

R.T.: 11.014 min
Delta R.T.: 0.014 min
Response: 167768
Conc: 2.45 ng/ml

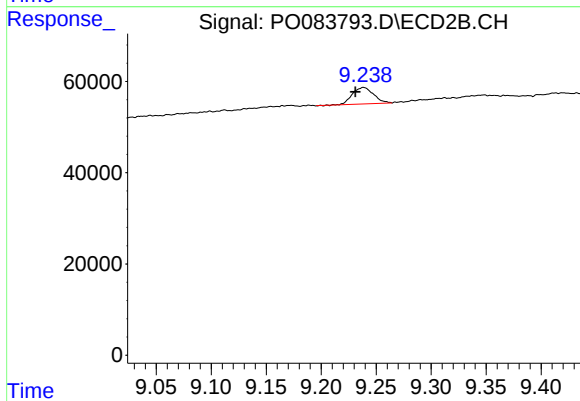

#2 Decachlorobiphenyl


R.T.: 9.239 min
Delta R.T.: 0.008 min
Response: 48394
Conc: 1.72 ng/ml

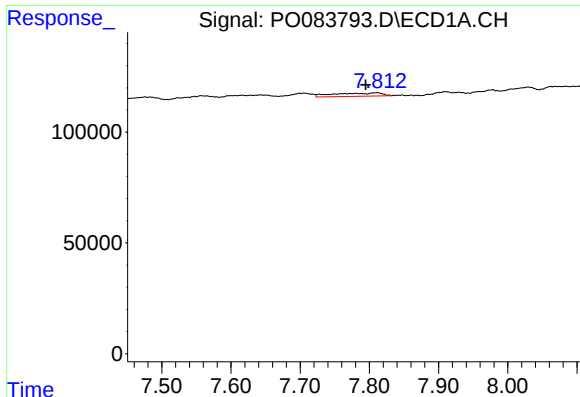

#28 AR-1254-3


R.T.: 7.812 min
Delta R.T.: 0.017 min
Response: 74357
Conc: 15.95 ng/ml

Instrument :
ECD_O
ClientSampleId :
CLI-2021-19-A

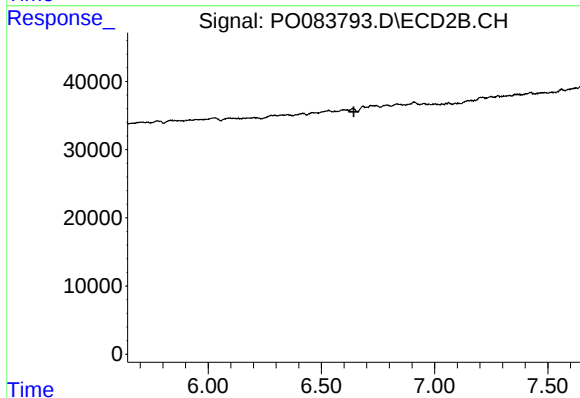


#28 AR-1254-3

R.T.: 0.000 min
Exp R.T. : 6.643 min
Response: 0
Conc: N.D.

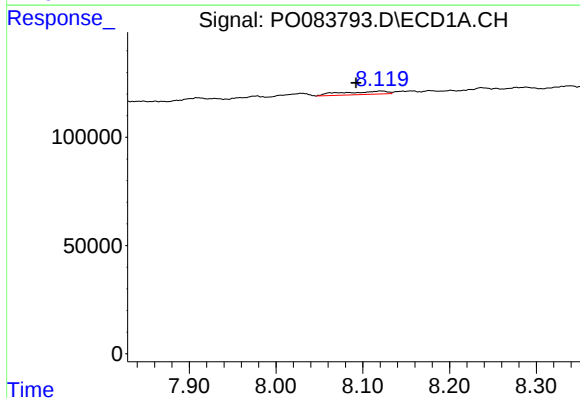


#29 AR-1254-4

R.T.: 8.120 min
Delta R.T.: 0.028 min
Response: 53369
Conc: 15.61 ng/ml

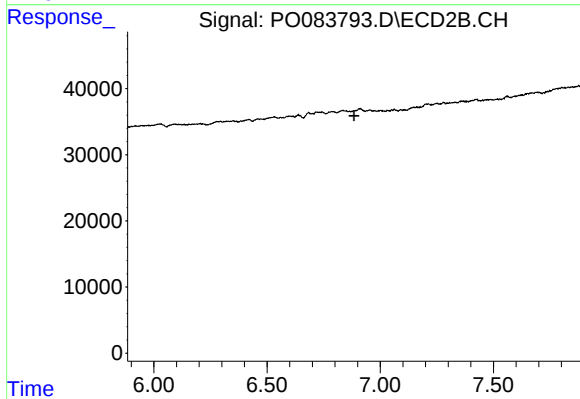

#29 AR-1254-4


R.T.: 0.000 min
Exp R.T. : 6.884 min
Response: 0
Conc: N.D.

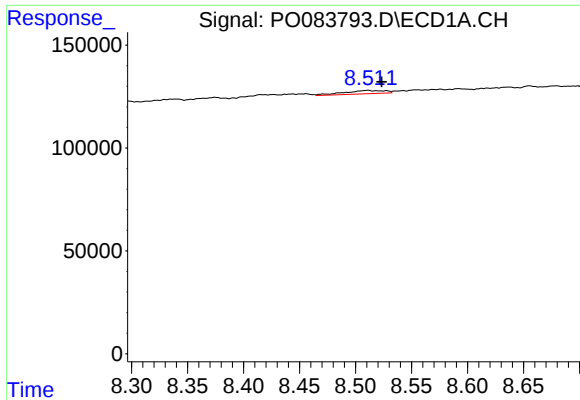

#30 AR-1254-5


R.T.: 8.511 min
Delta R.T.: -0.013 min
Response: 41365
Conc: 11.60 ng/ml

Instrument :
ECD_O
ClientSampleId :
CLI-2021-19-A

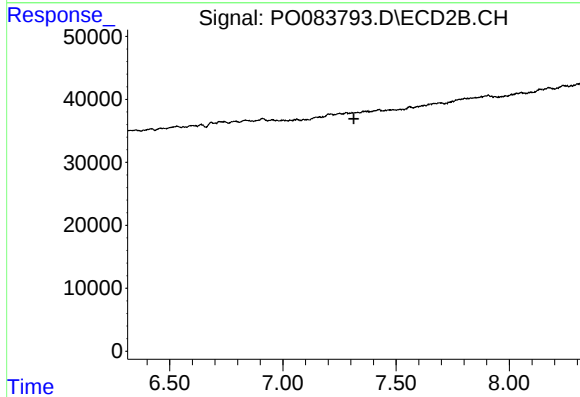


#30 AR-1254-5

R.T.: 0.000 min
Exp R.T. : 7.313 min
Response: 0
Conc: N.D.

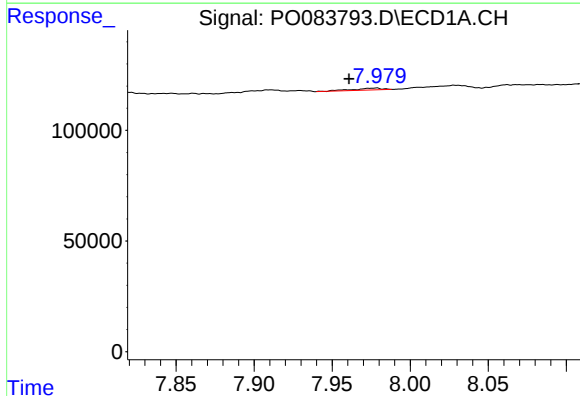


#31 AR-1260-1

R.T.: 7.978 min
Delta R.T.: 0.017 min
Response: 11161
Conc: 3.44 ng/ml

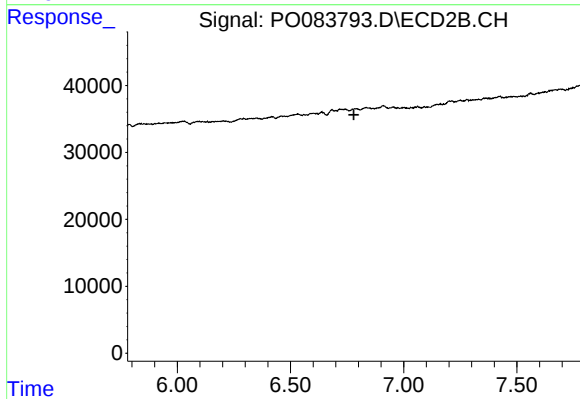

#31 AR-1260-1


R.T.: 0.000 min
Exp R.T. : 6.780 min
Response: 0
Conc: N.D.

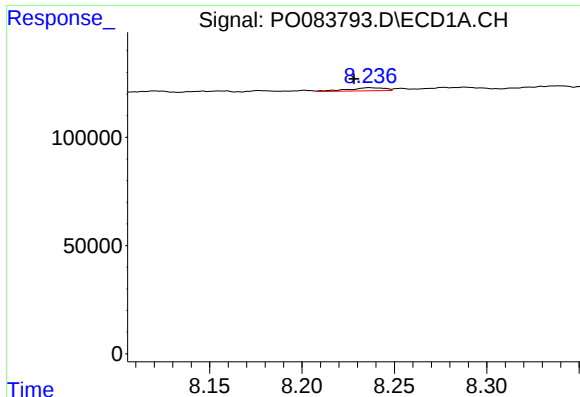

#32 AR-1260-2


R.T.: 8.237 min
Delta R.T.: 0.008 min
Response: 19493
Conc: 5.03 ng/ml

Instrument :
ECD_O
ClientSampleId :
CLI-2021-19-A

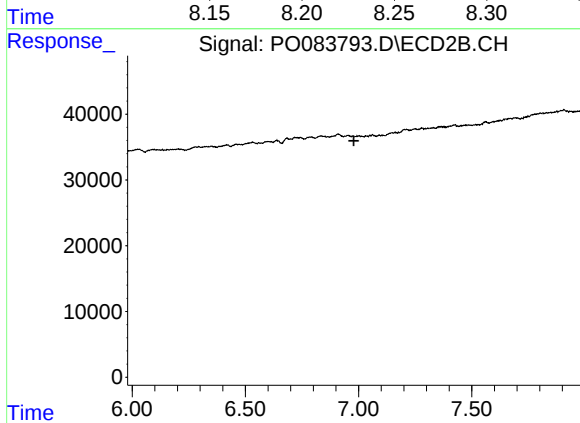


#32 AR-1260-2

R.T.: 0.000 min
Exp R.T. : 6.979 min
Response: 0
Conc: N.D.

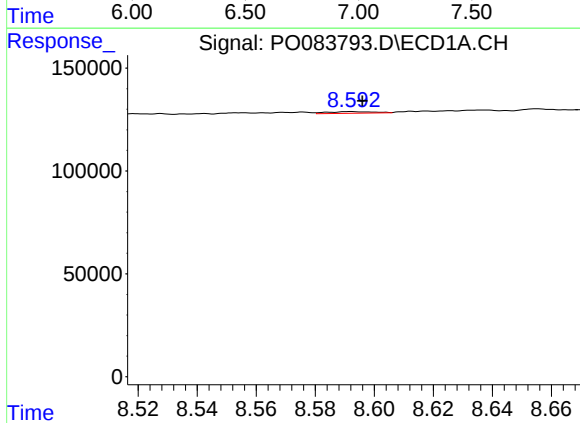


#33 AR-1260-3

R.T.: 8.592 min
Delta R.T.: -0.004 min
Response: 8672
Conc: 2.93 ng/ml

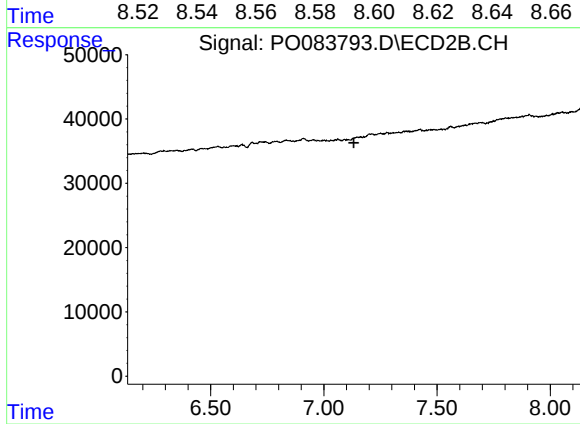

#33 AR-1260-3


R.T.: 0.000 min
Exp R.T. : 7.133 min
Response: 0
Conc: N.D.

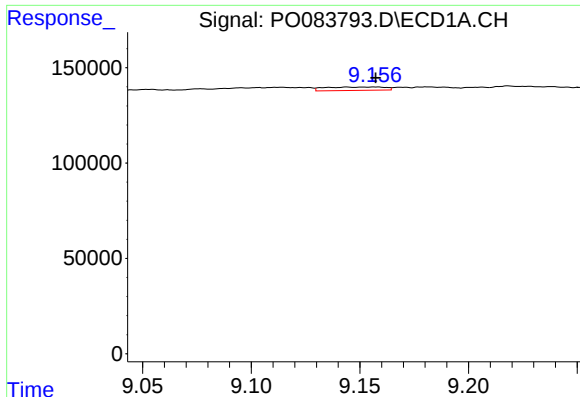

#35 AR-1260-5


R.T.: 9.144 min
Delta R.T.: -0.013 min
Response: 33845
Conc: 5.02 ng/ml

Instrument :
ECD_O
ClientSampleId :
CLI-2021-19-A

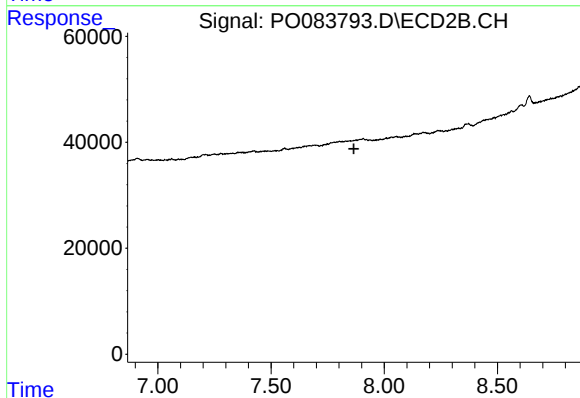


#35 AR-1260-5

R.T.: 0.000 min
Exp R.T. : 7.866 min
Response: 0
Conc: N.D.

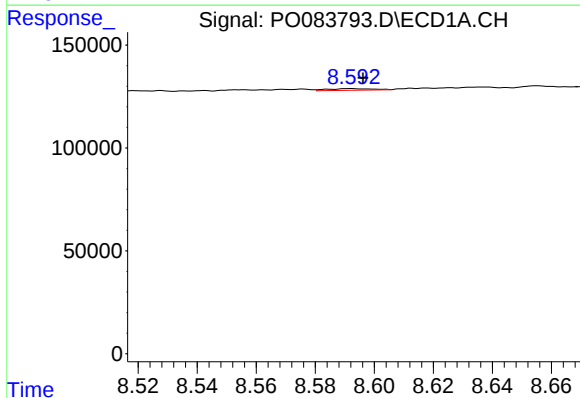


#36 AR-1262-1

R.T.: 8.592 min
Delta R.T.: -0.004 min
Response: 8672
Conc: 2.15 ng/ml

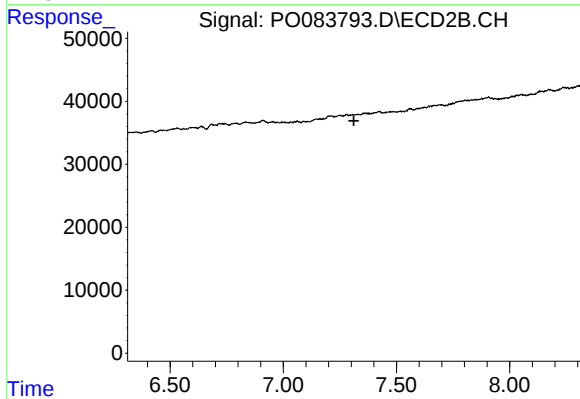

#36 AR-1262-1


R.T.: 0.000 min
Exp R.T. : 7.312 min
Response: 0
Conc: N.D.

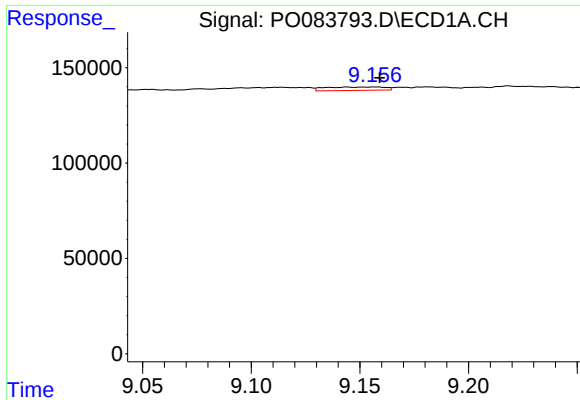

#37 AR-1262-2


R.T.: 9.144 min
Delta R.T.: -0.015 min
Response: 33845
Conc: 4.84 ng/ml

Instrument :
ECD_O
ClientSampleId :
CLI-2021-19-A

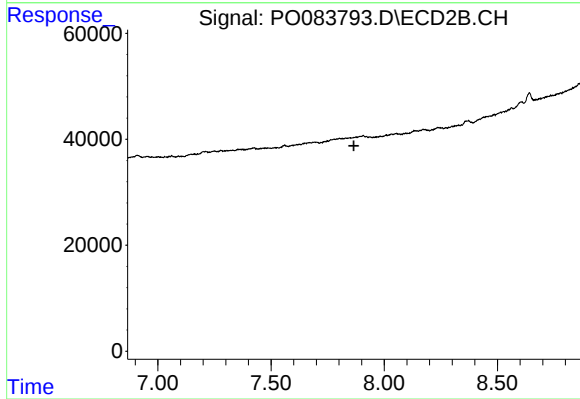


#37 AR-1262-2

R.T.: 0.000 min
Exp R.T. : 7.866 min
Response: 0
Conc: N.D.

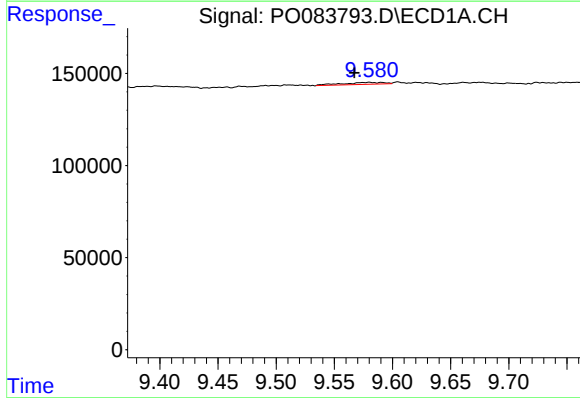


#39 AR-1262-4

R.T.: 9.580 min
Delta R.T.: 0.013 min
Response: 26263
Conc: 13.20 ng/ml

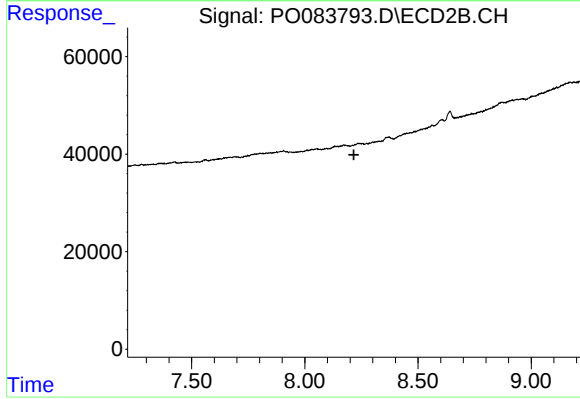

#39 AR-1262-4


R.T.: 0.000 min
Exp R.T. : 8.217 min
Response: 0
Conc: N.D.

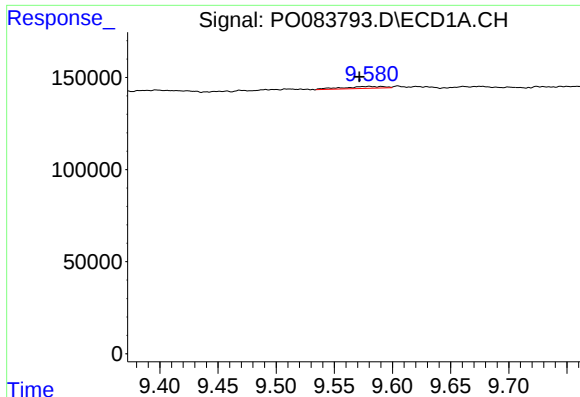

#42 AR-1268-2


R.T.: 9.580 min
Delta R.T.: 0.009 min
Response: 26263
Conc: 3.13 ng/ml

Instrument :
ECD_O
ClientSampleId :
CLI-2021-19-A

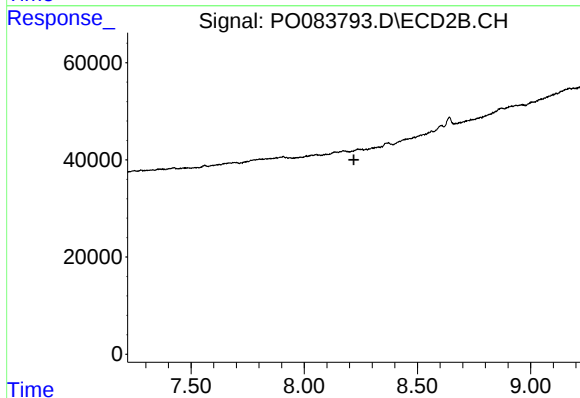


#42 AR-1268-2

R.T.: 0.000 min
Exp R.T. : 8.219 min
Response: 0
Conc: N.D.

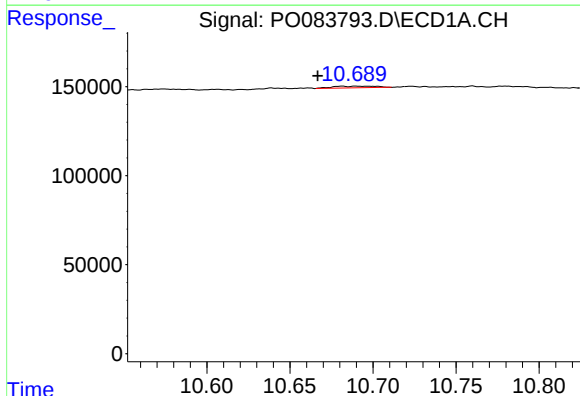

#45 AR-1268-5

R.T.: 10.681 min
Delta R.T.: 0.014 min
Response: 17508
Conc: 0.71 ng/ml

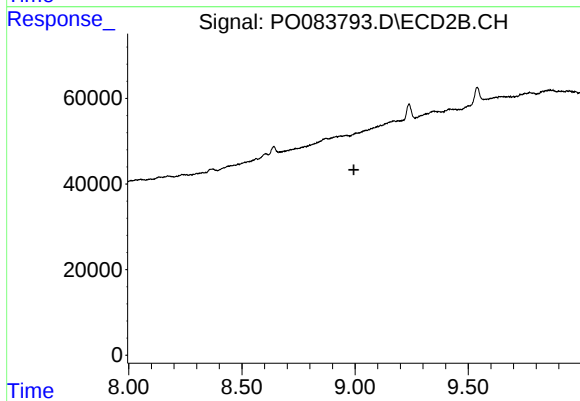

#45 AR-1268-5

R.T.: 0.000 min
Exp R.T. : 8.995 min
Response: 0
Conc: N.D.