

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO121621\
 Data File : P0083794.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 17 Dec 2021 3:47
 Operator : AJ\MA
 Sample : M5070-22 10X
 Misc :
 ALS Vial : 46 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 CLI-2021-19-B

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 17 04:45:45 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO121521.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Dec 16 04:05:27 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.935	3.941	113909	44150	1.196	1.505 #
2) SA Decachlor...	11.010	9.238	133372	45086	1.947	1.606
Target Compounds						
29) L6 AR-1254-4	8.110f	0.000	19750	0	5.778	N.D. #
30) L6 AR-1254-5	8.534	0.000	35851	0	10.056	N.D. #
31) L7 AR-1260-1	7.965	0.000	14991	0	4.626	N.D. #
32) L7 AR-1260-2	8.233	0.000	22469	0	5.801	N.D. #
39) L8 AR-1262-4	9.593f	0.000	26371	0	13.258	N.D. #
42) L9 AR-1268-2	9.593f	0.000	26371	0	3.142	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO121621\
Data File : P0083794.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 17 Dec 2021 3:47
Operator : AJ\MA
Sample : M5070-22 10X
Misc :
ALS Vial : 46 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
CLI-2021-19-B

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 17 04:45:45 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO121521.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Dec 16 04:05:27 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

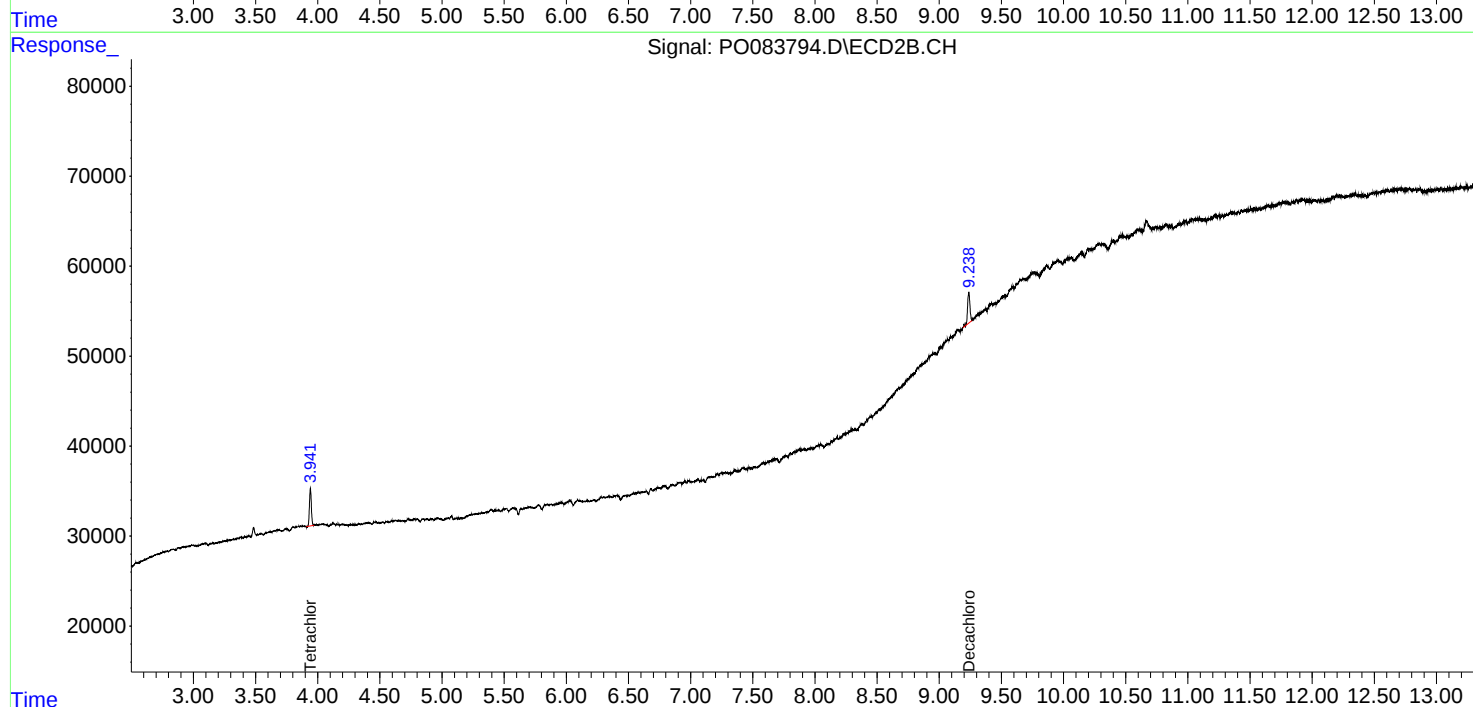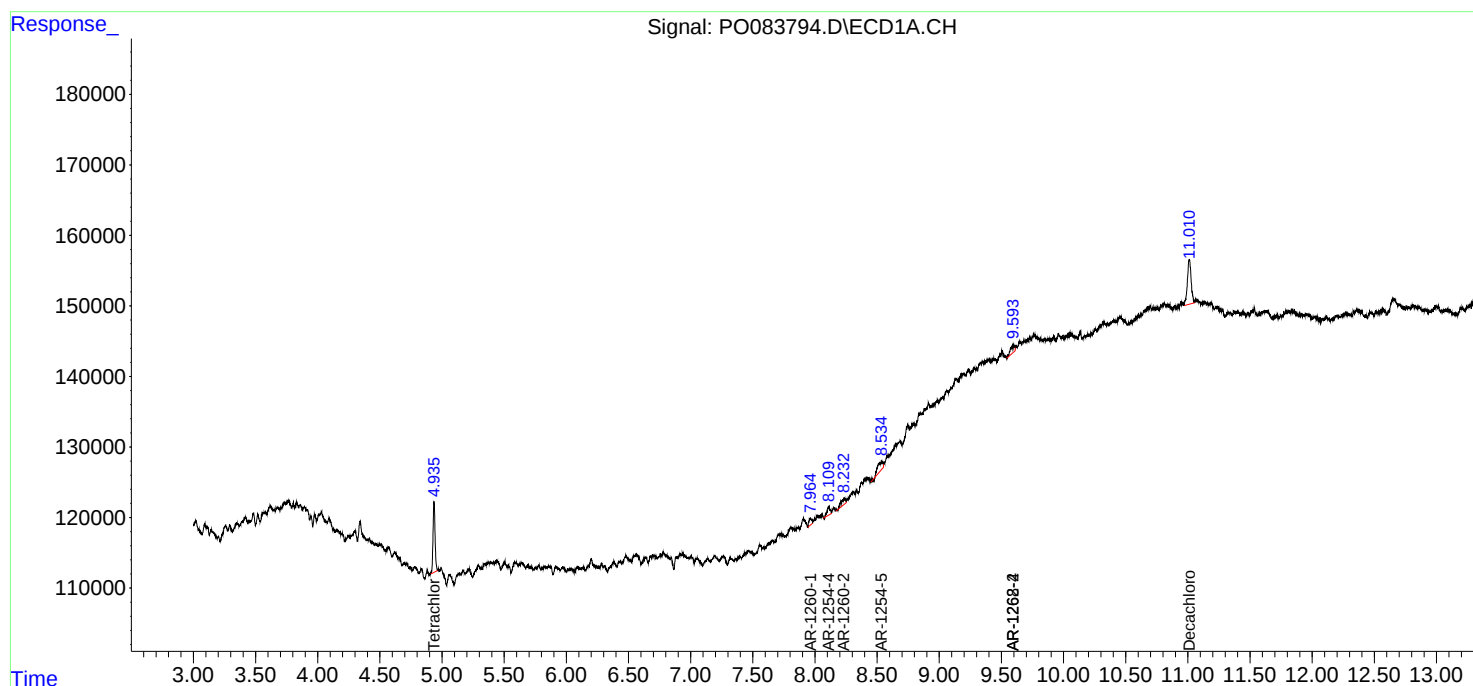


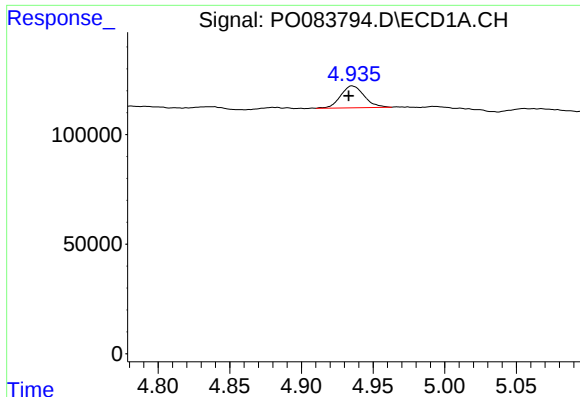

#1 Tetrachloro-m-xylene


R.T.: 4.935 min
Delta R.T.: 0.002 min
Response: 113909
Conc: 1.20 ng/ml

Instrument :
ECD_O
ClientSampleId :
CLI-2021-19-B

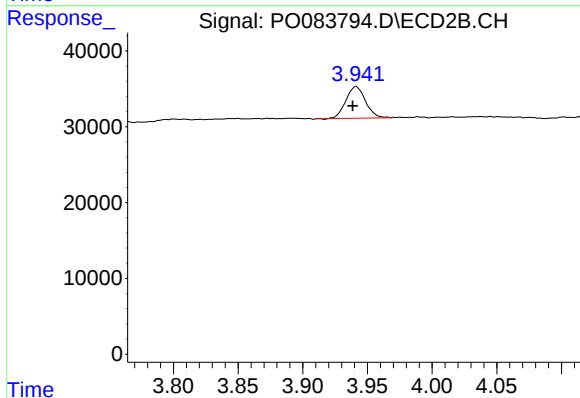


#1 Tetrachloro-m-xylene

R.T.: 3.941 min
Delta R.T.: 0.003 min
Response: 44150
Conc: 1.51 ng/ml

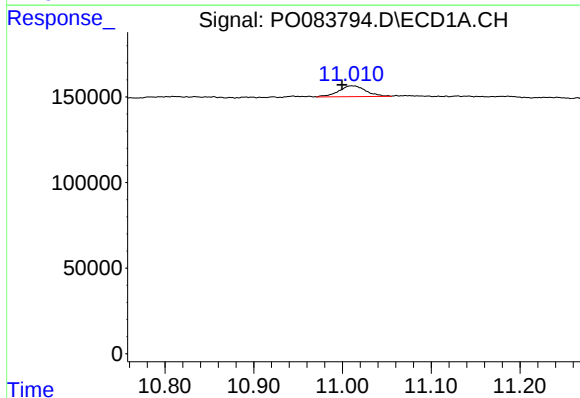


#2 Decachlorobiphenyl

R.T.: 11.010 min
Delta R.T.: 0.011 min
Response: 133372
Conc: 1.95 ng/ml

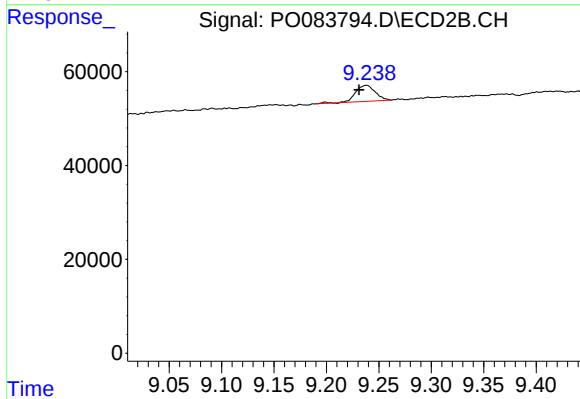

#2 Decachlorobiphenyl


R.T.: 9.238 min
Delta R.T.: 0.007 min
Response: 45086
Conc: 1.61 ng/ml

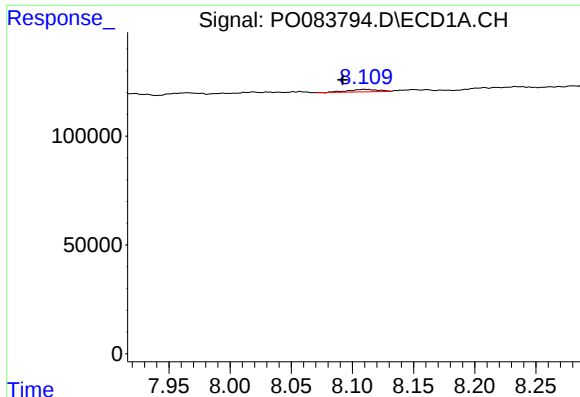

#29 AR-1254-4


R.T.: 8.110 min
Delta R.T.: 0.017 min
Response: 19750
Conc: 5.78 ng/ml

Instrument :
ECD_O
ClientSampleId :
CLI-2021-19-B

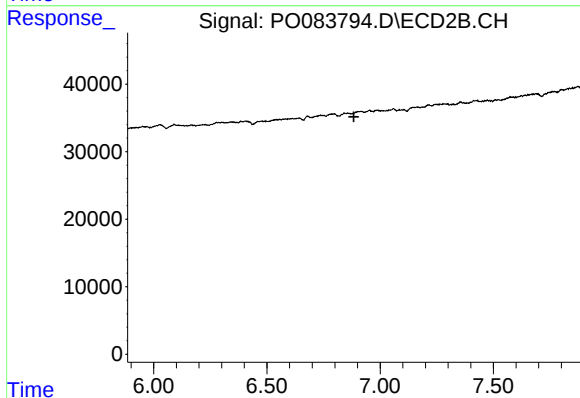


#29 AR-1254-4

R.T.: 0.000 min
Exp R.T. : 6.884 min
Response: 0
Conc: N.D.

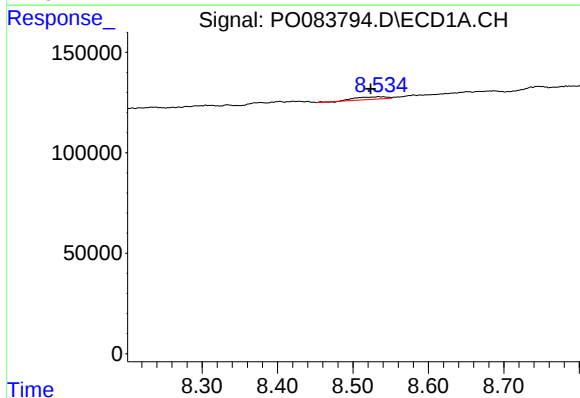


#30 AR-1254-5

R.T.: 8.534 min
Delta R.T.: 0.010 min
Response: 35851
Conc: 10.06 ng/ml

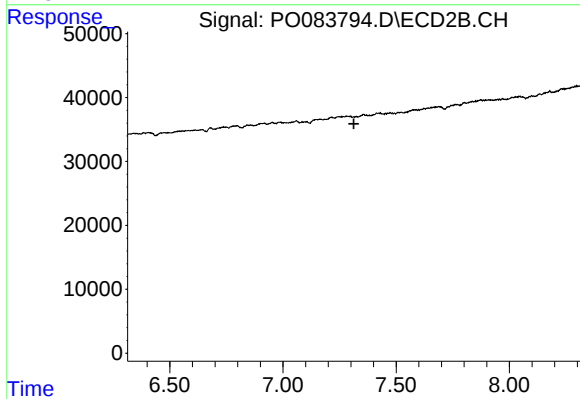

#30 AR-1254-5


R.T.: 0.000 min
Exp R.T. : 7.313 min
Response: 0
Conc: N.D.

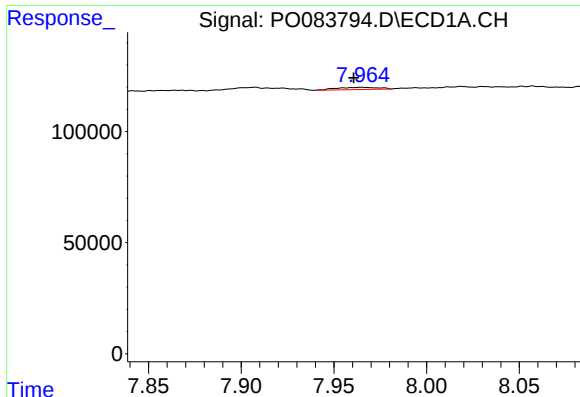

#31 AR-1260-1


R.T.: 7.965 min
Delta R.T.: 0.004 min
Response: 14991
Conc: 4.63 ng/ml

Instrument :
ECD_O
ClientSampleId :
CLI-2021-19-B

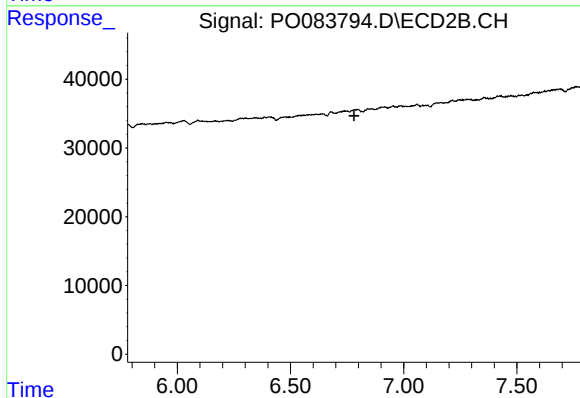


#31 AR-1260-1

R.T.: 0.000 min
Exp R.T. : 6.780 min
Response: 0
Conc: N.D.

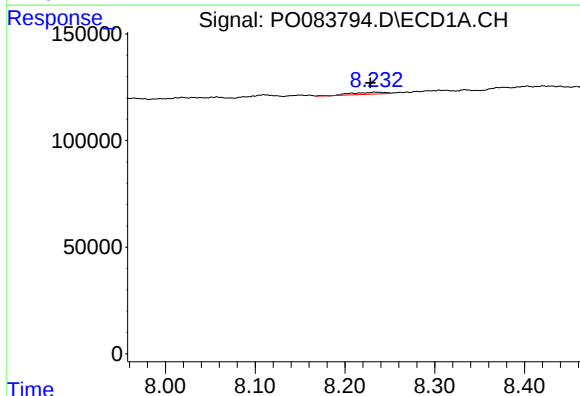


#32 AR-1260-2

R.T.: 8.233 min
Delta R.T.: 0.005 min
Response: 22469
Conc: 5.80 ng/ml

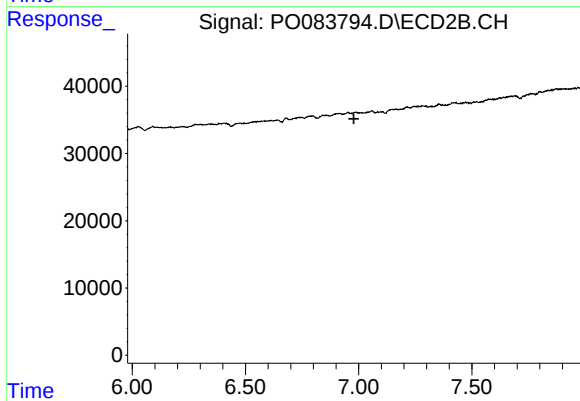

#32 AR-1260-2


R.T.: 0.000 min
Exp R.T. : 6.979 min
Response: 0
Conc: N.D.

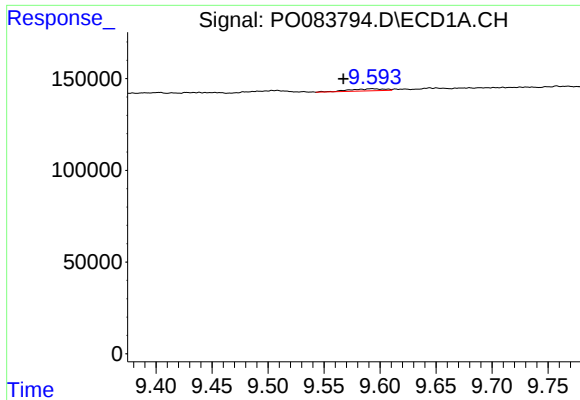

#39 AR-1262-4


R.T.: 9.593 min
Delta R.T.: 0.026 min
Response: 26371
Conc: 13.26 ng/ml

Instrument :
ECD_O
ClientSampleId :
CLI-2021-19-B

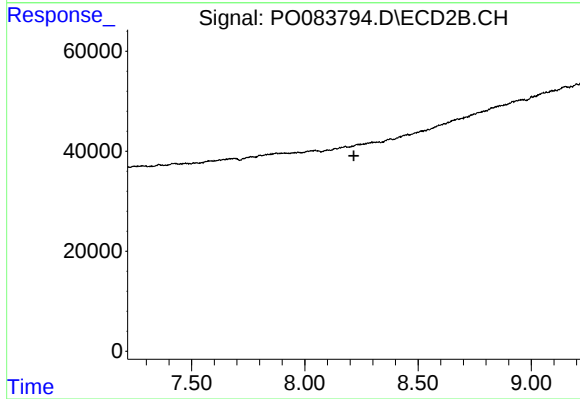


#39 AR-1262-4

R.T.: 0.000 min
Exp R.T. : 8.217 min
Response: 0
Conc: N.D.

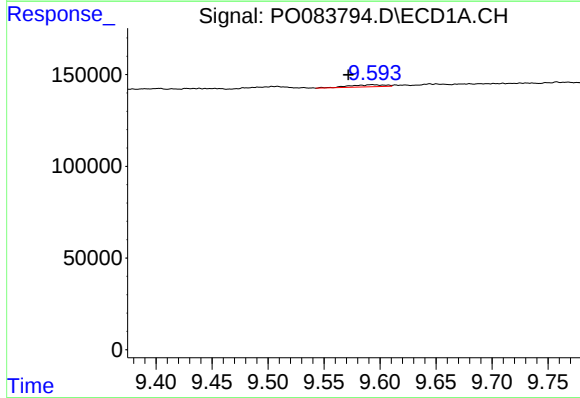

#42 AR-1268-2

R.T.: 9.593 min
Delta R.T.: 0.021 min
Response: 26371
Conc: 3.14 ng/ml

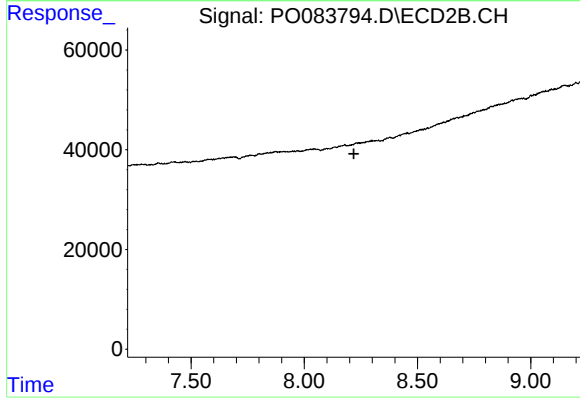

#42 AR-1268-2

R.T.: 0.000 min
Exp R.T. : 8.219 min
Response: 0
Conc: N.D.