

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO121621\
 Data File : P0083795.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 17 Dec 2021 4:04
 Operator : AJ\MA
 Sample : M5070-23 10X
 Misc :
 ALS Vial : 47 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 CLI-2021-20-A

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 17 04:46:03 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO121521.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Dec 16 04:05:27 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.936	3.942	103732	39826	1.089	1.358
2) SA Decachlor...	11.010	9.240	118987	49683	1.737	1.769
Target Compounds						
9) L2 AR-1221-2	5.292	0.000	9221	0	12.905	N.D. #
29) L6 AR-1254-4	8.067f	0.000	16863	0	4.933	N.D. #
30) L6 AR-1254-5	8.517	0.000	14197	0	3.982	N.D. #
31) L7 AR-1260-1	7.978f	0.000	17162	0	5.297	N.D. #
32) L7 AR-1260-2	8.239	0.000	25107	0	6.482	N.D. #
33) L7 AR-1260-3	8.599	0.000	5282	0	1.783	N.D. #
34) L7 AR-1260-4	8.851f	0.000	11249	0	3.288	N.D. #
35) L7 AR-1260-5	9.144	0.000	5153	0	0.765	N.D. #
36) L8 AR-1262-1	8.599	0.000	5282	0	1.310	N.D. #
37) L8 AR-1262-2	9.144f	0.000	5153	0	0.736	N.D. #
39) L8 AR-1262-4	0.000	8.243f	0	17951	N.D.	6.060 #
42) L9 AR-1268-2	0.000	8.243f	0	17951	N.D.	3.906 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO121621\
Data File : PO083795.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 17 Dec 2021 4:04
Operator : AJ\MA
Sample : M5070-23 10X
Misc :
ALS Vial : 47 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
CLI-2021-20-A

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 17 04:46:03 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO121521.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Dec 16 04:05:27 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

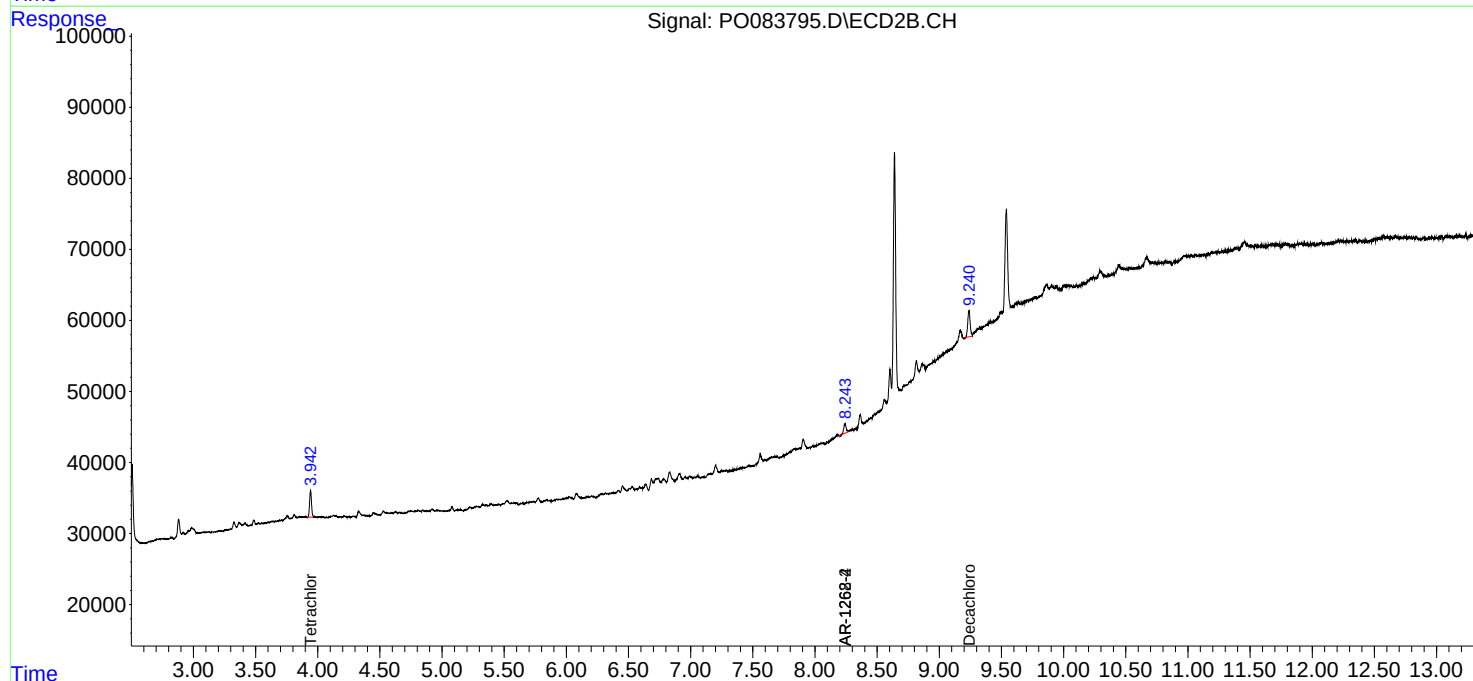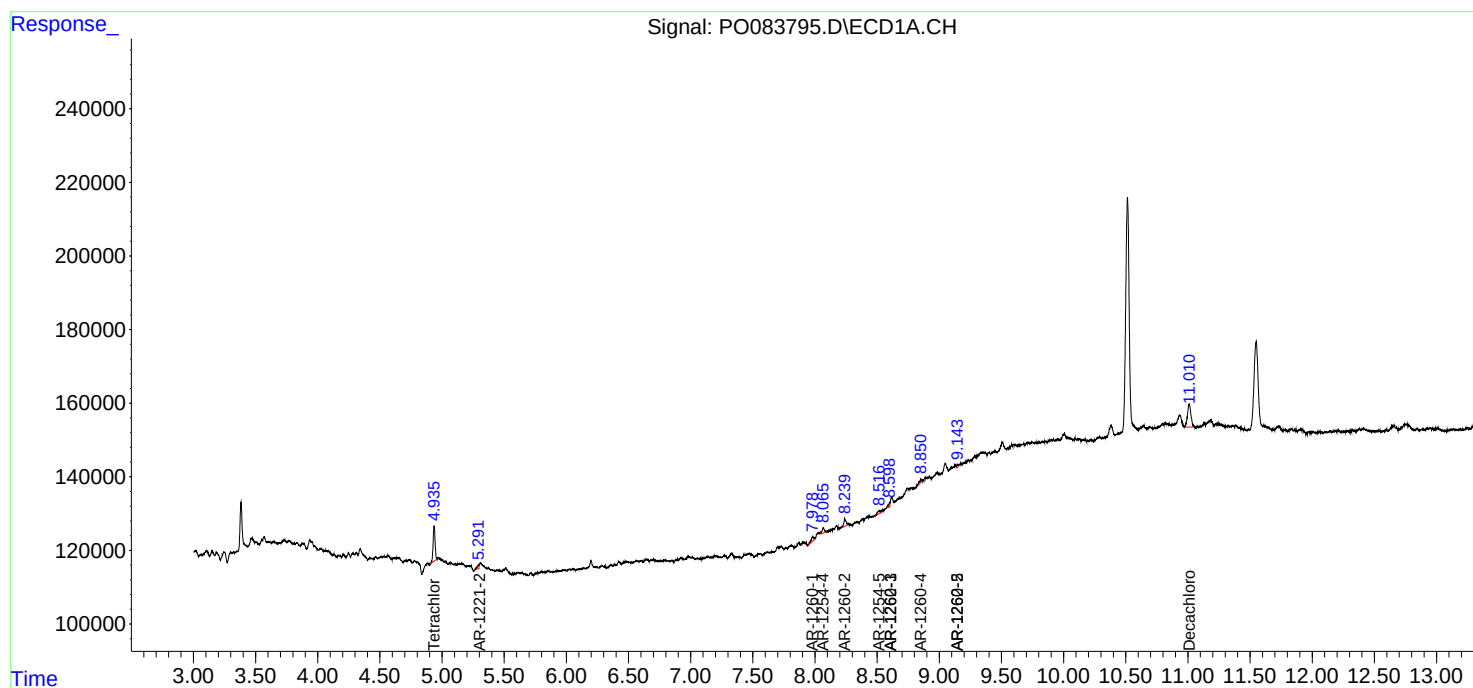


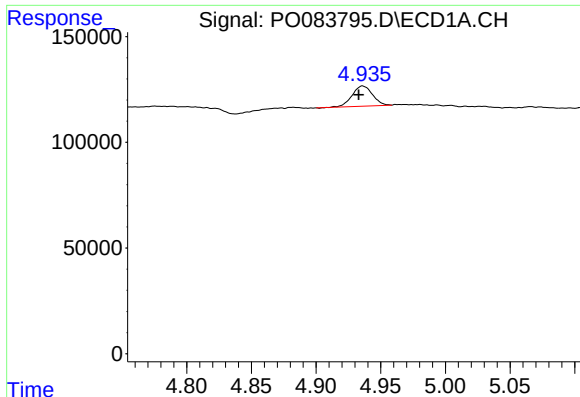

#1 Tetrachloro-m-xylene


R.T.: 4.936 min
Delta R.T.: 0.003 min
Response: 103732
Conc: 1.09 ng/ml

Instrument :
ECD_O
ClientSampleId :
CLI-2021-20-A

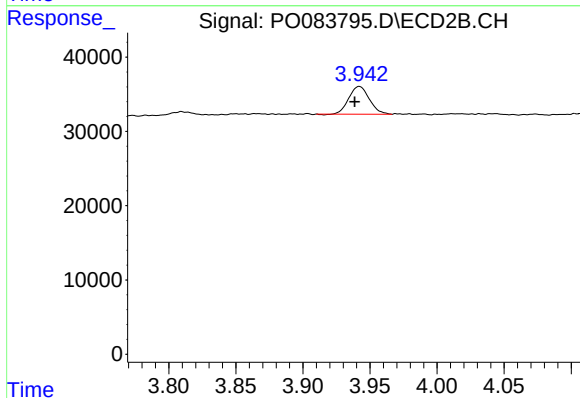


#1 Tetrachloro-m-xylene

R.T.: 3.942 min
Delta R.T.: 0.003 min
Response: 39826
Conc: 1.36 ng/ml

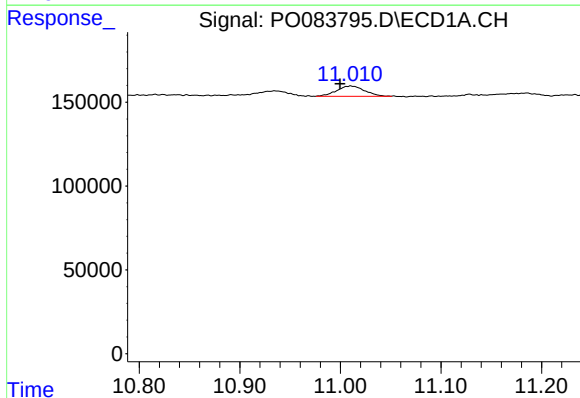


#2 Decachlorobiphenyl

R.T.: 11.010 min
Delta R.T.: 0.011 min
Response: 118987
Conc: 1.74 ng/ml

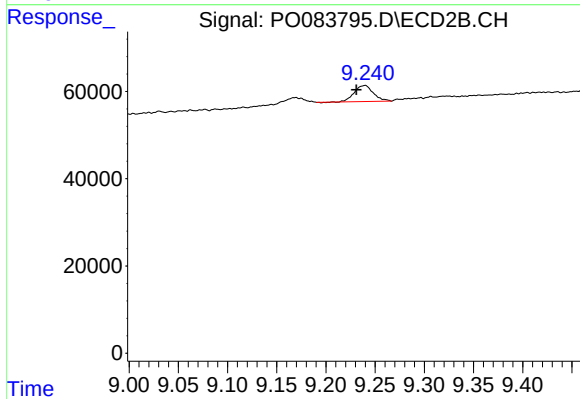

#2 Decachlorobiphenyl


R.T.: 9.240 min
Delta R.T.: 0.009 min
Response: 49683
Conc: 1.77 ng/ml

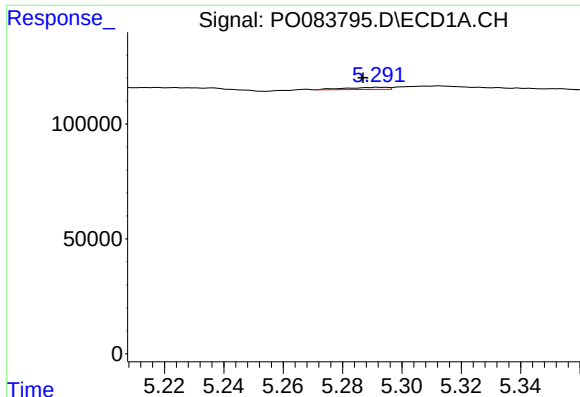

#9 AR-1221-2


R.T.: 5.292 min
Delta R.T.: 0.005 min
Response: 9221
Conc: 12.90 ng/ml

Instrument :
ECD_O
ClientSampleId :
CLI-2021-20-A

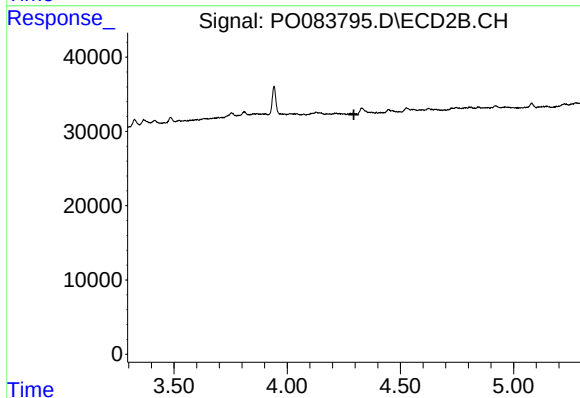


#9 AR-1221-2

R.T.: 0.000 min
Exp R.T. : 4.294 min
Response: 0
Conc: N.D.

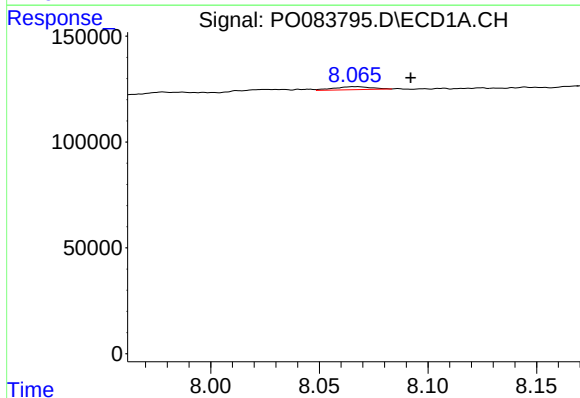


#29 AR-1254-4

R.T.: 8.067 min
Delta R.T.: -0.025 min
Response: 16863
Conc: 4.93 ng/ml

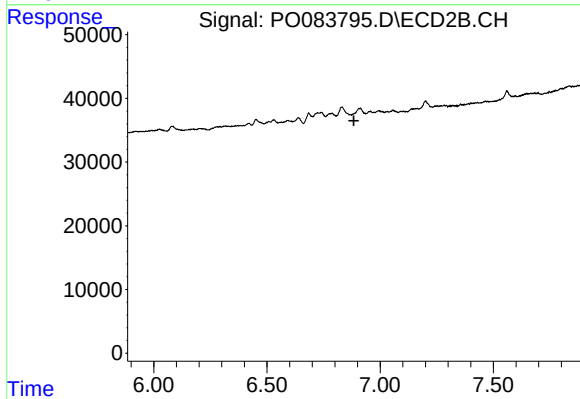

#29 AR-1254-4


R.T.: 0.000 min
Exp R.T. : 6.884 min
Response: 0
Conc: N.D.

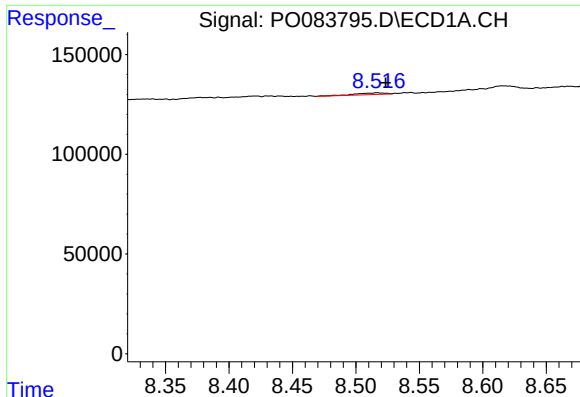

#30 AR-1254-5


R.T.: 8.517 min
Delta R.T.: -0.007 min
Response: 14197
Conc: 3.98 ng/ml

Instrument :
ECD_O
ClientSampleId :
CLI-2021-20-A

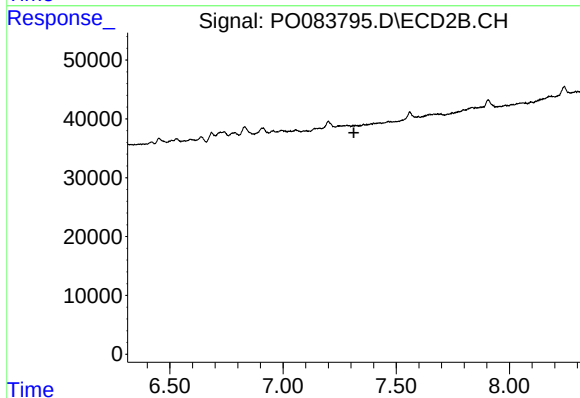


#30 AR-1254-5

R.T.: 0.000 min
Exp R.T. : 7.313 min
Response: 0
Conc: N.D.

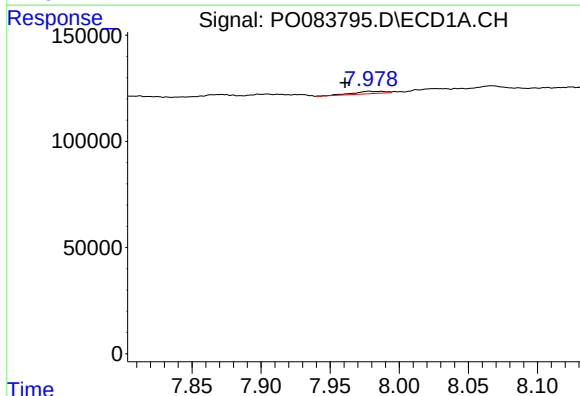


#31 AR-1260-1

R.T.: 7.978 min
Delta R.T.: 0.017 min
Response: 17162
Conc: 5.30 ng/ml

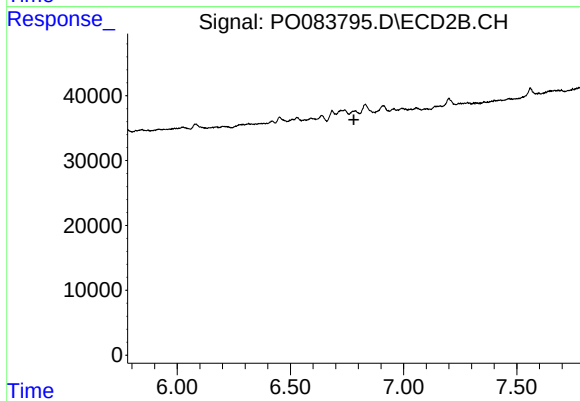

#31 AR-1260-1


R.T.: 0.000 min
Exp R.T. : 6.780 min
Response: 0
Conc: N.D.

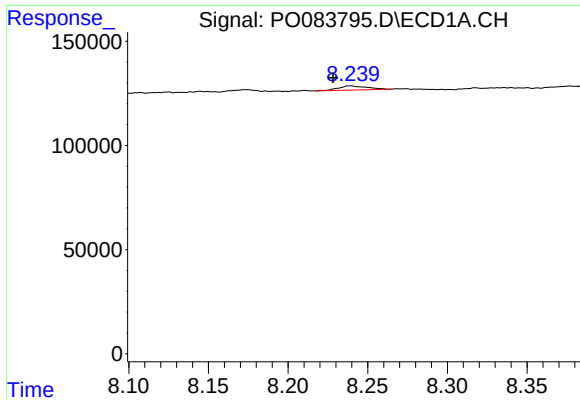

#32 AR-1260-2


R.T.: 8.239 min
Delta R.T.: 0.011 min
Response: 25107
Conc: 6.48 ng/ml

Instrument :
ECD_O
ClientSampleId :
CLI-2021-20-A

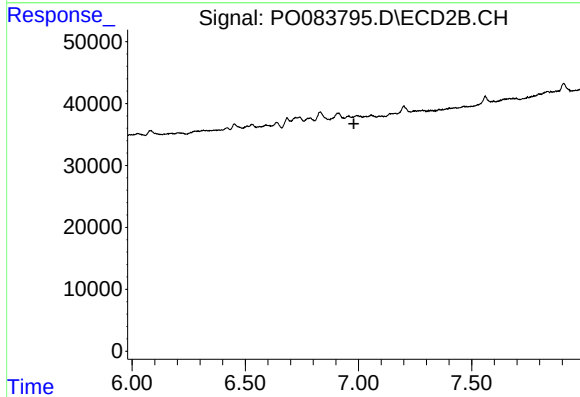


#32 AR-1260-2

R.T.: 0.000 min
Exp R.T. : 6.979 min
Response: 0
Conc: N.D.

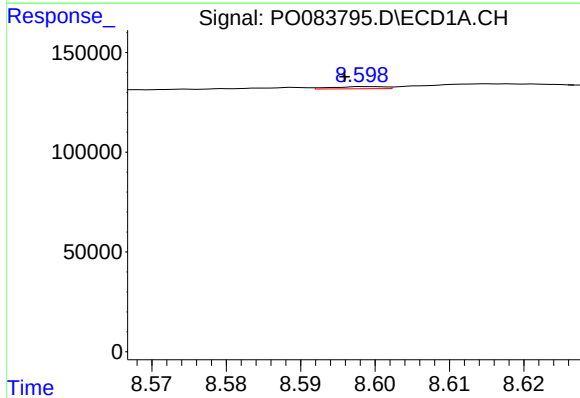


#33 AR-1260-3

R.T.: 8.599 min
Delta R.T.: 0.003 min
Response: 5282
Conc: 1.78 ng/ml

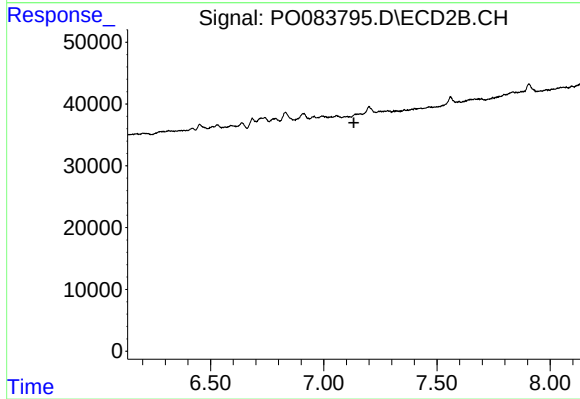

#33 AR-1260-3


R.T.: 0.000 min
Exp R.T. : 7.133 min
Response: 0
Conc: N.D.

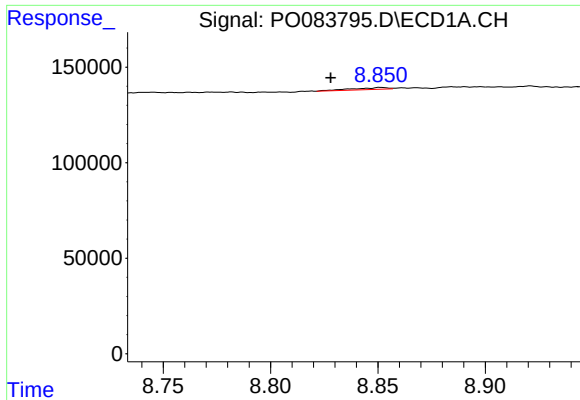

#34 AR-1260-4


R.T.: 8.851 min
Delta R.T.: 0.023 min
Response: 11249
Conc: 3.29 ng/ml

Instrument :
ECD_O
ClientSampleId :
CLI-2021-20-A

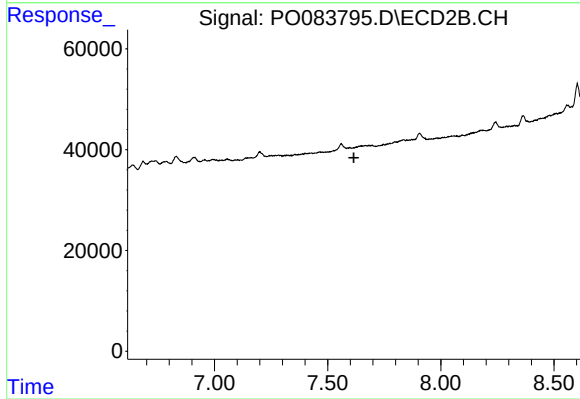


#34 AR-1260-4

R.T.: 0.000 min
Exp R.T. : 7.616 min
Response: 0
Conc: N.D.

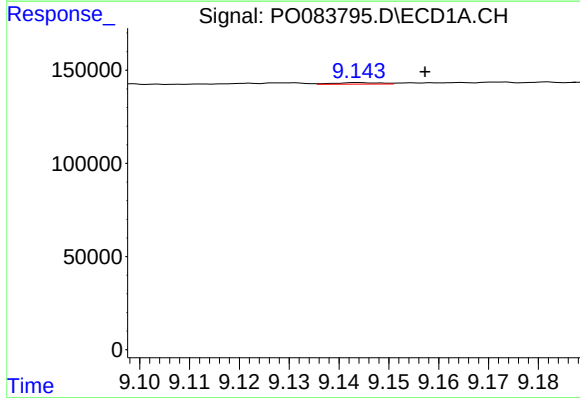


#35 AR-1260-5

R.T.: 9.144 min
Delta R.T.: -0.013 min
Response: 5153
Conc: 0.76 ng/ml

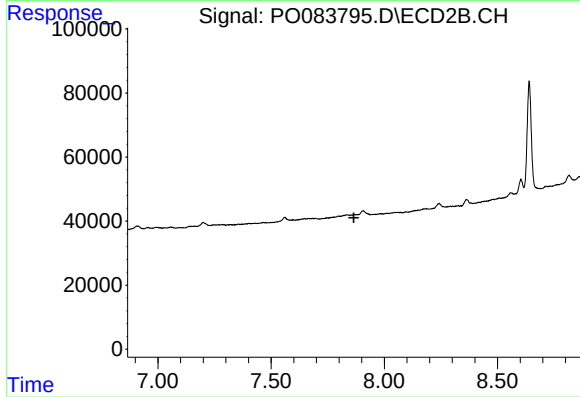

#35 AR-1260-5


R.T.: 0.000 min
Exp R.T. : 7.866 min
Response: 0
Conc: N.D.

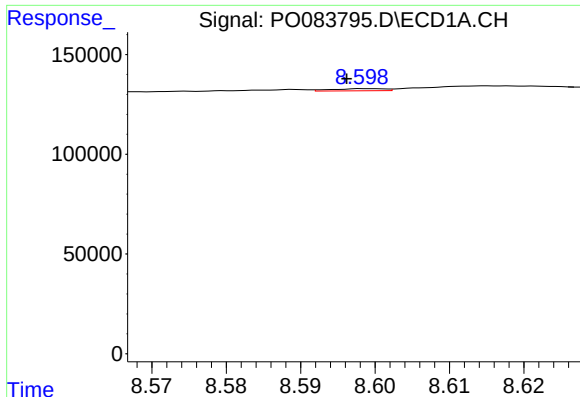

#36 AR-1262-1


R.T.: 8.599 min
Delta R.T.: 0.003 min
Response: 5282
Conc: 1.31 ng/ml

Instrument :
ECD_O
ClientSampleId :
CLI-2021-20-A

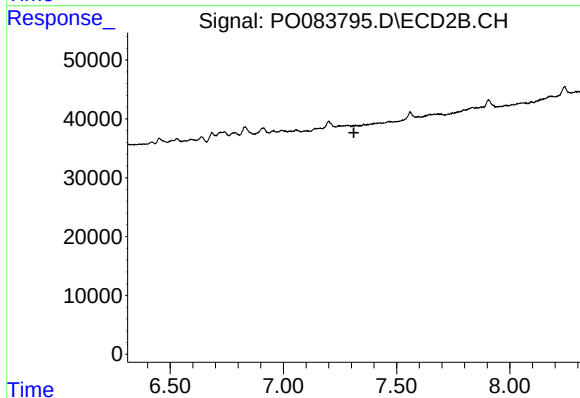


#36 AR-1262-1

R.T.: 0.000 min
Exp R.T. : 7.312 min
Response: 0
Conc: N.D.

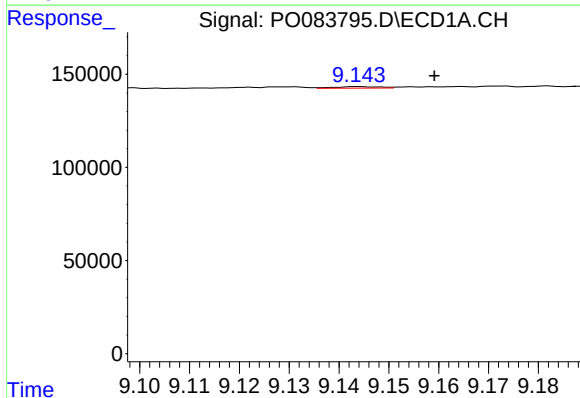


#37 AR-1262-2

R.T.: 9.144 min
Delta R.T.: -0.015 min
Response: 5153
Conc: 0.74 ng/ml

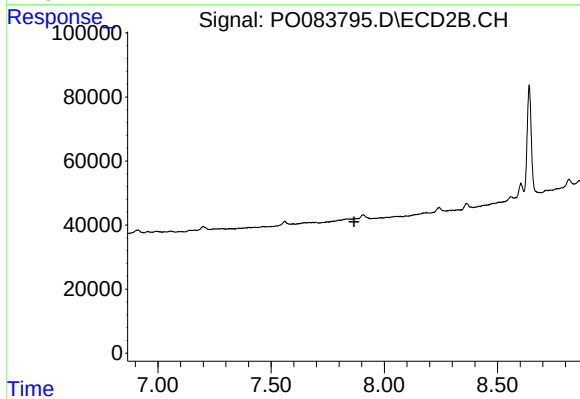

#37 AR-1262-2


R.T.: 0.000 min
Exp R.T. : 7.866 min
Response: 0
Conc: N.D.

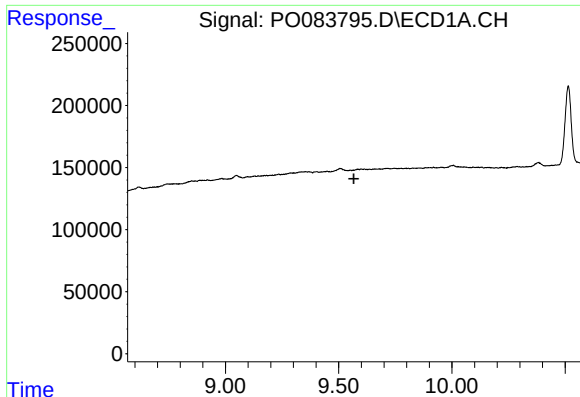

#39 AR-1262-4


R.T.: 0.000 min
Exp R.T.: 9.567 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
CLI-2021-20-A

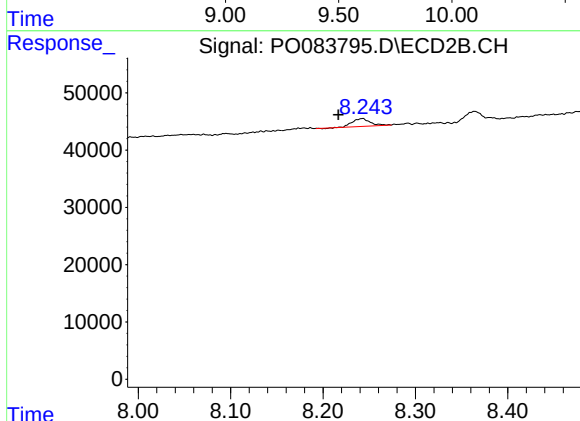


#39 AR-1262-4

R.T.: 8.243 min
Delta R.T.: 0.027 min
Response: 17951
Conc: 6.06 ng/ml

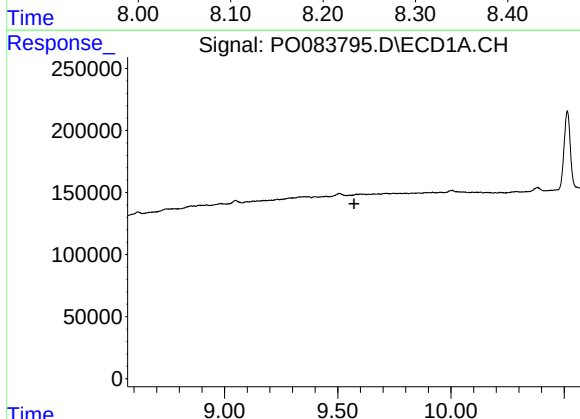

#42 AR-1268-2

R.T.: 0.000 min
Exp R.T.: 9.572 min
Response: 0
Conc: N.D.

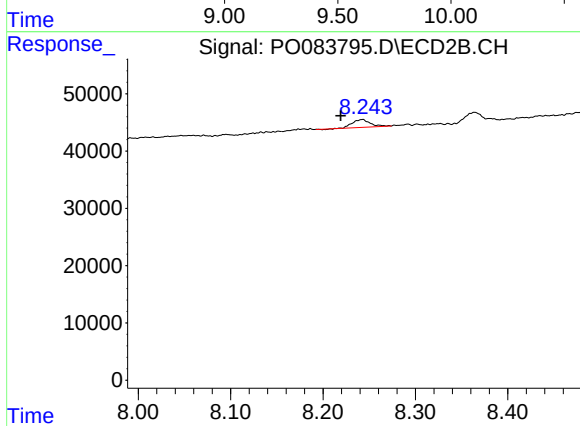

#42 AR-1268-2

R.T.: 8.243 min
Delta R.T.: 0.024 min
Response: 17951
Conc: 3.91 ng/ml