

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO121621\
 Data File : PO083796.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 17 Dec 2021 4:21
 Operator : AJ\MA
 Sample : M5070-24 10X
 Misc :
 ALS Vial : 48 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 CLI-2021-20-B

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 17 04:46:18 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO121521.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Dec 16 04:05:27 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.936	3.941	107453	40901	1.128	1.394
2) SA Decachlor...	11.013	9.239	121673	52587	1.776	1.873
Target Compounds						
30) L6 AR-1254-5	8.512	0.000	11786	0	3.306	N.D. #
32) L7 AR-1260-2	8.243	0.000	14293	0	3.690	N.D. #
33) L7 AR-1260-3	8.616f	0.000	10307	0	3.479	N.D. #
34) L7 AR-1260-4	8.829	0.000	14047	0	4.106	N.D. #
35) L7 AR-1260-5	9.149	0.000	9288	0	1.378	N.D. #
36) L8 AR-1262-1	8.616f	0.000	10307	0	2.556	N.D. #
37) L8 AR-1262-2	9.166	0.000	3969	0	0.567	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO121621\
Data File : P0083796.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 17 Dec 2021 4:21
Operator : AJ\MA
Sample : M5070-24 10X
Misc :
ALS Vial : 48 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
CLI-2021-20-B

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 17 04:46:18 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO121521.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Dec 16 04:05:27 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

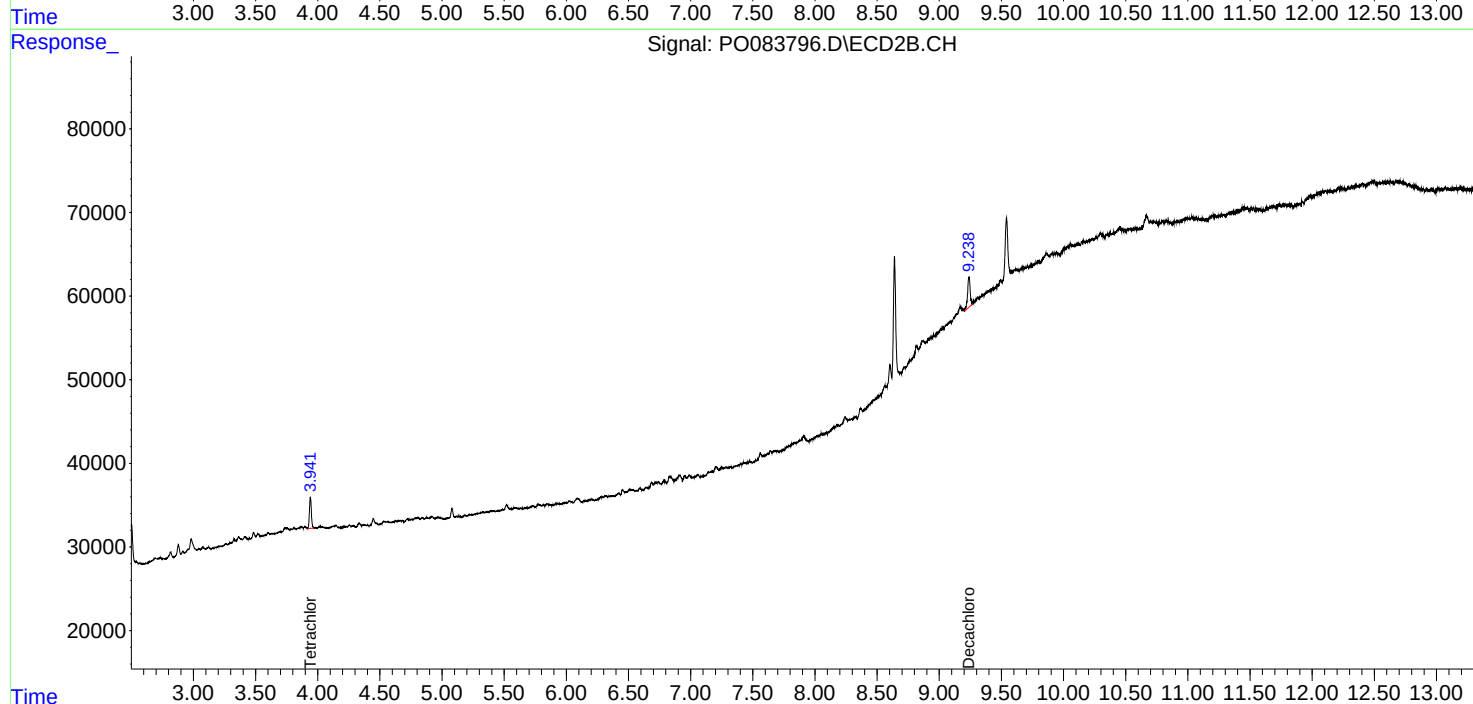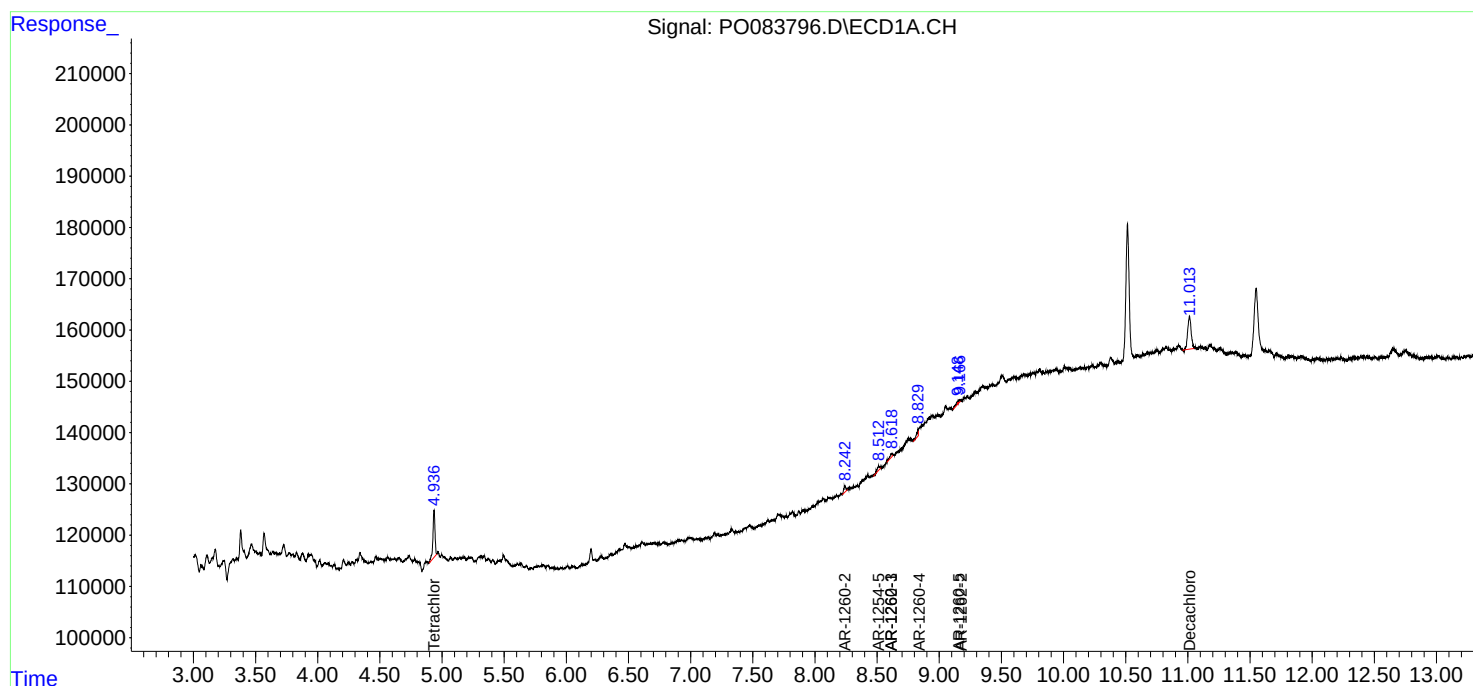


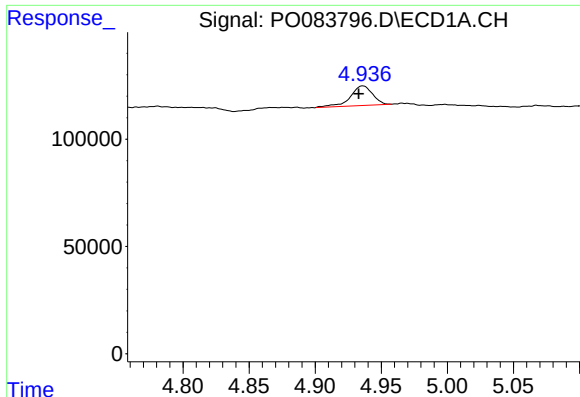

#1 Tetrachloro-m-xylene


R.T.: 4.936 min
Delta R.T.: 0.003 min
Response: 107453
Conc: 1.13 ng/ml

Instrument :
ECD_O
ClientSampleId :
CLI-2021-20-B

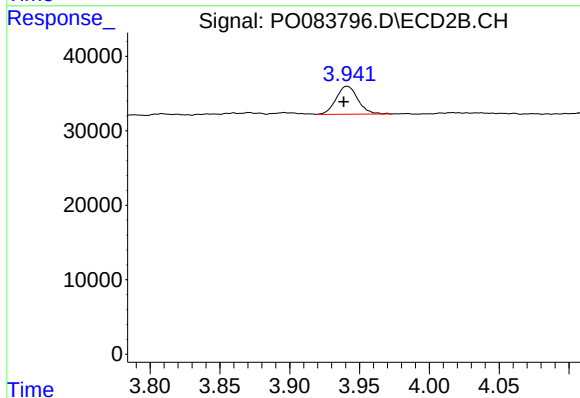


#1 Tetrachloro-m-xylene

R.T.: 3.941 min
Delta R.T.: 0.002 min
Response: 40901
Conc: 1.39 ng/ml

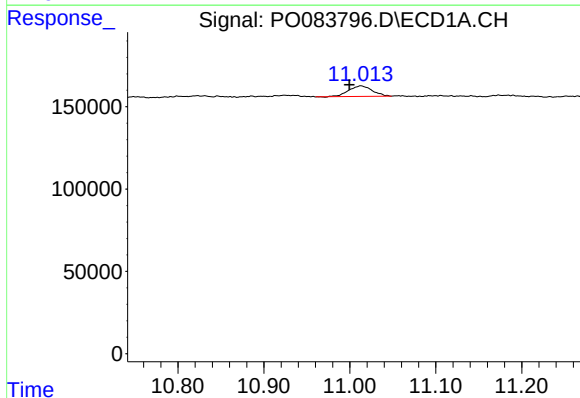


#2 Decachlorobiphenyl

R.T.: 11.013 min
Delta R.T.: 0.013 min
Response: 121673
Conc: 1.78 ng/ml

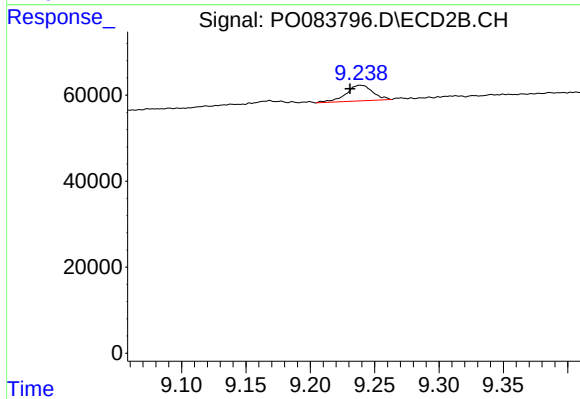

#2 Decachlorobiphenyl


R.T.: 9.239 min
Delta R.T.: 0.008 min
Response: 52587
Conc: 1.87 ng/ml

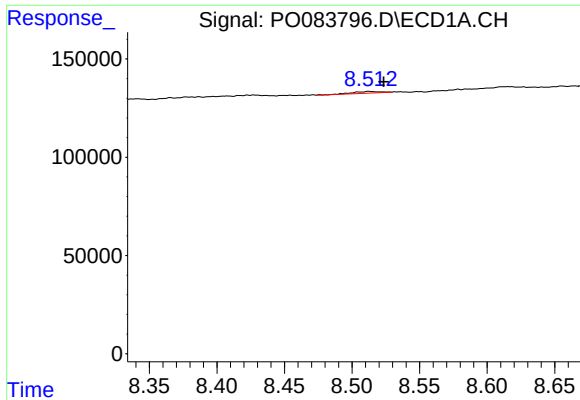

#30 AR-1254-5


R.T.: 8.512 min
Delta R.T.: -0.011 min
Response: 11786
Conc: 3.31 ng/ml

Instrument :
ECD_O
ClientSampleId :
CLI-2021-20-B

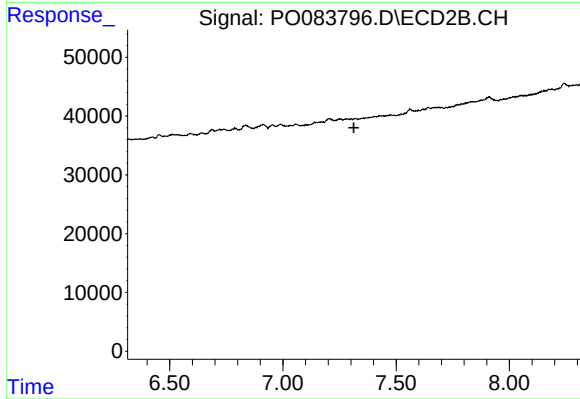


#30 AR-1254-5

R.T.: 0.000 min
Exp R.T. : 7.313 min
Response: 0
Conc: N.D.

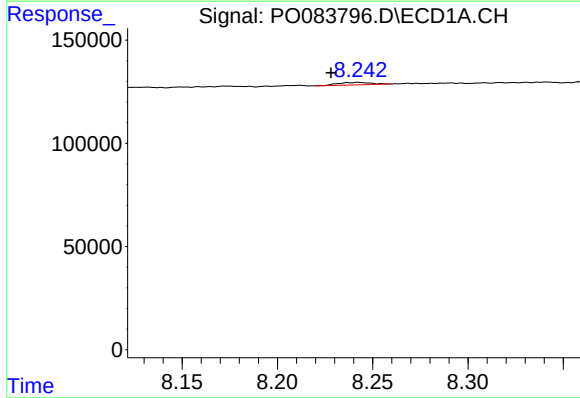


#32 AR-1260-2

R.T.: 8.243 min
Delta R.T.: 0.014 min
Response: 14293
Conc: 3.69 ng/ml

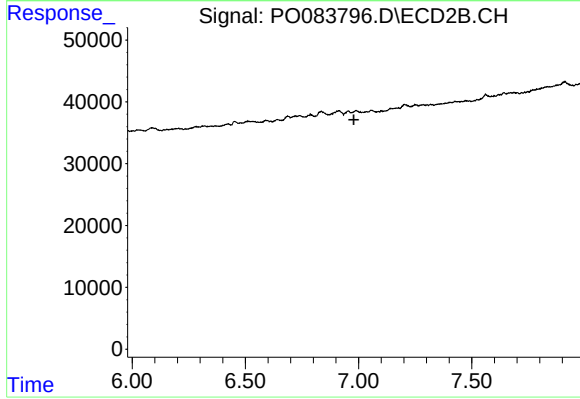

#32 AR-1260-2


R.T.: 0.000 min
Exp R.T. : 6.979 min
Response: 0
Conc: N.D.

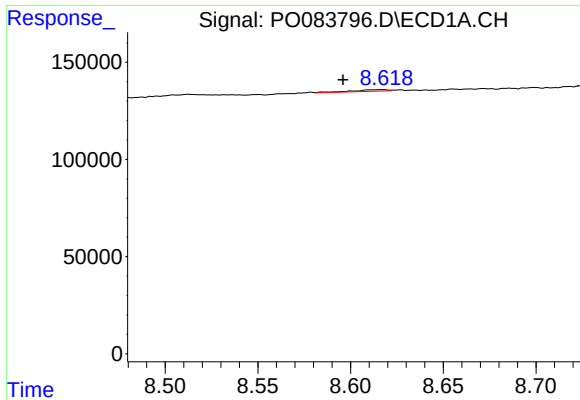

#33 AR-1260-3


R.T.: 8.616 min
Delta R.T.: 0.020 min
Response: 10307
Conc: 3.48 ng/ml

Instrument :
ECD_O
ClientSampleId :
CLI-2021-20-B

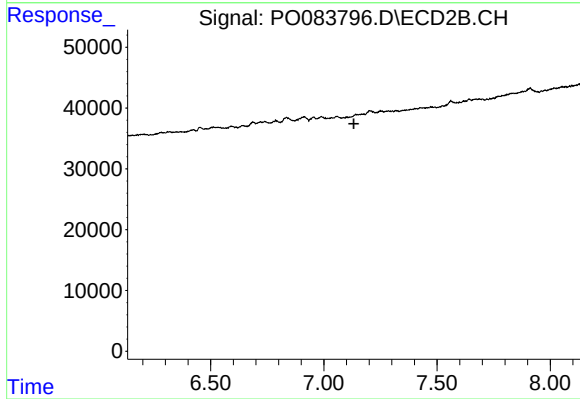


#33 AR-1260-3

R.T.: 0.000 min
Exp R.T. : 7.133 min
Response: 0
Conc: N.D.

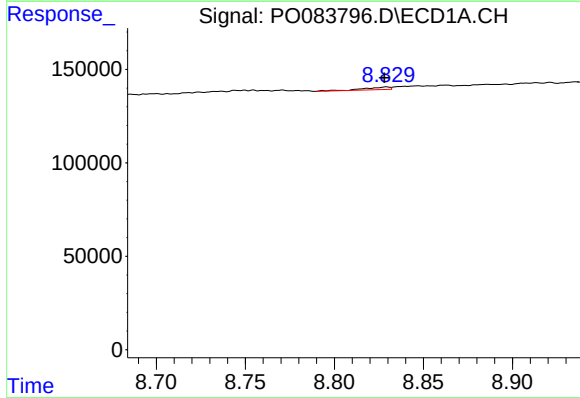


#34 AR-1260-4

R.T.: 8.829 min
Delta R.T.: 0.001 min
Response: 14047
Conc: 4.11 ng/ml

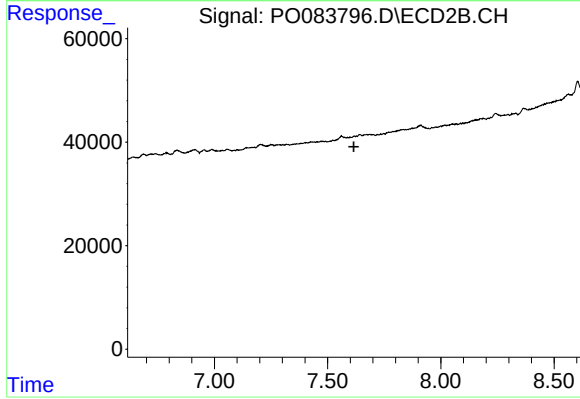

#34 AR-1260-4


R.T.: 0.000 min
Exp R.T. : 7.616 min
Response: 0
Conc: N.D.

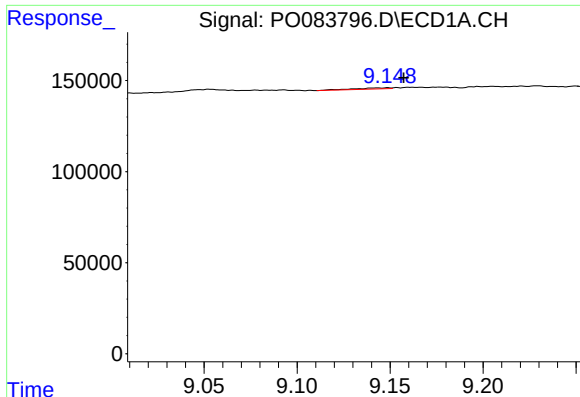

#35 AR-1260-5


R.T.: 9.149 min
Delta R.T.: -0.008 min
Response: 9288
Conc: 1.38 ng/ml

Instrument :
ECD_O
ClientSampleId :
CLI-2021-20-B

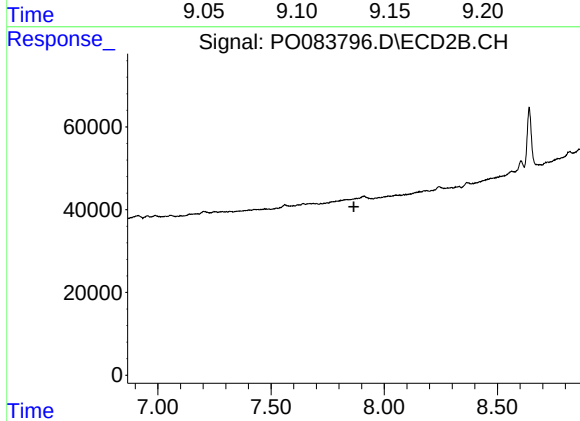


#35 AR-1260-5

R.T.: 0.000 min
Exp R.T. : 7.866 min
Response: 0
Conc: N.D.

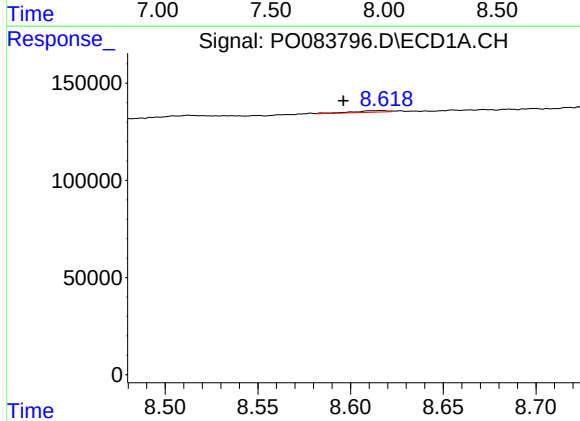


#36 AR-1262-1

R.T.: 8.616 min
Delta R.T.: 0.020 min
Response: 10307
Conc: 2.56 ng/ml

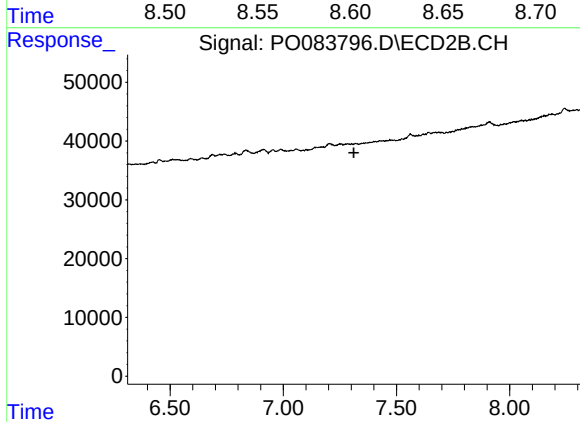

#36 AR-1262-1


R.T.: 0.000 min
Exp R.T. : 7.312 min
Response: 0
Conc: N.D.

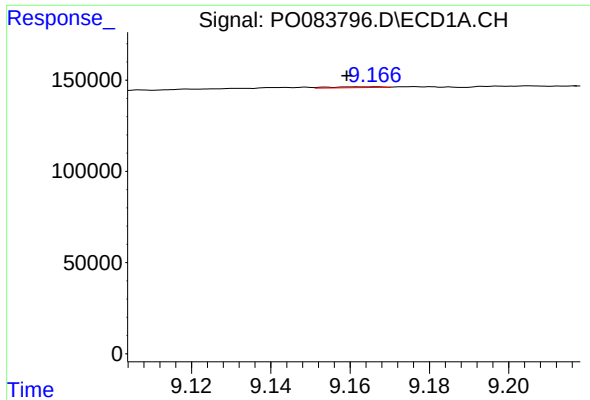

#37 AR-1262-2

R.T.: 9.166 min
Delta R.T.: 0.007 min
Response: 3969
Conc: 0.57 ng/ml

Instrument :
ECD_O
ClientSampleId :
CLI-2021-20-B

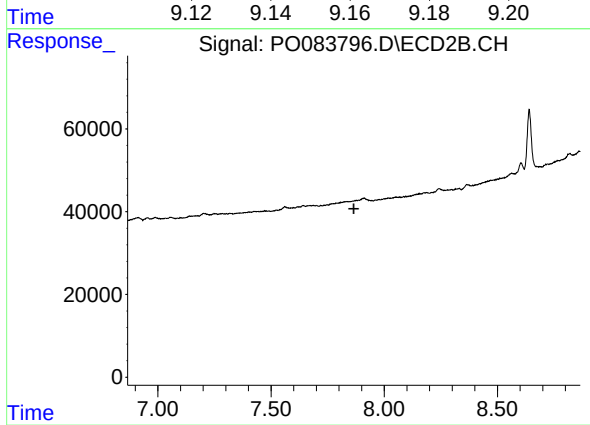

#37 AR-1262-2

R.T.: 0.000 min
Exp R.T. : 7.866 min
Response: 0
Conc: N.D.