

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO121621\
 Data File : PO083798.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 17 Dec 2021 4:56
 Operator : AJ\MA
 Sample : M5070-26 10X
 Misc :
 ALS Vial : 50 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 CLI-2021-20-B

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 17 06:06:37 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO121521.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Dec 16 04:05:27 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.936	3.941	155503	51981	1.632	1.772
2) SA Decachlor...	11.014	9.240	137138	35794	2.002	1.275 #
Target Compounds						
28) L6 AR-1254-3	7.804	0.000	42529	0	9.121	N.D. #
30) L6 AR-1254-5	8.524	0.000	8621	0	2.418	N.D. #
31) L7 AR-1260-1	7.968	0.000	21694	0	6.695	N.D. #
32) L7 AR-1260-2	8.235	0.000	13670	0	3.529	N.D. #
33) L7 AR-1260-3	8.595	0.000	8436	0	2.848	N.D. #
34) L7 AR-1260-4	8.842	0.000	7010	0	2.049	N.D. #
36) L8 AR-1262-1	8.595	0.000	8436	0	2.092	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO121621\
Data File : P0083798.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 17 Dec 2021 4:56
Operator : AJ\MA
Sample : M5070-26 10X
Misc :
ALS Vial : 50 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
CLI-2021-20-B

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 17 06:06:37 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO121521.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Dec 16 04:05:27 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

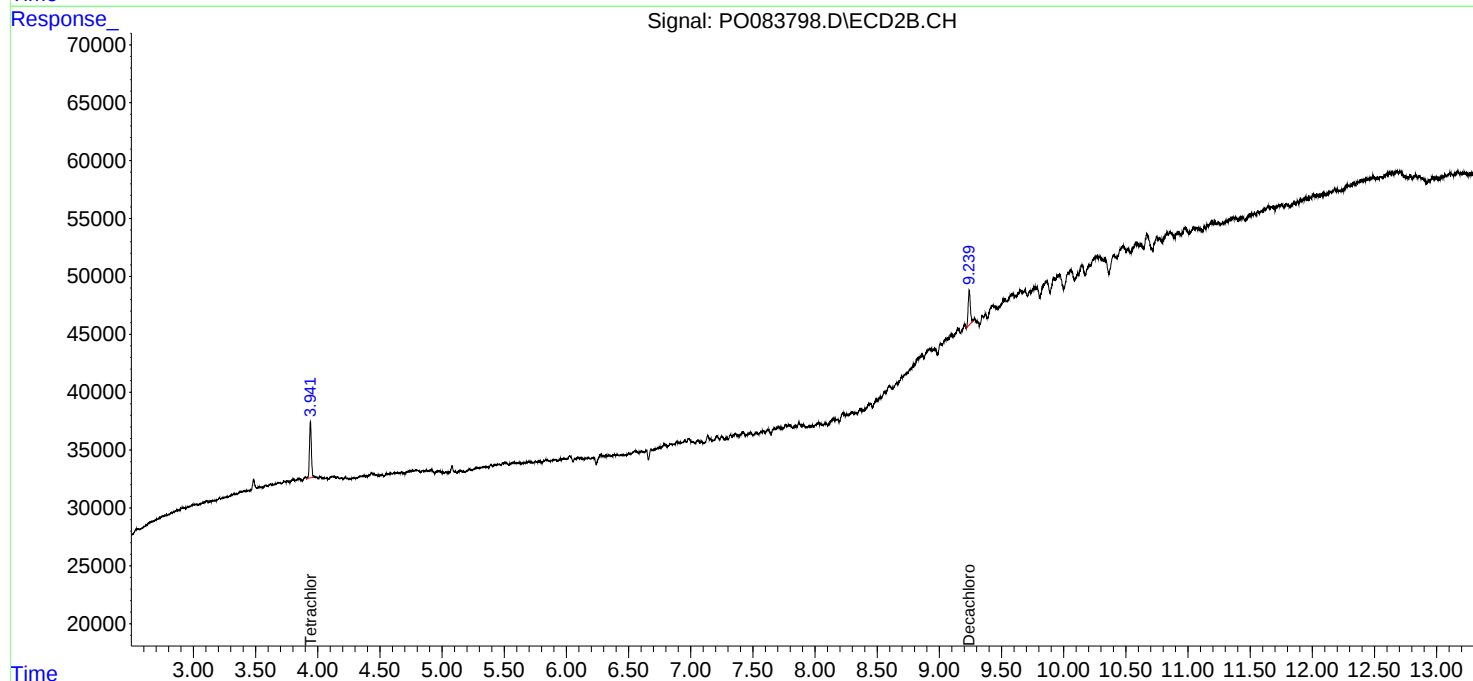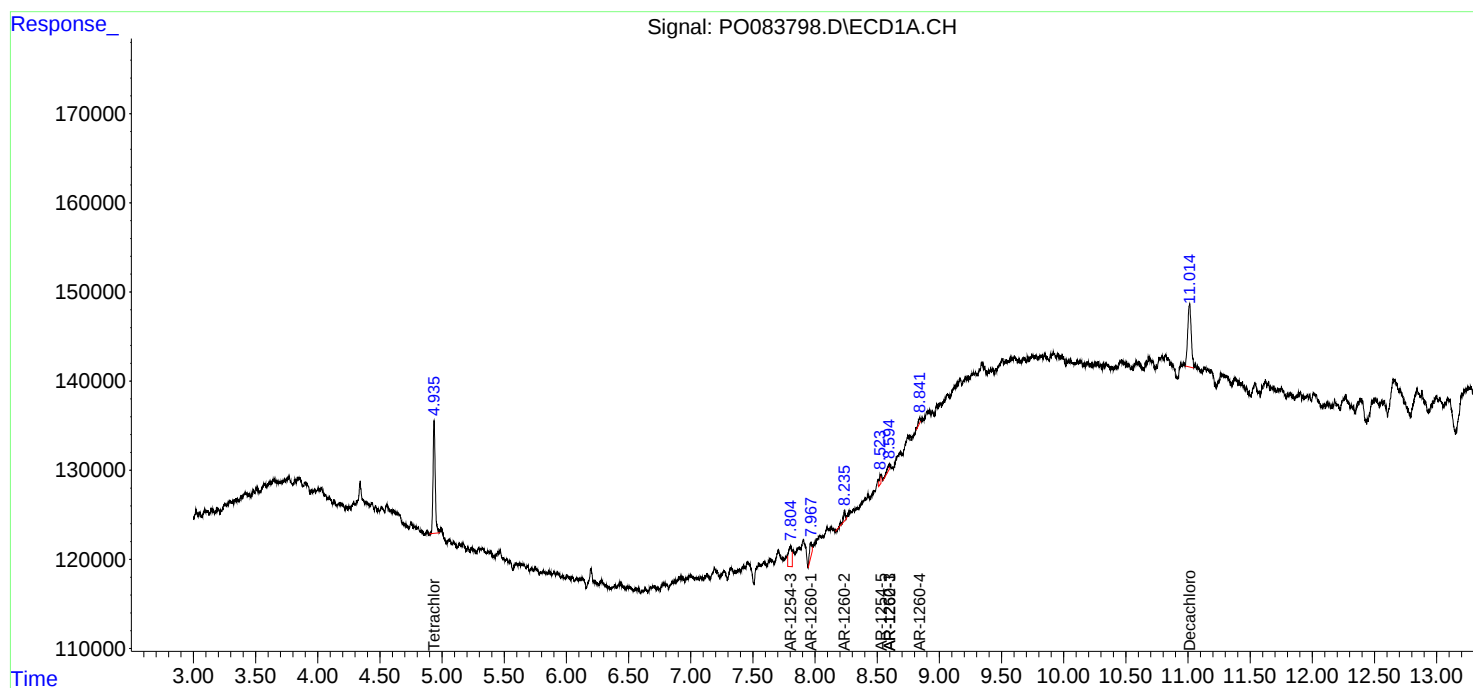


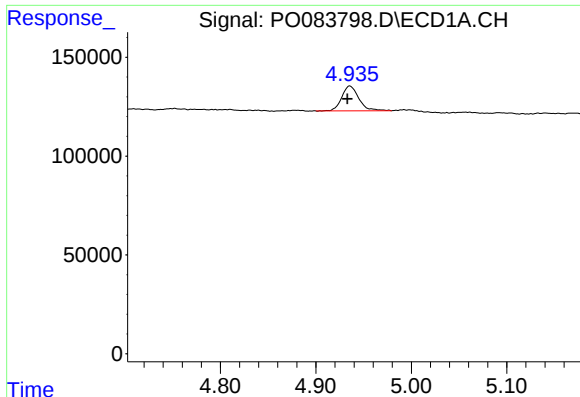

#1 Tetrachloro-m-xylene


R.T.: 4.936 min
Delta R.T.: 0.003 min
Response: 155503
Conc: 1.63 ng/ml

Instrument :
ECD_O
ClientSampleId :
CLI-2021-20-B

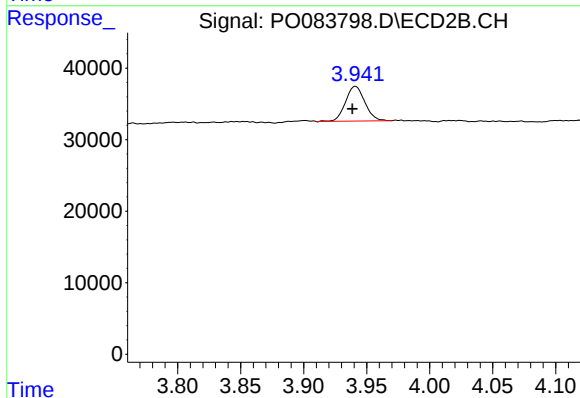


#1 Tetrachloro-m-xylene

R.T.: 3.941 min
Delta R.T.: 0.002 min
Response: 51981
Conc: 1.77 ng/ml

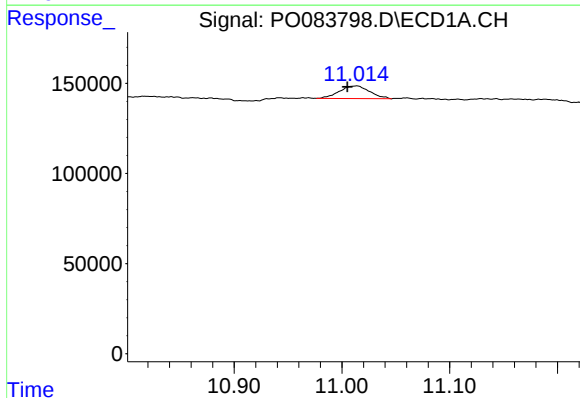


#2 Decachlorobiphenyl

R.T.: 11.014 min
Delta R.T.: 0.009 min
Response: 137138
Conc: 2.00 ng/ml

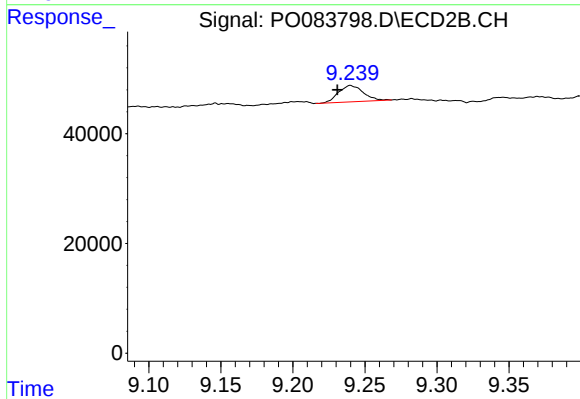

#2 Decachlorobiphenyl


R.T.: 9.240 min
Delta R.T.: 0.009 min
Response: 35794
Conc: 1.27 ng/ml

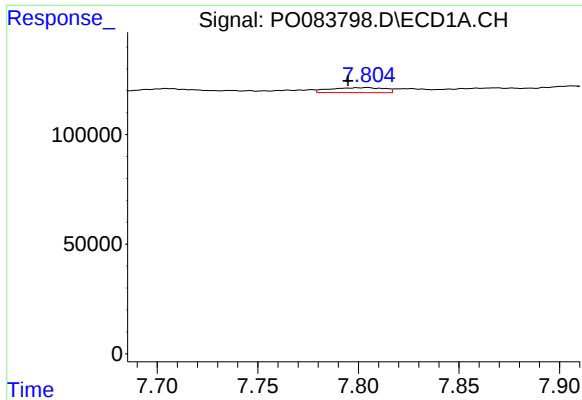

#28 AR-1254-3


R.T.: 7.804 min
Delta R.T.: 0.010 min
Response: 42529
Conc: 9.12 ng/ml

Instrument :
ECD_O
ClientSampleId :
CLI-2021-20-B

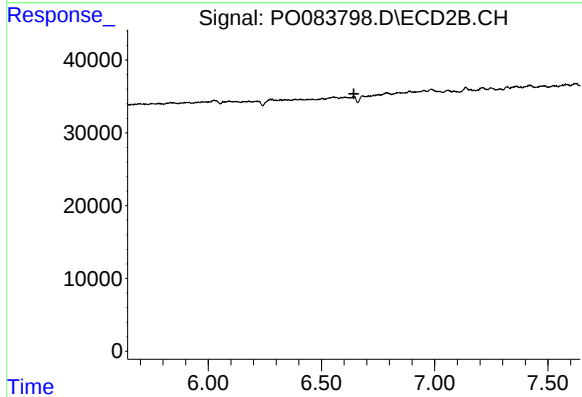


#28 AR-1254-3

R.T.: 0.000 min
Exp R.T. : 6.643 min
Response: 0
Conc: N.D.

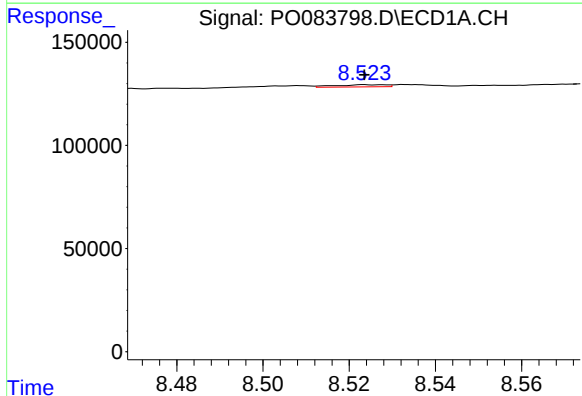


#30 AR-1254-5

R.T.: 8.524 min
Delta R.T.: 0.000 min
Response: 8621
Conc: 2.42 ng/ml

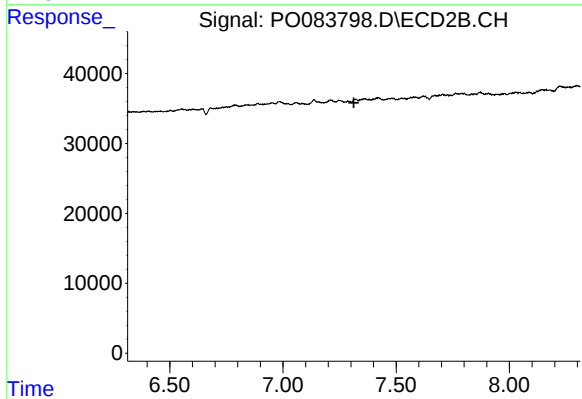

#30 AR-1254-5


R.T.: 0.000 min
Exp R.T. : 7.313 min
Response: 0
Conc: N.D.

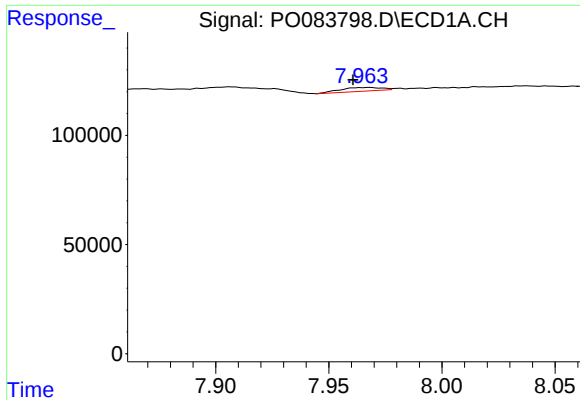

#31 AR-1260-1


R.T.: 7.968 min
Delta R.T.: 0.007 min
Response: 21694
Conc: 6.70 ng/ml

Instrument :
ECD_O
ClientSampleId :
CLI-2021-20-B

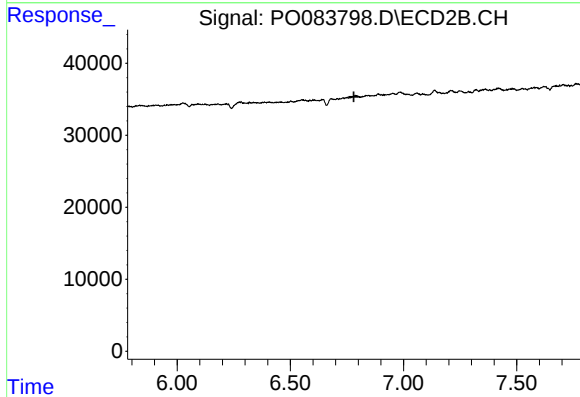


#31 AR-1260-1

R.T.: 0.000 min
Exp R.T. : 6.780 min
Response: 0
Conc: N.D.

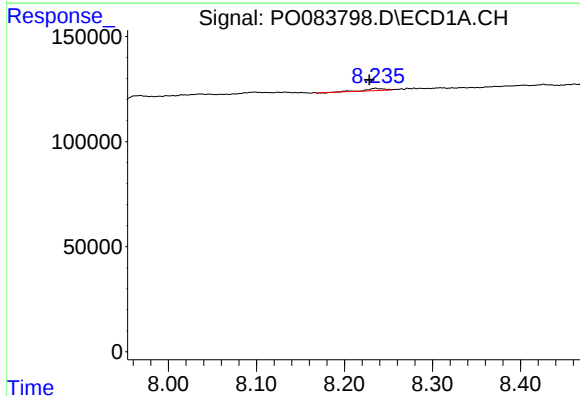


#32 AR-1260-2

R.T.: 8.235 min
Delta R.T.: 0.007 min
Response: 13670
Conc: 3.53 ng/ml

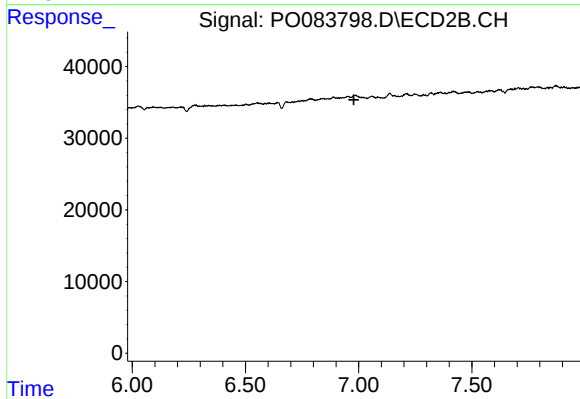

#32 AR-1260-2


R.T.: 0.000 min
Exp R.T. : 6.979 min
Response: 0
Conc: N.D.

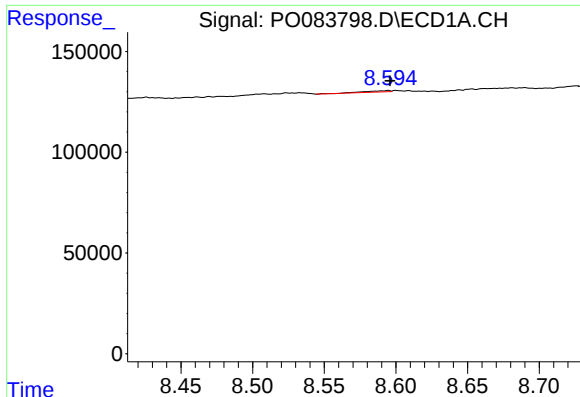

#33 AR-1260-3


R.T.: 8.595 min
Delta R.T.: -0.001 min
Response: 8436
Conc: 2.85 ng/ml

Instrument :
ECD_O
ClientSampleId :
CLI-2021-20-B

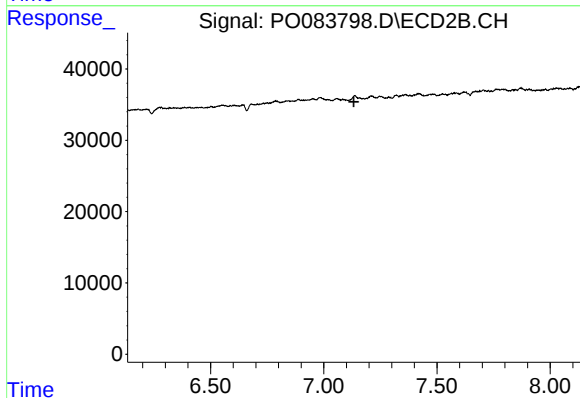


#33 AR-1260-3

R.T.: 0.000 min
Exp R.T. : 7.133 min
Response: 0
Conc: N.D.

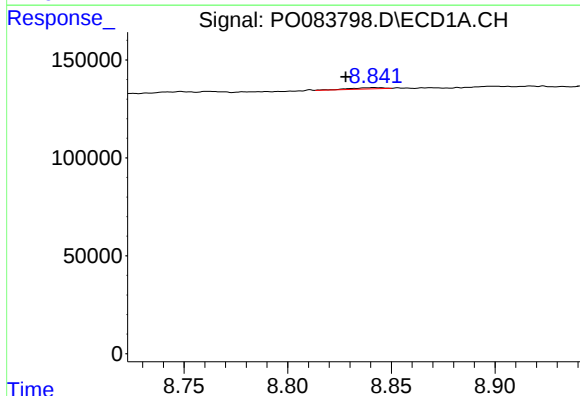


#34 AR-1260-4

R.T.: 8.842 min
Delta R.T.: 0.014 min
Response: 7010
Conc: 2.05 ng/ml

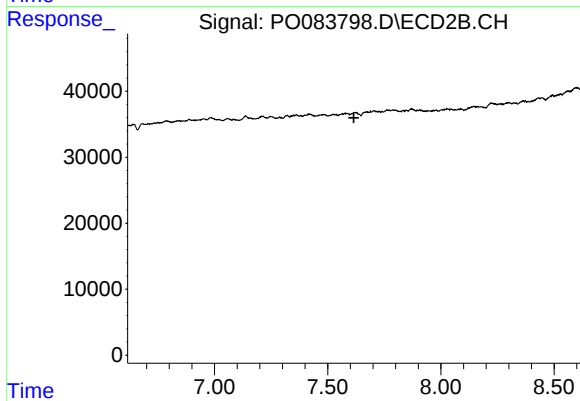

#34 AR-1260-4


R.T.: 0.000 min
Exp R.T. : 7.616 min
Response: 0
Conc: N.D.

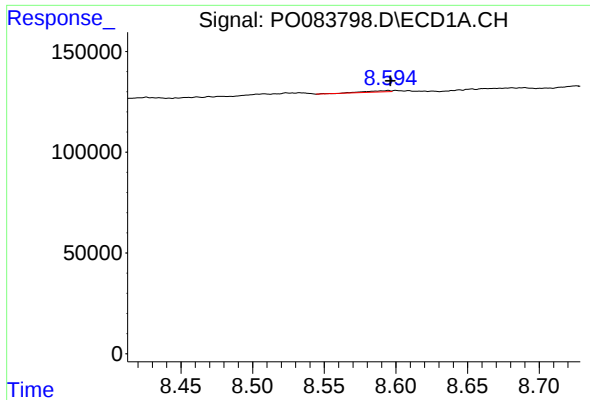

#36 AR-1262-1

R.T.: 8.595 min
Delta R.T.: -0.002 min
Response: 8436
Conc: 2.09 ng/ml

Instrument :
ECD_O
ClientSampleId :
CLI-2021-20-B

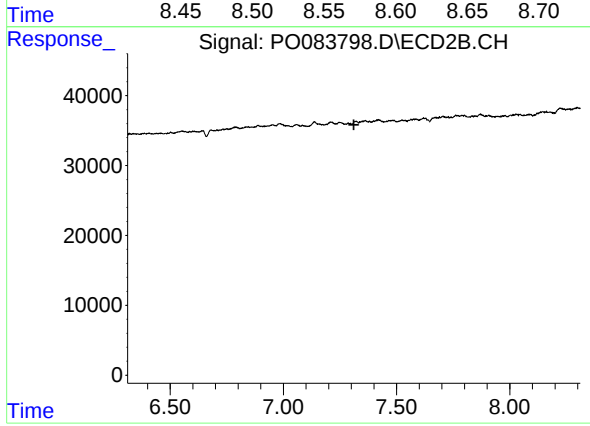

#36 AR-1262-1

R.T.: 0.000 min
Exp R.T. : 7.312 min
Response: 0
Conc: N.D.