

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO121621\
 Data File : PO083800.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 17 Dec 2021 5:30
 Operator : AJ\MA
 Sample : M5070-28 10X
 Misc :
 ALS Vial : 52 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 CLI-2021-22-B

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 17 06:07:10 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO121521.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Dec 16 04:05:27 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.935	3.942	104523	39357	1.097	1.342
2) SA Decachlor...	11.012	9.238	136316	43112	1.990	1.535
Target Compounds						
30) L6 AR-1254-5	8.529	0.000	42668	0	11.969	N.D. #
32) L7 AR-1260-2	8.239	0.000	12806	0	3.306	N.D. #
33) L7 AR-1260-3	8.597	0.000	24509	0	8.274	N.D. #
34) L7 AR-1260-4	8.843f	0.000	22844	0	6.678	N.D. #
35) L7 AR-1260-5	9.150	0.000	11496	0	1.706	N.D. #
36) L8 AR-1262-1	8.597	0.000	24509	0	6.077	N.D. #
37) L8 AR-1262-2	9.150	0.000	11496	0	1.643	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO121621\
Data File : P0083800.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 17 Dec 2021 5:30
Operator : AJ\MA
Sample : M5070-28 10X
Misc :
ALS Vial : 52 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
CLI-2021-22-B

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 17 06:07:10 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO121521.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Dec 16 04:05:27 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

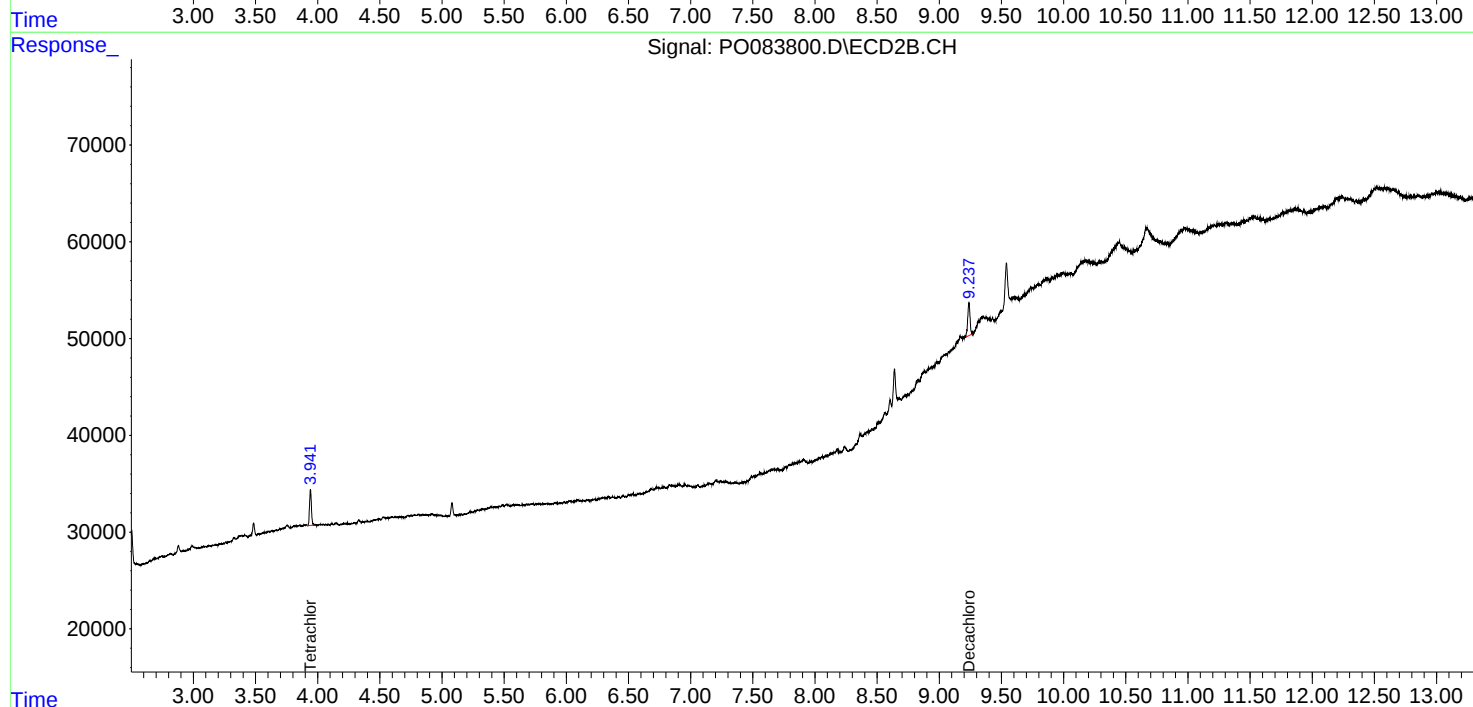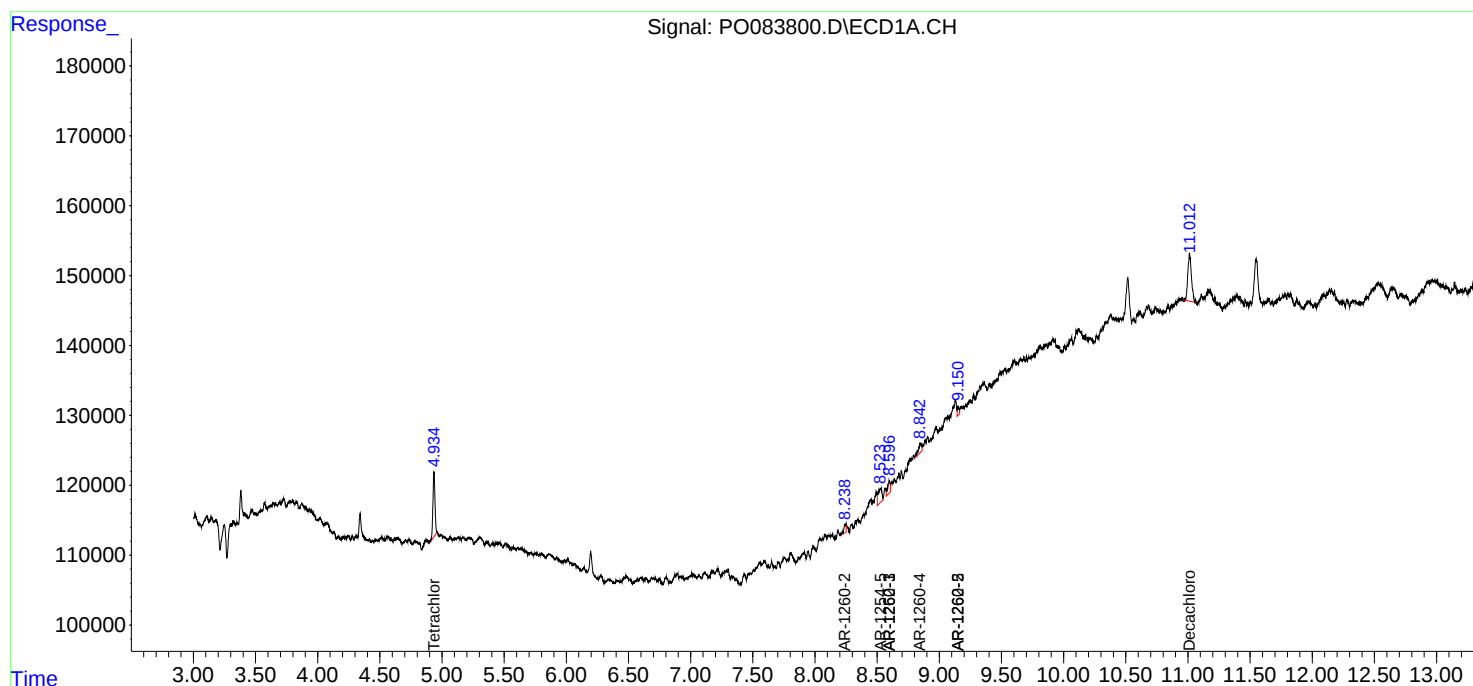


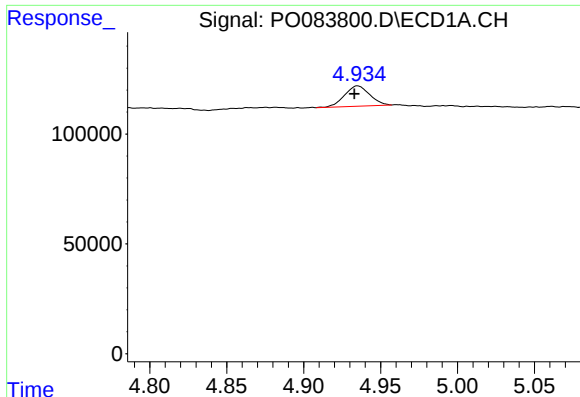

#1 Tetrachloro-m-xylene


R.T.: 4.935 min
Delta R.T.: 0.002 min
Response: 104523
Conc: 1.10 ng/ml

Instrument :
ECD_O
ClientSampleId :
CLI-2021-22-B

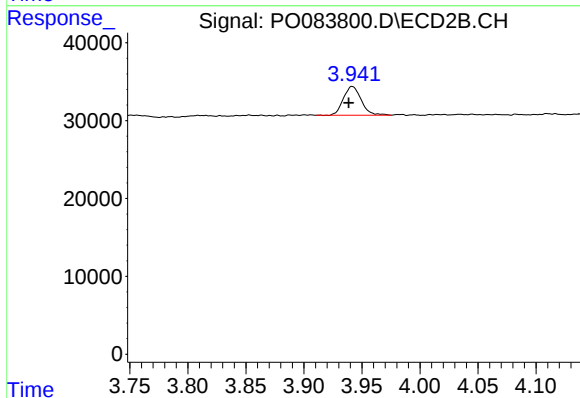


#1 Tetrachloro-m-xylene

R.T.: 3.942 min
Delta R.T.: 0.003 min
Response: 39357
Conc: 1.34 ng/ml

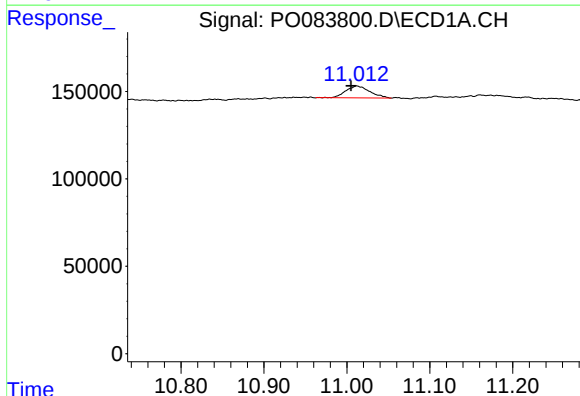


#2 Decachlorobiphenyl

R.T.: 11.012 min
Delta R.T.: 0.007 min
Response: 136316
Conc: 1.99 ng/ml

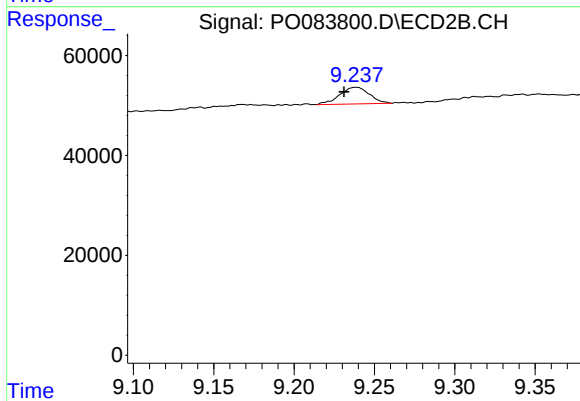

#2 Decachlorobiphenyl


R.T.: 9.238 min
Delta R.T.: 0.007 min
Response: 43112
Conc: 1.54 ng/ml

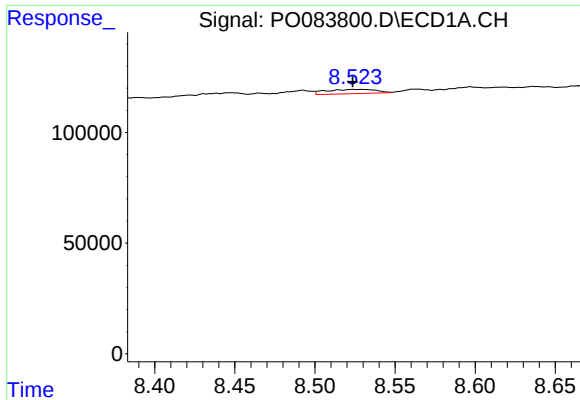

#30 AR-1254-5


R.T.: 8.529 min
Delta R.T.: 0.005 min
Response: 42668
Conc: 11.97 ng/ml

Instrument :
ECD_O
ClientSampleId :
CLI-2021-22-B

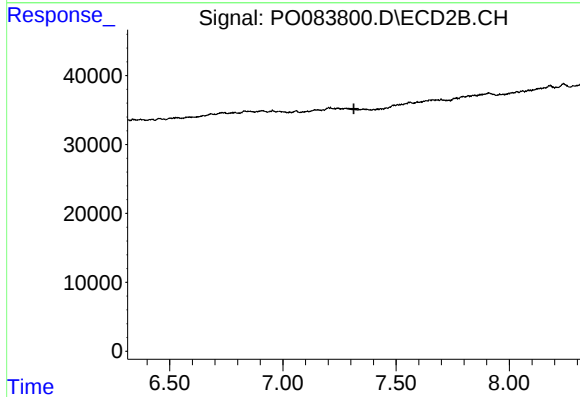


#30 AR-1254-5

R.T.: 0.000 min
Exp R.T. : 7.313 min
Response: 0
Conc: N.D.

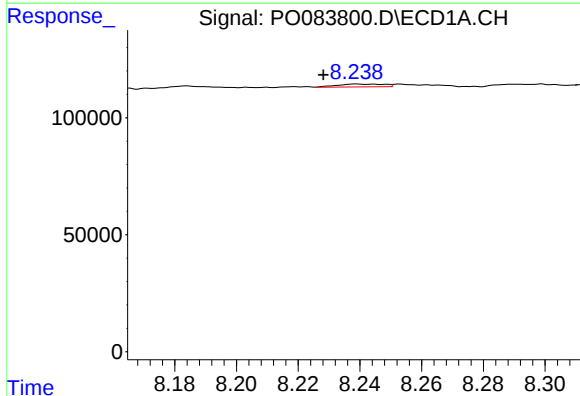


#32 AR-1260-2

R.T.: 8.239 min
Delta R.T.: 0.011 min
Response: 12806
Conc: 3.31 ng/ml

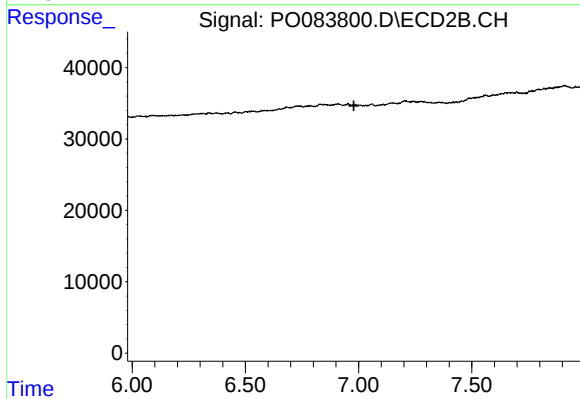

#32 AR-1260-2


R.T.: 0.000 min
Exp R.T. : 6.979 min
Response: 0
Conc: N.D.

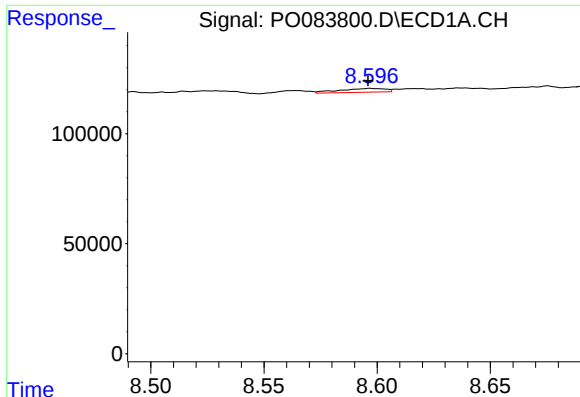

#33 AR-1260-3


R.T.: 8.597 min
Delta R.T.: 0.001 min
Response: 24509
Conc: 8.27 ng/ml

Instrument :
ECD_O
ClientSampleId :
CLI-2021-22-B

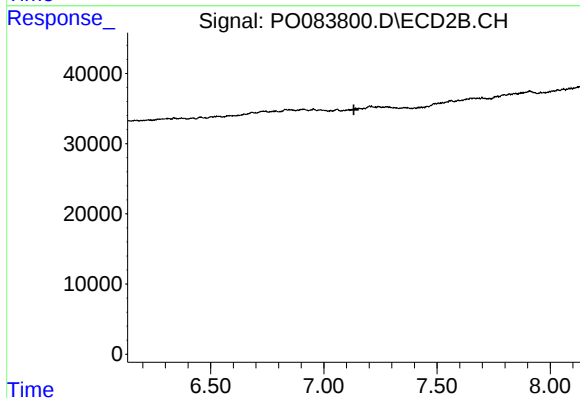


#33 AR-1260-3

R.T.: 0.000 min
Exp R.T. : 7.133 min
Response: 0
Conc: N.D.

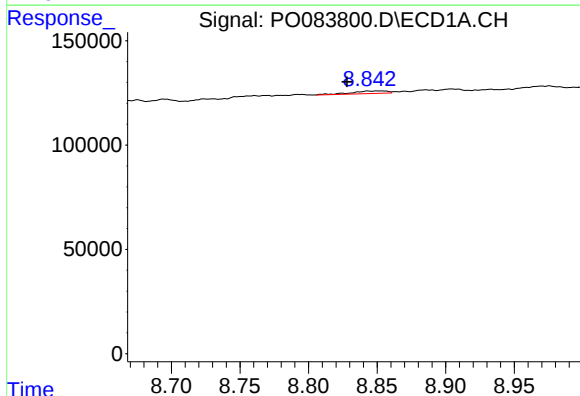


#34 AR-1260-4

R.T.: 8.843 min
Delta R.T.: 0.015 min
Response: 22844
Conc: 6.68 ng/ml

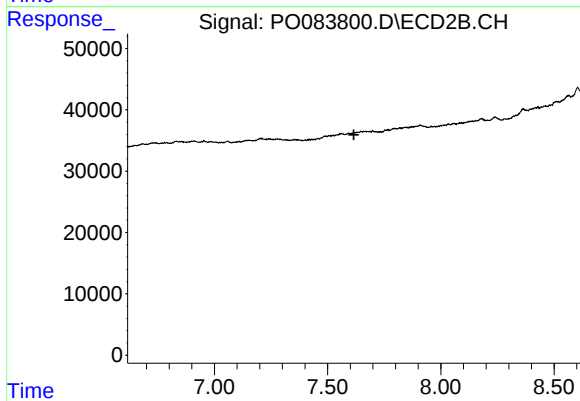

#34 AR-1260-4


R.T.: 0.000 min
Exp R.T. : 7.616 min
Response: 0
Conc: N.D.

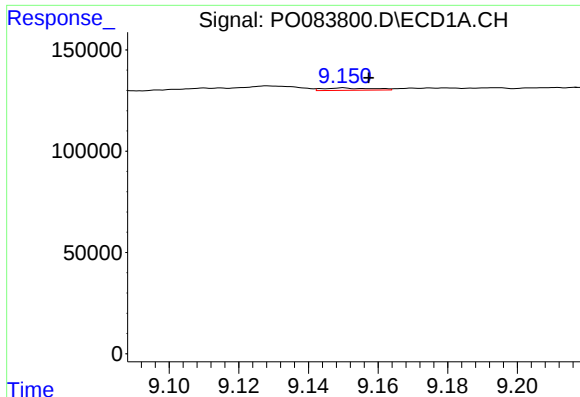

#35 AR-1260-5


R.T.: 9.150 min
Delta R.T.: -0.007 min
Response: 11496
Conc: 1.71 ng/ml

Instrument :
ECD_O
ClientSampleId :
CLI-2021-22-B

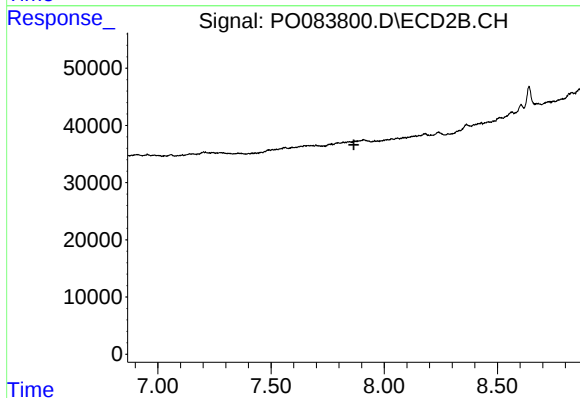


#35 AR-1260-5

R.T.: 0.000 min
Exp R.T. : 7.866 min
Response: 0
Conc: N.D.

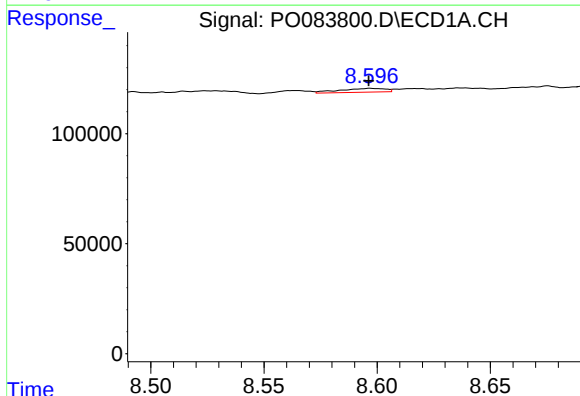


#36 AR-1262-1

R.T.: 8.597 min
Delta R.T.: 0.000 min
Response: 24509
Conc: 6.08 ng/ml

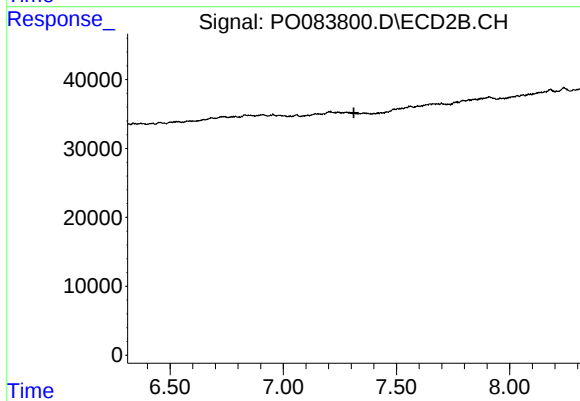

#36 AR-1262-1


R.T.: 0.000 min
Exp R.T. : 7.312 min
Response: 0
Conc: N.D.

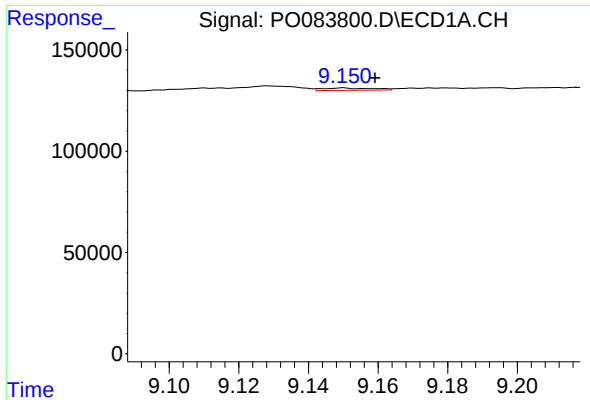

#37 AR-1262-2

R.T.: 9.150 min
Delta R.T.: -0.009 min
Response: 11496
Conc: 1.64 ng/ml

Instrument :
ECD_O
ClientSampleId :
CLI-2021-22-B

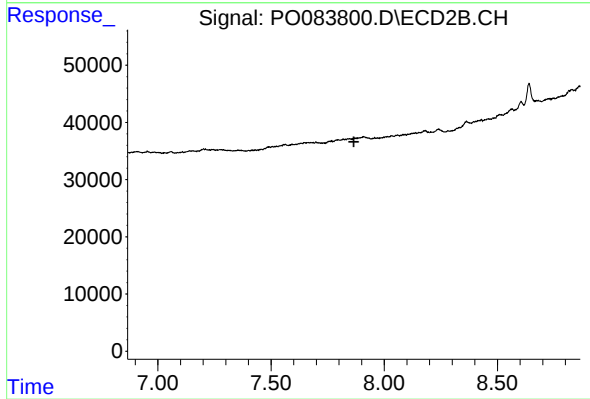

#37 AR-1262-2

R.T.: 0.000 min
Exp R.T. : 7.866 min
Response: 0
Conc: N.D.