

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO121621\
 Data File : PO083751.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 16 Dec 2021 13:34
 Operator : AJ\MA
 Sample : M5077-06
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 06-A-06-B-06-C

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 17 01:29:39 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO121521.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Dec 16 04:05:27 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.934	3.939	2115948	640217	22.210	21.826
2)	SA Decachlor...	11.007	9.236	1475413	527944	21.541	18.802

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO121621\
Data File : PO083751.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 16 Dec 2021 13:34
Operator : AJ\MA
Sample : M5077-06
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
06-A-06-B-06-C

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 17 01:29:39 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO121521.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Dec 16 04:05:27 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

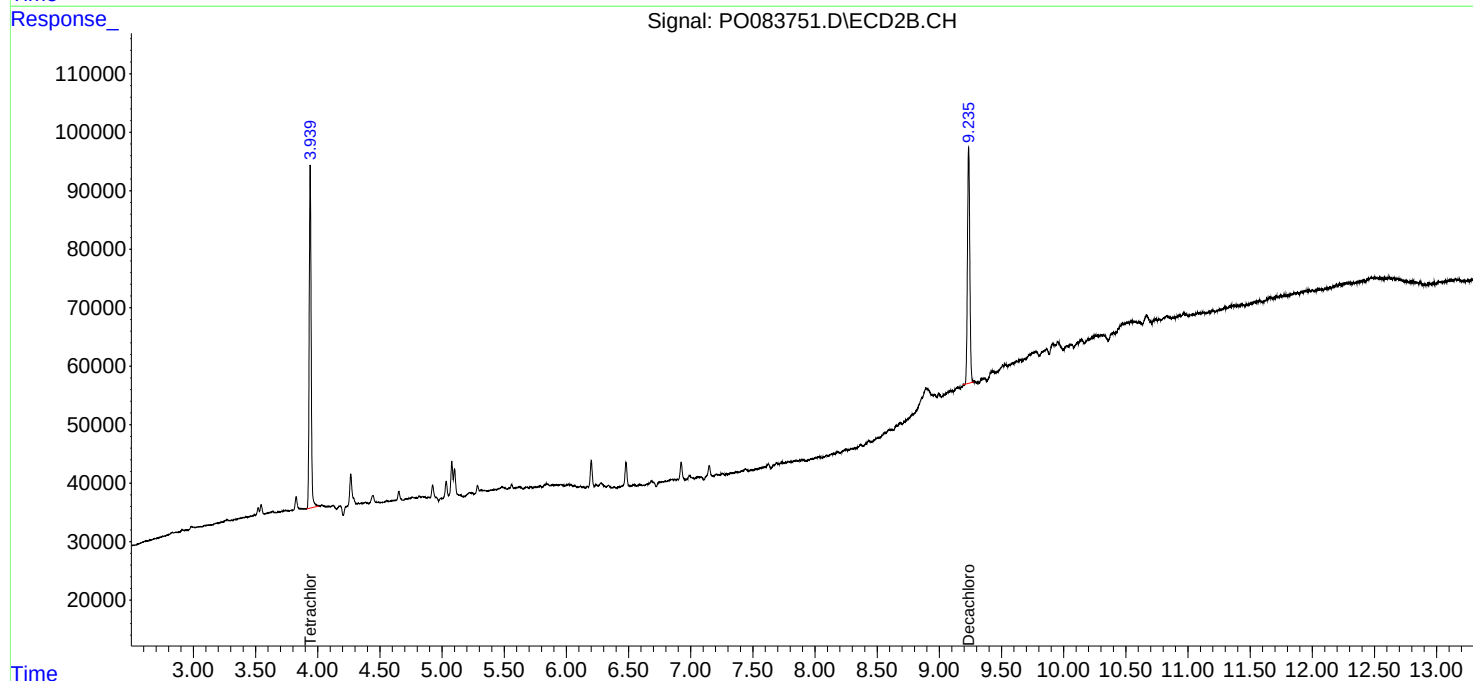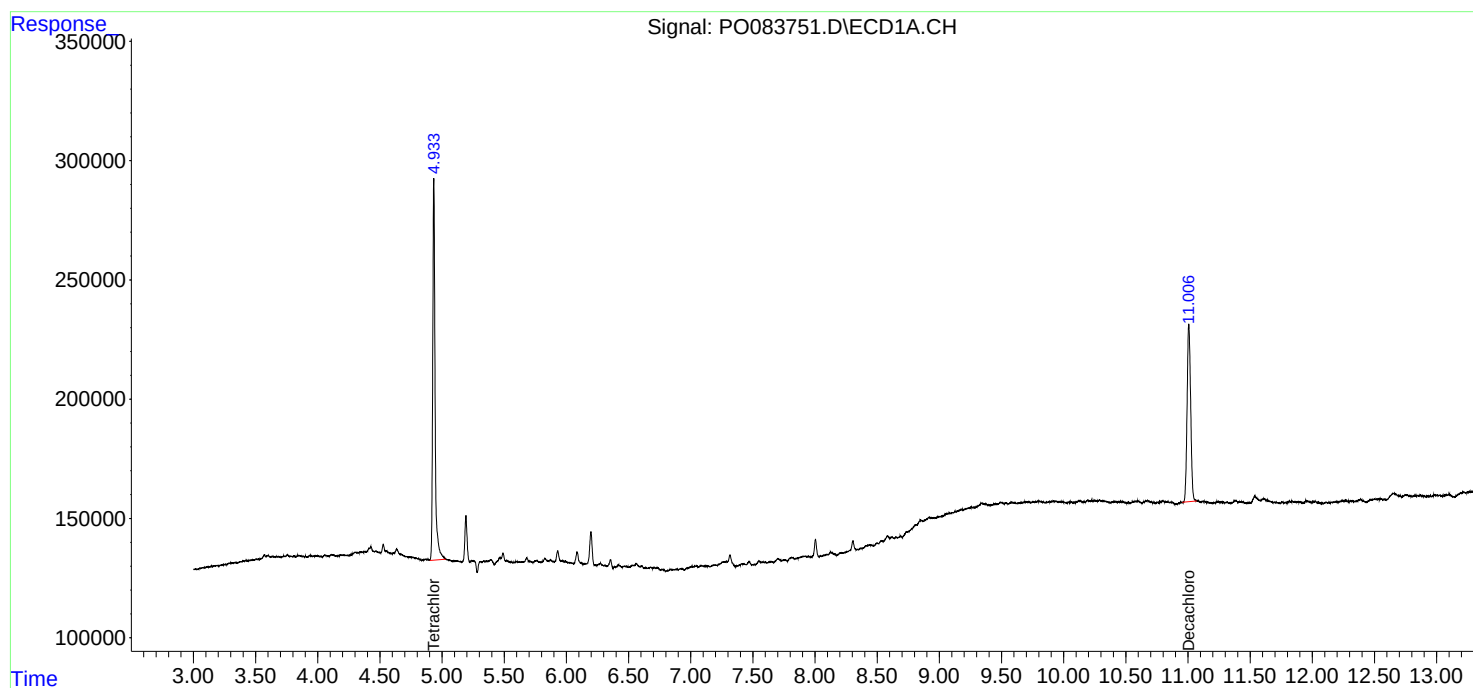


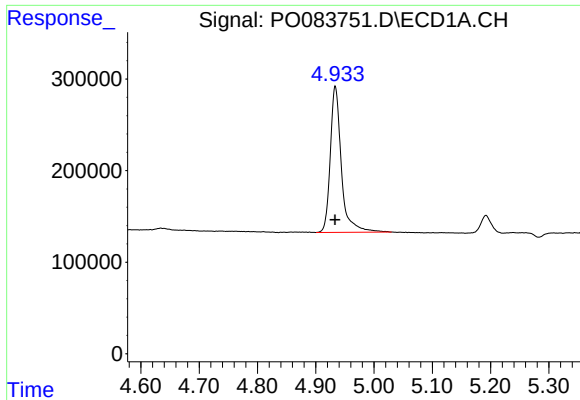

#1 Tetrachloro-m-xylene


R.T.: 4.934 min
Delta R.T.: 0.000 min
Response: 2115948
Conc: 22.21 ng/ml

Instrument :
ECD_O
ClientSampleId :
06-A-06-B-06-C

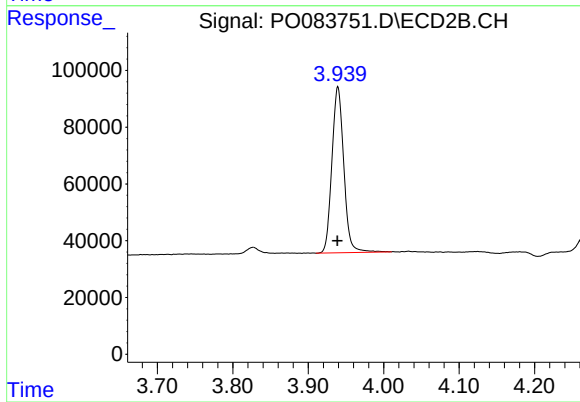


#1 Tetrachloro-m-xylene

R.T.: 3.939 min
Delta R.T.: 0.000 min
Response: 640217
Conc: 21.83 ng/ml

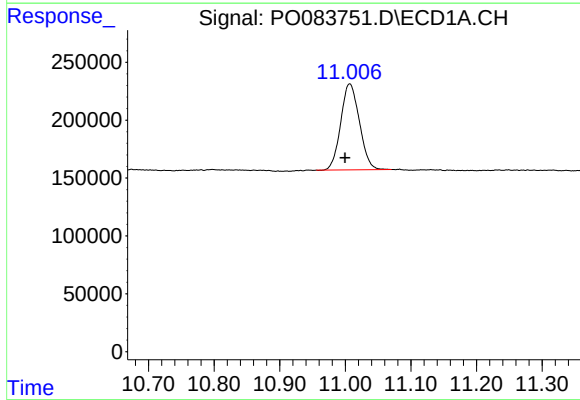

#2 Decachlorobiphenyl

R.T.: 11.007 min
Delta R.T.: 0.007 min
Response: 1475413
Conc: 21.54 ng/ml

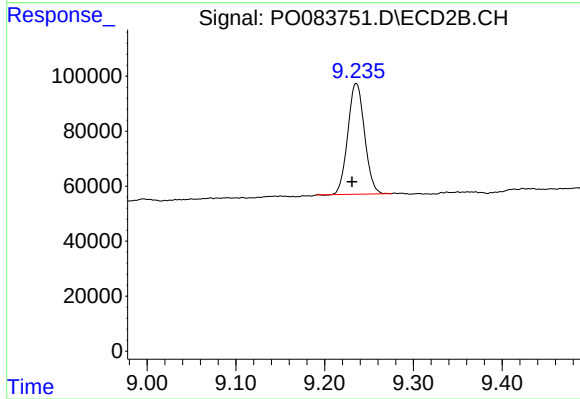

#2 Decachlorobiphenyl

R.T.: 9.236 min
Delta R.T.: 0.005 min
Response: 527944
Conc: 18.80 ng/ml