

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0121621\
 Data File : P0083793.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 17 Dec 2021 3:30
 Operator : AJ\MA
 Sample : M5070-21 10X
 Misc :
 ALS Vial : 45 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 CLI-2021-19-A

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 17 04:45:29 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0121521.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Dec 16 04:05:27 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.936	3.941	146035	51340	1.533	1.750
2) SA Decachlor...	11.014	9.239	167768	48394	2.449	1.723 #

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO121621\
Data File : PO083793.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 17 Dec 2021 3:30
Operator : AJ\MA
Sample : M5070-21 10X
Misc :
ALS Vial : 45 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
CLI-2021-19-A

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 17 04:45:29 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO121521.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Dec 16 04:05:27 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

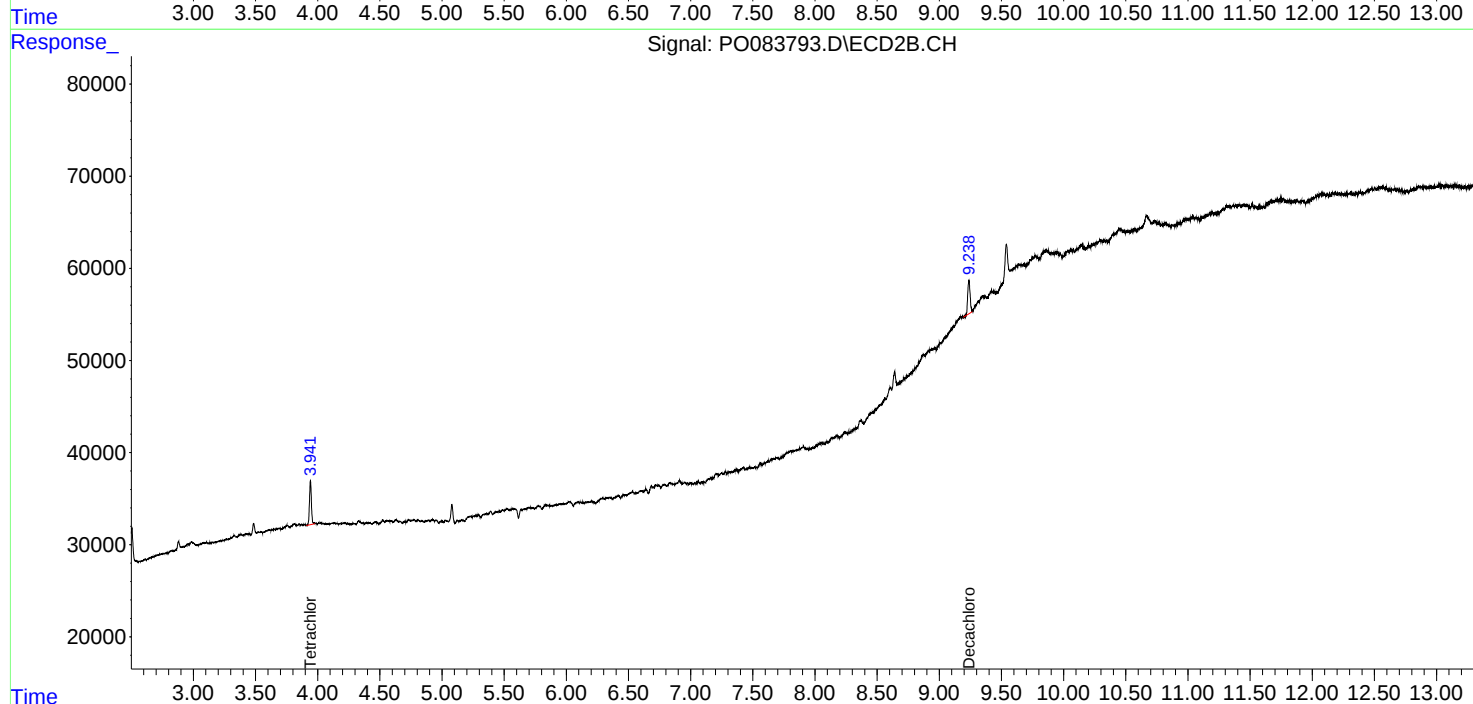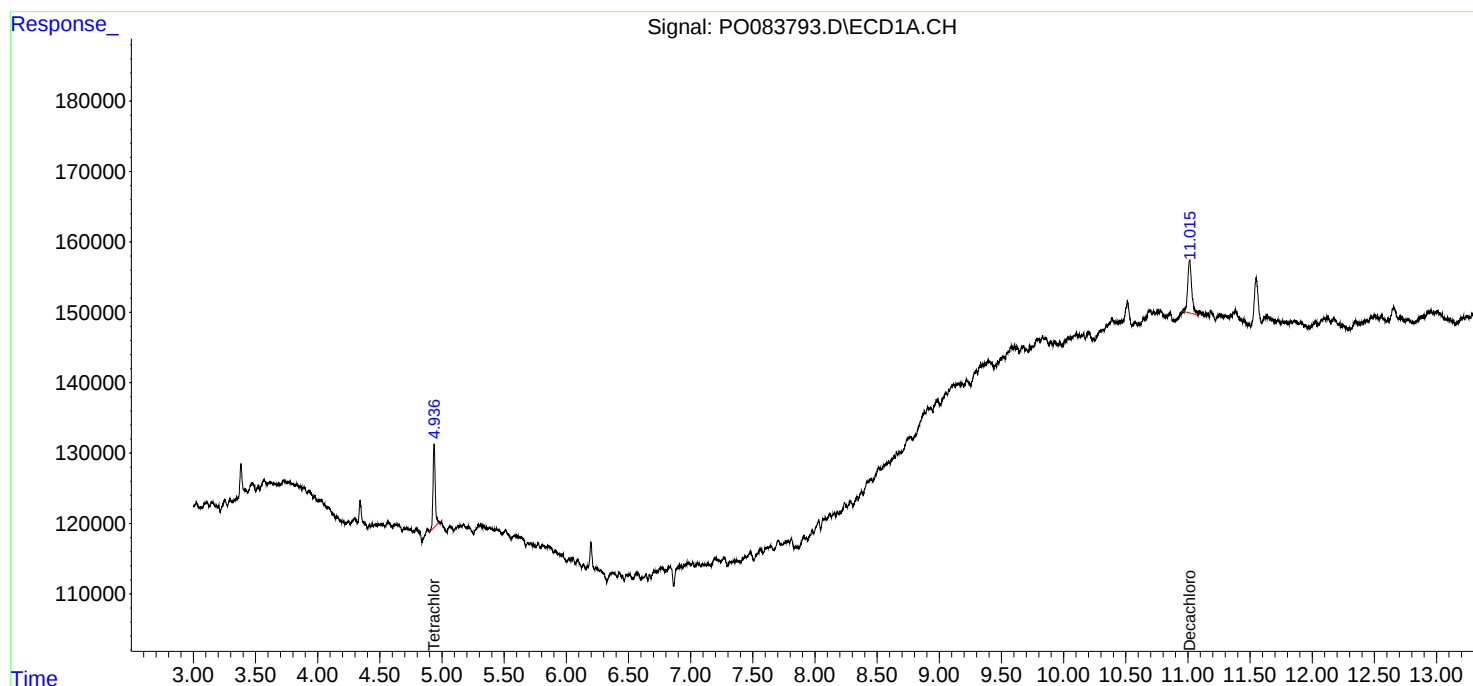


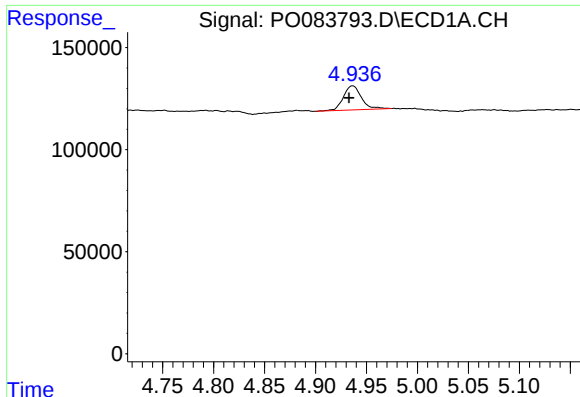

#1 Tetrachloro-m-xylene


R.T.: 4.936 min
Delta R.T.: 0.003 min
Response: 146035
Conc: 1.53 ng/ml

Instrument :
ECD_O
ClientSampleId :
CLI-2021-19-A

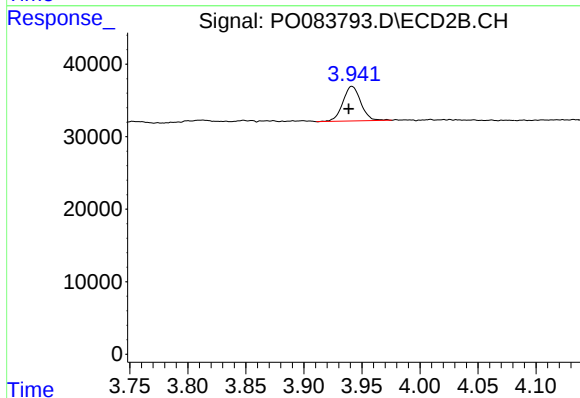


#1 Tetrachloro-m-xylene

R.T.: 3.941 min
Delta R.T.: 0.003 min
Response: 51340
Conc: 1.75 ng/ml

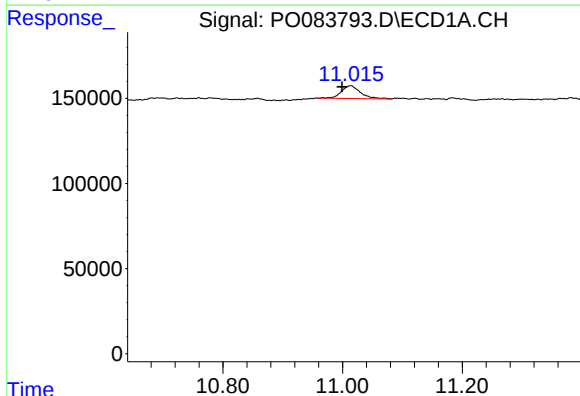

#2 Decachlorobiphenyl

R.T.: 11.014 min
Delta R.T.: 0.014 min
Response: 167768
Conc: 2.45 ng/ml

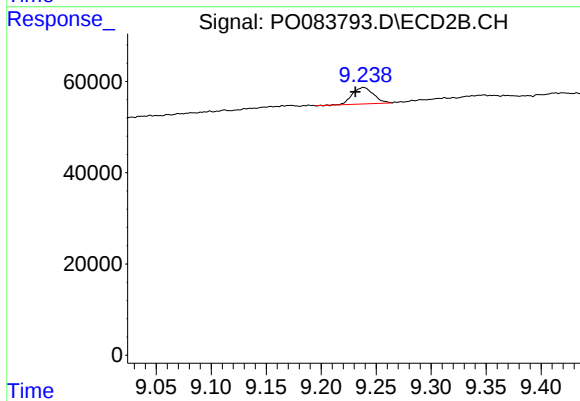

#2 Decachlorobiphenyl

R.T.: 9.239 min
Delta R.T.: 0.008 min
Response: 48394
Conc: 1.72 ng/ml