

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO121621\
 Data File : PO083797.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 17 Dec 2021 4:39
 Operator : AJ\MA
 Sample : M5070-25 10X
 Misc :
 ALS Vial : 49 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 CLI-2021-21-A

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 17 06:06:23 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO121521.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Dec 16 04:05:27 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.937	3.942	134774	39447	1.415	1.345
2)	SA Decachlor...	11.014	9.240	115509	50268	1.686	1.790

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO121621\
Data File : P0083797.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 17 Dec 2021 4:39
Operator : AJ\MA
Sample : M5070-25 10X
Misc :
ALS Vial : 49 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
CLI-2021-21-A

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 17 06:06:23 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO121521.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Dec 16 04:05:27 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

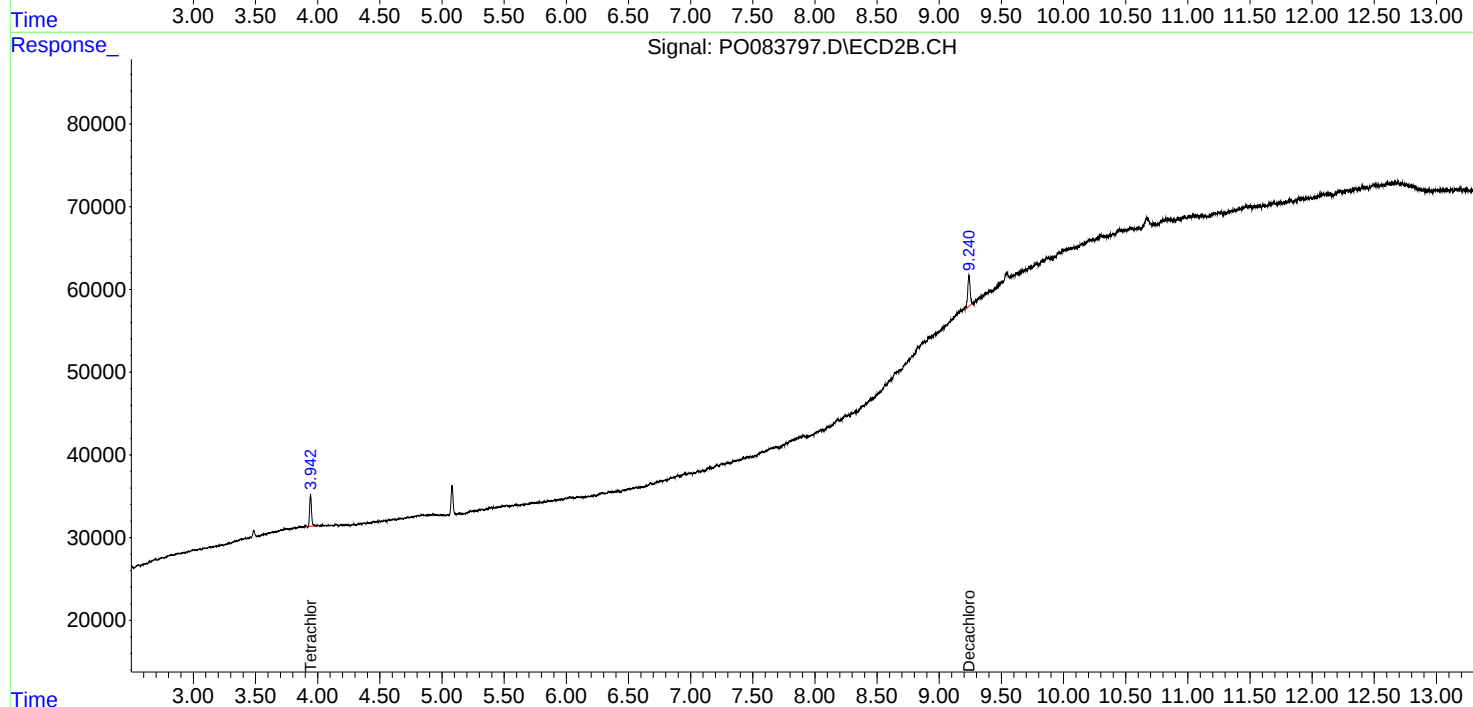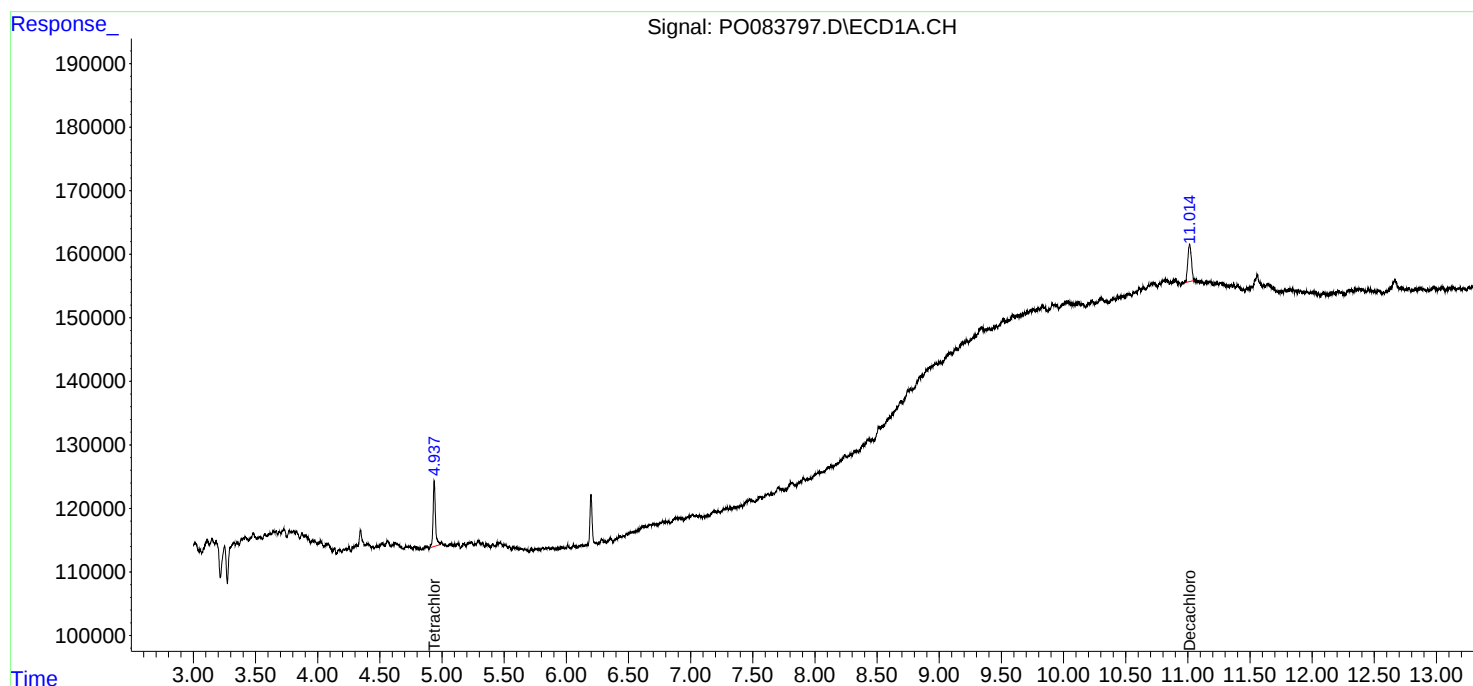


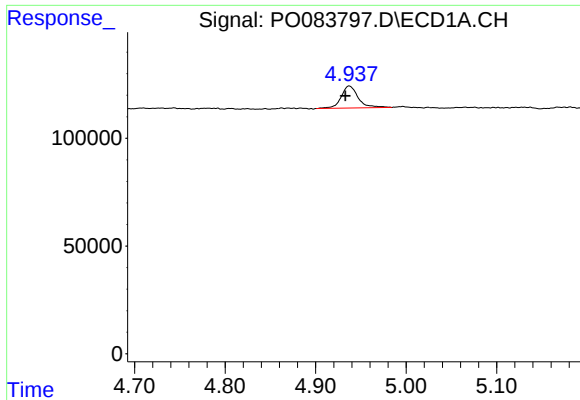

#1 Tetrachloro-m-xylene


R.T.: 4.937 min
Delta R.T.: 0.004 min
Response: 134774
Conc: 1.41 ng/ml

Instrument :
ECD_O
ClientSampleId :
CLI-2021-21-A

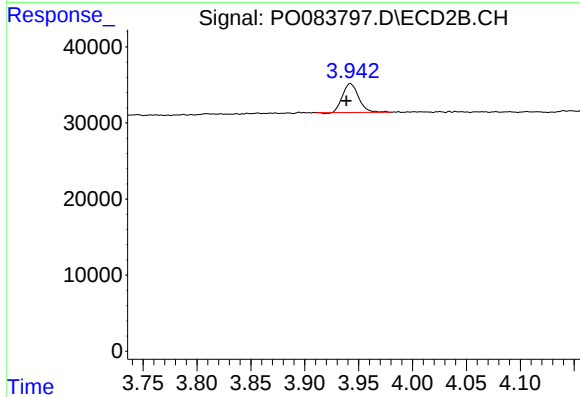


#1 Tetrachloro-m-xylene

R.T.: 3.942 min
Delta R.T.: 0.004 min
Response: 39447
Conc: 1.34 ng/ml

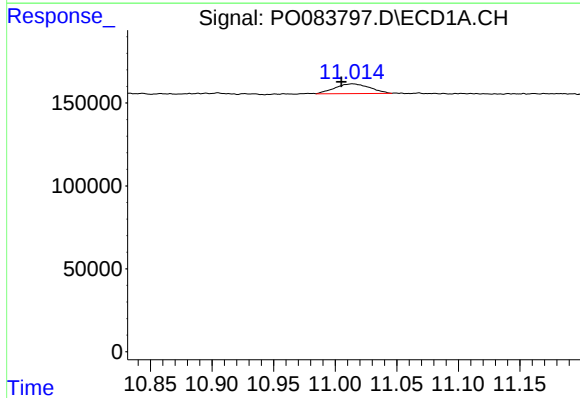

#2 Decachlorobiphenyl

R.T.: 11.014 min
Delta R.T.: 0.009 min
Response: 115509
Conc: 1.69 ng/ml

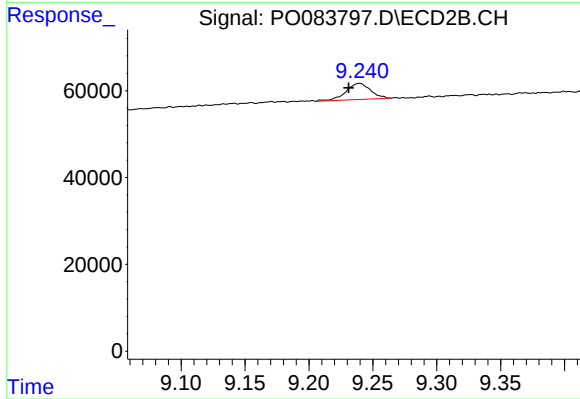

#2 Decachlorobiphenyl

R.T.: 9.240 min
Delta R.T.: 0.009 min
Response: 50268
Conc: 1.79 ng/ml