

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0121621\
 Data File : P0083799.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 17 Dec 2021 5:13
 Operator : AJ\MA
 Sample : M5070-27 10X
 Misc :
 ALS Vial : 51 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 CLI-2021-22-A

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 17 06:06:54 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0121521.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Dec 16 04:05:27 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.935	3.941	144052	47490	1.512	1.619
2) SA Decachlor...	11.010	9.239	147372	36685	2.152	1.306 #

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO121621\
Data File : PO083799.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 17 Dec 2021 5:13
Operator : AJ\MA
Sample : M5070-27 10X
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
CLI-2021-22-A

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 17 06:06:54 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO121521.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Dec 16 04:05:27 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

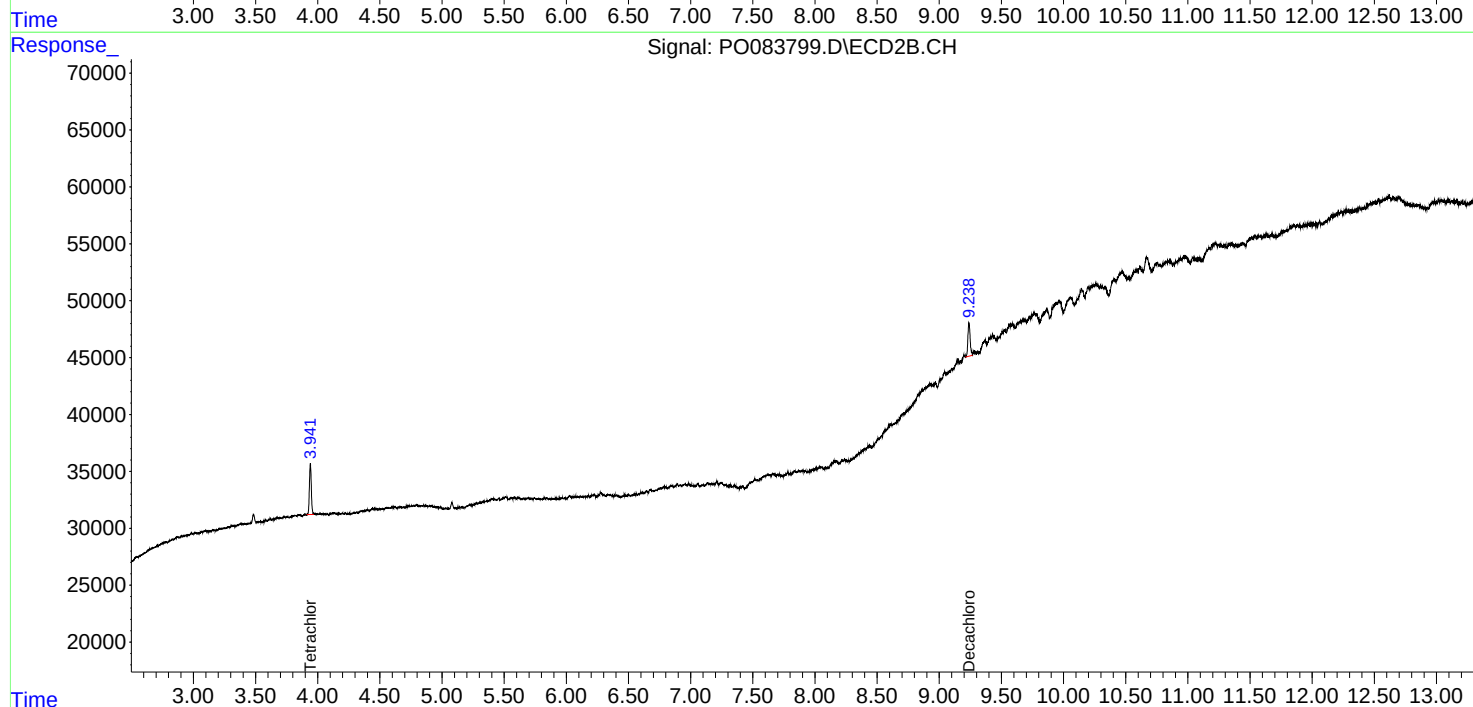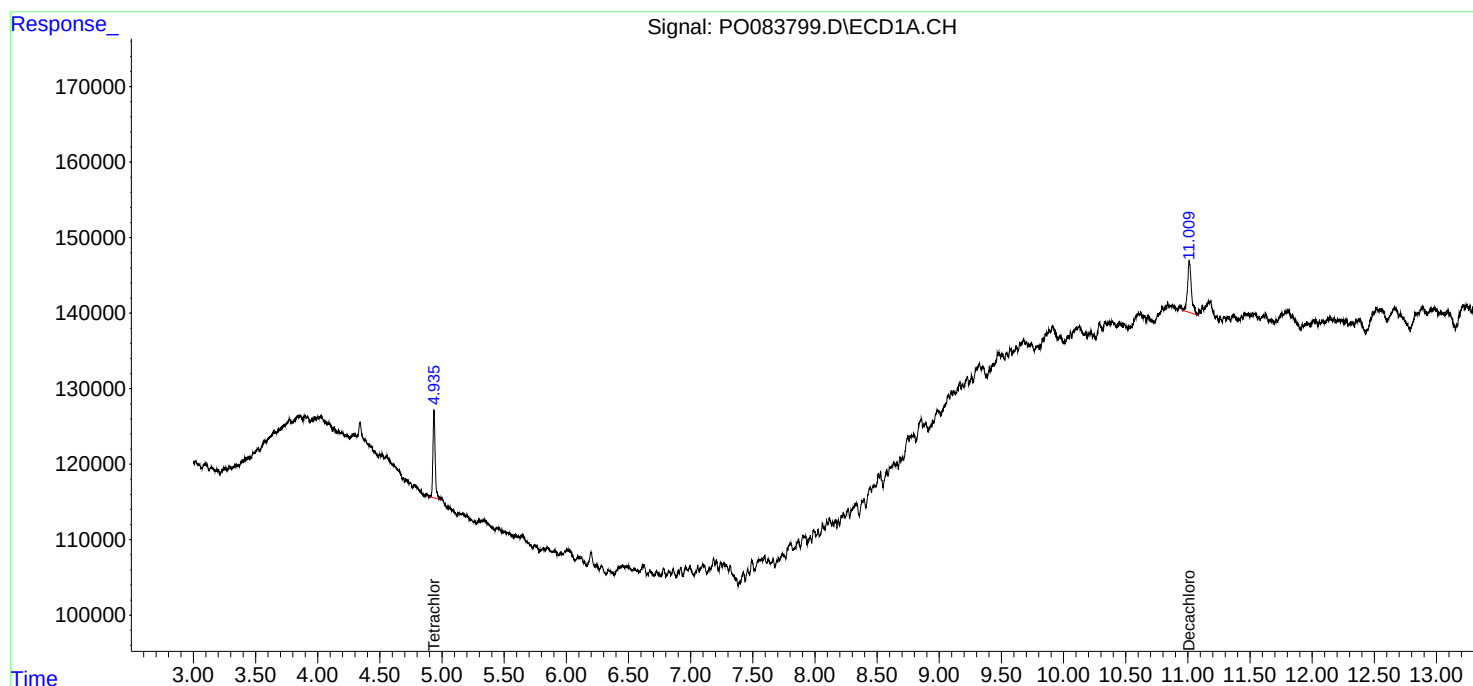


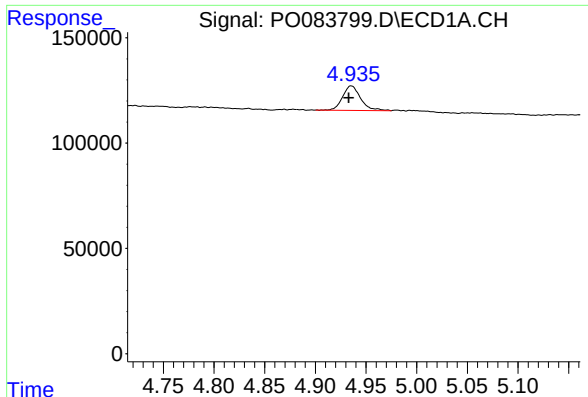

#1 Tetrachloro-m-xylene


R.T.: 4.935 min
Delta R.T.: 0.002 min
Response: 144052
Conc: 1.51 ng/ml

Instrument :
ECD_O
ClientSampleId :
CLI-2021-22-A

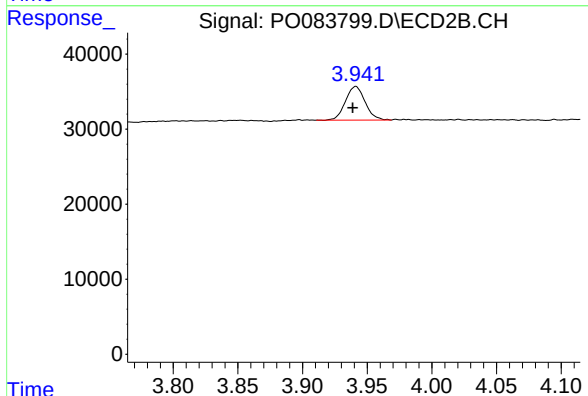


#1 Tetrachloro-m-xylene

R.T.: 3.941 min
Delta R.T.: 0.003 min
Response: 47490
Conc: 1.62 ng/ml

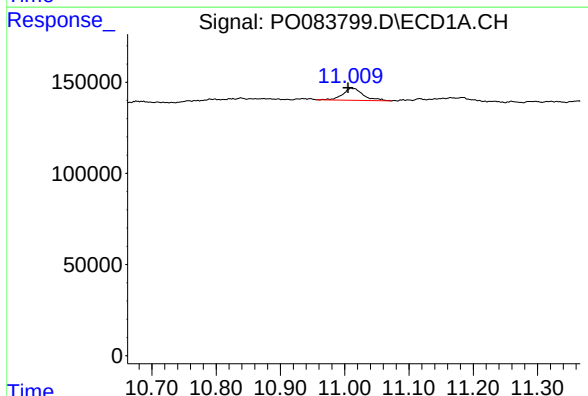

#2 Decachlorobiphenyl

R.T.: 11.010 min
Delta R.T.: 0.005 min
Response: 147372
Conc: 2.15 ng/ml

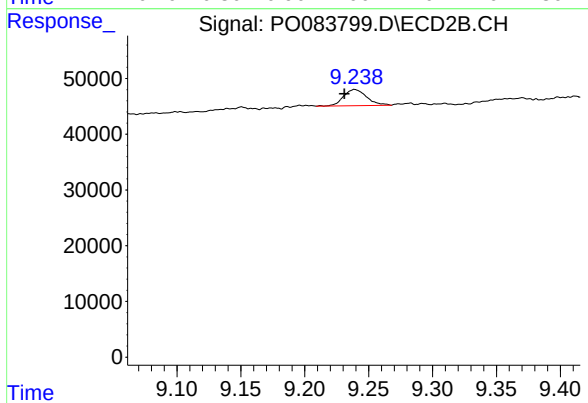

#2 Decachlorobiphenyl

R.T.: 9.239 min
Delta R.T.: 0.008 min
Response: 36685
Conc: 1.31 ng/ml