

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO121622\
 Data File : PO091433.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 Dec 2022 10:36
 Operator : YP/AJ
 Sample : N6067-03
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 WC-LIQUID-20221214

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 16 20:38:06 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO112522.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Nov 28 11:25:59 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.296	3.474	31109283	14177011	9.201	13.508 #
2) SA Decachlor...	10.049	8.477	14510435	6215666	5.463	6.402

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO121622\
Data File : P0091433.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 Dec 2022 10:36
Operator : YP/AJ
Sample : N6067-03
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
WC-LIQUID-20221214

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 16 20:38:06 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO112522.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Nov 28 11:25:59 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

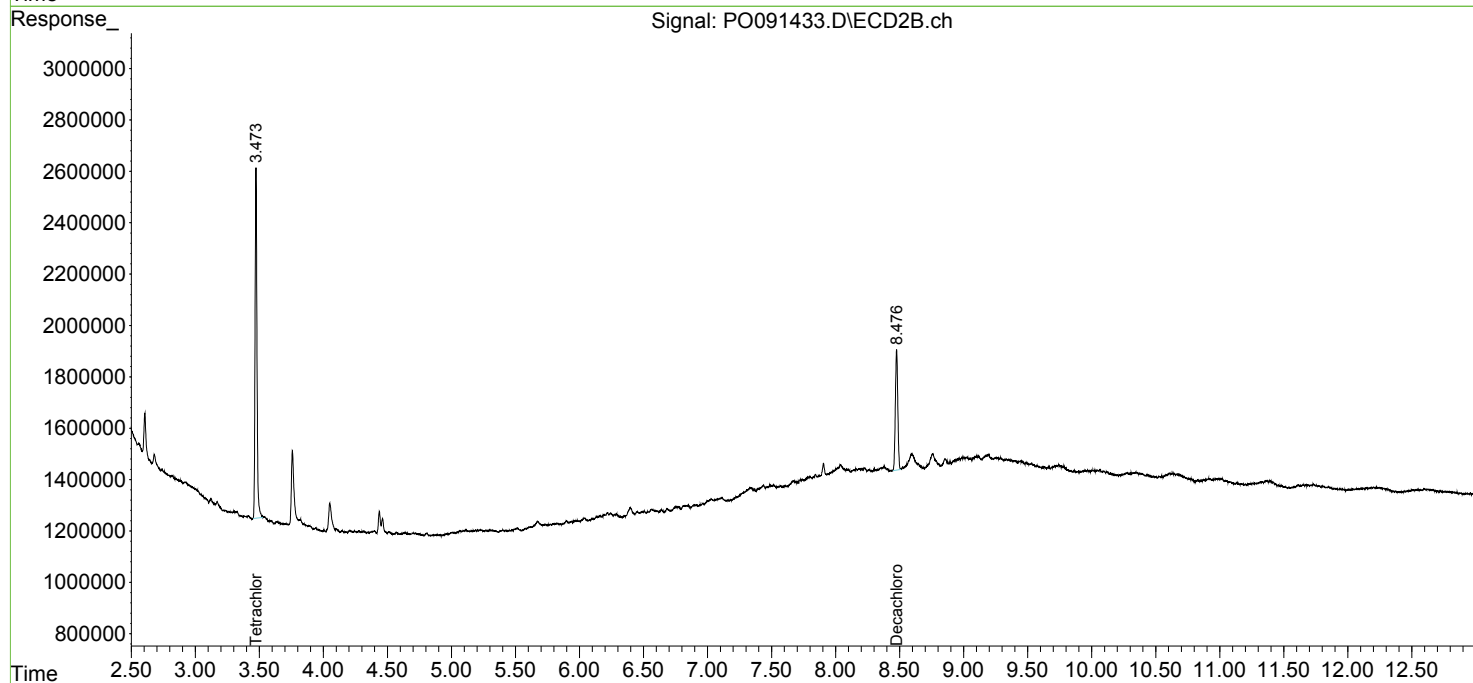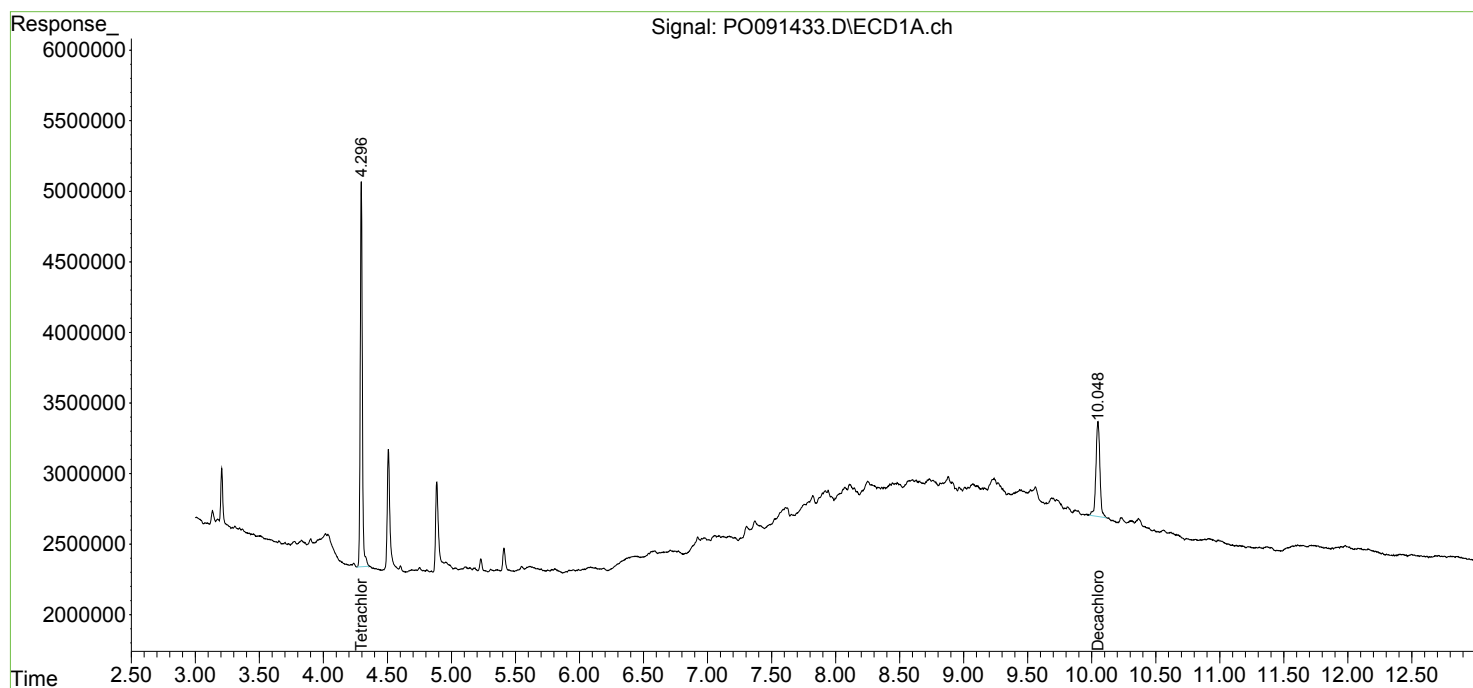


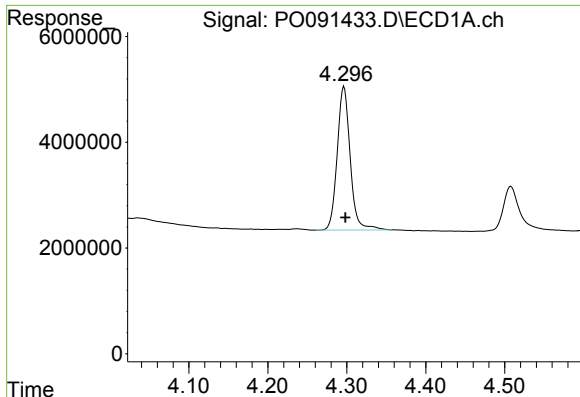

#1 Tetrachloro-m-xylene


R.T.: 4.296 min
Delta R.T.: -0.002 min
Response: 31109283
Conc: 9.20 ng/ml

Instrument :
ECD_O
ClientSampleId :
WC-LIQUID-20221214

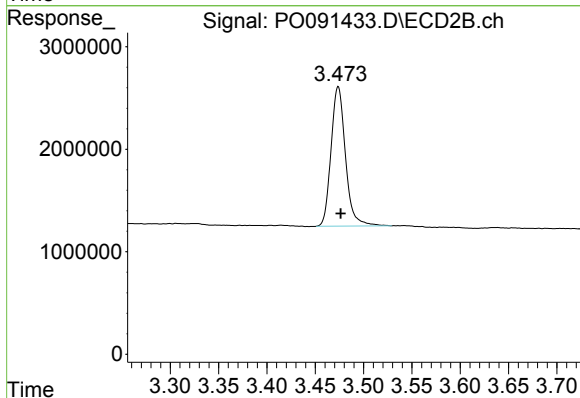


#1 Tetrachloro-m-xylene

R.T.: 3.474 min
Delta R.T.: -0.002 min
Response: 14177011
Conc: 13.51 ng/ml

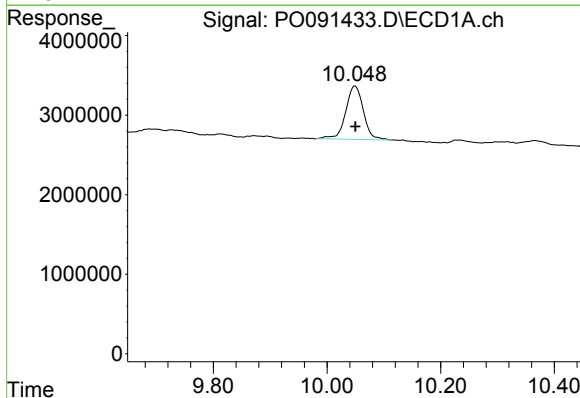

#2 Decachlorobiphenyl

R.T.: 10.049 min
Delta R.T.: 0.000 min
Response: 14510435
Conc: 5.46 ng/ml

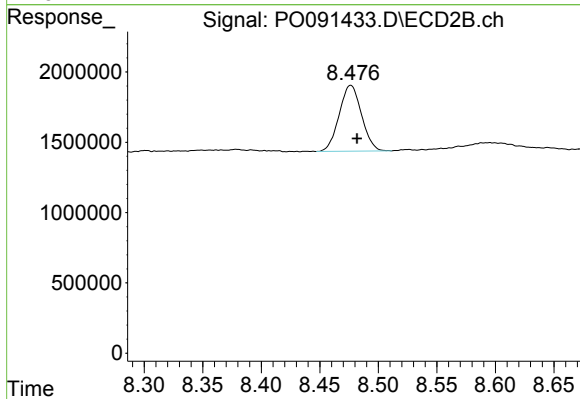

#2 Decachlorobiphenyl

R.T.: 8.477 min
Delta R.T.: -0.005 min
Response: 6215666
Conc: 6.40 ng/ml