

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO121622\
 Data File : PO091446.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 Dec 2022 15:17
 Operator : YP/AJ
 Sample : N6071-11
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 FVSUB-TP8-COMP-08

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 16 20:50:10 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO112522.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Nov 28 11:25:59 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.297	3.474	61610099	23875544	18.222	22.748
2) SA Decachlor...	10.049	8.476	32187633	13170815	12.118	13.566

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO121622\
Data File : P0091446.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 Dec 2022 15:17
Operator : YP/AJ
Sample : N6071-11
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
FVSUB-TP8-COMP-08

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 16 20:50:10 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO112522.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Nov 28 11:25:59 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

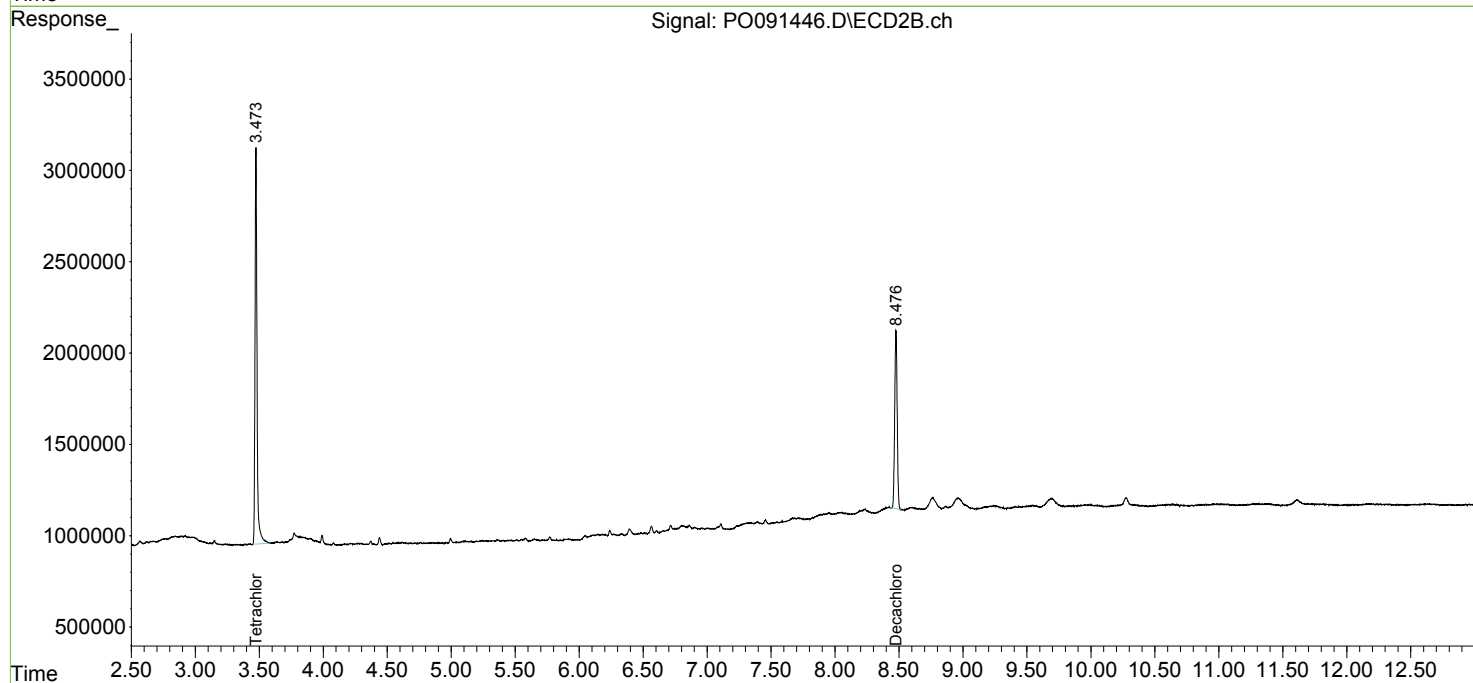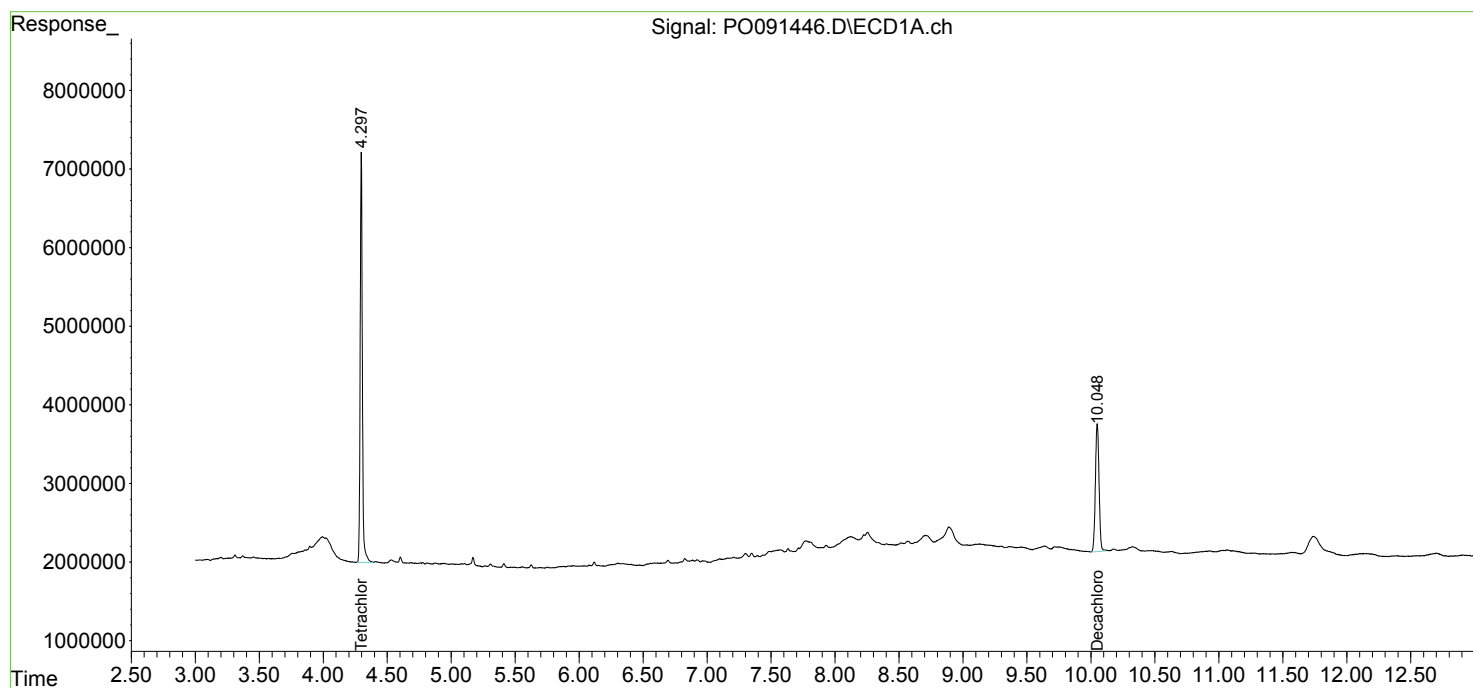


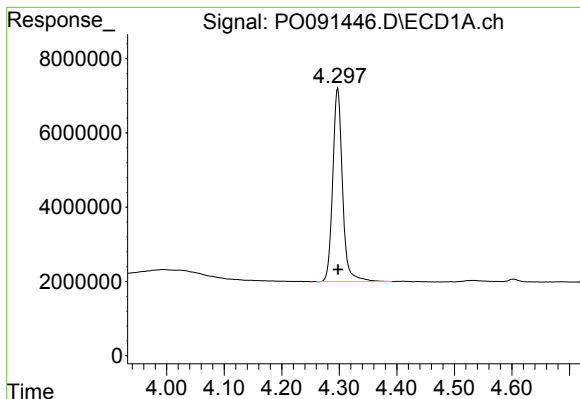

#1 Tetrachloro-m-xylene


R.T.: 4.297 min
Delta R.T.: 0.000 min
Response: 61610099
Conc: 18.22 ng/ml

Instrument :
ECD_O
ClientSampleId :
FVSUB-TP8-COMP-08

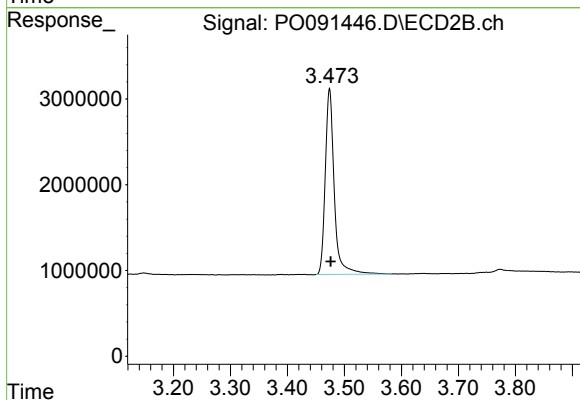


#1 Tetrachloro-m-xylene

R.T.: 3.474 min
Delta R.T.: -0.002 min
Response: 23875544
Conc: 22.75 ng/ml

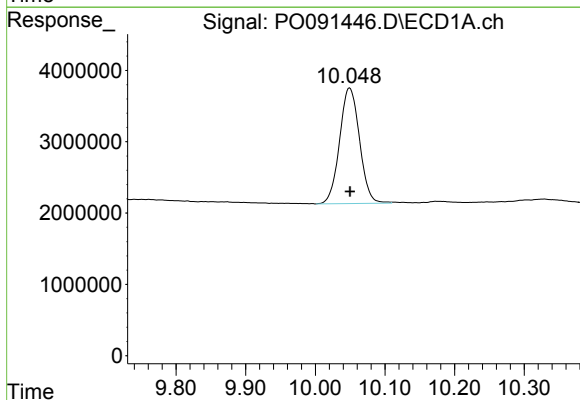

#2 Decachlorobiphenyl

R.T.: 10.049 min
Delta R.T.: 0.000 min
Response: 32187633
Conc: 12.12 ng/ml

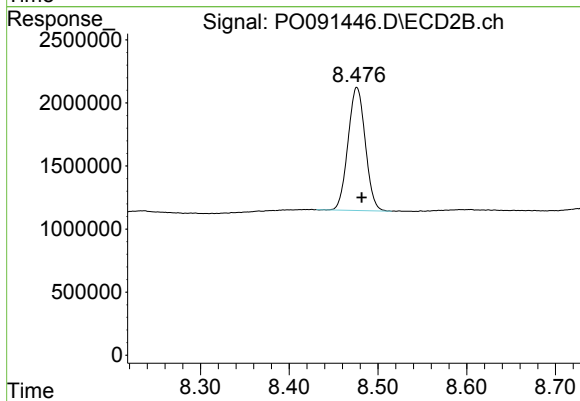

#2 Decachlorobiphenyl

R.T.: 8.476 min
Delta R.T.: -0.006 min
Response: 13170815
Conc: 13.57 ng/ml