

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0121624\
 Data File : P0108567.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 Dec 2024 20:07
 Operator : YP/AJ
 Sample : P5287-05
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 220-2-TRANS-WATER

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 17 00:31:19 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0120624.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Dec 07 05:58:15 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.708	3.705	124.1E6	79563691	14.263	15.695
2) SA Decachlor...	8.776	8.725	96196611	61137005	13.170	15.778

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO121624\
Data File : PO108567.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 Dec 2024 20:07
Operator : YP/AJ
Sample : P5287-05
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
220-2-TRANS-WATER

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 17 00:31:19 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO120624.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Dec 07 05:58:15 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

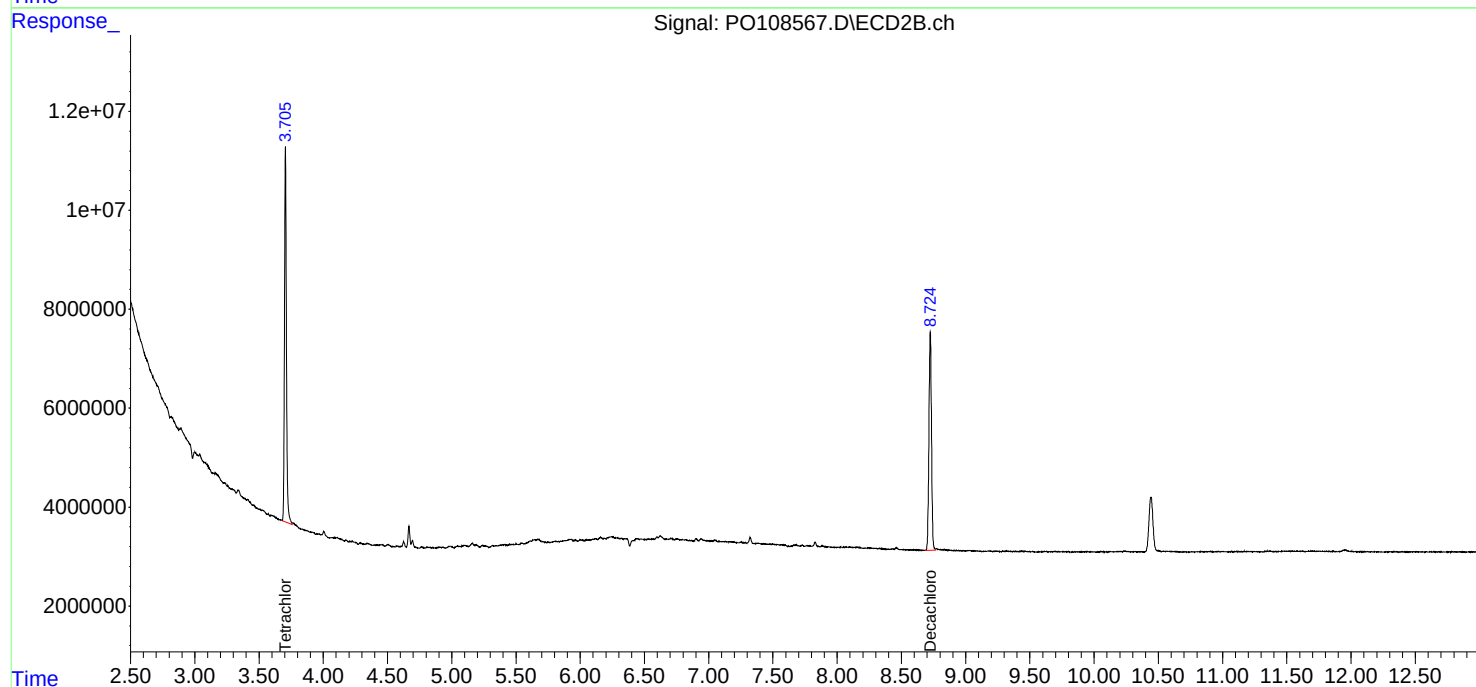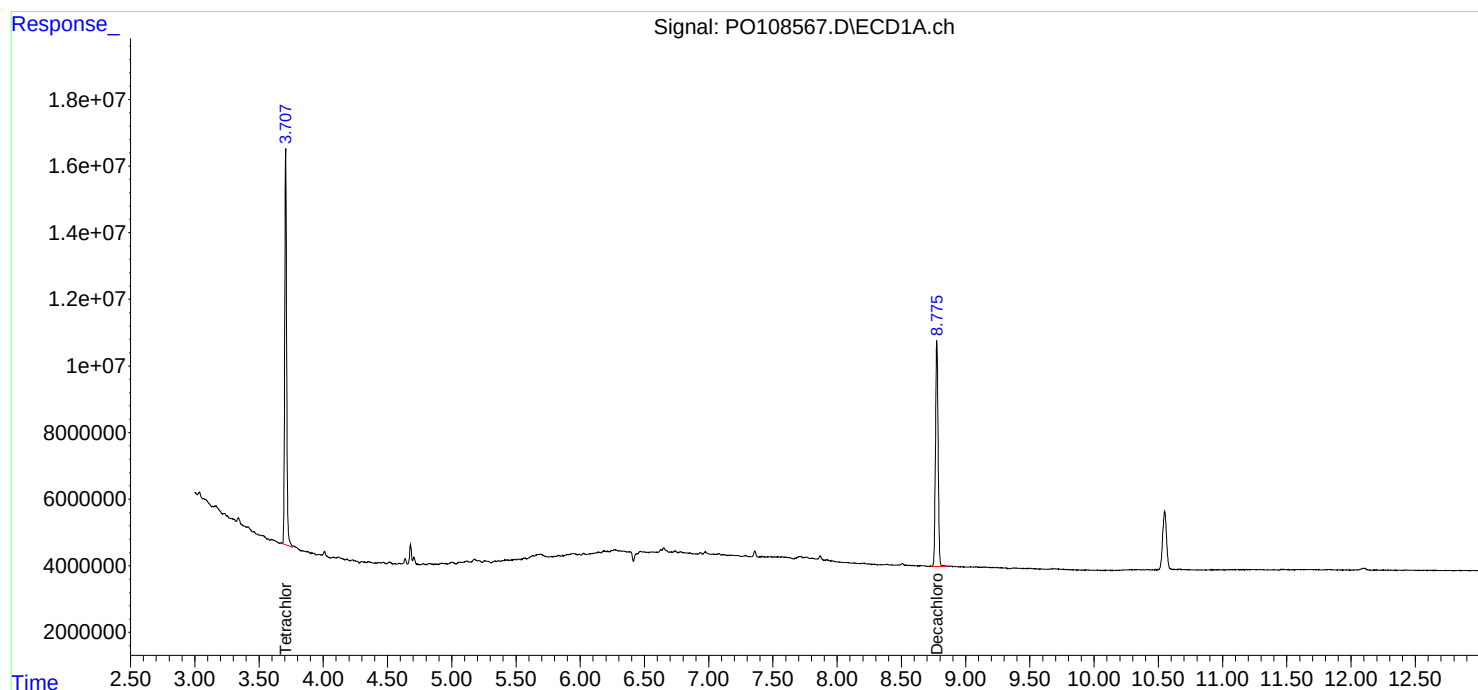


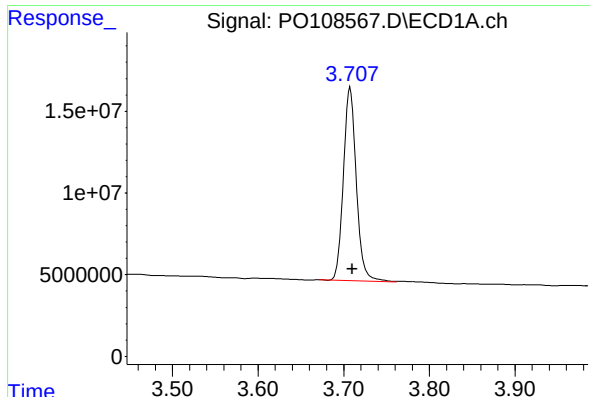

#1 Tetrachloro-m-xylene


R.T.: 3.708 min
Delta R.T.: -0.002 min
Response: 124091329
Conc: 14.26 ng/ml

Instrument :
ECD_O
ClientSampleId :
220-2-TRANS-WATER

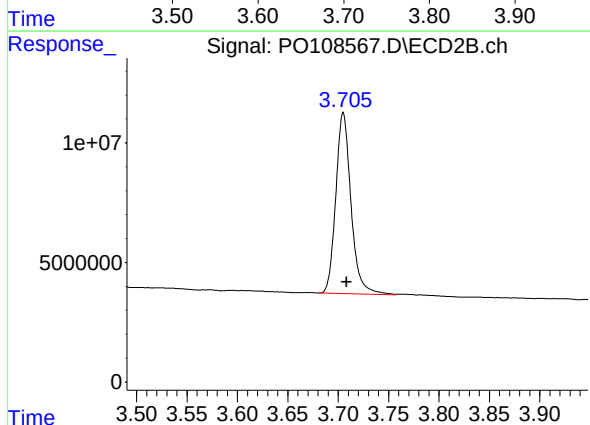


#1 Tetrachloro-m-xylene

R.T.: 3.705 min
Delta R.T.: -0.003 min
Response: 79563691
Conc: 15.69 ng/ml

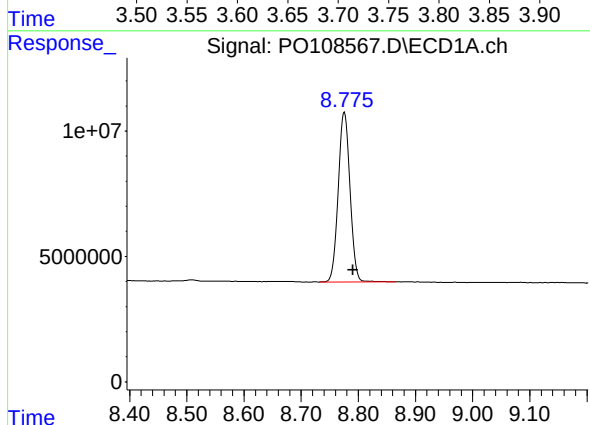

#2 Decachlorobiphenyl

R.T.: 8.776 min
Delta R.T.: -0.015 min
Response: 96196611
Conc: 13.17 ng/ml

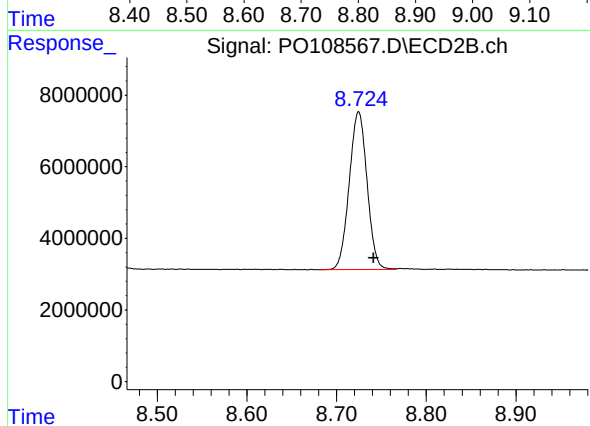

#2 Decachlorobiphenyl

R.T.: 8.725 min
Delta R.T.: -0.017 min
Response: 61137005
Conc: 15.78 ng/ml