

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0121820\
 Data File : P0073941.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 18 Dec 2020 14:57
 Operator : DD\AJ
 Sample : L5140-01
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 18 15:13:08 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0121020.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Dec 11 03:58:06 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.938	3.998	1919626	1117450	20.996	20.834
2)	SA Decachlor...	10.960	9.260	1510452	873542	18.278	18.669
Target Compounds							
8)	L2 AR-1221-1	5.197	0.000	114279	0	107.858	N.D. #
9)	L2 AR-1221-2	5.292	0.000	23021	0	29.307	N.D. #
27)	L6 AR-1254-2	7.416	0.000	167359	0	28.386	N.D. #
28)	L6 AR-1254-3	7.805	0.000	27933	0	4.559	N.D. #
30)	L6 AR-1254-5	8.517	0.000	13324	0	2.587	N.D. #
33)	L7 AR-1260-3	8.587	0.000	7610	0	1.665	N.D. #
34)	L7 AR-1260-4	8.845f	0.000	1401	0	0.296	N.D. #
36)	L8 AR-1262-1	8.587	0.000	7610	0	1.016	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO121820\
Data File : PO073941.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 18 Dec 2020 14:57
Operator : DD\AJ
Sample : L5140-01
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 18 15:13:08 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO121020.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Dec 11 03:58:06 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

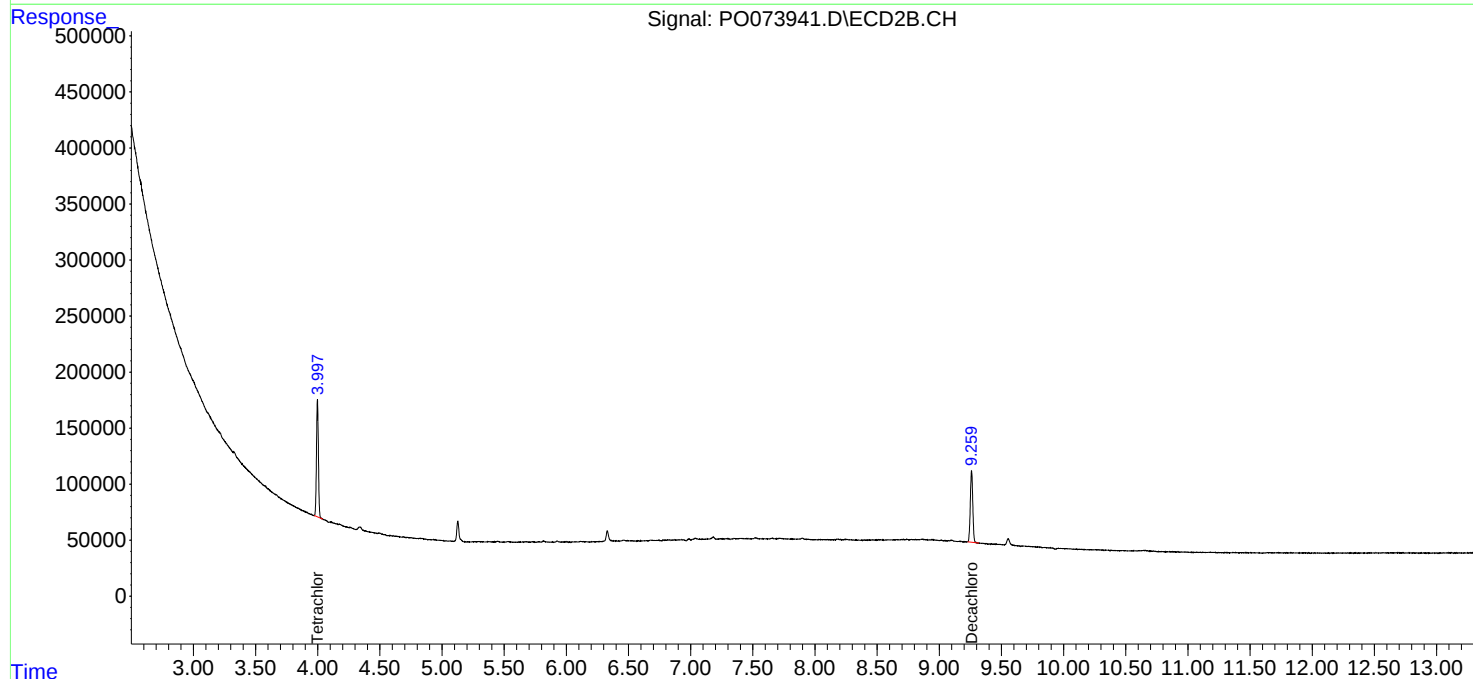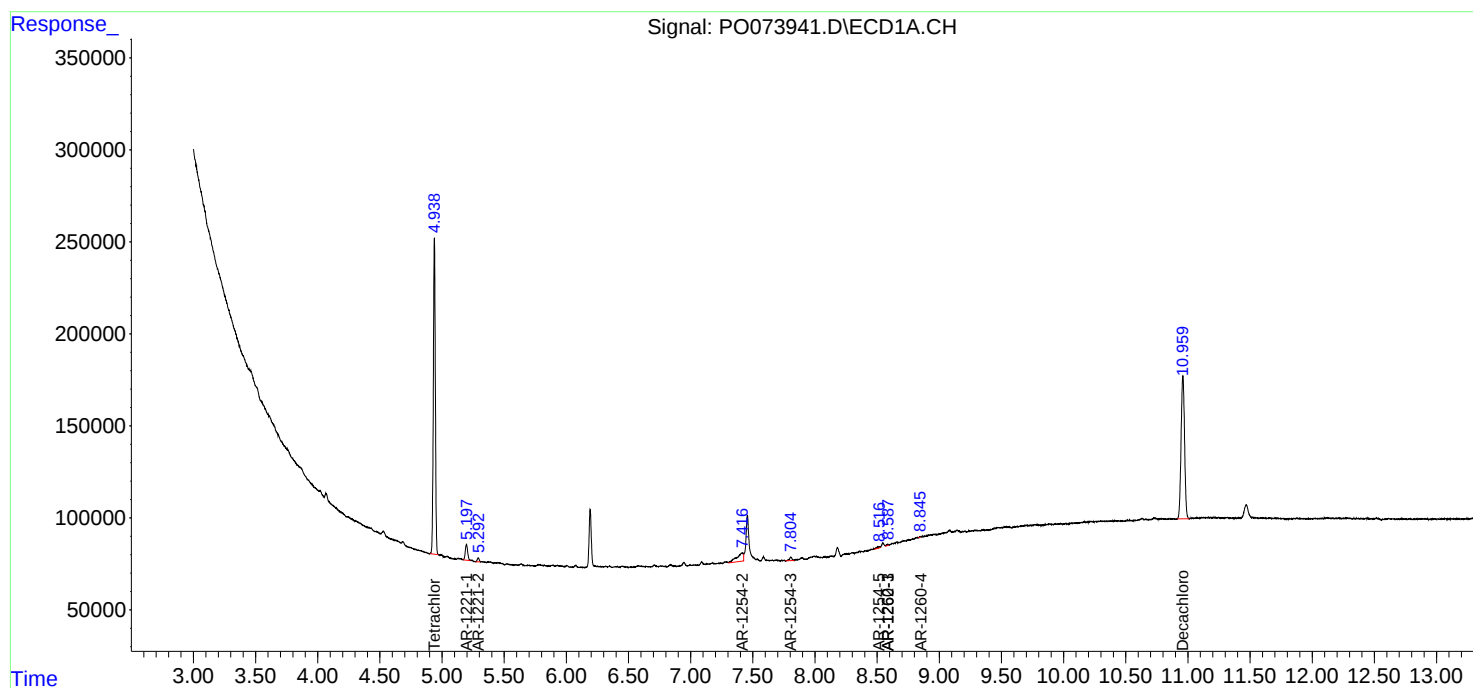


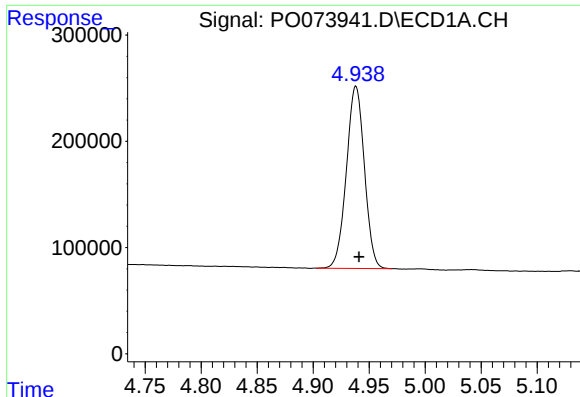

#1 Tetrachloro-m-xylene


R.T.: 4.938 min
Delta R.T.: -0.003 min
Response: 1919626
Conc: 21.00 ng/ml

Instrument :
ECD_O
ClientSampleId :

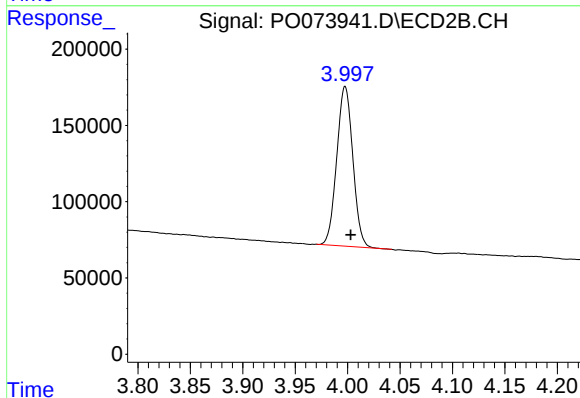


#1 Tetrachloro-m-xylene

R.T.: 3.998 min
Delta R.T.: -0.005 min
Response: 1117450
Conc: 20.83 ng/ml

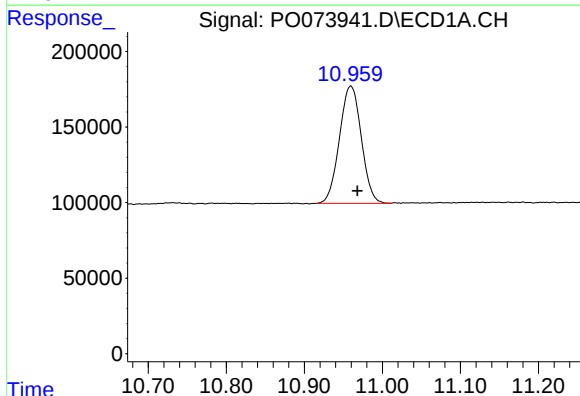


#2 Decachlorobiphenyl

R.T.: 10.960 min
Delta R.T.: -0.009 min
Response: 1510452
Conc: 18.28 ng/ml

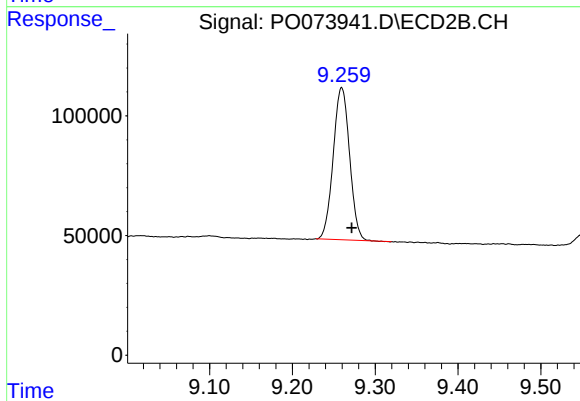

#2 Decachlorobiphenyl


R.T.: 9.260 min
Delta R.T.: -0.012 min
Response: 873542
Conc: 18.67 ng/ml

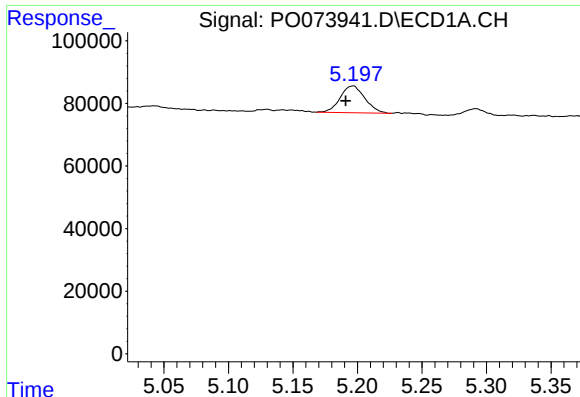

#8 AR-1221-1


R.T.: 5.197 min
Delta R.T.: 0.006 min
Response: 114279
Conc: 107.86 ng/ml

Instrument :
ECD_O
ClientSampleId :

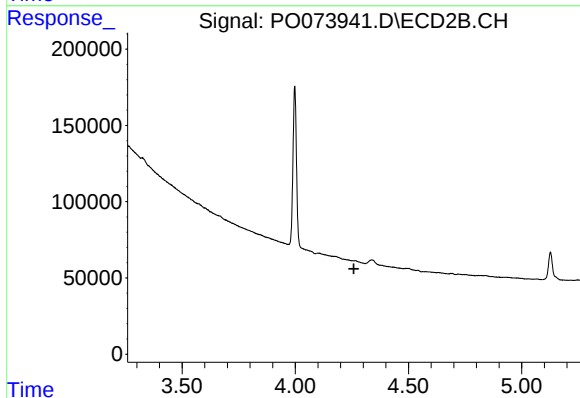


#8 AR-1221-1

R.T.: 0.000 min
Exp R.T. : 4.259 min
Response: 0
Conc: N.D.

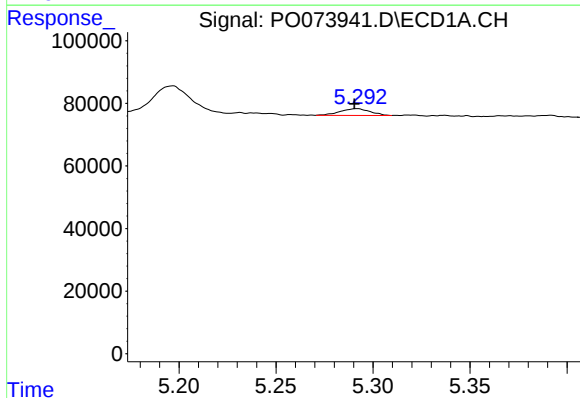


#9 AR-1221-2

R.T.: 5.292 min
Delta R.T.: 0.002 min
Response: 23021
Conc: 29.31 ng/ml

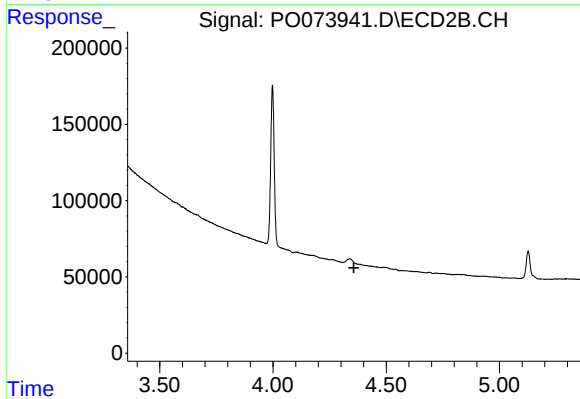

#9 AR-1221-2


R.T.: 0.000 min
Exp R.T. : 4.357 min
Response: 0
Conc: N.D.

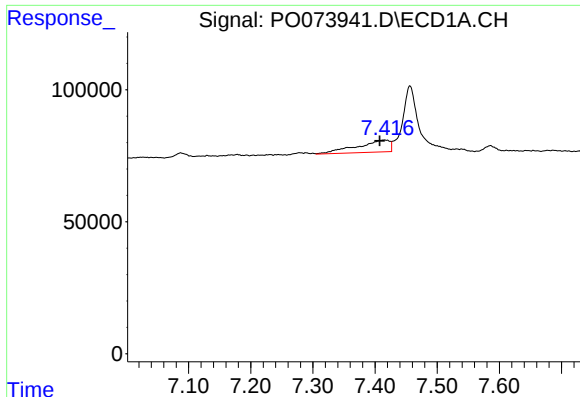

#27 AR-1254-2


R.T.: 7.416 min
Delta R.T.: 0.008 min
Response: 167359
Conc: 28.39 ng/ml

Instrument :
ECD_O
ClientSampleId :

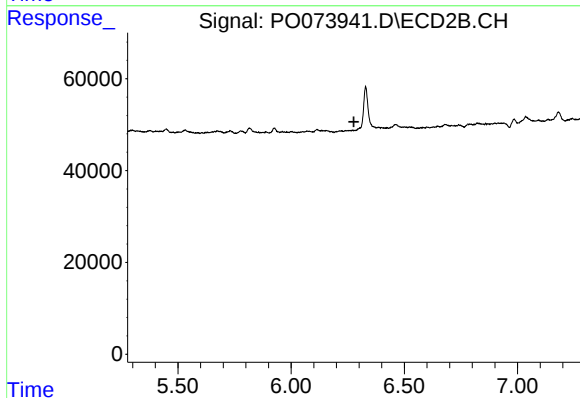


#27 AR-1254-2

R.T.: 0.000 min
Exp R.T. : 6.277 min
Response: 0
Conc: N.D.

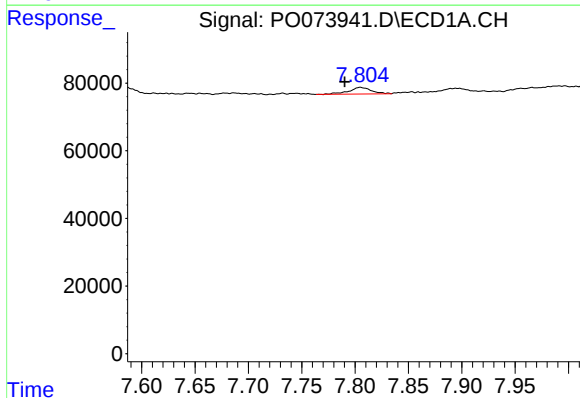


#28 AR-1254-3

R.T.: 7.805 min
Delta R.T.: 0.015 min
Response: 27933
Conc: 4.56 ng/ml

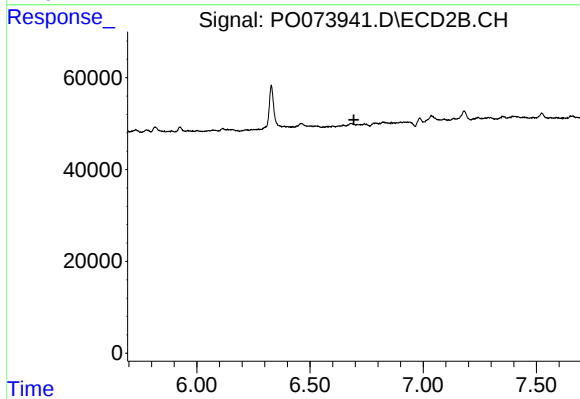

#28 AR-1254-3


R.T.: 0.000 min
Exp R.T. : 6.694 min
Response: 0
Conc: N.D.

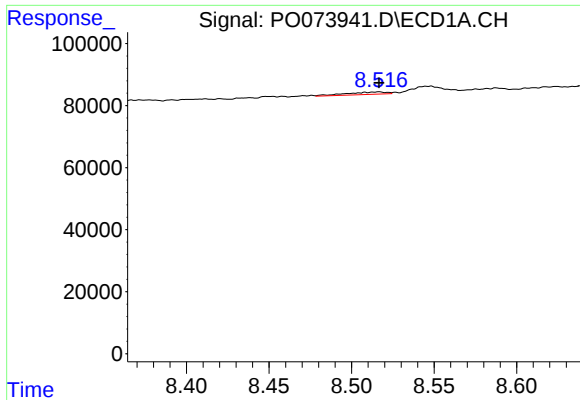

#30 AR-1254-5


R.T.: 8.517 min
Delta R.T.: 0.000 min
Response: 13324
Conc: 2.59 ng/ml

Instrument :
ECD_O
ClientSampleId :

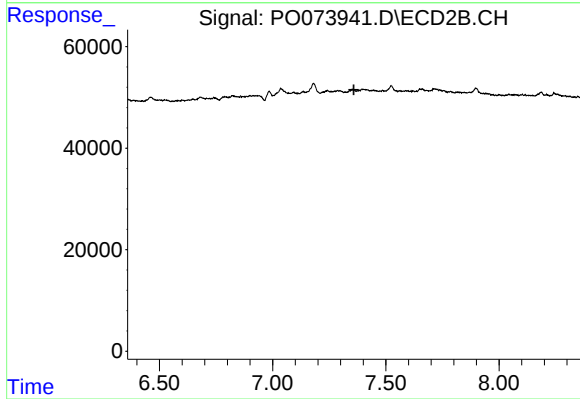


#30 AR-1254-5

R.T.: 0.000 min
Exp R.T. : 7.359 min
Response: 0
Conc: N.D.

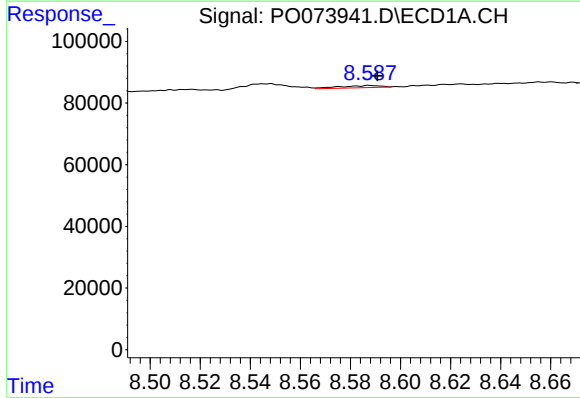


#33 AR-1260-3

R.T.: 8.587 min
Delta R.T.: -0.003 min
Response: 7610
Conc: 1.66 ng/ml

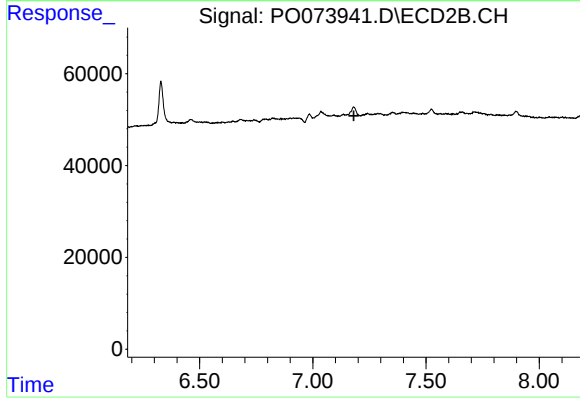

#33 AR-1260-3


R.T.: 0.000 min
Exp R.T. : 7.182 min
Response: 0
Conc: N.D.

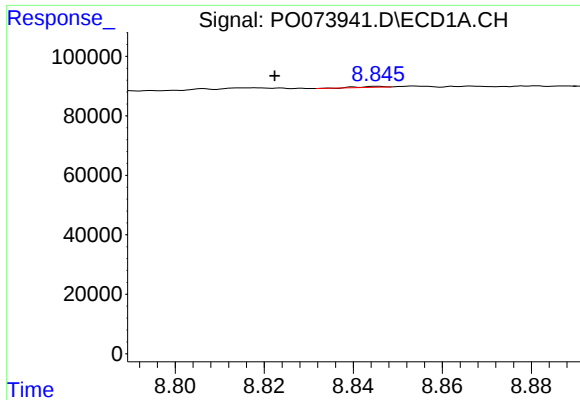

#34 AR-1260-4


R.T.: 8.845 min
Delta R.T.: 0.023 min
Response: 1401
Conc: 0.30 ng/ml

Instrument :
ECD_O
ClientSampleId :

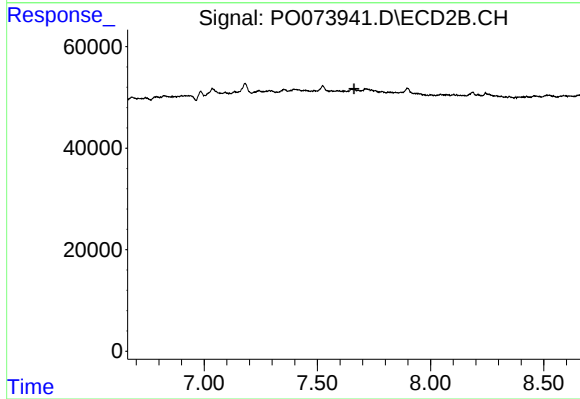


#34 AR-1260-4

R.T.: 0.000 min
Exp R.T. : 7.662 min
Response: 0
Conc: N.D.

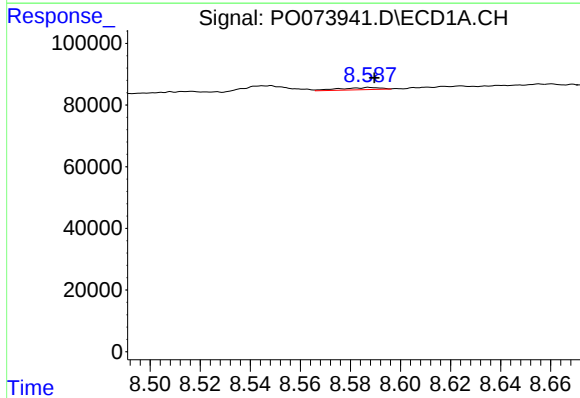

#36 AR-1262-1

R.T.: 8.587 min
Delta R.T.: -0.002 min
Response: 7610
Conc: 1.02 ng/ml

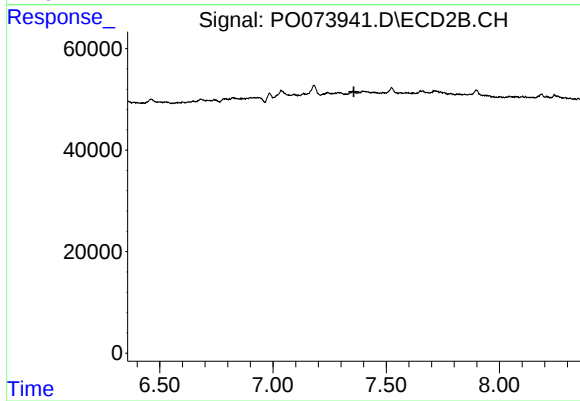

#36 AR-1262-1

R.T.: 0.000 min
Exp R.T. : 7.357 min
Response: 0
Conc: N.D.