

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO121820\
 Data File : PO073937.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 18 Dec 2020 13:48
 Operator : DD\AJ
 Sample : L5140-01
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 GROUNDWATER-SAMPLE-1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 18 14:10:00 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO121020.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Dec 11 03:58:06 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.936	3.996	1945942	1124287	21.284	20.961
2) SA Decachlor...	10.957	9.257f	1491924	862134	18.053	18.425

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO121820\
Data File : PO073937.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 18 Dec 2020 13:48
Operator : DD\AJ
Sample : L5140-01
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
GROUNDWATER-SAMPLE-1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 18 14:10:00 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO121020.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Dec 11 03:58:06 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

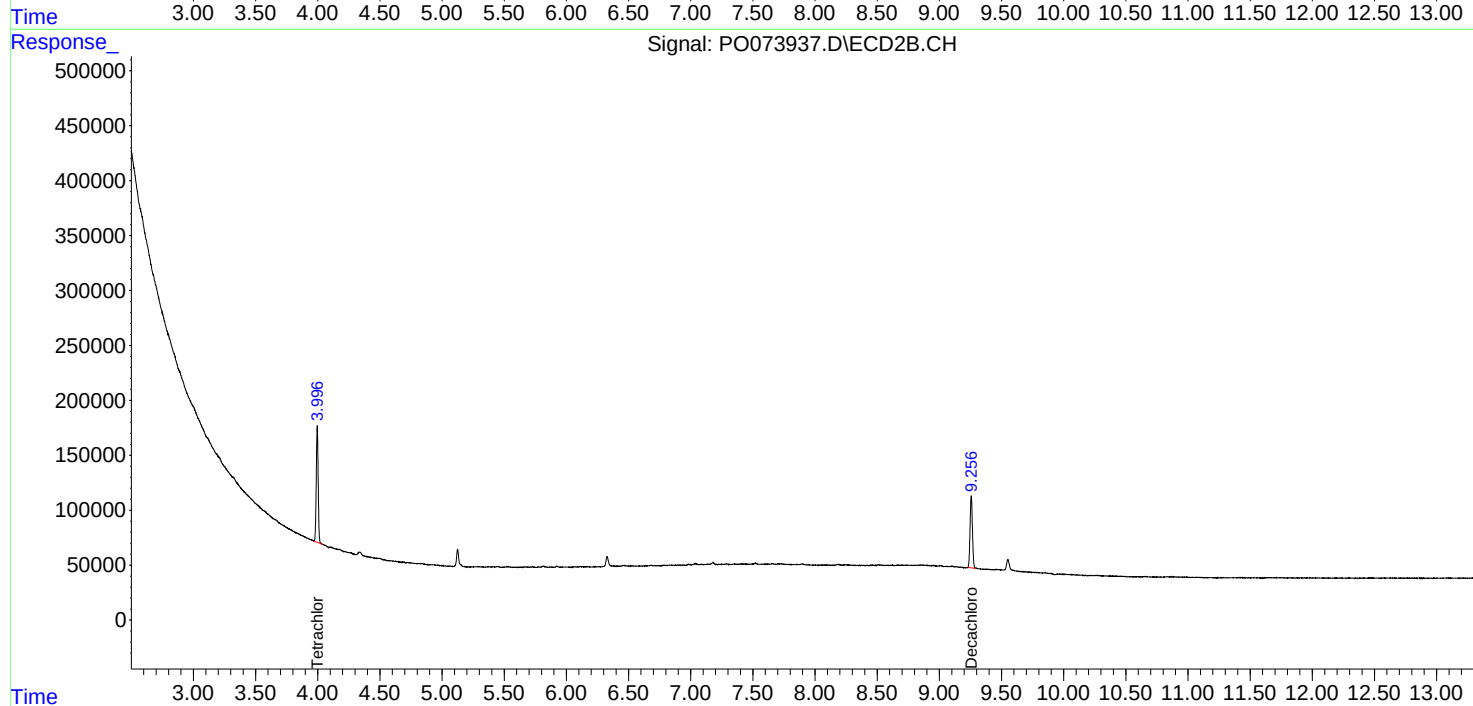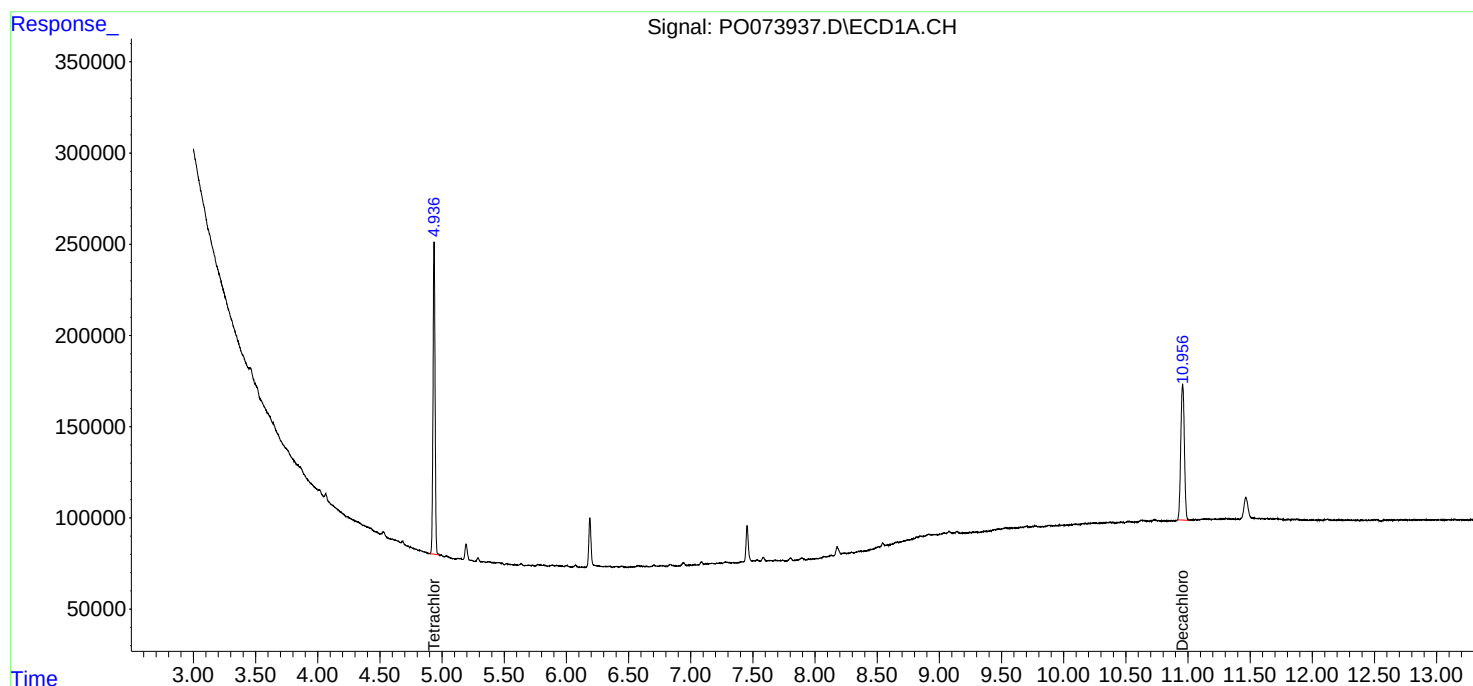


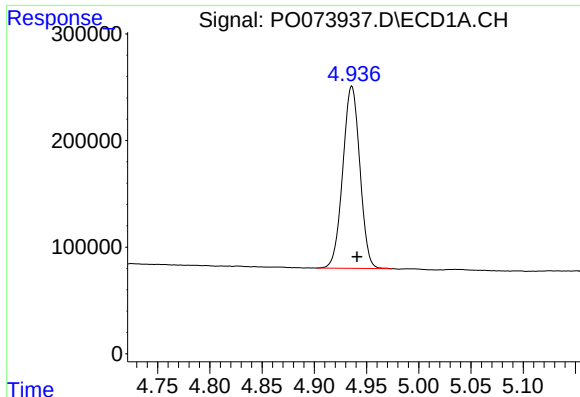

#1 Tetrachloro-m-xylene


R.T.: 4.936 min
Delta R.T.: -0.005 min
Response: 1945942
Conc: 21.28 ng/ml

Instrument :
ECD_O
ClientSampleId :
GROUNDWATER-SAMPLE-1

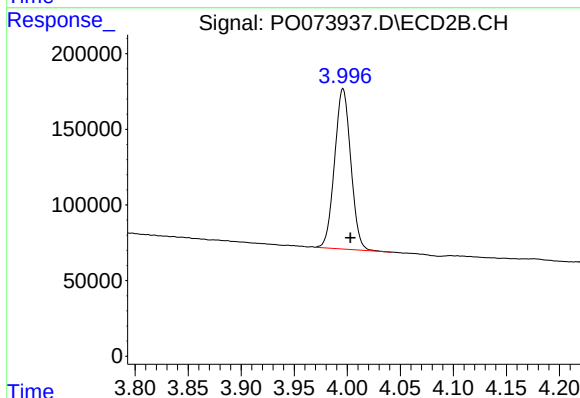


#1 Tetrachloro-m-xylene

R.T.: 3.996 min
Delta R.T.: -0.007 min
Response: 1124287
Conc: 20.96 ng/ml

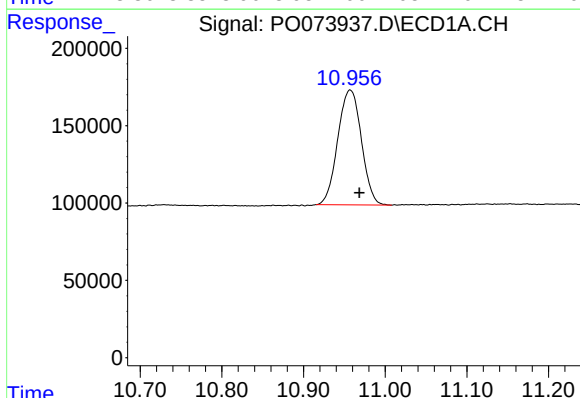

#2 Decachlorobiphenyl

R.T.: 10.957 min
Delta R.T.: -0.011 min
Response: 1491924
Conc: 18.05 ng/ml

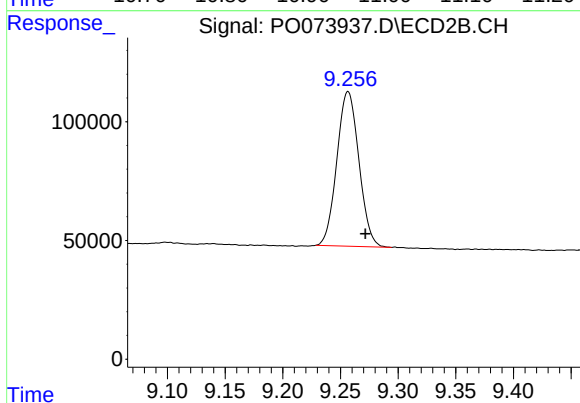

#2 Decachlorobiphenyl

R.T.: 9.257 min
Delta R.T.: -0.015 min
Response: 862134
Conc: 18.43 ng/ml