

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO121820\
 Data File : PO073951.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 18 Dec 2020 18:11
 Operator : DD\AJ
 Sample : L5126-04
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 190-ACADEMY-ST-OILY-WATER

Manual Integrations
 APPROVED

Ankita
 12/21/2020 12:25:56 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 19 00:36:28 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO121020.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Dec 11 03:58:06 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.937	4.000	1132705	695677	12.389m	12.970
2) SA Decachlor...	10.956	9.257	1739594	970773	21.050	20.747

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO121820\
Data File : PO073951.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 18 Dec 2020 18:11
Operator : DD\AJ
Sample : L5126-04
Misc :
ALS Vial : 21 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
190-ACADEMY-ST-OILY-WATER


Manual Integrations
APPROVED

Ankita
12/21/2020 12:25:56 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 19 00:36:28 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO121020.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Dec 11 03:58:06 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

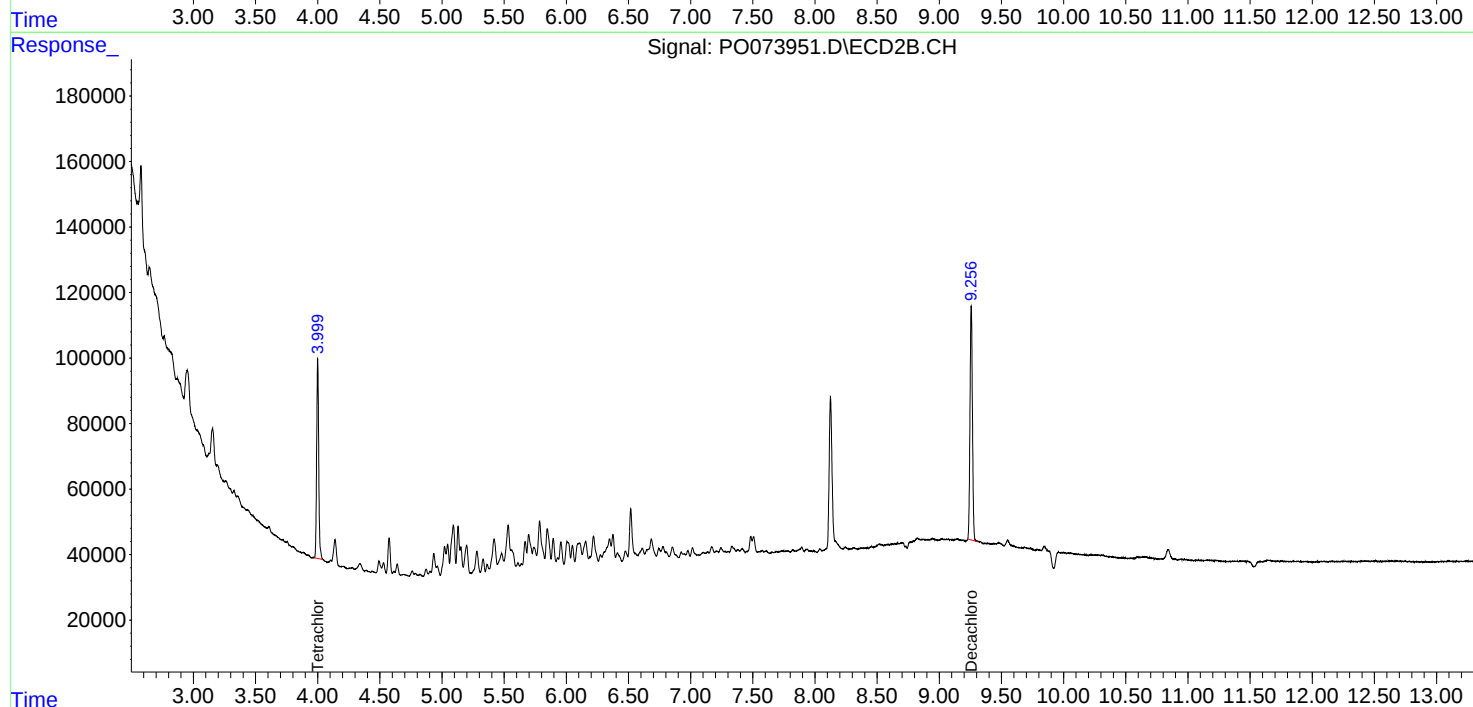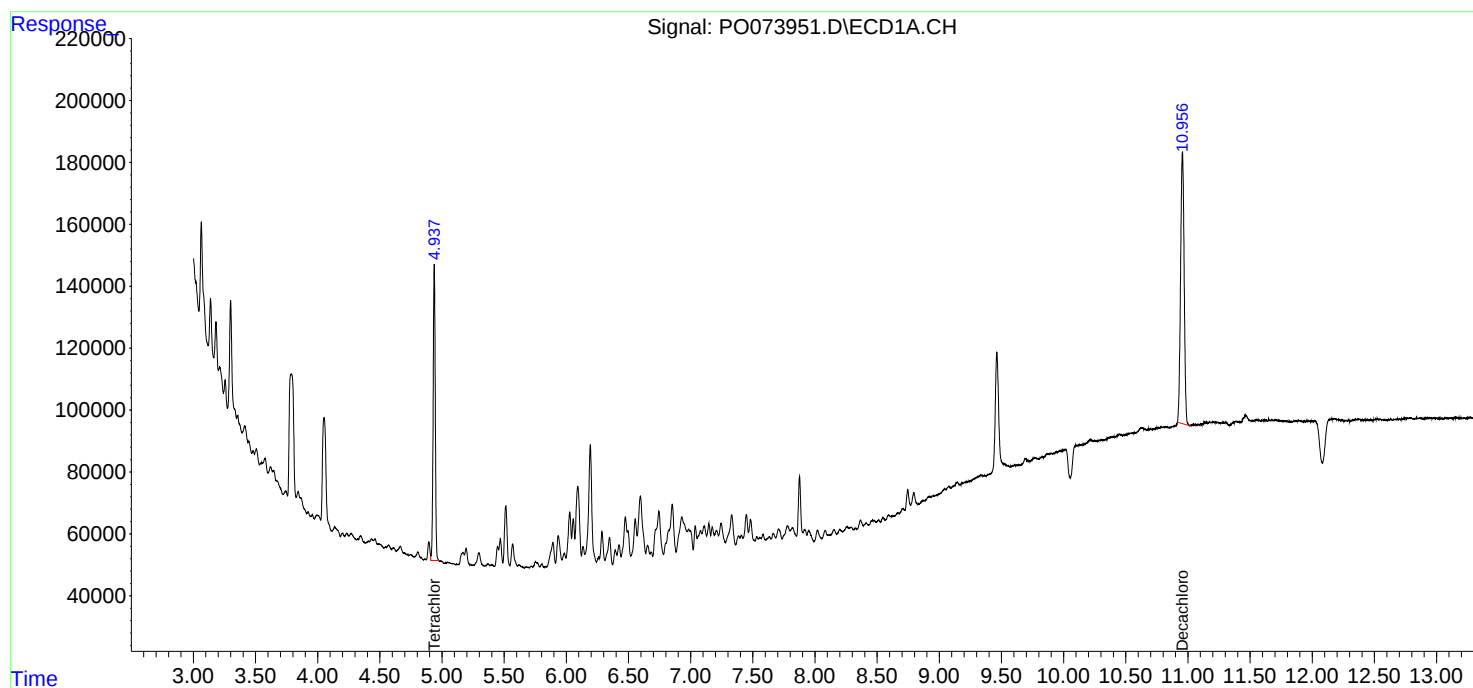

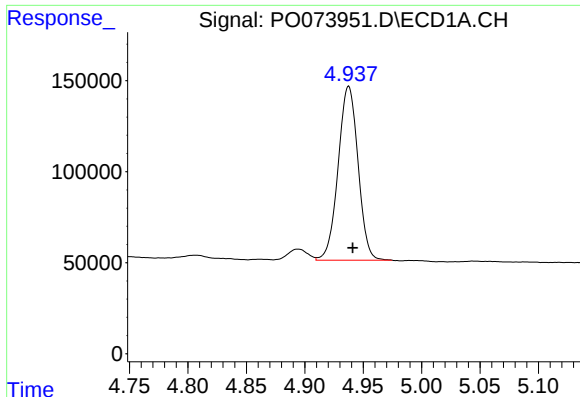


#1 Tetrachloro-m-xylene

R.T.: 4.937 min
Delta R.T.: -0.004 min
Response: 1132705
Conc: 12.39 ng/ml m

Instrument :
ECD_O
ClientSampleId :
190-ACADEMY-ST-OILY-WATER


Manual Integrations
APPROVED

Ankita
12/21/2020 12:25:56 PM

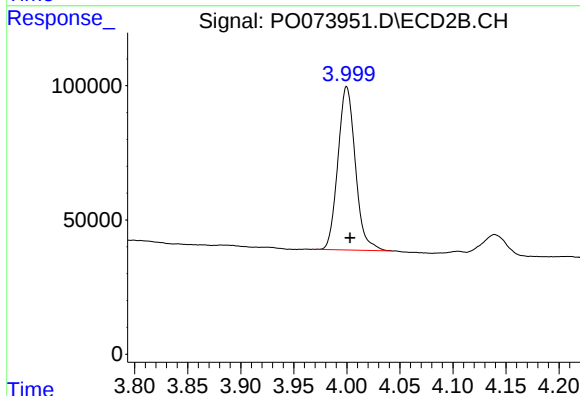


#1 Tetrachloro-m-xylene

R.T.: 4.000 min
Delta R.T.: -0.003 min
Response: 695677
Conc: 12.97 ng/ml

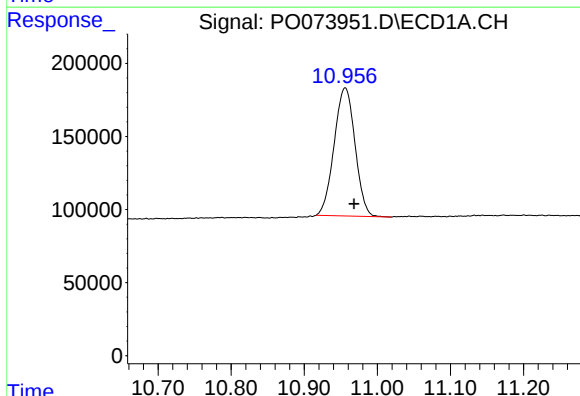

#2 Decachlorobiphenyl

R.T.: 10.956 min
Delta R.T.: -0.012 min
Response: 1739594
Conc: 21.05 ng/ml

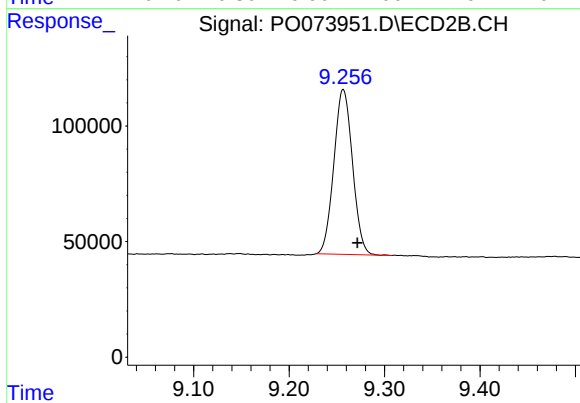

#2 Decachlorobiphenyl

R.T.: 9.257 min
Delta R.T.: -0.015 min
Response: 970773
Conc: 20.75 ng/ml