

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\PO121823\
 Data File : PO100564.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Dec 2023 19:57
 Operator : YP/AJ
 Sample : 05884-07
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 ECD_0
 ClientSampleId :
 WATER-COMP

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 12/19/2023
 Supervised By :Ankita Jodhani 12/19/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 19 03:00:13 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\PO121523.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Dec 16 05:19:37 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.512f	3.732f	33938237	31976093	21.455m	21.058m
2) SA Decachlor...	10.487f	8.868f	23696877	26166661	21.105m	21.012m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO121823\
Data File : PO100564.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Dec 2023 19:57
Operator : YP/AJ
Sample : 05884-07
Misc :
ALS Vial : 26 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
WATER-COMP


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 12/19/2023
Supervised By :Ankita Jodhani 12/19/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 19 03:00:13 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO121523.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Dec 16 05:19:37 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

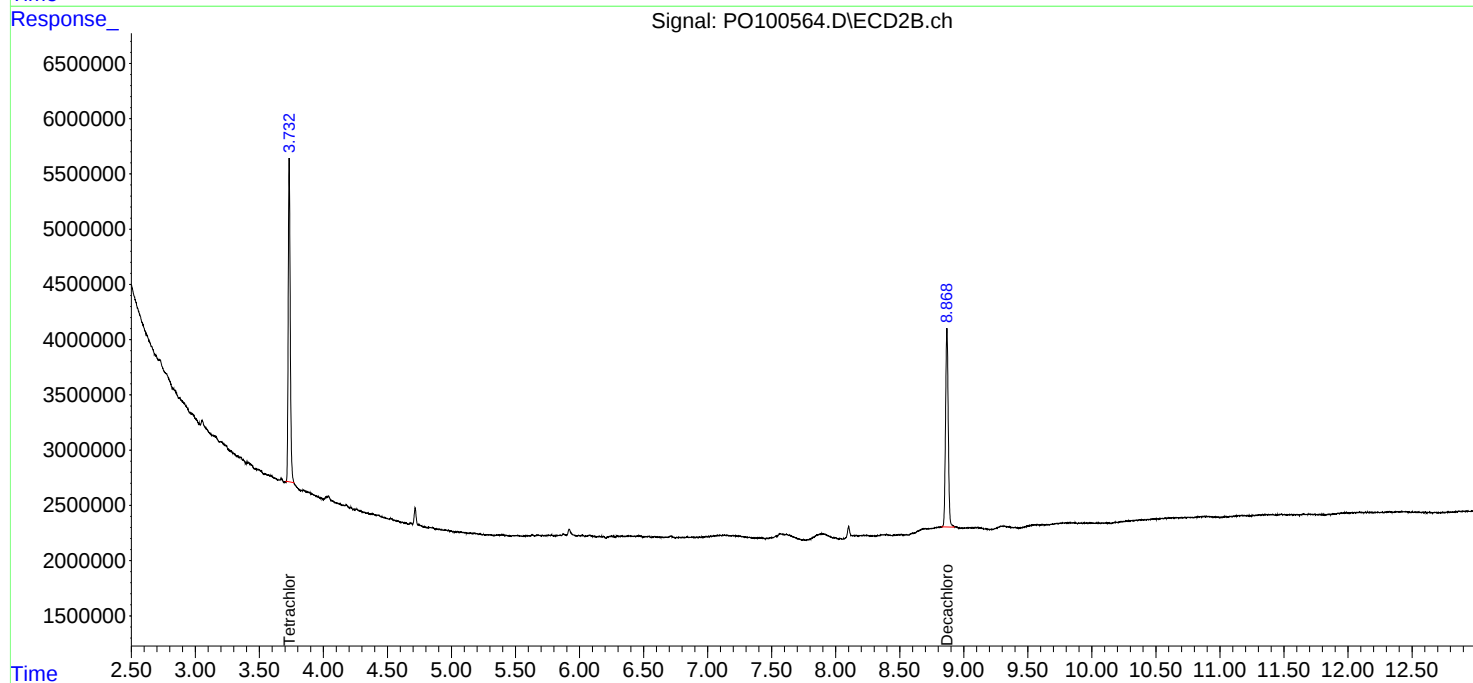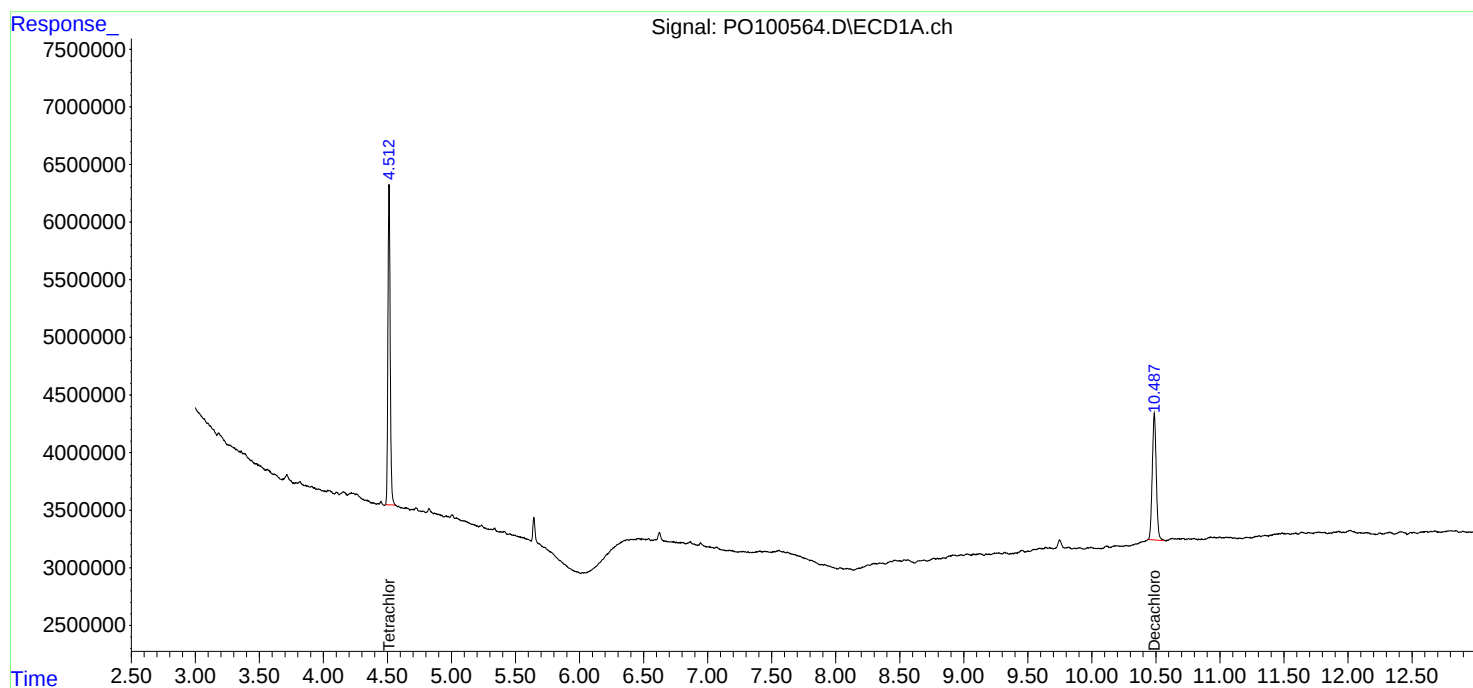

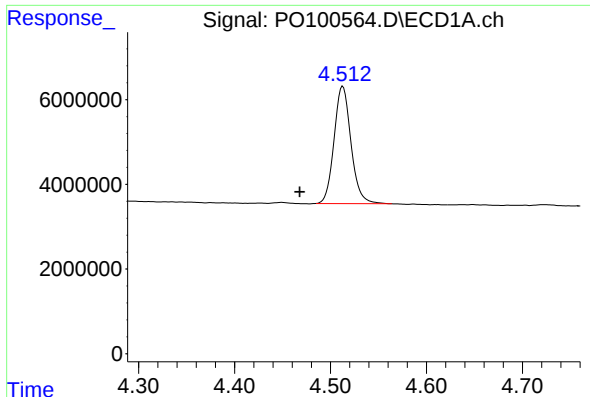


#1 Tetrachloro-m-xylene

R.T.: 4.512 min
Delta R.T.: 0.044 min
Response: 33938237
Conc: 21.45 ng/ml

Instrument :
ECD_O
ClientSampleId :
WATER-COMP


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 12/19/2023
Supervised By :Ankita Jodhani 12/19/2023

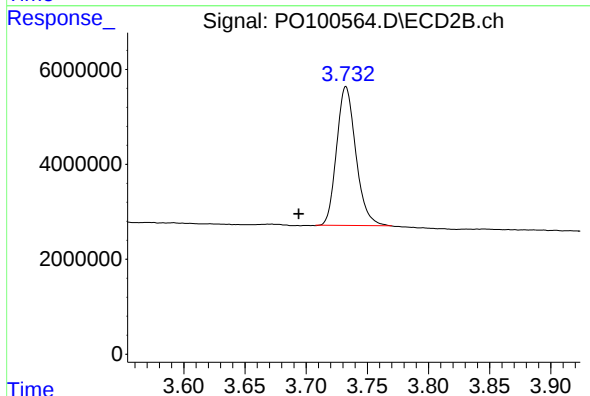


#1 Tetrachloro-m-xylene

R.T.: 3.732 min
Delta R.T.: 0.038 min
Response: 31976093
Conc: 21.06 ng/ml m

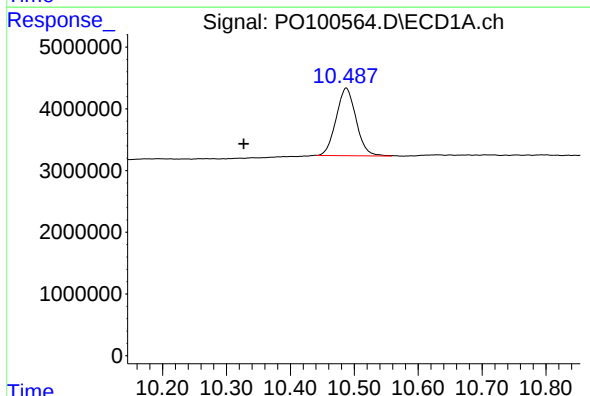

#2 Decachlorobiphenyl

R.T.: 10.487 min
Delta R.T.: 0.160 min
Response: 23696877
Conc: 21.10 ng/ml m

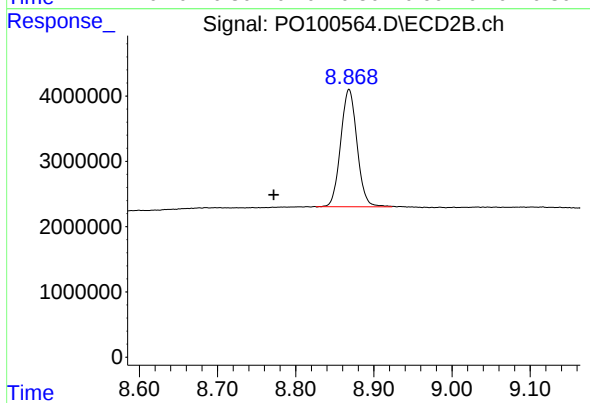

#2 Decachlorobiphenyl

R.T.: 8.868 min
Delta R.T.: 0.096 min
Response: 26166661
Conc: 21.01 ng/ml m