

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO121823\
 Data File : PO100570.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Dec 2023 22:07
 Operator : YP/AJ
 Sample : 05886-01
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 AUD-1295

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 12/19/2023
 Supervised By :Ankita Jodhani 12/19/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 19 03:02:08 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO121523.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Dec 16 05:19:37 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.515f	3.692	397.9E6	343.4E6	251.567m	226.165m
2) SA Decachlor...	10.570f	8.934f	18469109	19849304	16.449m	15.939m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO121823\
Data File : PO100570.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Dec 2023 22:07
Operator : YP/AJ
Sample : 05886-01
Misc :
ALS Vial : 27 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
AUD-1295


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 12/19/2023
Supervised By :Ankita Jodhani 12/19/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 19 03:02:08 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO121523.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Dec 16 05:19:37 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

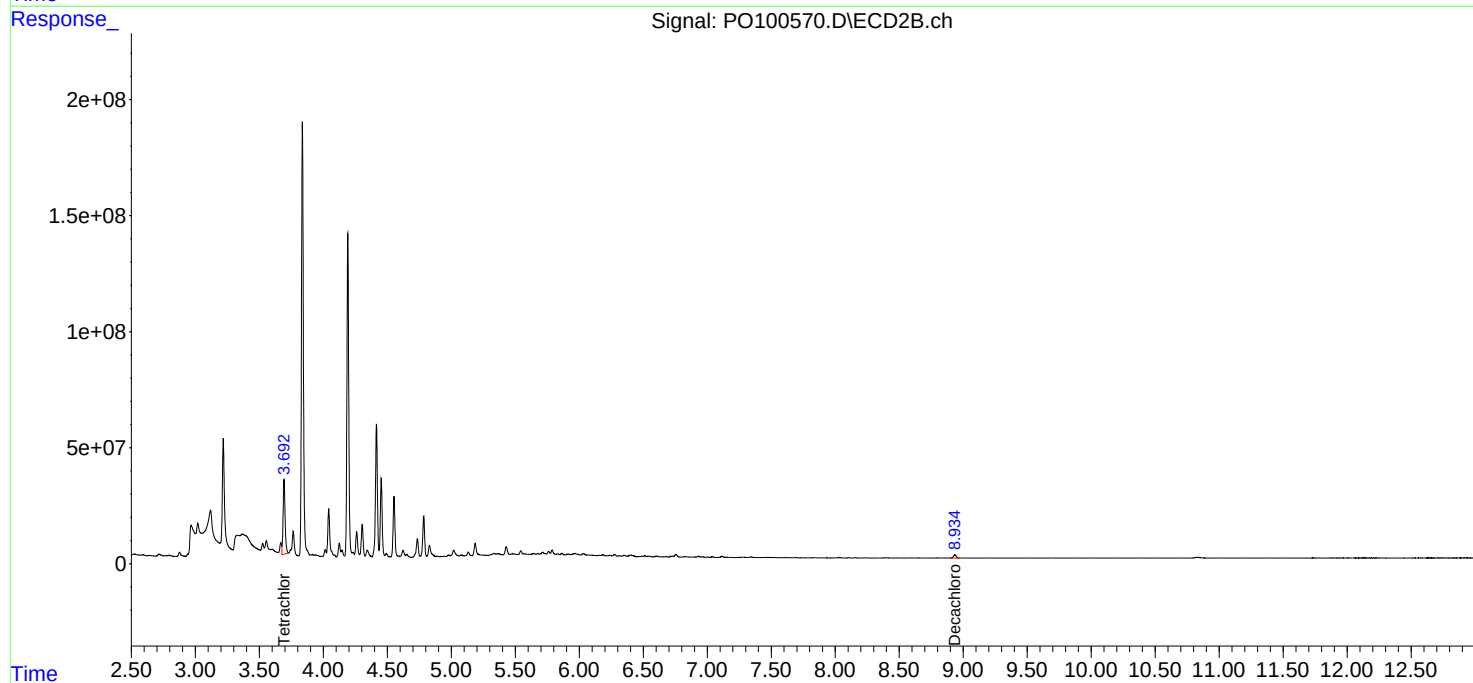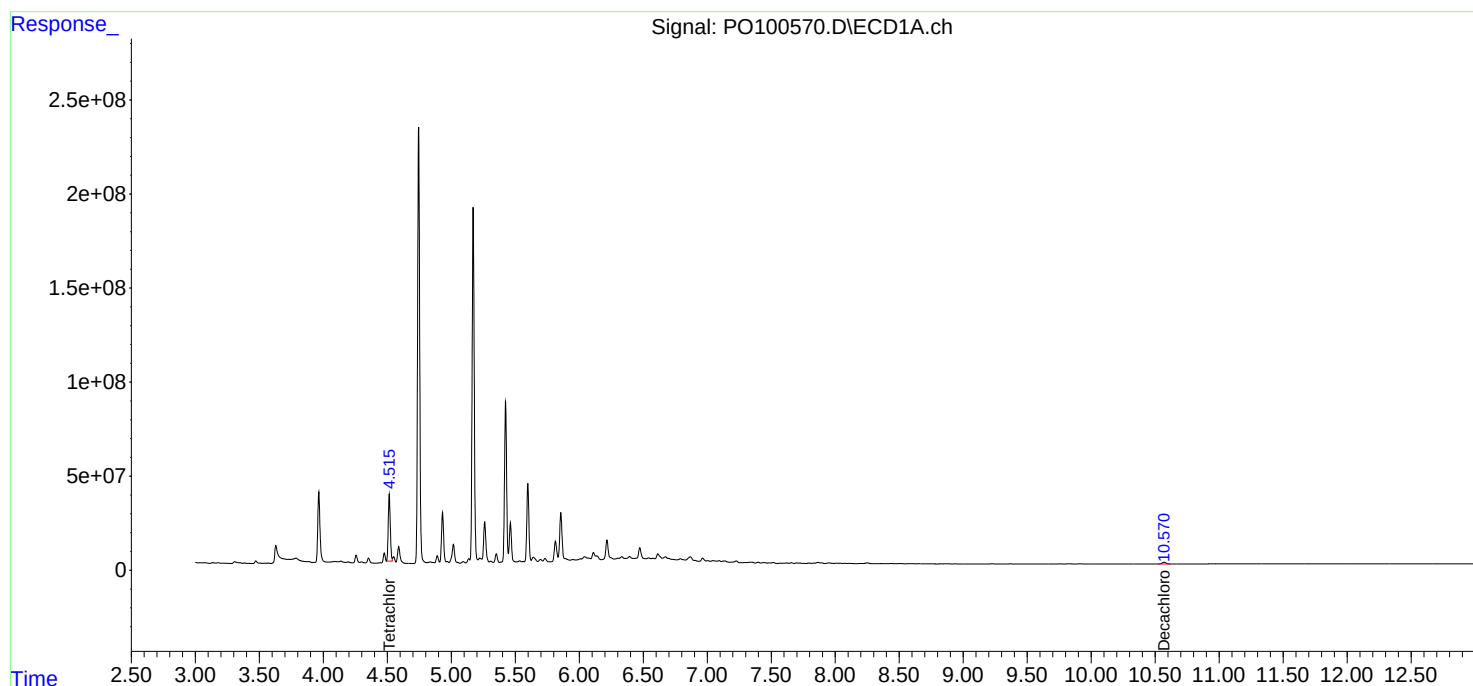

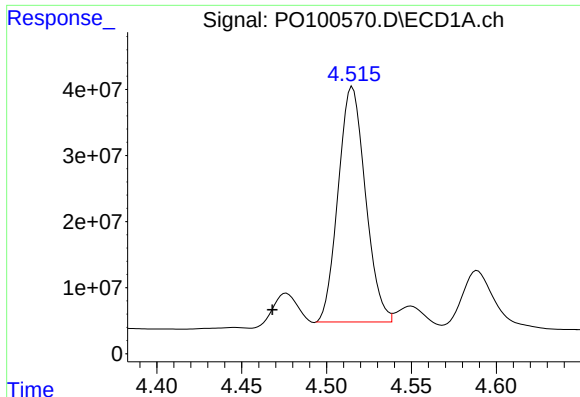


#1 Tetrachloro-m-xylene

R.T.: 4.515 min
Delta R.T.: 0.047 min
Response: 397943096
Conc: 251.57 ng/ml

Instrument :
ECD_O
ClientSampleId :
AUD-1295


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 12/19/2023
Supervised By :Ankita Jodhani 12/19/2023

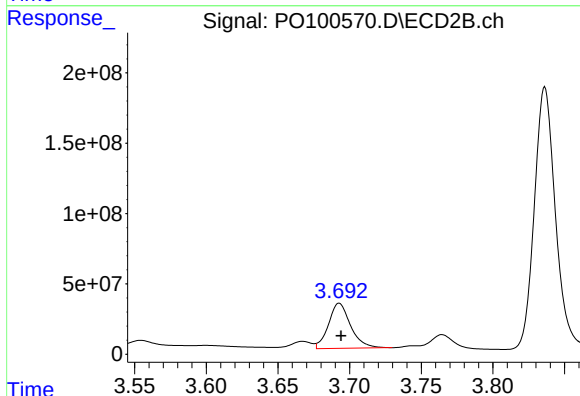


#1 Tetrachloro-m-xylene

R.T.: 3.692 min
Delta R.T.: -0.002 min
Response: 343429949
Conc: 226.17 ng/ml m

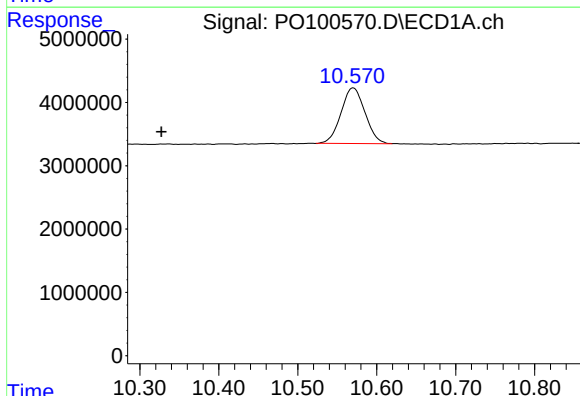

#2 Decachlorobiphenyl

R.T.: 10.570 min
Delta R.T.: 0.243 min
Response: 18469109
Conc: 16.45 ng/ml m

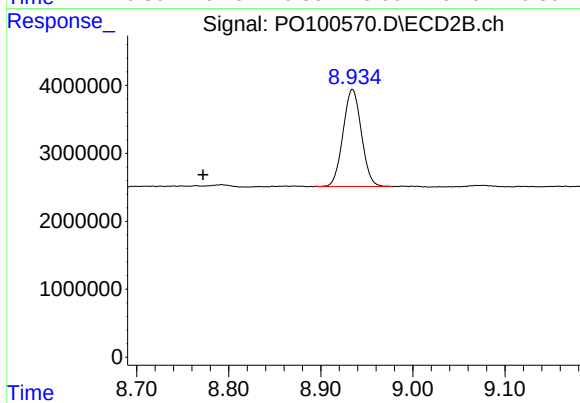

#2 Decachlorobiphenyl

R.T.: 8.934 min
Delta R.T.: 0.162 min
Response: 19849304
Conc: 15.94 ng/ml m