

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO121824\
 Data File : PO108615.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Dec 2024 12:46
 Operator : YP/AJ
 Sample : P5307-11
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 11A-11B-11C-1952-BLDG

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 12/19/2024
 Supervised By :Ankita Jodhani 12/19/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 19 03:46:45 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO120624.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Dec 07 05:58:15 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.705	3.702	131.8E6	89715071	15.144m	17.697m
2) SA Decachlor...	8.774	8.723	120.3E6	76293295	16.477	19.689

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO121824\
Data File : PO108615.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Dec 2024 12:46
Operator : YP/AJ
Sample : P5307-11
Misc :
ALS Vial : 10 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
11A-11B-11C-1952-BLDG


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 12/19/2024
Supervised By :Ankita Jodhani 12/19/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 19 03:46:45 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO120624.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Dec 07 05:58:15 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

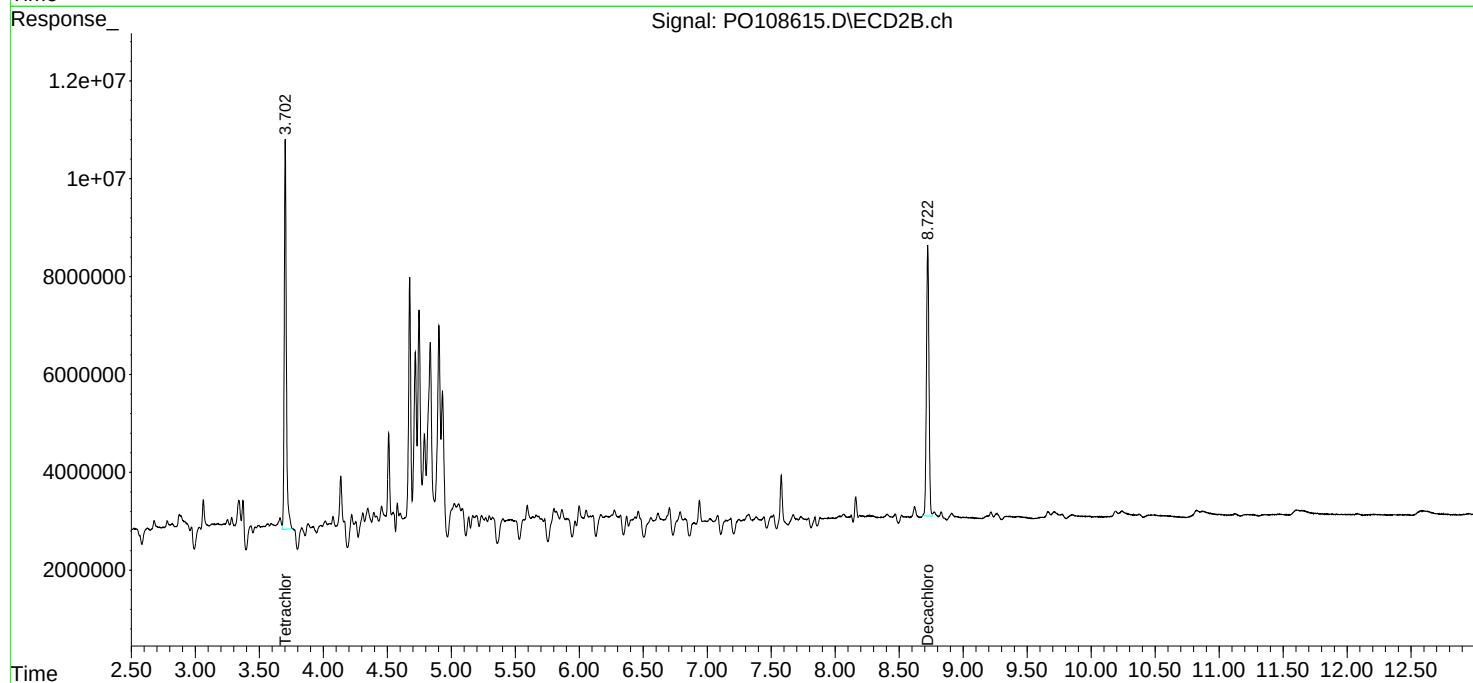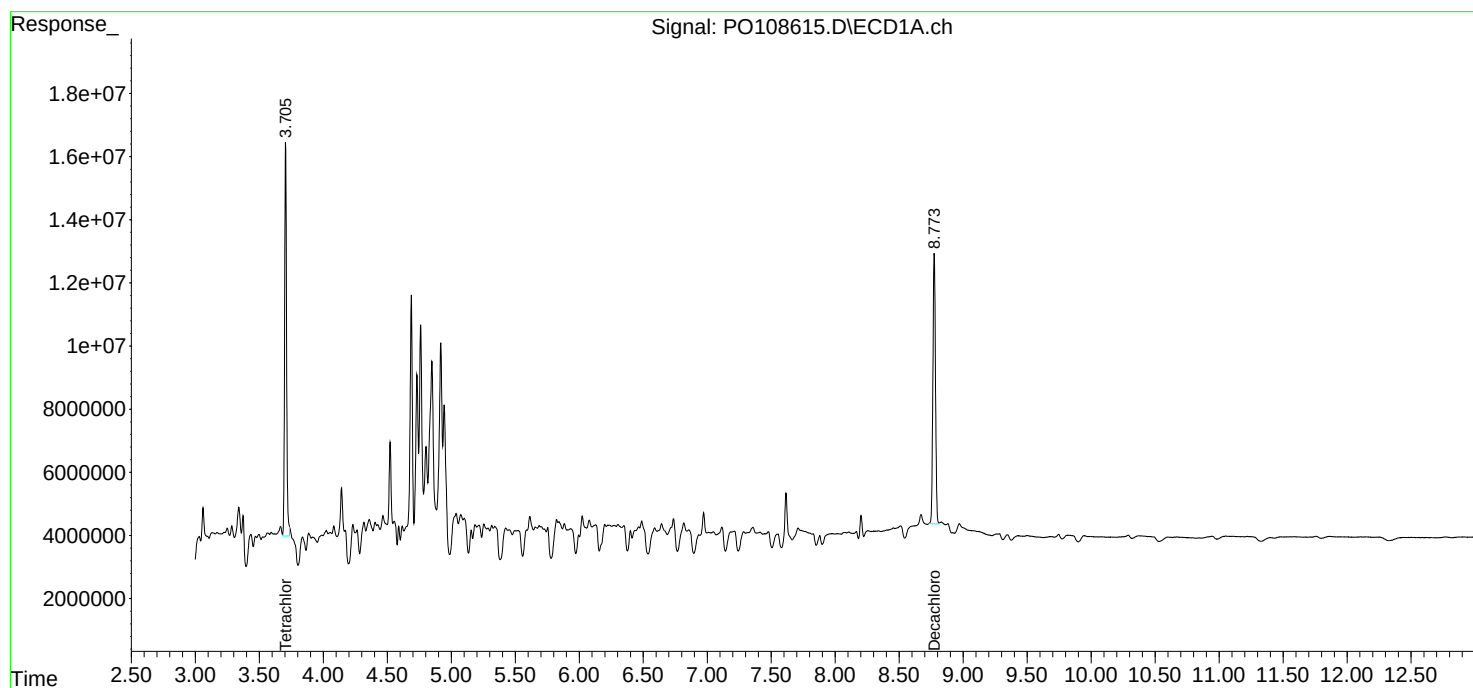

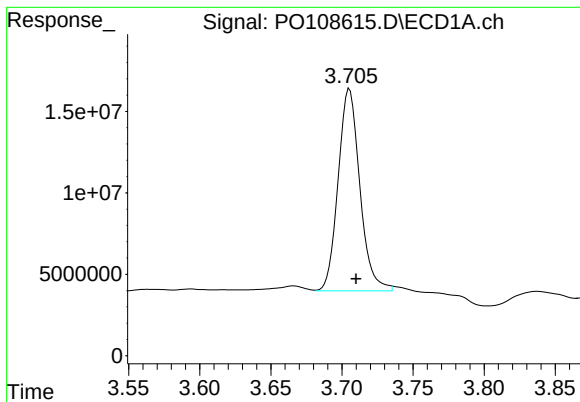


#1 Tetrachloro-m-xylene

R.T.: 3.705 min
Delta R.T.: -0.005 min
Response: 131757570
Conc: 15.14 ng/ml

Instrument :
ECD_O
ClientSampleId :
11A-11B-11C-1952-BLDG


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 12/19/2024
Supervised By :Ankita Jodhani 12/19/2024

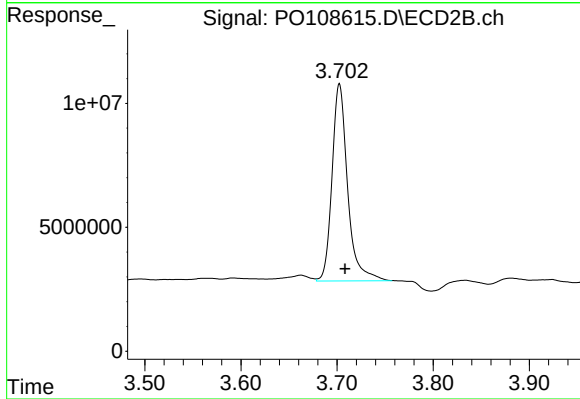


#1 Tetrachloro-m-xylene

R.T.: 3.702 min
Delta R.T.: -0.006 min
Response: 89715071
Conc: 17.70 ng/ml m

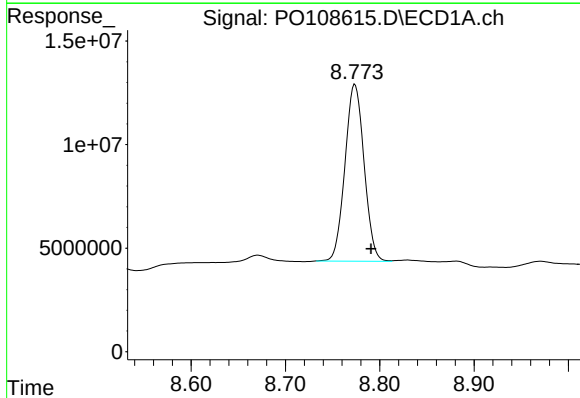

#2 Decachlorobiphenyl

R.T.: 8.774 min
Delta R.T.: -0.017 min
Response: 120349115
Conc: 16.48 ng/ml

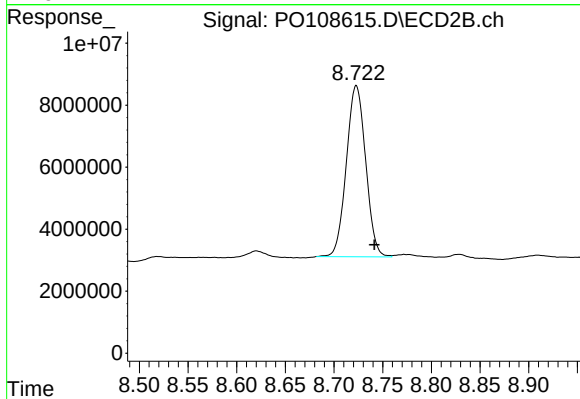

#2 Decachlorobiphenyl

R.T.: 8.723 min
Delta R.T.: -0.019 min
Response: 76293295
Conc: 19.69 ng/ml