

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0121918\
Data File : P0052739.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 19 Dec 2018 13:01
Operator : SM/SJ
Sample : J6438-13
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
COMP-3

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 19 13:29:13 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0121518.M
Quant Title : GC EXTRACTABLES
QLast Update : Sun Dec 16 03:01:24 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

1) SA Tetrachlo...	4.249	3.274	14654452	4349388	18.687	20.525
2) SA Decachlor...	9.796	7.956	8105283	3289134	16.086m	14.908

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO121918\
Data File : PO052739.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 19 Dec 2018 13:01
Operator : SM/SJ
Sample : J6438-13
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
COMP-3

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 19 13:29:13 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO121518.M
Quant Title : GC EXTRACTABLES
QLast Update : Sun Dec 16 03:01:24 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

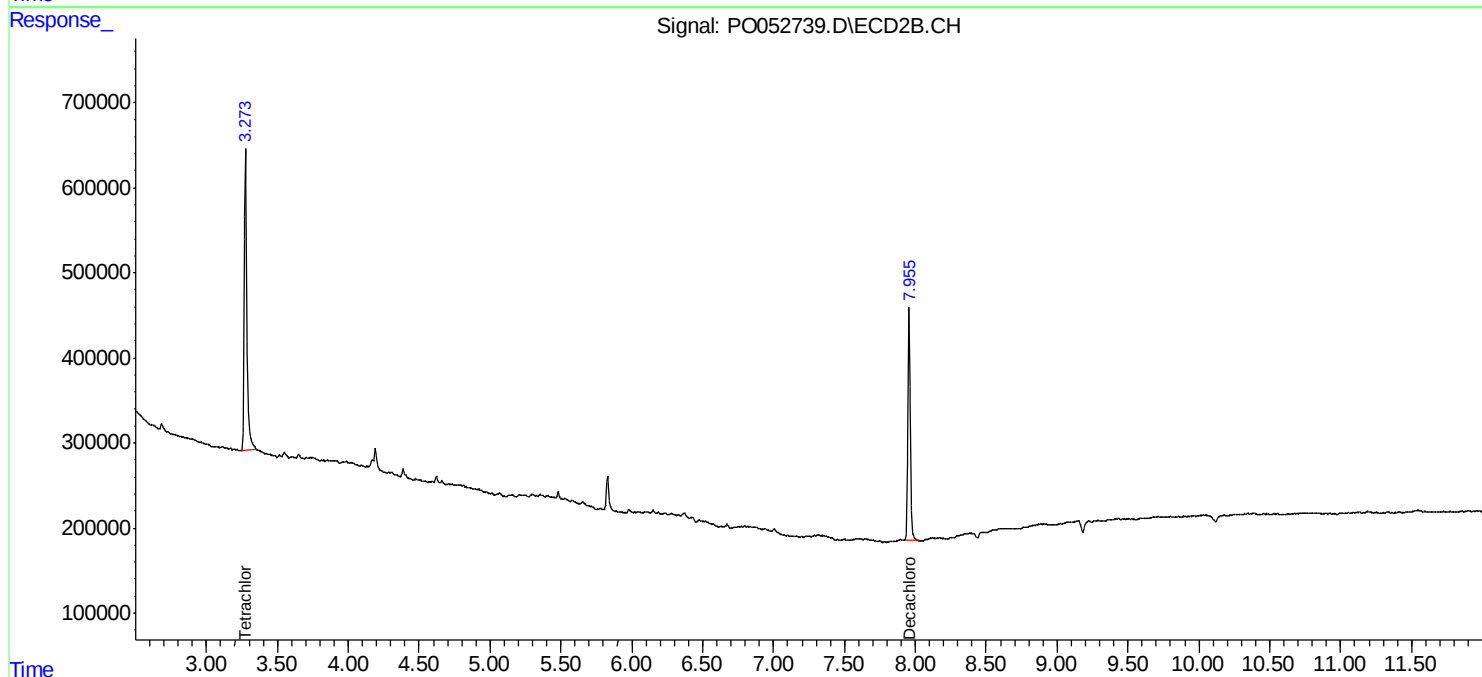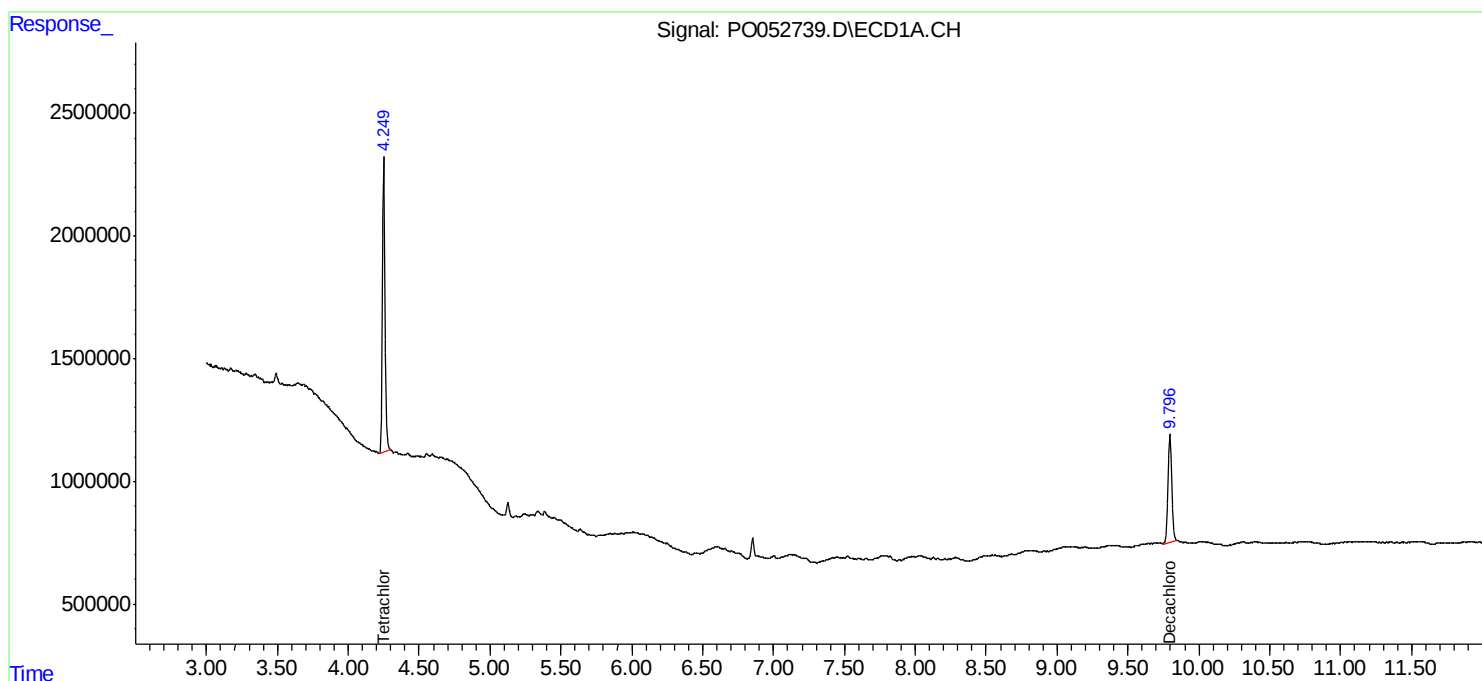


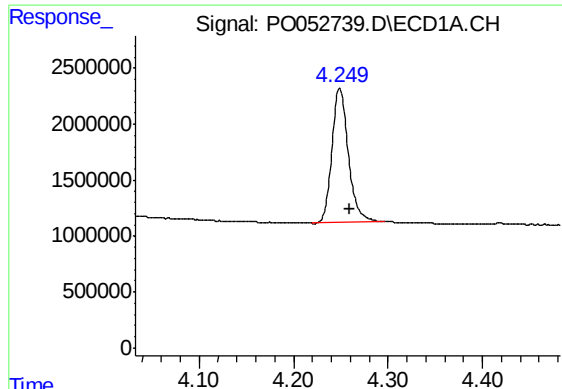

#1 Tetrachloro-m-xylene


R.T.: 4.249 min
Delta R.T.: -0.010 min
Response: 14654452
Conc: 18.69 ng/ml

Instrument :
ECD_O
ClientSampleId :
COMP-3

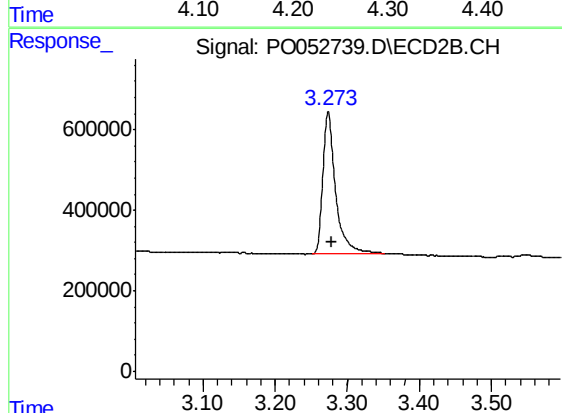


#1 Tetrachloro-m-xylene

R.T.: 3.274 min
Delta R.T.: -0.005 min
Response: 4349388
Conc: 20.53 ng/ml

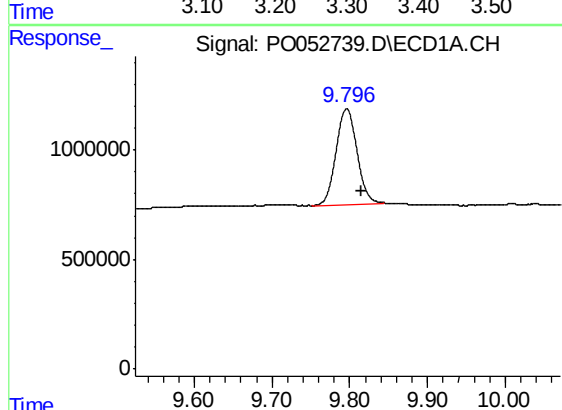

#2 Decachlorobiphenyl

R.T.: 9.796 min
Delta R.T.: -0.018 min
Response: 8105283
Conc: 16.09 ng/ml m

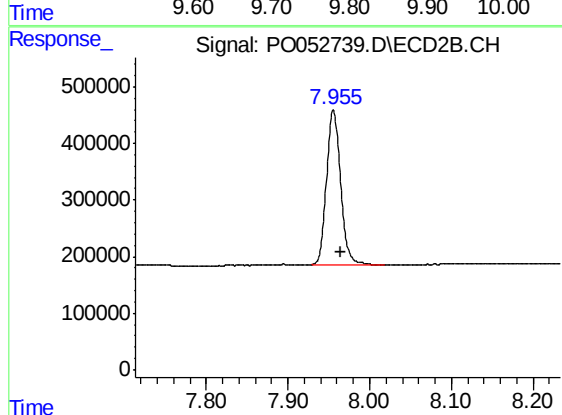

#2 Decachlorobiphenyl

R.T.: 7.956 min
Delta R.T.: -0.009 min
Response: 3289134
Conc: 14.91 ng/ml