

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO122018\
 Data File : PO052827.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 20 Dec 2018 23:04
 Operator : SM/SJ
 Sample : J6470-02 10X
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 21 02:35:56 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO121518.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sun Dec 16 03:01:24 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.249	0.000	517507	0	0.660	N.D. #
2) SA Decachlor...	0.000	7.951	0	313986	N.D.	1.423 #
Target Compounds						
6) L1 AR-1016-4	5.591	0.000	474556	0	31.585	N.D. #
14) L3 AR-1232-4	5.591	0.000	474556	0	69.066	N.D. #
15) L3 AR-1232-5	5.707	0.000	498739	0	108.106	N.D. #
19) L4 AR-1242-4	5.591	0.000	474556	0	36.200	N.D. #
22) L5 AR-1248-2	5.707	0.000	498739	0	26.179	N.D. #
28) L6 AR-1254-3	6.847	0.000	176933	0	4.491	N.D. #
34) L7 AR-1260-4	7.877	0.000	71943	0	2.890	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO122018\
Data File : PO052827.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 20 Dec 2018 23:04
Operator : SM/SJ
Sample : J6470-02 10X
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 21 02:35:56 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO121518.M
Quant Title : GC EXTRACTABLES
QLast Update : Sun Dec 16 03:01:24 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

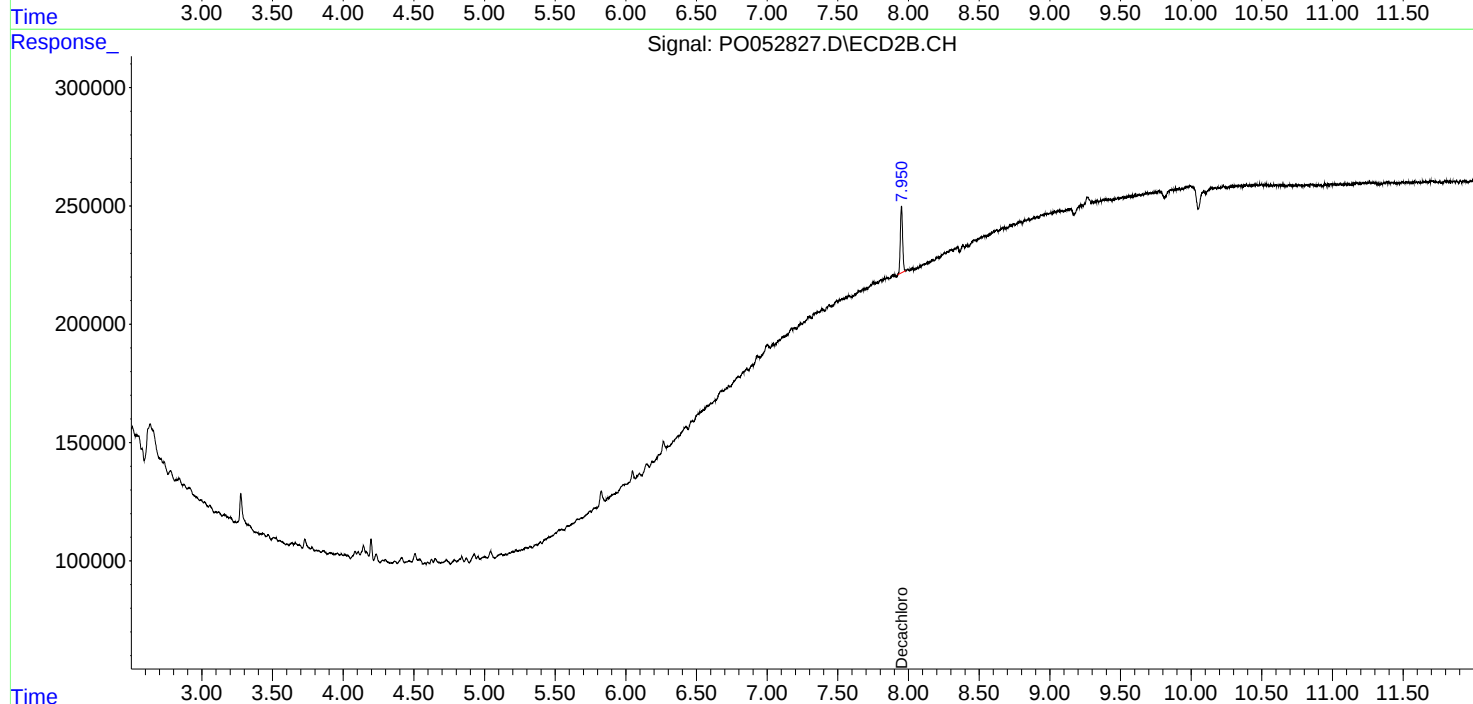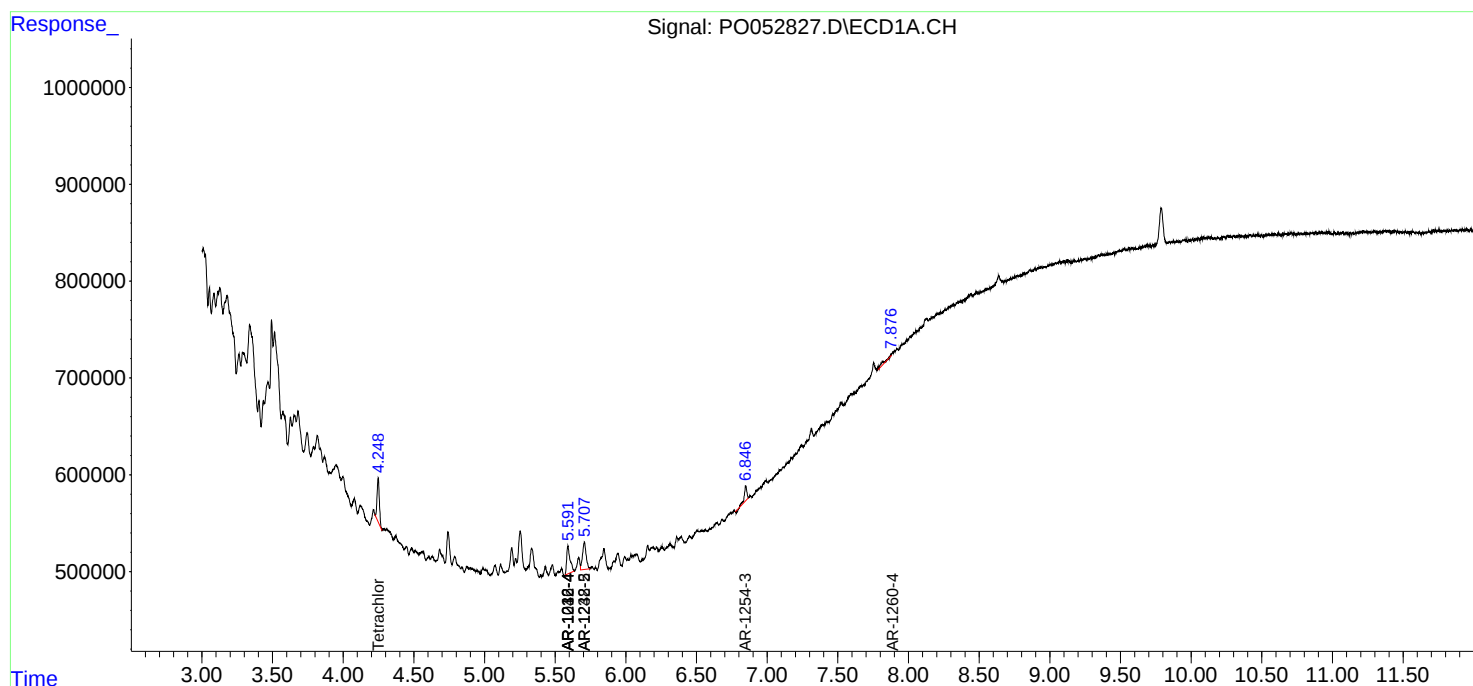


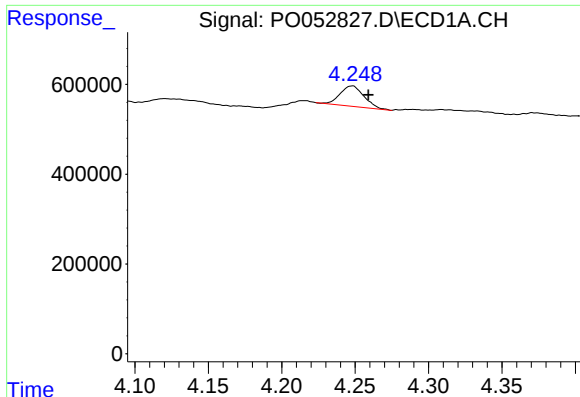

#1 Tetrachloro-m-xylene


R.T.: 4.249 min
Delta R.T.: -0.010 min
Response: 517507
Conc: 0.66 ng/ml

Instrument :
ECD_O
ClientSampleId :

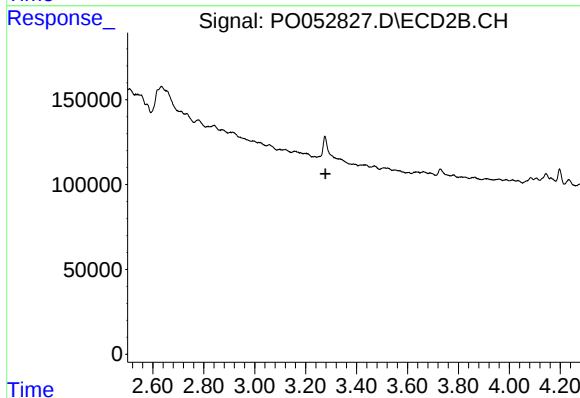


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T. : 3.278 min
Response: 0
Conc: N.D.

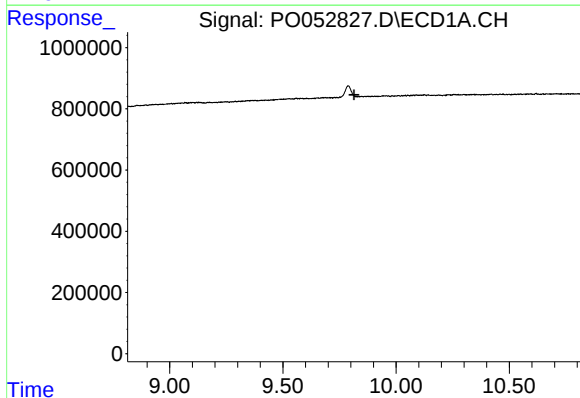


#2 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 9.814 min
Response: 0
Conc: N.D.

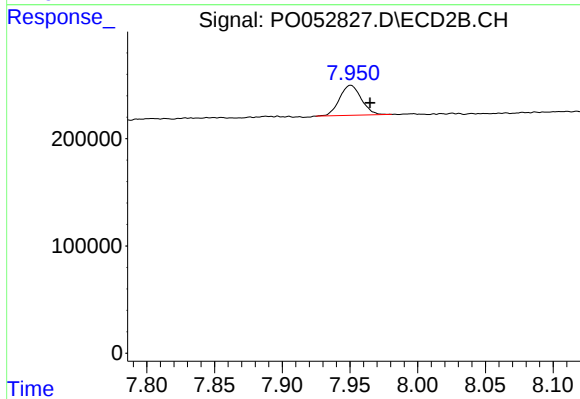

#2 Decachlorobiphenyl


R.T.: 7.951 min
Delta R.T.: -0.014 min
Response: 313986
Conc: 1.42 ng/ml

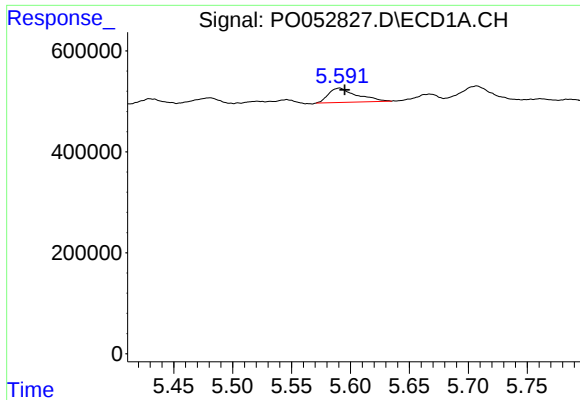

#6 AR-1016-4


R.T.: 5.591 min
Delta R.T.: -0.004 min
Response: 474556
Conc: 31.58 ng/ml

Instrument :
ECD_O
ClientSampleId :

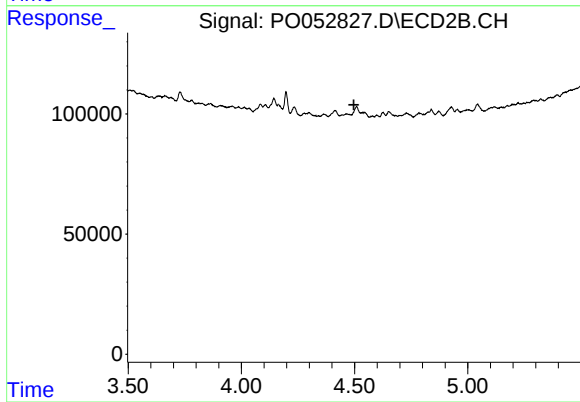


#6 AR-1016-4

R.T.: 0.000 min
Exp R.T. : 4.497 min
Response: 0
Conc: N.D.

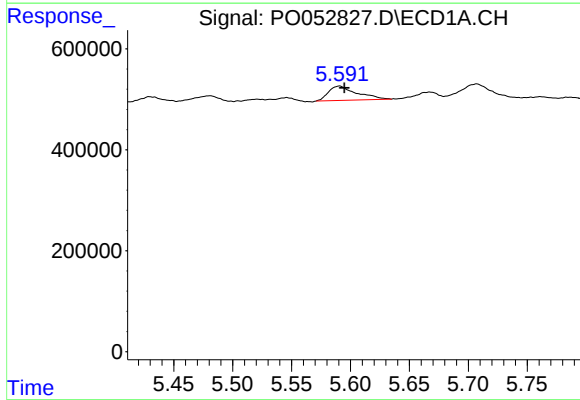


#14 AR-1232-4

R.T.: 5.591 min
Delta R.T.: -0.004 min
Response: 474556
Conc: 69.07 ng/ml

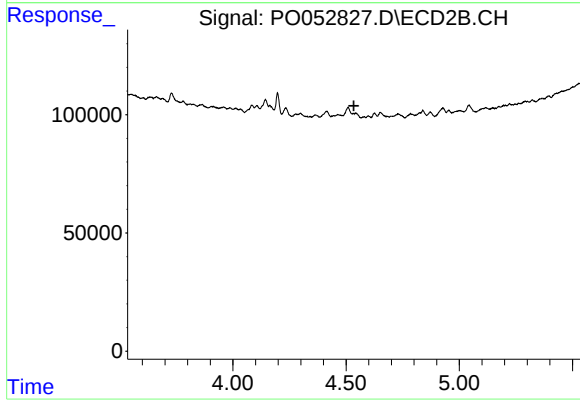

#14 AR-1232-4


R.T.: 0.000 min
Exp R.T. : 4.535 min
Response: 0
Conc: N.D.

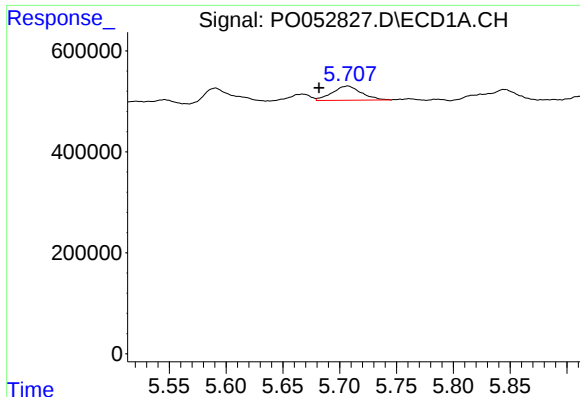

#15 AR-1232-5


R.T.: 5.707 min
Delta R.T.: 0.025 min
Response: 498739
Conc: 108.11 ng/ml

Instrument :
ECD_O
ClientSampleId :

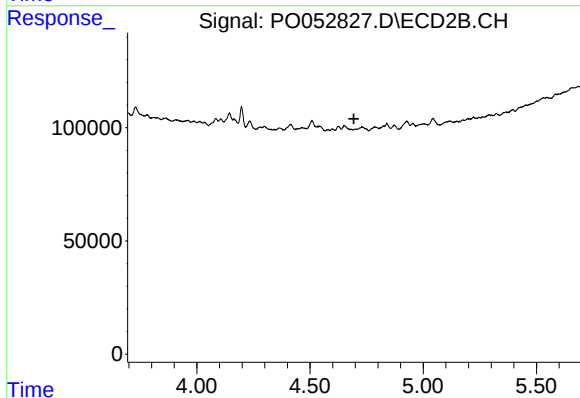


#15 AR-1232-5

R.T.: 0.000 min
Exp R.T. : 4.693 min
Response: 0
Conc: N.D.

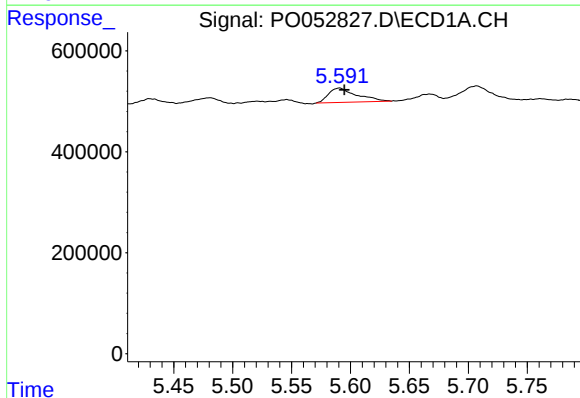


#19 AR-1242-4

R.T.: 5.591 min
Delta R.T.: -0.004 min
Response: 474556
Conc: 36.20 ng/ml

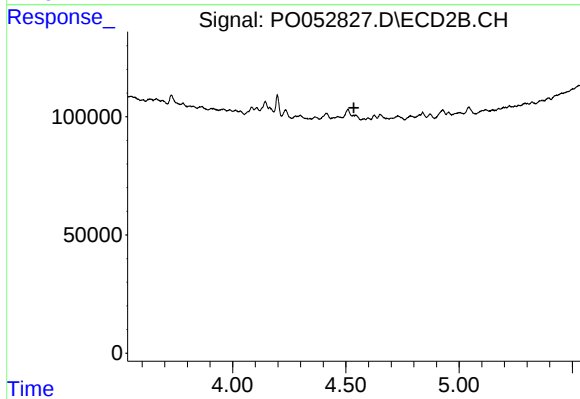

#19 AR-1242-4


R.T.: 0.000 min
Exp R.T. : 4.535 min
Response: 0
Conc: N.D.

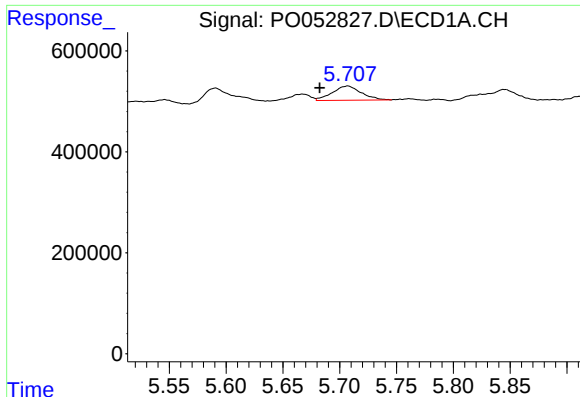

#22 AR-1248-2


R.T.: 5.707 min
Delta R.T.: 0.025 min
Response: 498739
Conc: 26.18 ng/ml

Instrument :
ECD_O
ClientSampleId :

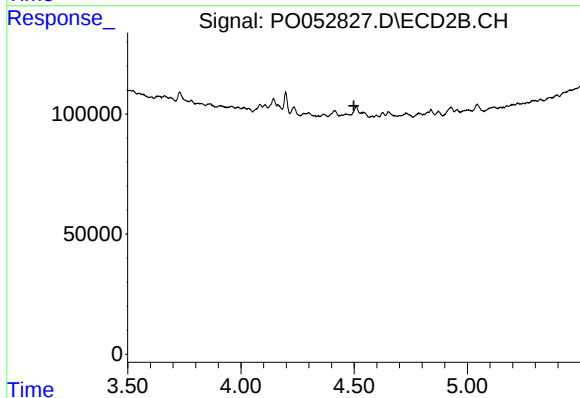


#22 AR-1248-2

R.T.: 0.000 min
Exp R.T. : 4.499 min
Response: 0
Conc: N.D.

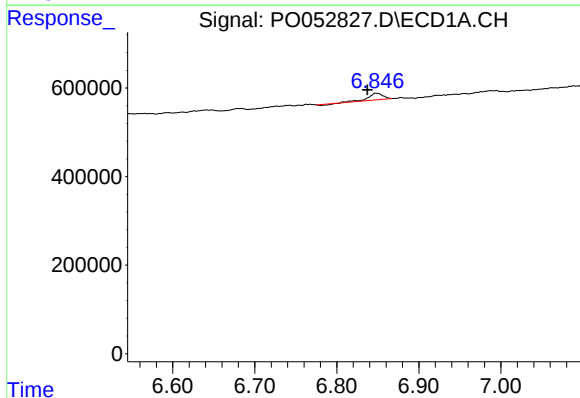


#28 AR-1254-3

R.T.: 6.847 min
Delta R.T.: 0.009 min
Response: 176933
Conc: 4.49 ng/ml

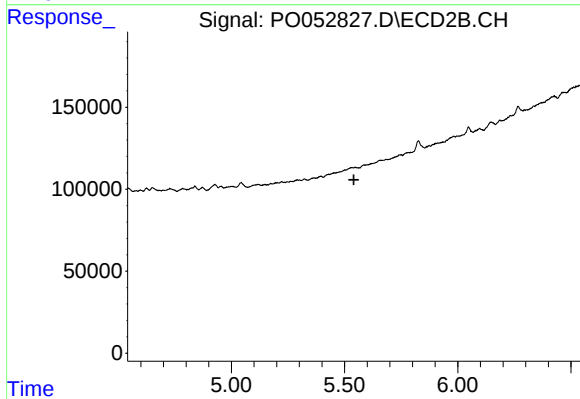

#28 AR-1254-3


R.T.: 0.000 min
Exp R.T. : 5.541 min
Response: 0
Conc: N.D.

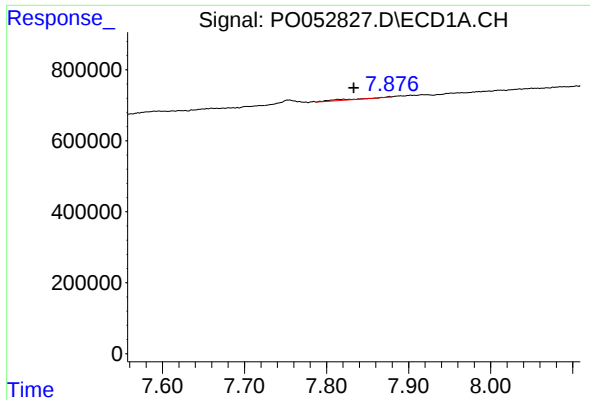

#34 AR-1260-4

R.T.: 7.877 min
Delta R.T.: 0.044 min
Response: 71943
Conc: 2.89 ng/ml

Instrument :
ECD_O
ClientSampleId :

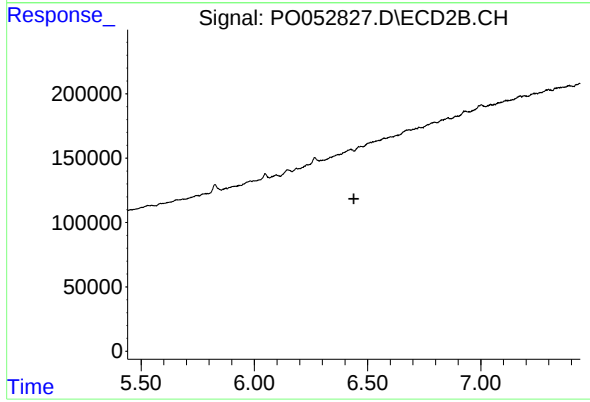

#34 AR-1260-4

R.T.: 0.000 min
Exp R.T. : 6.440 min
Response: 0
Conc: N.D.