

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0122018\
 Data File : P0052858.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 21 Dec 2018 9:14
 Operator : SM/SJ
 Sample : J6482-07 10X
 Misc :
 ALS Vial : 48 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 DPC-91468-OD-01

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 21 10:45:08 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0121518.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sun Dec 16 03:01:24 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.243	3.270	1034774	263804	1.320	1.245
2) SA Decachlor...	9.789	7.951	875970	381450	1.739m	1.729

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO122018\
Data File : PO052858.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 21 Dec 2018 9:14
Operator : SM/SJ
Sample : J6482-07 10X
Misc :
ALS Vial : 48 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
DPC-91468-OD-01

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 21 10:45:08 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO121518.M
Quant Title : GC EXTRACTABLES
QLast Update : Sun Dec 16 03:01:24 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

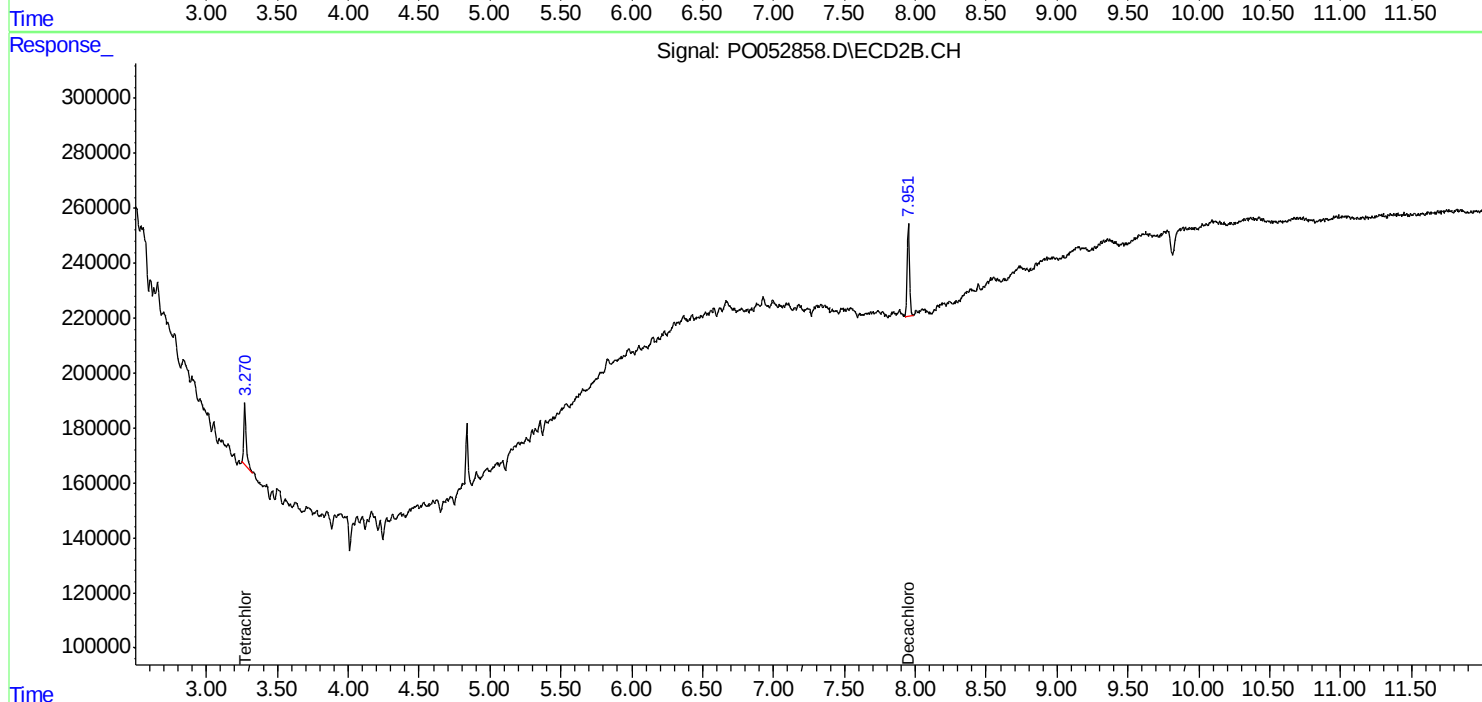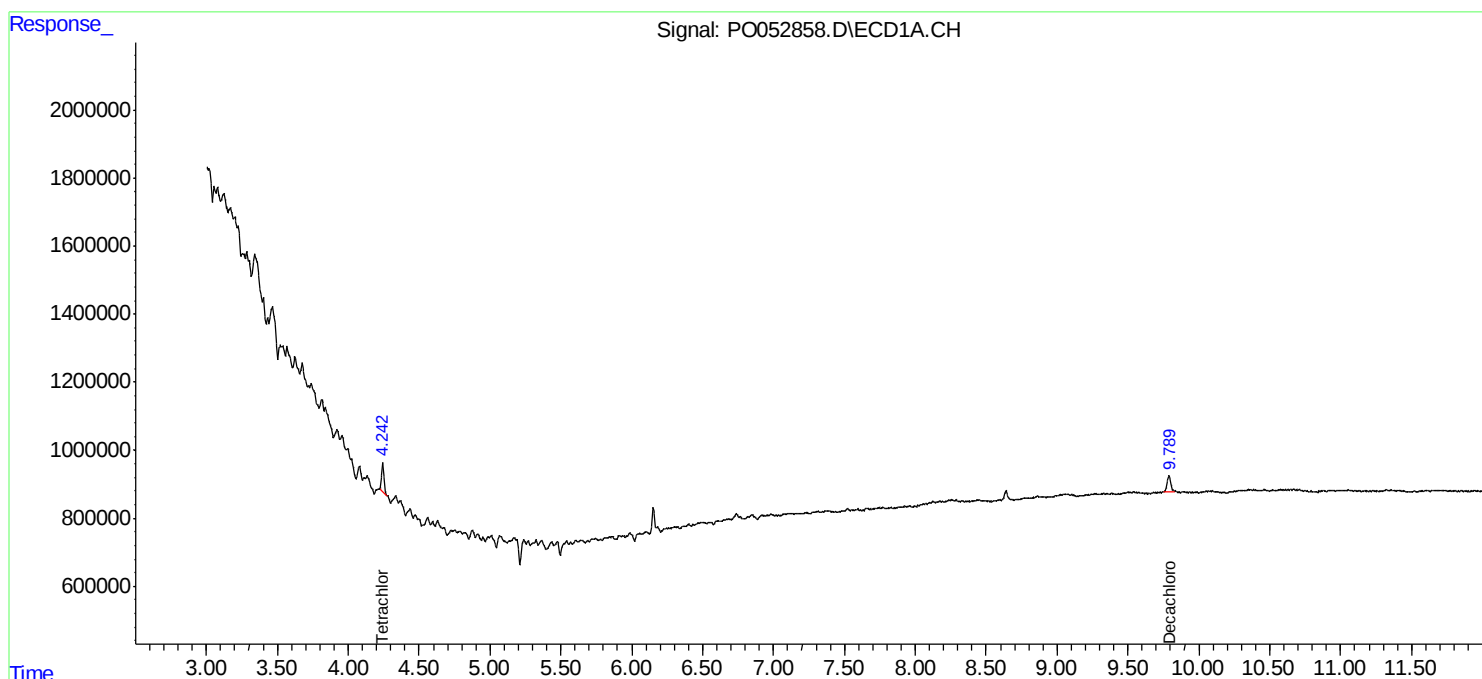


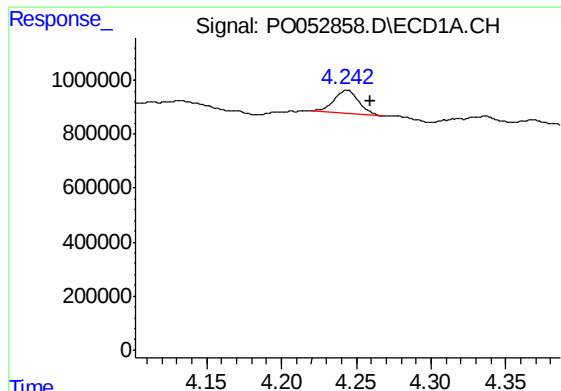

#1 Tetrachloro-m-xylene


R.T.: 4.243 min
Delta R.T.: -0.016 min
Response: 1034774
Conc: 1.32 ng/ml

Instrument :
ECD_O
ClientSampleId :
DPC-91468-OD-01

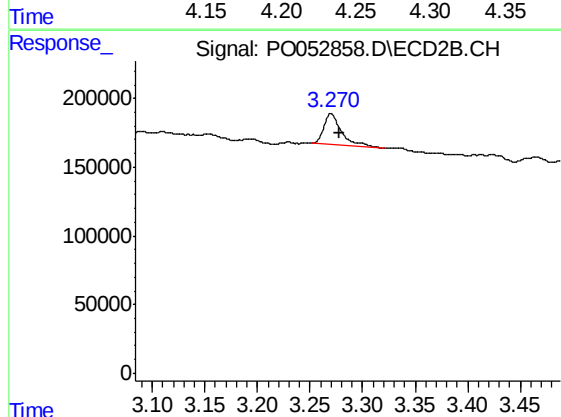


#1 Tetrachloro-m-xylene

R.T.: 3.270 min
Delta R.T.: -0.008 min
Response: 263804
Conc: 1.24 ng/ml

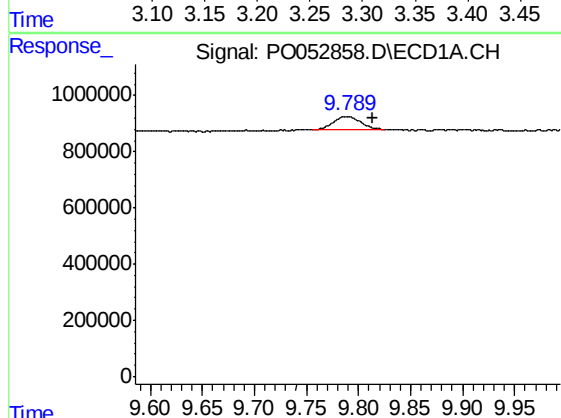

#2 Decachlorobiphenyl

R.T.: 9.789 min
Delta R.T.: -0.025 min
Response: 875970
Conc: 1.74 ng/ml m

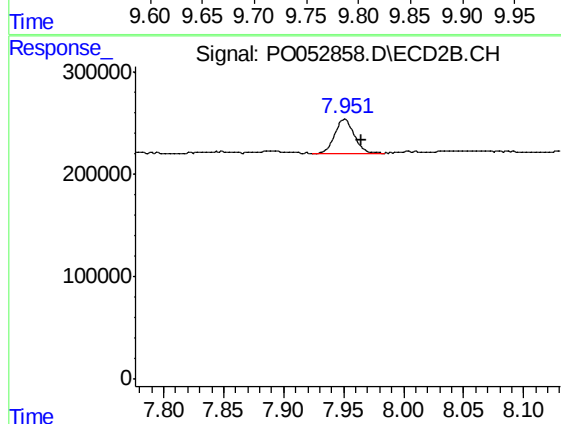

#2 Decachlorobiphenyl

R.T.: 7.951 min
Delta R.T.: -0.014 min
Response: 381450
Conc: 1.73 ng/ml