

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\PO122019\
 Data File : PO064819.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 20 Dec 2019 12:11
 Operator : SM/AJ
 Sample : K6358-02
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_0
 ClientSampleId :
 PCB-121619-02

Manual Integrations
 APPROVED

Ankita
 12/24/2019 9:16:44 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 20 13:11:17 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\PO121319.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Dec 13 08:19:24 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.198	3.460	342290	410838	14.060m	16.207m
2)	SA Decachlor...	9.721	8.382	400753	510474	13.058m	14.699
Target Compounds							
26)	L6 AR-1254-1	6.194	5.318	200055	313398	157.086	154.328
27)	L6 AR-1254-2	6.411	5.464	224672	209270	108.013	114.770
28)	L6 AR-1254-3	6.774	5.863	146220	265511	61.236	85.471m#
29)	L6 AR-1254-4	7.057	6.091	63618	60549	34.021	29.478m
30)	L6 AR-1254-5	7.464	6.482	1001805	1244744	476.138m	417.016m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO122019\
Data File : P0064819.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 20 Dec 2019 12:11
Operator : SM/AJ
Sample : K6358-02
Misc :
ALS Vial : 4 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampled :
PCB-121619-02


Manual Integrations
APPROVED

Ankita
12/24/2019 9:16:44 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 20 13:11:17 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO121319.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Dec 13 08:19:24 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

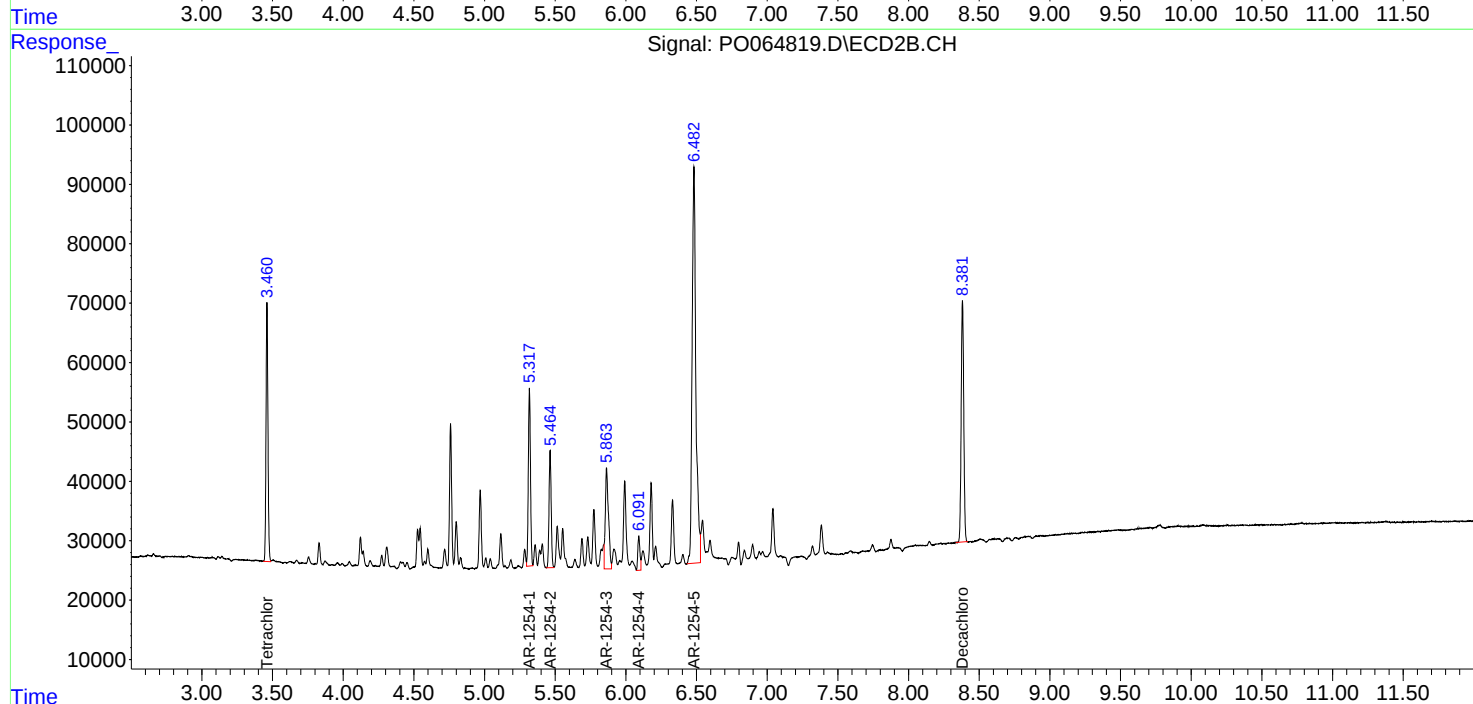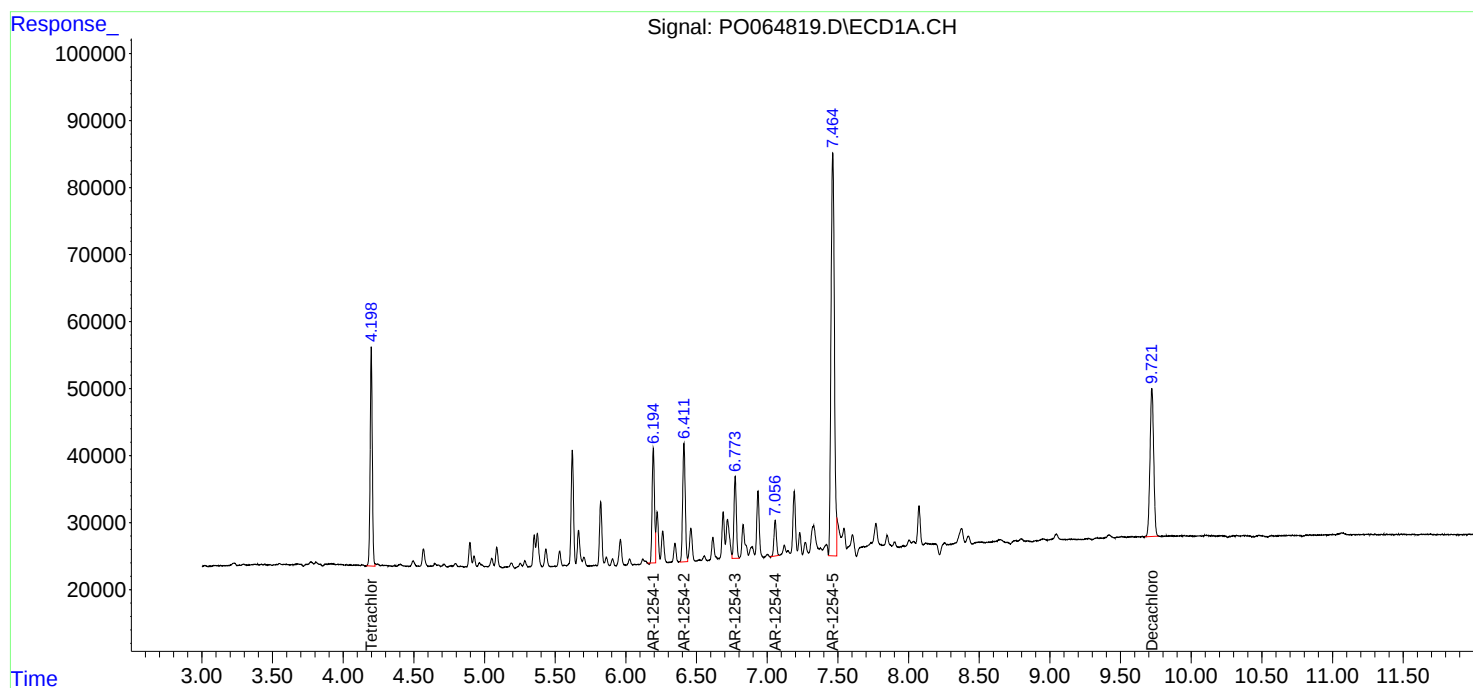

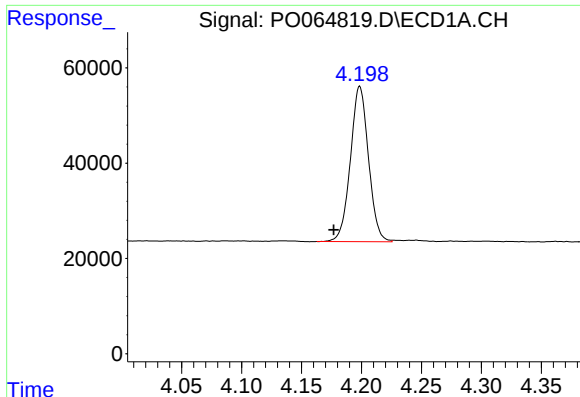


#1 Tetrachloro-m-xylene

R.T.: 4.198 min
Delta R.T.: 0.021 min
Response: 342290
Conc: 14.06 ng/ml m

Instrument :
ECD_O
ClientSampleId :
PCB-121619-02


Manual Integrations
APPROVED

Ankita
12/24/2019 9:16:44 AM

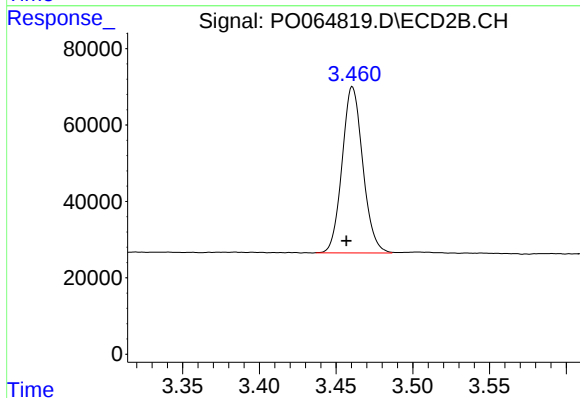


#1 Tetrachloro-m-xylene

R.T.: 3.460 min
Delta R.T.: 0.003 min
Response: 410838
Conc: 16.21 ng/ml m

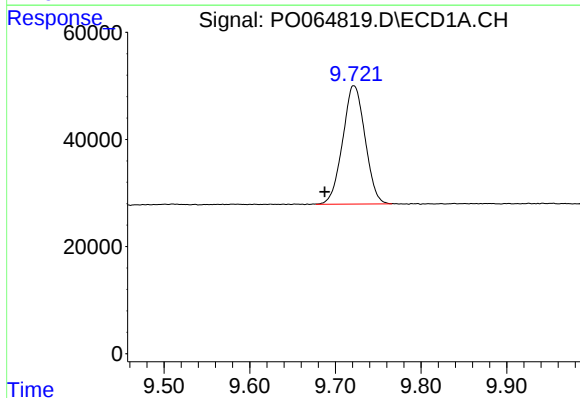


#2 Decachlorobiphenyl

R.T.: 9.721 min
Delta R.T.: 0.034 min
Response: 400753
Conc: 13.06 ng/ml m

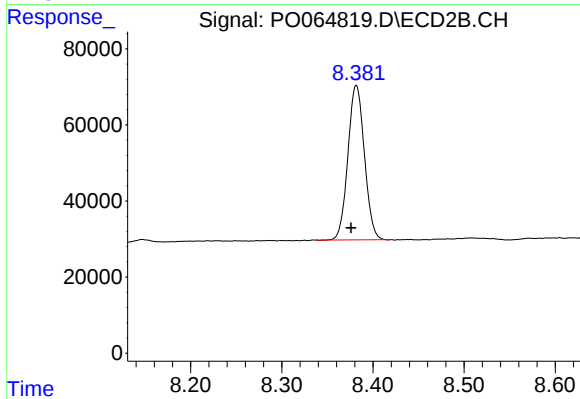

#2 Decachlorobiphenyl

R.T.: 8.382 min
Delta R.T.: 0.006 min
Response: 510474
Conc: 14.70 ng/ml

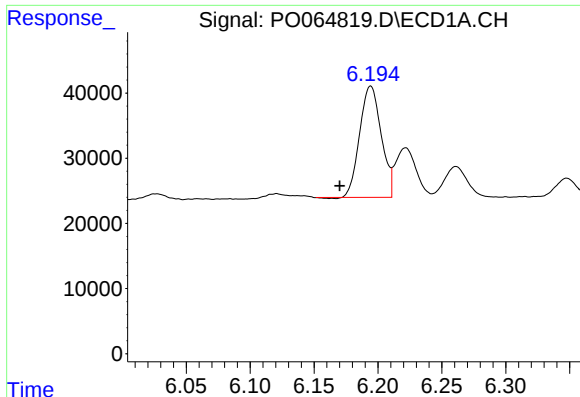


#26 AR-1254-1

R.T.: 6.194 min
Delta R.T.: 0.024 min
Response: 200055
Conc: 157.09 ng/ml

Instrument :
ECD_O
ClientSampleId :
PCB-121619-02


Manual Integrations
APPROVED

Ankita
12/24/2019 9:16:44 AM

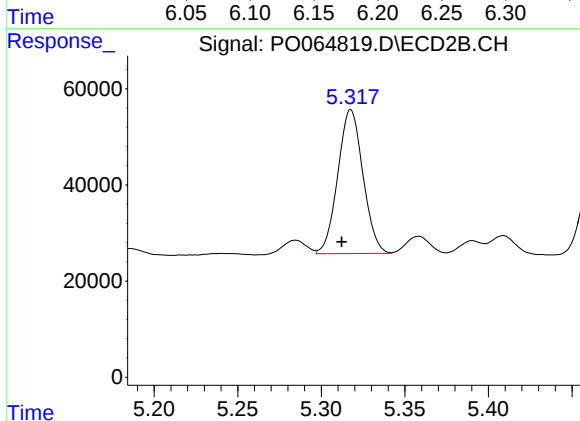


#26 AR-1254-1

R.T.: 5.318 min
Delta R.T.: 0.005 min
Response: 313398
Conc: 154.33 ng/ml

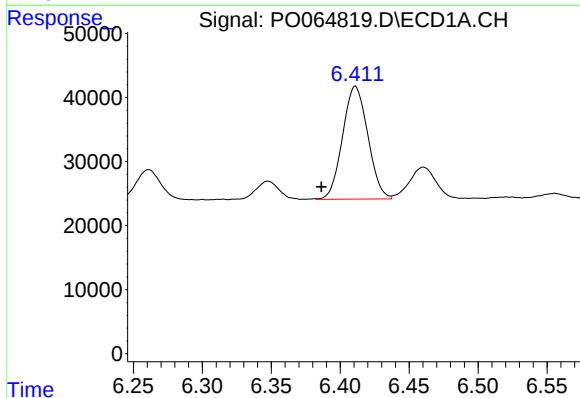


#27 AR-1254-2

R.T.: 6.411 min
Delta R.T.: 0.025 min
Response: 224672
Conc: 108.01 ng/ml

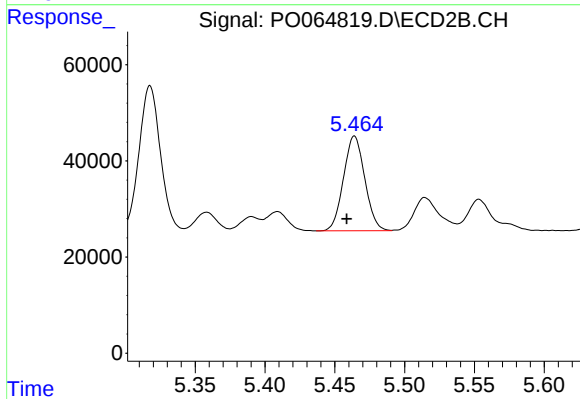

#27 AR-1254-2

R.T.: 5.464 min
Delta R.T.: 0.006 min
Response: 209270
Conc: 114.77 ng/ml

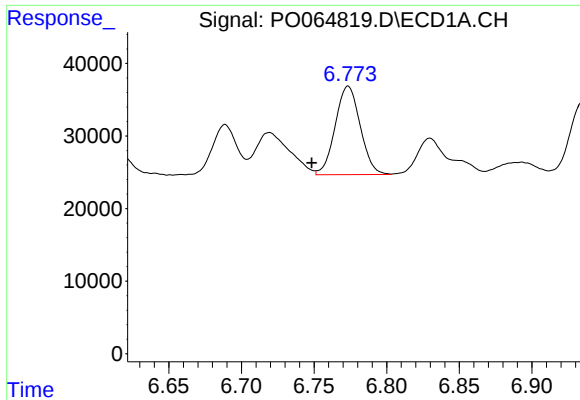


#28 AR-1254-3

R.T.: 6.774 min
Delta R.T.: 0.025 min
Response: 146220
Conc: 61.24 ng/ml

Instrument :
ECD_O
ClientSampleId :
PCB-121619-02


Manual Integrations
APPROVED

Ankita
12/24/2019 9:16:44 AM

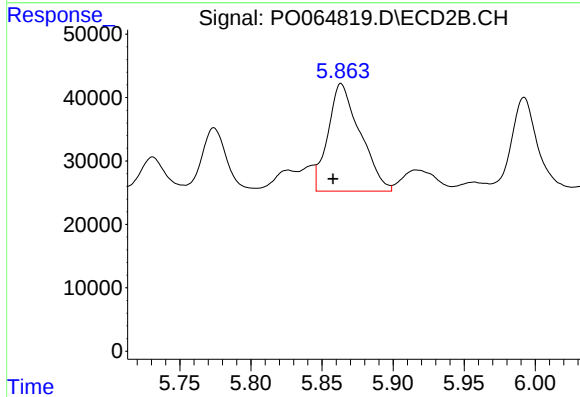


#28 AR-1254-3

R.T.: 5.863 min
Delta R.T.: 0.005 min
Response: 265511
Conc: 85.47 ng/ml m

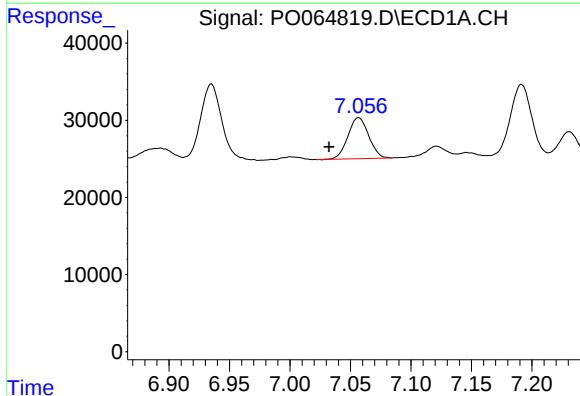


#29 AR-1254-4

R.T.: 7.057 min
Delta R.T.: 0.024 min
Response: 63618
Conc: 34.02 ng/ml

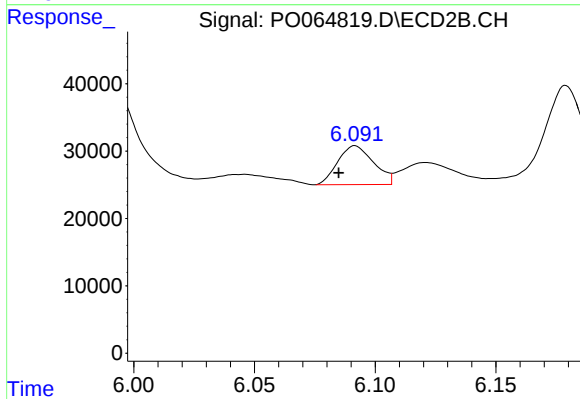

#29 AR-1254-4

R.T.: 6.091 min
Delta R.T.: 0.006 min
Response: 60549
Conc: 29.48 ng/ml m

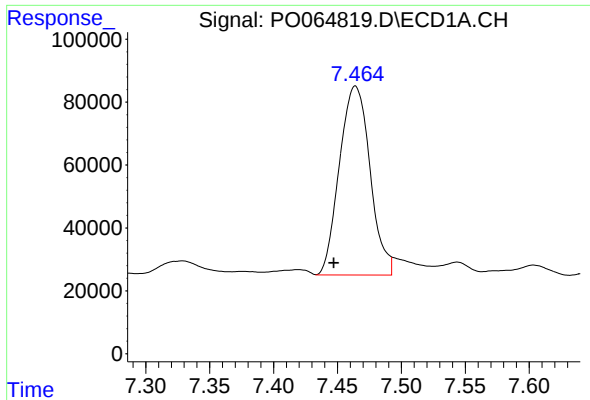


#30 AR-1254-5

R.T.: 7.464 min
Delta R.T.: 0.016 min
Response: 1001805
Conc: 476.14 ng/ml m

Instrument :
ECD_O
ClientSampleId :
PCB-121619-02

Manual Integrations
APPROVED

Ankita
12/24/2019 9:16:44 AM

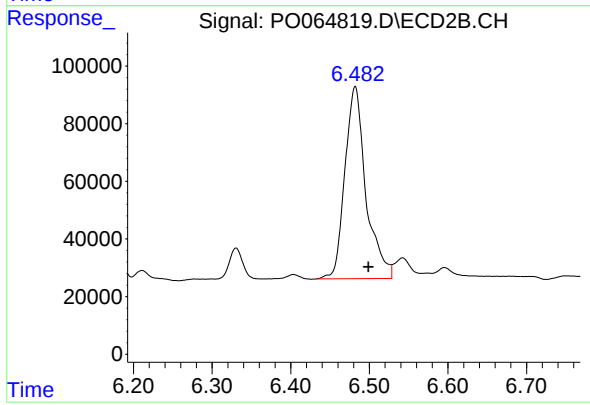

#30 AR-1254-5

R.T.: 6.482 min
Delta R.T.: -0.017 min
Response: 1244744
Conc: 417.02 ng/ml m