

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO122019\
 Data File : P0064848.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 20 Dec 2019 20:21
 Operator : SM/AJ
 Sample : K6348-01
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 MW-8

Manual Integrations
 APPROVED

Ankita
 12/23/2019 11:10:13 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 21 05:31:14 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO121319.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Dec 13 08:19:24 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.184	3.459	542317	598812	22.276m	23.622
2) SA Decachlor...	9.700	8.372	388337	472134	12.653	13.595

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO122019\
Data File : P0064848.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 20 Dec 2019 20:21
Operator : SM/AJ
Sample : K6348-01
Misc :
ALS Vial : 22 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampled :
MW-8


Manual Integrations
APPROVED

Ankita
12/23/2019 11:10:13 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 21 05:31:14 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO121319.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Dec 13 08:19:24 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

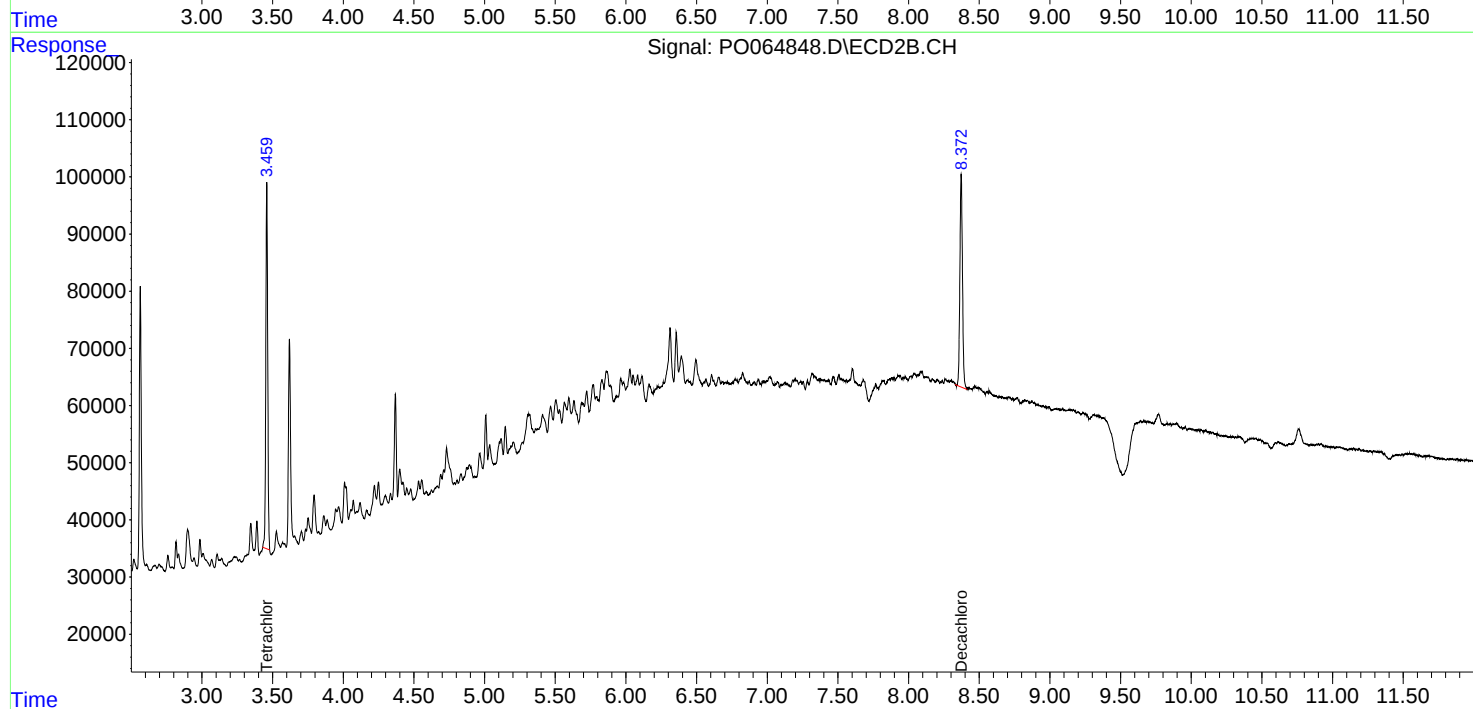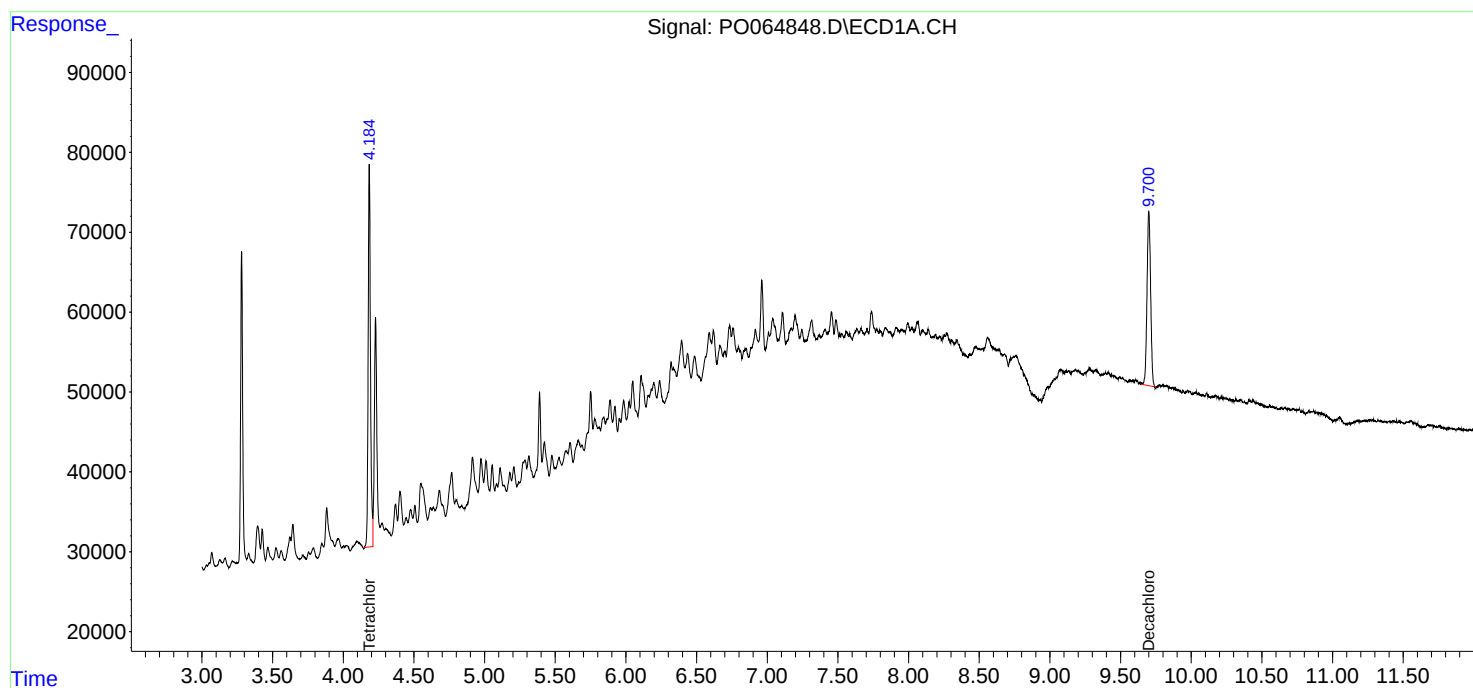

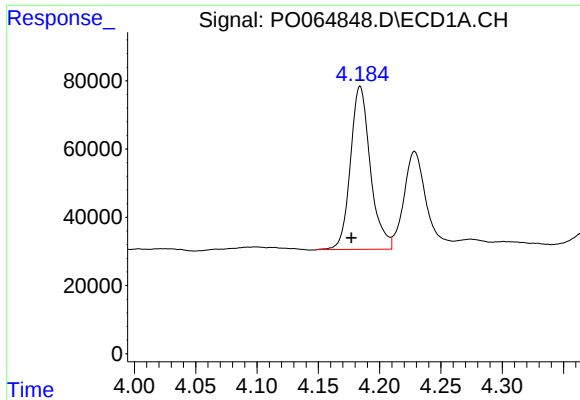


#1 Tetrachloro-m-xylene

R.T.: 4.184 min
Delta R.T.: 0.007 min
Response: 542317
Conc: 22.28 ng/ml m

Instrument :
ECD_O
ClientSampleId :
MW-8


Manual Integrations
APPROVED

Ankita
12/23/2019 11:10:13 AM

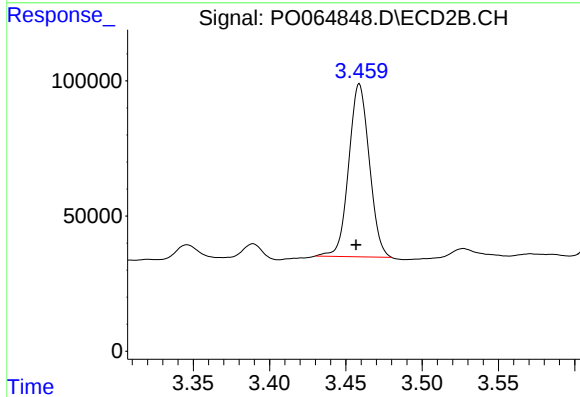


#1 Tetrachloro-m-xylene

R.T.: 3.459 min
Delta R.T.: 0.002 min
Response: 598812
Conc: 23.62 ng/ml

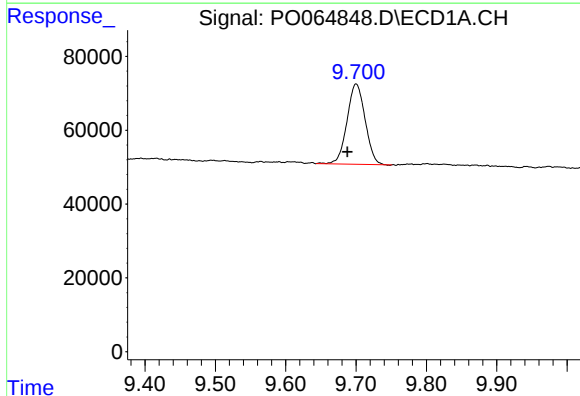

#2 Decachlorobiphenyl

R.T.: 9.700 min
Delta R.T.: 0.013 min
Response: 388337
Conc: 12.65 ng/ml

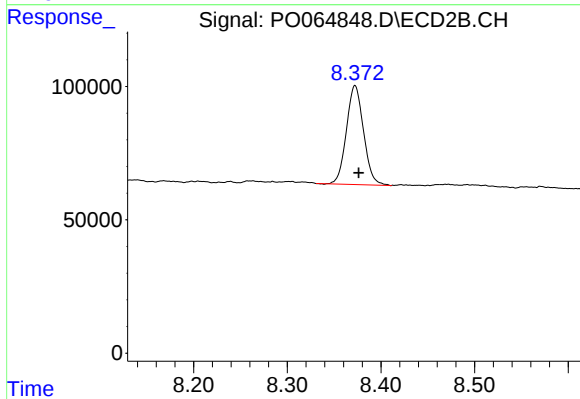

#2 Decachlorobiphenyl

R.T.: 8.372 min
Delta R.T.: -0.004 min
Response: 472134
Conc: 13.59 ng/ml