

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO122021\
 Data File : PO083868.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 20 Dec 2021 14:53
 Operator : AJ\MA
 Sample : PB141553BL
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 20 17:08:40 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO121521.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Dec 16 04:05:27 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.935	3.941	1982394	622168	20.808	21.210
2)	SA Decachlor...	11.007	9.236	1529593	625573	22.332	22.279
Target Compounds							
9)	L2 AR-1221-2	5.291	0.000	23510	0	32.903	N.D. #
28)	L6 AR-1254-3	7.794	0.000	52051	0	11.163	N.D. #
30)	L6 AR-1254-5	8.524	0.000	38469	0	10.791	N.D. #
32)	L7 AR-1260-2	0.000	6.995f	0	102861	N.D.	49.816 #
33)	L7 AR-1260-3	8.568f	0.000	4062	0	1.371	N.D. #
36)	L8 AR-1262-1	8.568f	0.000	4062	0	1.007	N.D. #
40)	L8 AR-1262-5	0.000	8.721	0	50939	N.D.	36.639 #
44)	L9 AR-1268-4	0.000	8.721	0	50939	N.D.	31.062 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO122021\
Data File : PO083868.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 20 Dec 2021 14:53
Operator : AJ\MA
Sample : PB141553BL
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 20 17:08:40 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO121521.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Dec 16 04:05:27 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

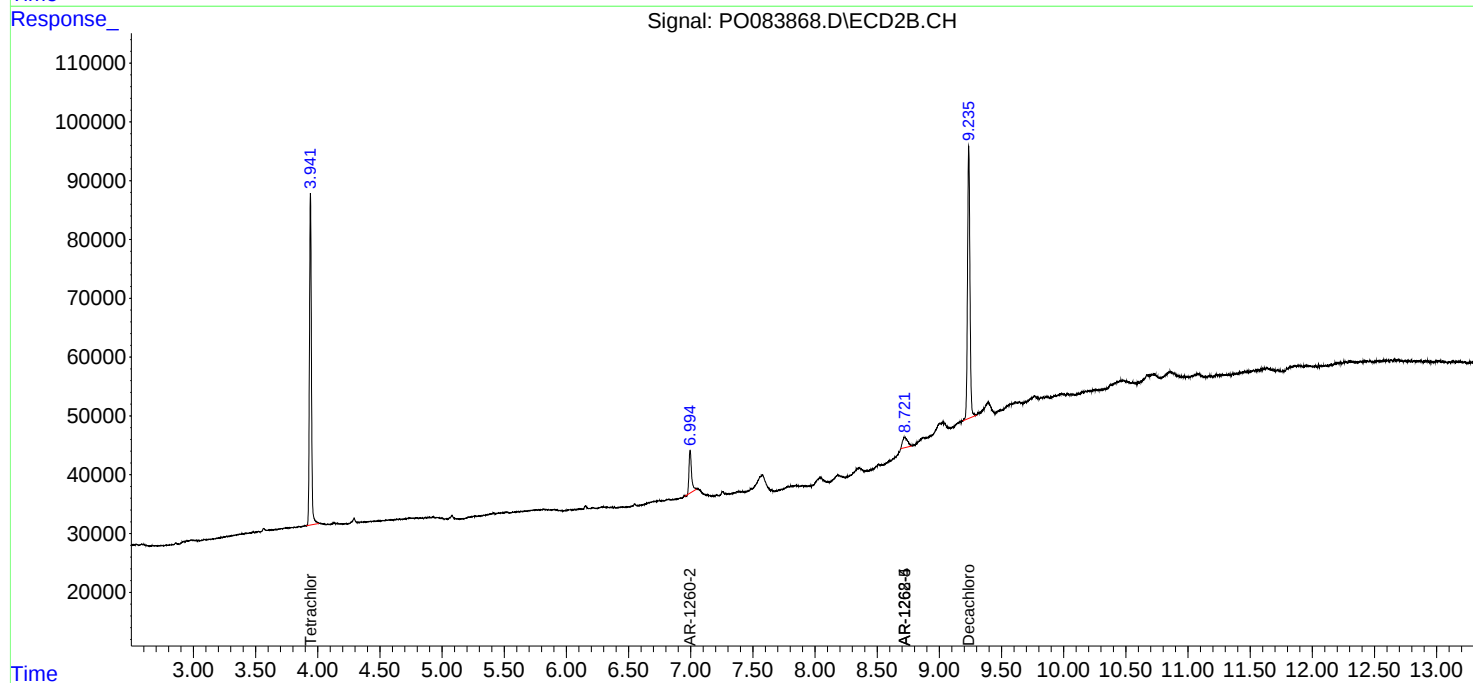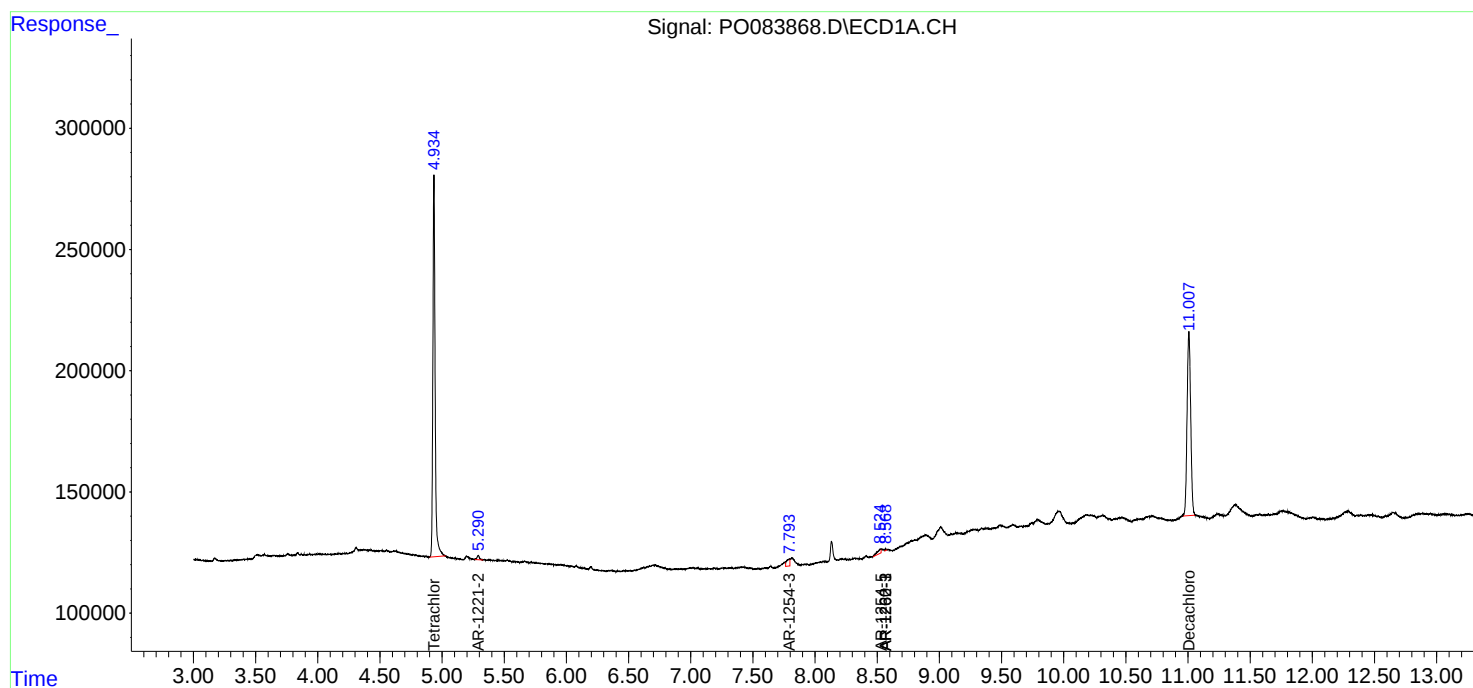


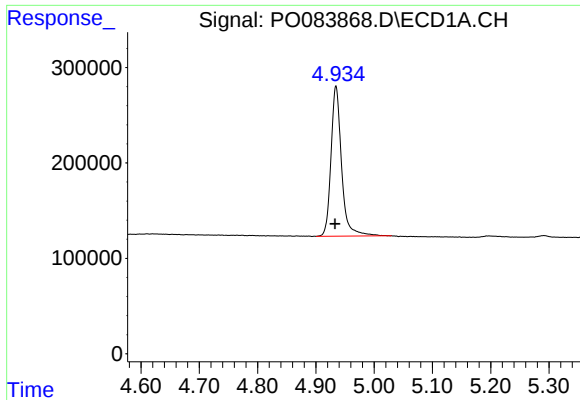

#1 Tetrachloro-m-xylene


R.T.: 4.935 min
Delta R.T.: 0.002 min
Response: 1982394
Conc: 20.81 ng/ml

Instrument :
ECD_O
ClientSampleId :

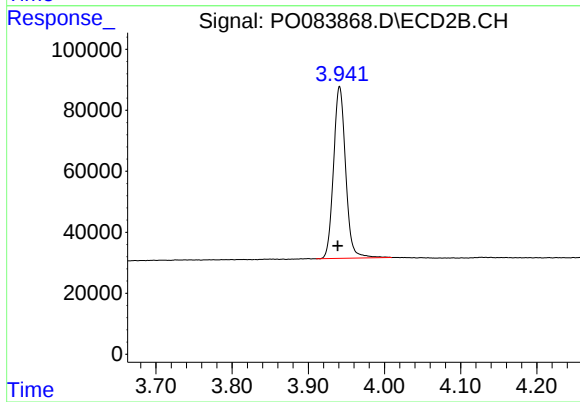


#1 Tetrachloro-m-xylene

R.T.: 3.941 min
Delta R.T.: 0.003 min
Response: 622168
Conc: 21.21 ng/ml

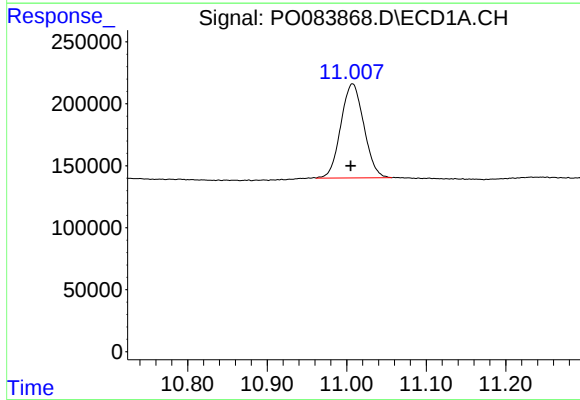


#2 Decachlorobiphenyl

R.T.: 11.007 min
Delta R.T.: 0.002 min
Response: 1529593
Conc: 22.33 ng/ml

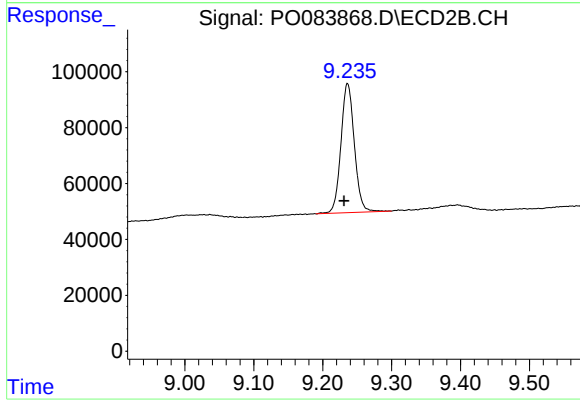

#2 Decachlorobiphenyl


R.T.: 9.236 min
Delta R.T.: 0.005 min
Response: 625573
Conc: 22.28 ng/ml

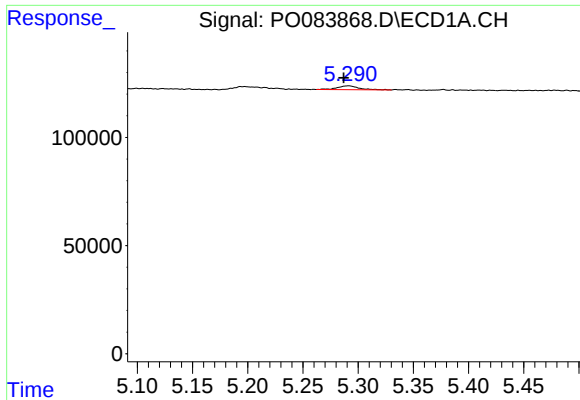

#9 AR-1221-2


R.T.: 5.291 min
Delta R.T.: 0.004 min
Response: 23510
Conc: 32.90 ng/ml

Instrument :
ECD_O
ClientSampleId :

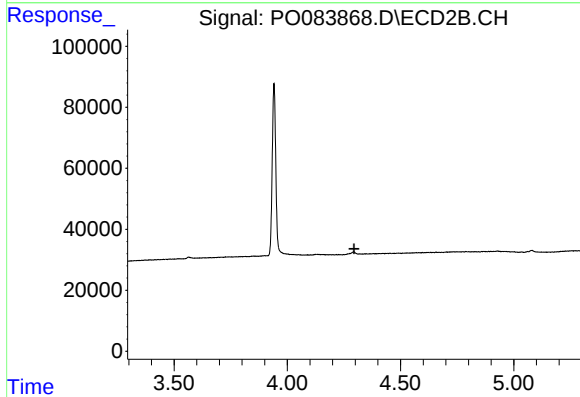


#9 AR-1221-2

R.T.: 0.000 min
Exp R.T. : 4.294 min
Response: 0
Conc: N.D.

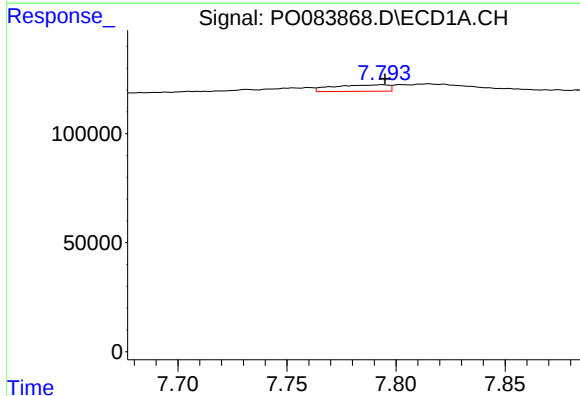


#28 AR-1254-3

R.T.: 7.794 min
Delta R.T.: -0.001 min
Response: 52051
Conc: 11.16 ng/ml

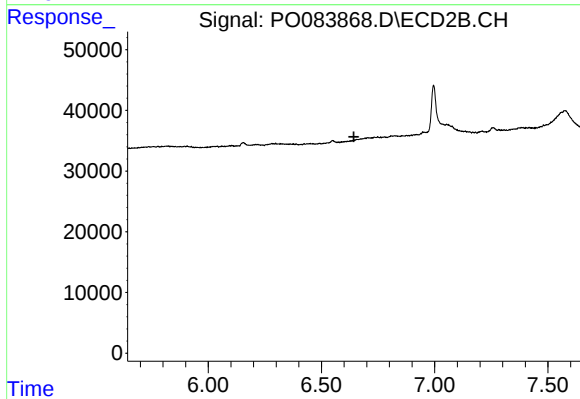

#28 AR-1254-3


R.T.: 0.000 min
Exp R.T. : 6.643 min
Response: 0
Conc: N.D.

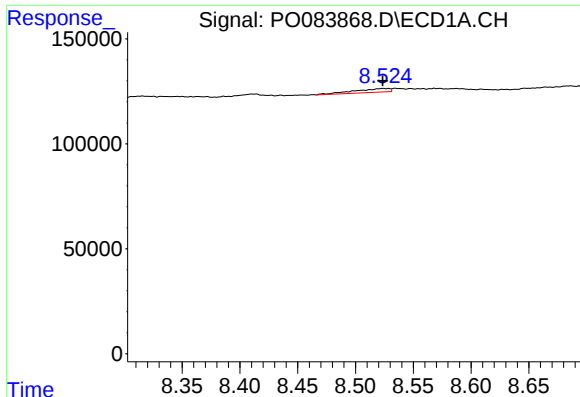

#30 AR-1254-5


R.T.: 8.524 min
Delta R.T.: 0.000 min
Response: 38469
Conc: 10.79 ng/ml

Instrument :
ECD_O
ClientSampleId :

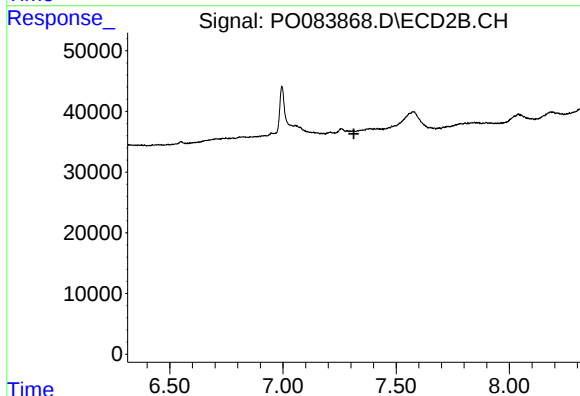


#30 AR-1254-5

R.T.: 0.000 min
Exp R.T. : 7.313 min
Response: 0
Conc: N.D.

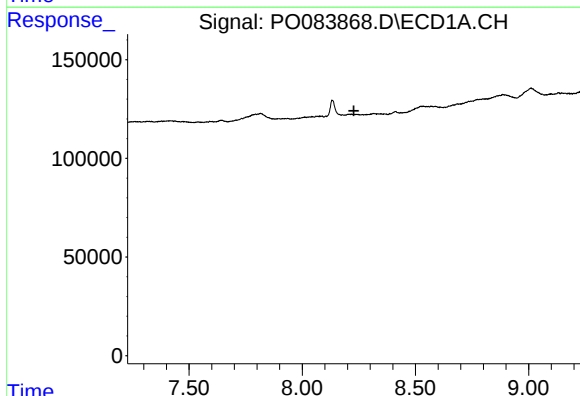


#32 AR-1260-2

R.T.: 0.000 min
Exp R.T. : 8.228 min
Response: 0
Conc: N.D.

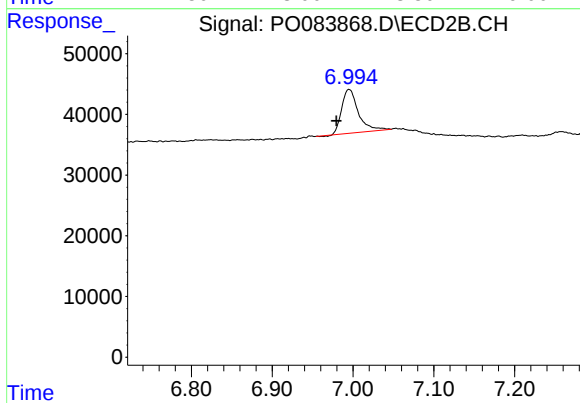

#32 AR-1260-2


R.T.: 6.995 min
Delta R.T.: 0.016 min
Response: 102861
Conc: 49.82 ng/ml

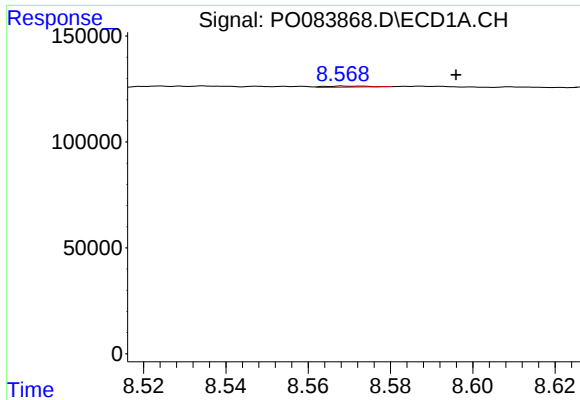

#33 AR-1260-3


R.T.: 8.568 min
Delta R.T.: -0.028 min
Response: 4062
Conc: 1.37 ng/ml

Instrument :
ECD_O
ClientSampleId :

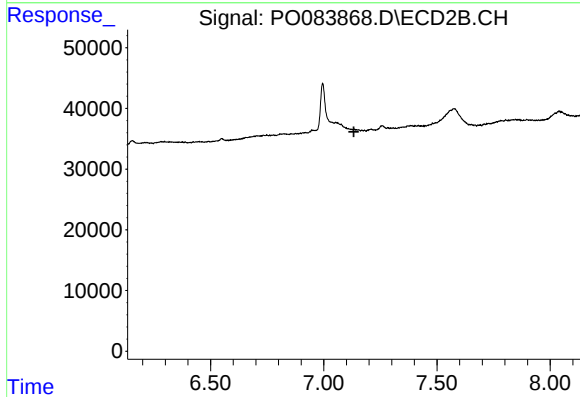


#33 AR-1260-3

R.T.: 0.000 min
Exp R.T. : 7.133 min
Response: 0
Conc: N.D.

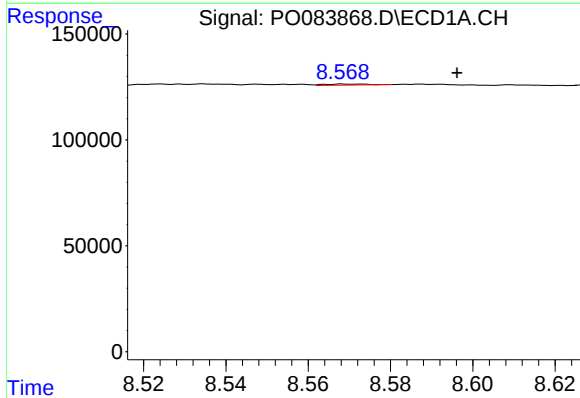


#36 AR-1262-1

R.T.: 8.568 min
Delta R.T.: -0.028 min
Response: 4062
Conc: 1.01 ng/ml

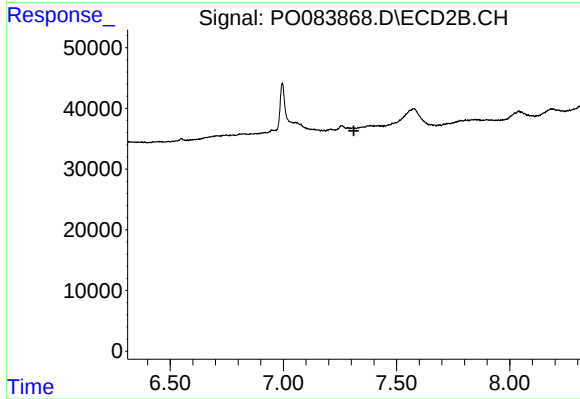

#36 AR-1262-1


R.T.: 0.000 min
Exp R.T. : 7.312 min
Response: 0
Conc: N.D.

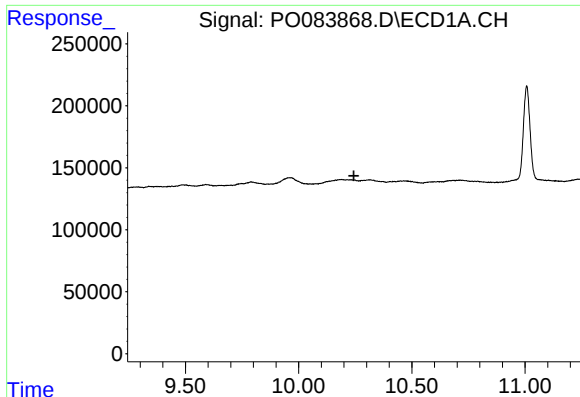

#40 AR-1262-5


R.T.: 0.000 min
Exp R.T. : 10.244 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :

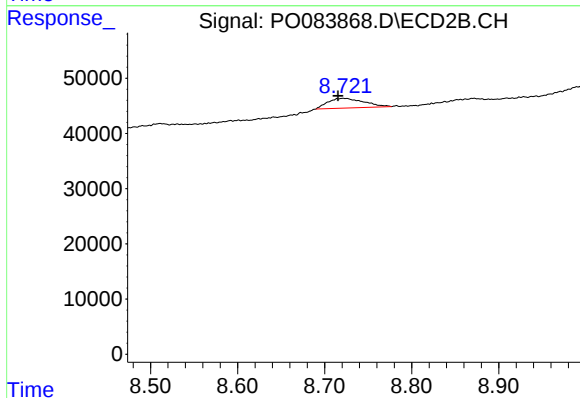


#40 AR-1262-5

R.T.: 8.721 min
Delta R.T.: 0.005 min
Response: 50939
Conc: 36.64 ng/ml

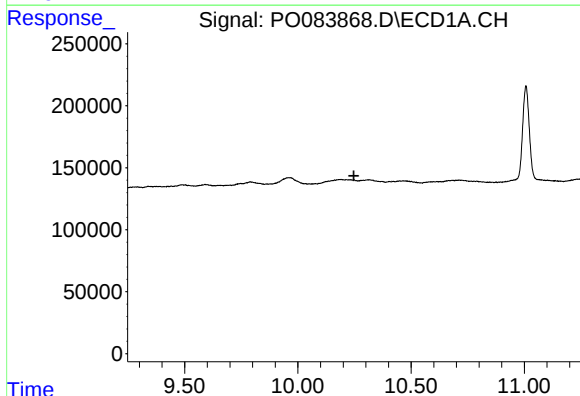

#44 AR-1268-4

R.T.: 0.000 min
Exp R.T. : 10.247 min
Response: 0
Conc: N.D.

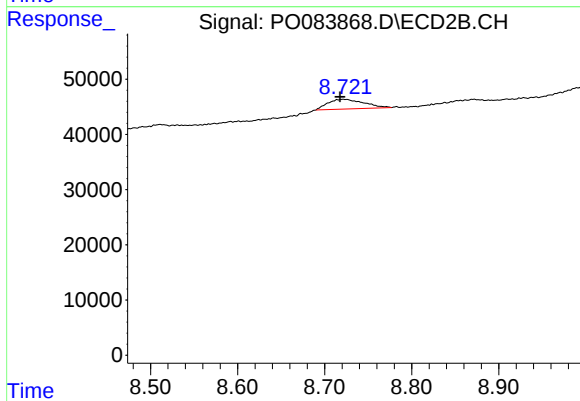

#44 AR-1268-4

R.T.: 8.721 min
Delta R.T.: 0.003 min
Response: 50939
Conc: 31.06 ng/ml