

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO122022\
 Data File : PO091550.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Dec 2022 19:45
 Operator : YP/AJ
 Sample : N6101-09 10X
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 KZZ178J-2-1

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 12/21/2022
 Supervised By :Ankita Jodhani 12/21/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 20 20:43:05 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO112522.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Nov 28 11:25:59 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.294	3.470	5126102	1655160	1.516	1.577
2) SA Decachlor...	10.035	8.467	5092396	1862905	1.917	1.919m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO122022\
Data File : PO091550.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Dec 2022 19:45
Operator : YP/AJ
Sample : N6101-09 10X
Misc :
ALS Vial : 17 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
KZZ178J-2-1


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 12/21/2022
Supervised By :Ankita Jodhani 12/21/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 20 20:43:05 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO112522.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Nov 28 11:25:59 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

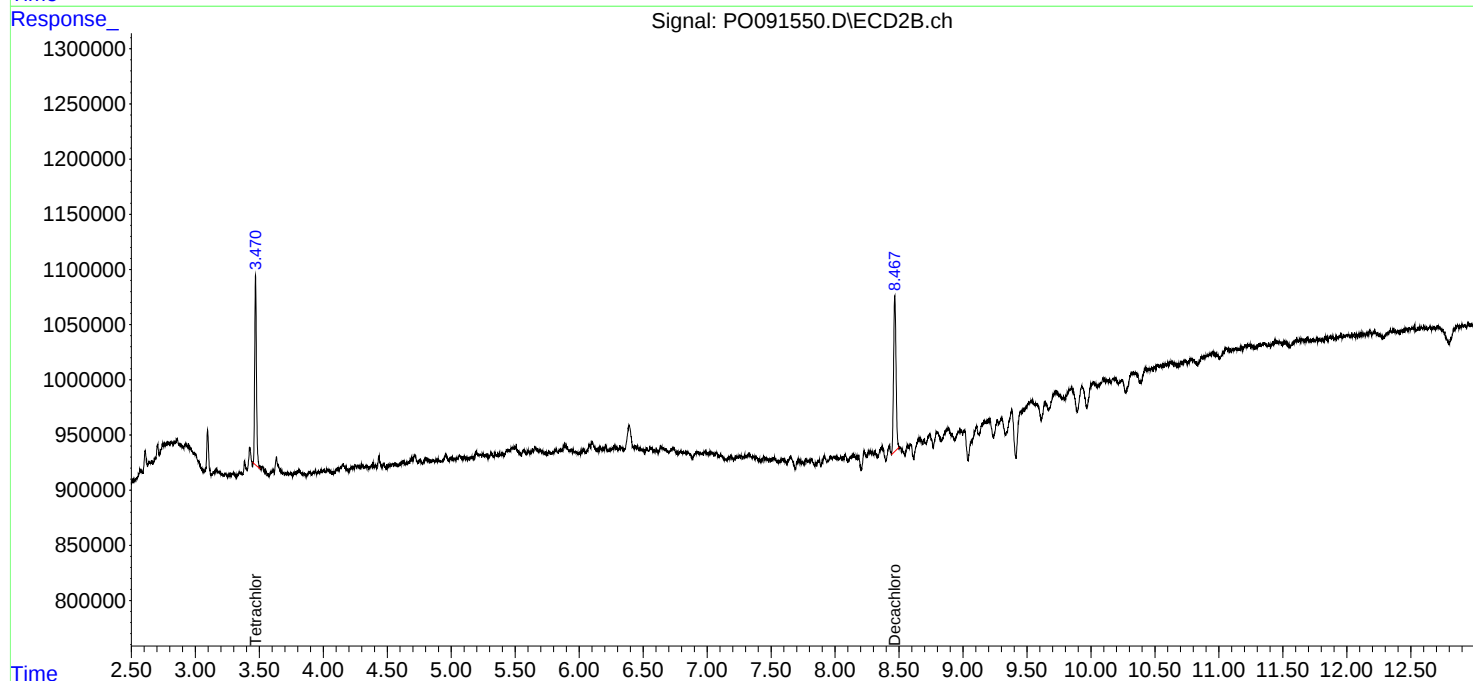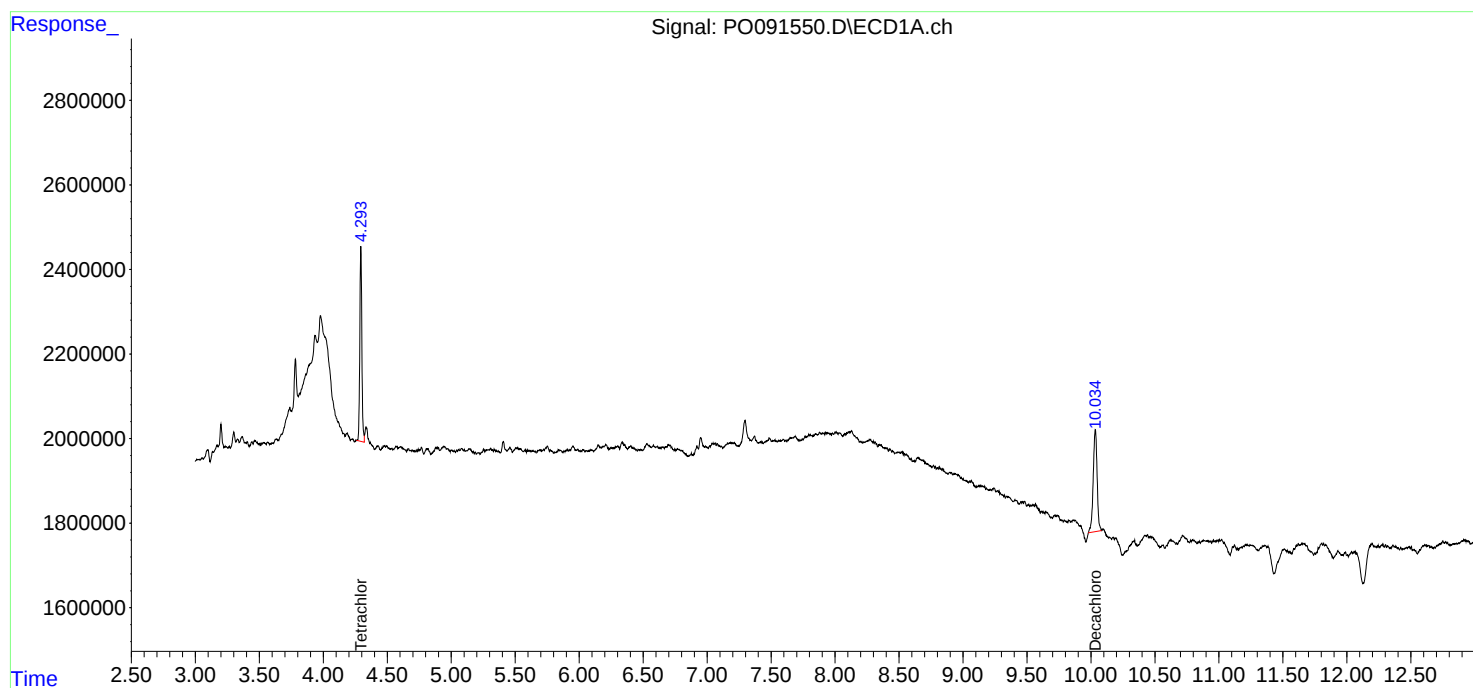

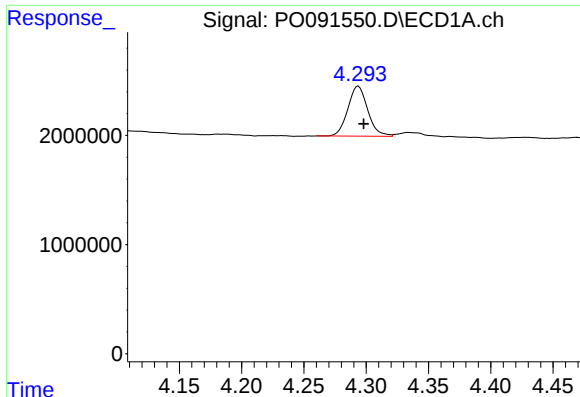


#1 Tetrachloro-m-xylene

R.T.: 4.294 min
Delta R.T.: -0.004 min
Response: 5126102
Conc: 1.52 ng/ml

Instrument :
ECD_O
ClientSampleId :
KZZ178J-2-1


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 12/21/2022
Supervised By :Ankita Jodhani 12/21/2022

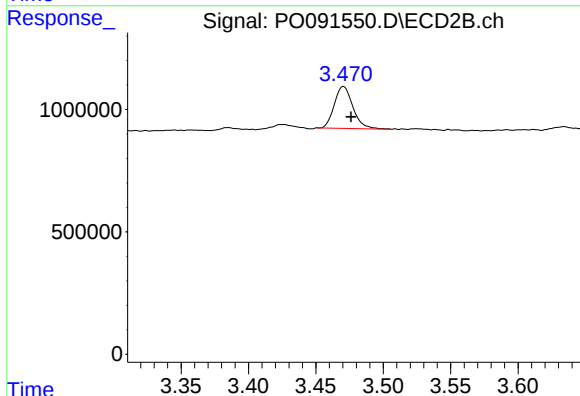


#1 Tetrachloro-m-xylene

R.T.: 3.470 min
Delta R.T.: -0.006 min
Response: 1655160
Conc: 1.58 ng/ml

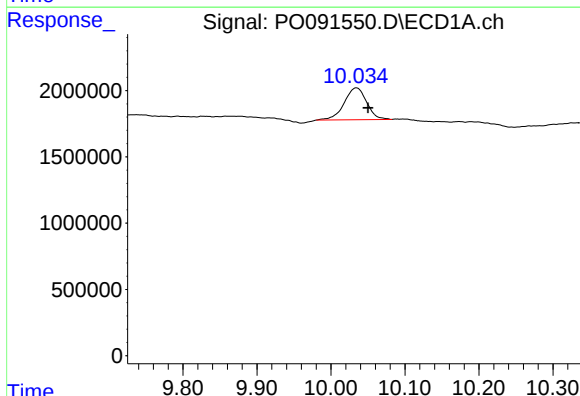

#2 Decachlorobiphenyl

R.T.: 10.035 min
Delta R.T.: -0.015 min
Response: 5092396
Conc: 1.92 ng/ml

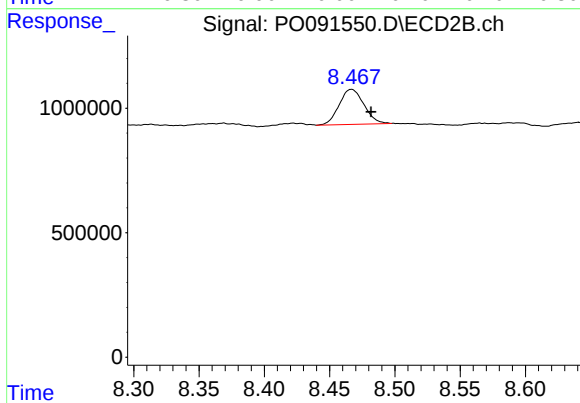

#2 Decachlorobiphenyl

R.T.: 8.467 min
Delta R.T.: -0.015 min
Response: 1862905
Conc: 1.92 ng/ml m