

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO122022\
 Data File : PO091556.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Dec 2022 21:28
 Operator : YP/AJ
 Sample : N6111-03 10X
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 BC274770-2-1

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 12/21/2022
 Supervised By :Ankita Jodhani 12/21/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 20 23:32:02 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO112522.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Nov 28 11:25:59 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.293	3.470	5540148	1949864	1.639	1.858
2) SA Decachlor...	10.034	8.467	5569577	2207362	2.097	2.274m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO122022\
Data File : PO091556.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Dec 2022 21:28
Operator : YP/AJ
Sample : N6111-03 10X
Misc :
ALS Vial : 23 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
BC274770-2-1


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 12/21/2022
Supervised By :Ankita Jodhani 12/21/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 20 23:32:02 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO112522.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Nov 28 11:25:59 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

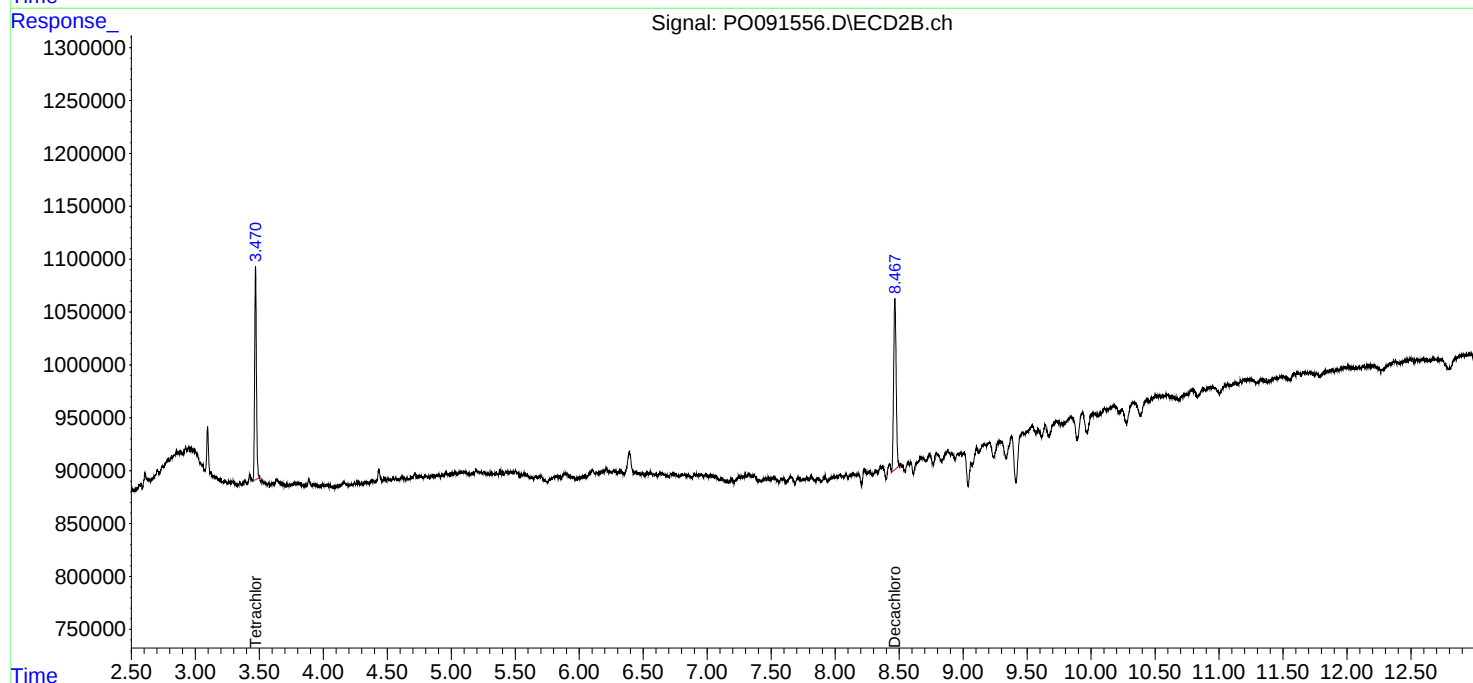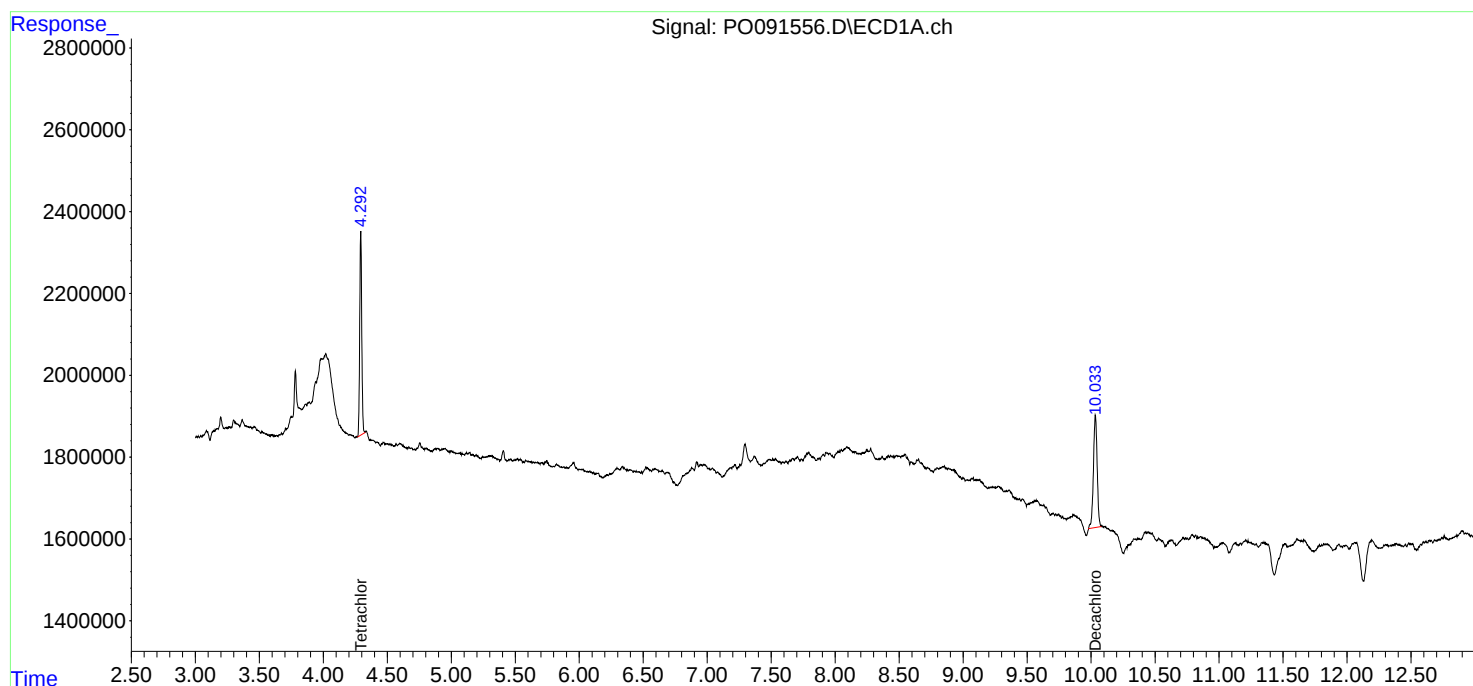

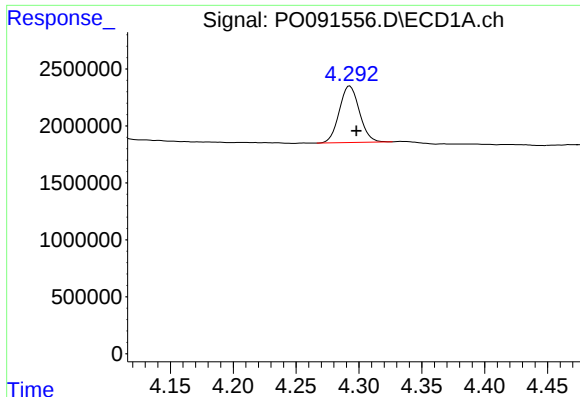


#1 Tetrachloro-m-xylene

R.T.: 4.293 min
Delta R.T.: -0.005 min
Response: 5540148
Conc: 1.64 ng/ml

Instrument :
ECD_O
ClientSampleId :
BC274770-2-1


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 12/21/2022
Supervised By :Ankita Jodhani 12/21/2022

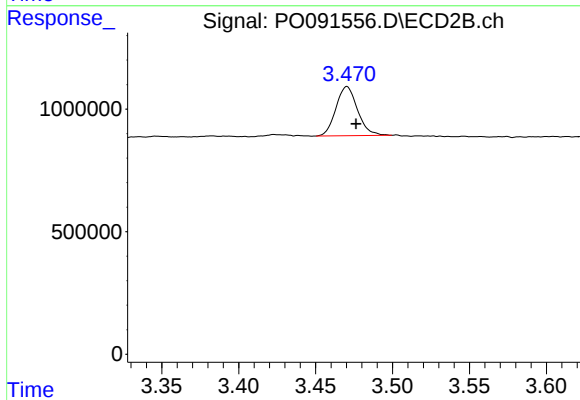


#1 Tetrachloro-m-xylene

R.T.: 3.470 min
Delta R.T.: -0.006 min
Response: 1949864
Conc: 1.86 ng/ml

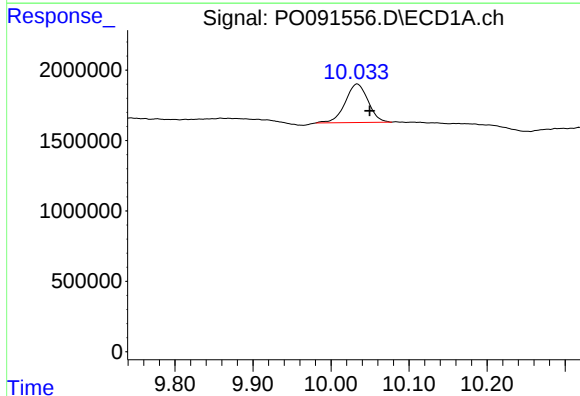

#2 Decachlorobiphenyl

R.T.: 10.034 min
Delta R.T.: -0.016 min
Response: 5569577
Conc: 2.10 ng/ml

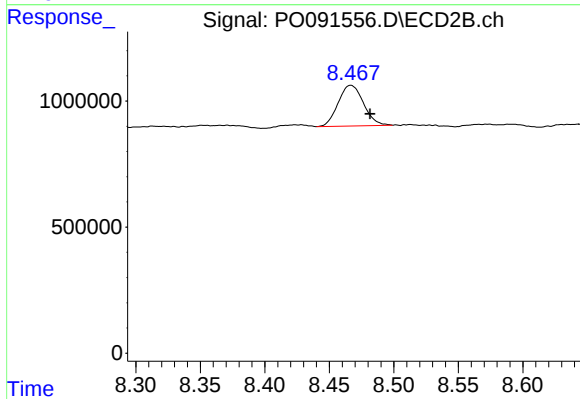

#2 Decachlorobiphenyl

R.T.: 8.467 min
Delta R.T.: -0.015 min
Response: 2207362
Conc: 2.27 ng/ml m