



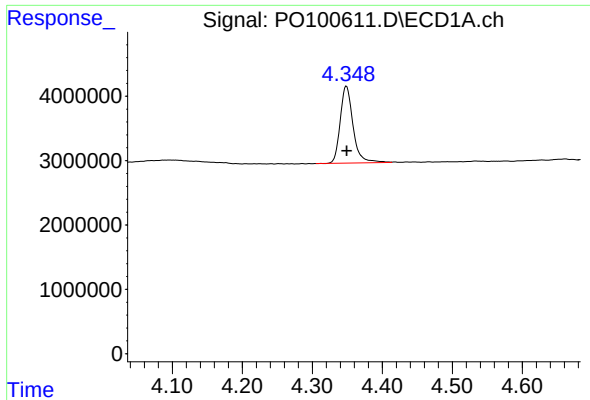

#1 Tetrachloro-m-xylene

R.T.: 4.349 min
Delta R.T.: 0.000 min
Response: 15217656
Conc: 4.64 ng/ml

Instrument :
ECD_O
ClientSampleId :

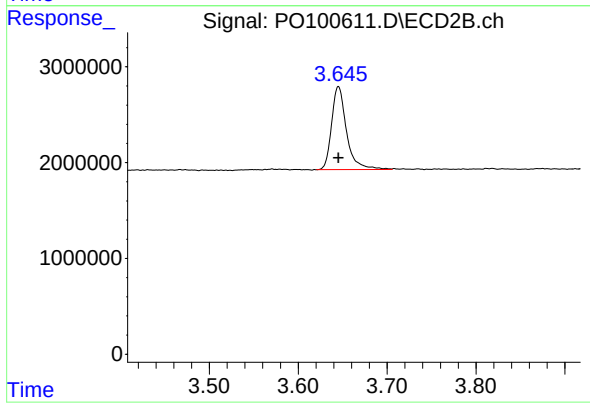

#1 Tetrachloro-m-xylene

R.T.: 3.645 min
Delta R.T.: 0.000 min
Response: 10118106
Conc: 4.71 ng/ml