

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\PO122024\
 Data File : PO108731.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Dec 2024 22:38
 Operator : YP/AJ
 Sample : P5356-01
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 ECD_0
 ClientSampleId :
 STAND-PIPE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 21 01:27:51 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\PO120624.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Dec 07 05:58:15 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.707	3.704	138.7E6	86780903	15.943	17.119
2)	SA Decachlor...	8.775	8.725	73232484	45869943	10.026	11.838
Target Compounds							
3)	L1 AR-1016-1	0.000	4.831	0	1182334	N.D.	7.368 #
4)	L1 AR-1016-2	0.000	4.831	0	1182334	N.D.	5.324 #
5)	L1 AR-1016-3	0.000	5.000	0	336841	N.D.	2.677 #
6)	L1 AR-1016-4	0.000	5.040	0	479402	N.D.	4.574 #
7)	L1 AR-1016-5	5.334f	5.238	12000197	3245618	47.682	24.004 #
8)	L2 AR-1221-1	3.981f	3.944	5646246	84450	49.903	1.359 #
9)	L2 AR-1221-2	4.008	4.003	2263997	1416688	26.107	29.860
10)	L2 AR-1221-3	0.000	4.078	0	378984	N.D.	2.696 #
11)	L3 AR-1232-1	0.000	4.078	0	378984	N.D.	3.382 #
12)	L3 AR-1232-2	0.000	4.831	0	1182334	N.D.	11.180 #
13)	L3 AR-1232-3	0.000	5.000	0	336841	N.D.	5.582 #
14)	L3 AR-1232-4	0.000	5.069	0	470536	N.D.	8.470 #
15)	L3 AR-1232-5	0.000	5.238	0	3245618	N.D.	56.371 #
16)	L4 AR-1242-1	0.000	4.831	0	1182334	N.D.	8.708 #
17)	L4 AR-1242-2	0.000	4.831	0	1182334	N.D.	6.375 #
18)	L4 AR-1242-3	0.000	5.000	0	336841	N.D.	3.196 #
19)	L4 AR-1242-4	0.000	5.069	0	470536	N.D.	4.384 #
20)	L4 AR-1242-5	0.000	5.604	0	3345208	N.D.	26.465 #
21)	L5 AR-1248-1	0.000	4.831	0	1182334	N.D.	11.248 #
22)	L5 AR-1248-2	0.000	5.040	0	479402	N.D.	3.210 #
23)	L5 AR-1248-3	0.000	5.069	0	470536	N.D.	2.970 #
24)	L5 AR-1248-4	0.000	5.238	0	3245618	N.D.	17.779 #
25)	L5 AR-1248-5	0.000	5.637	0	3373776	N.D.	19.212 #
26)	L6 AR-1254-1	0.000	5.604	0	3345208	N.D.	12.352 #
27)	L6 AR-1254-2	0.000	5.736	0	1542326	N.D.	6.426 #
28)	L6 AR-1254-3	6.108f	6.152	1949804	1049546	2.708	2.795
29)	L6 AR-1254-4	6.437	6.405	-2940577	2295517	N.D.	10.546 #
30)	L6 AR-1254-5	0.000	6.789	0	3121994	N.D.	9.673 #
31)	L7 AR-1260-1	0.000	6.293	0	1748756	N.D.	7.472 #
32)	L7 AR-1260-2	6.472	6.462	3235515	3692095	5.822	13.159 #
33)	L7 AR-1260-3	0.000	6.618	0	3181632	N.D.	12.071 #
34)	L7 AR-1260-4	0.000	7.104	0	1754150	N.D.	8.245 #
35)	L7 AR-1260-5	0.000	7.329	0	1333601	N.D.	2.756 #
36)	L8 AR-1262-1	0.000	6.826	0	1388147	N.D.	4.107 #
37)	L8 AR-1262-2	0.000	7.329	0	1333601	N.D.	2.332 #
38)	L8 AR-1262-3	0.000	7.647	0	105135	N.D.	0.468 #
39)	L8 AR-1262-4	0.000	7.674	0	177111	N.D.	0.432 #
40)	L8 AR-1262-5	0.000	8.182	0	57996	N.D.	0.314 #
41)	L9 AR-1268-1	0.000	7.647	0	105135	N.D.	0.163 #

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO122024\
Data File : PO108731.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Dec 2024 22:38
Operator : YP/AJ
Sample : P5356-01
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
STAND-PIPE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 21 01:27:51 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO120624.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Dec 07 05:58:15 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
42)	L9 AR-1268-2	0.000	7.674	0	177111	N.D.	0.305 #
43)	L9 AR-1268-3	0.000	7.915	0	23452	N.D.	0.047 #
44)	L9 AR-1268-4	0.000	8.182	0	57996	N.D.	0.286 #
45)	L9 AR-1268-5	0.000	8.464	0	218469	N.D.	0.147 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO122024\
Data File : PO108731.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Dec 2024 22:38
Operator : YP/AJ
Sample : P5356-01
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
STAND-PIPE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 21 01:27:51 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO120624.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Dec 07 05:58:15 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

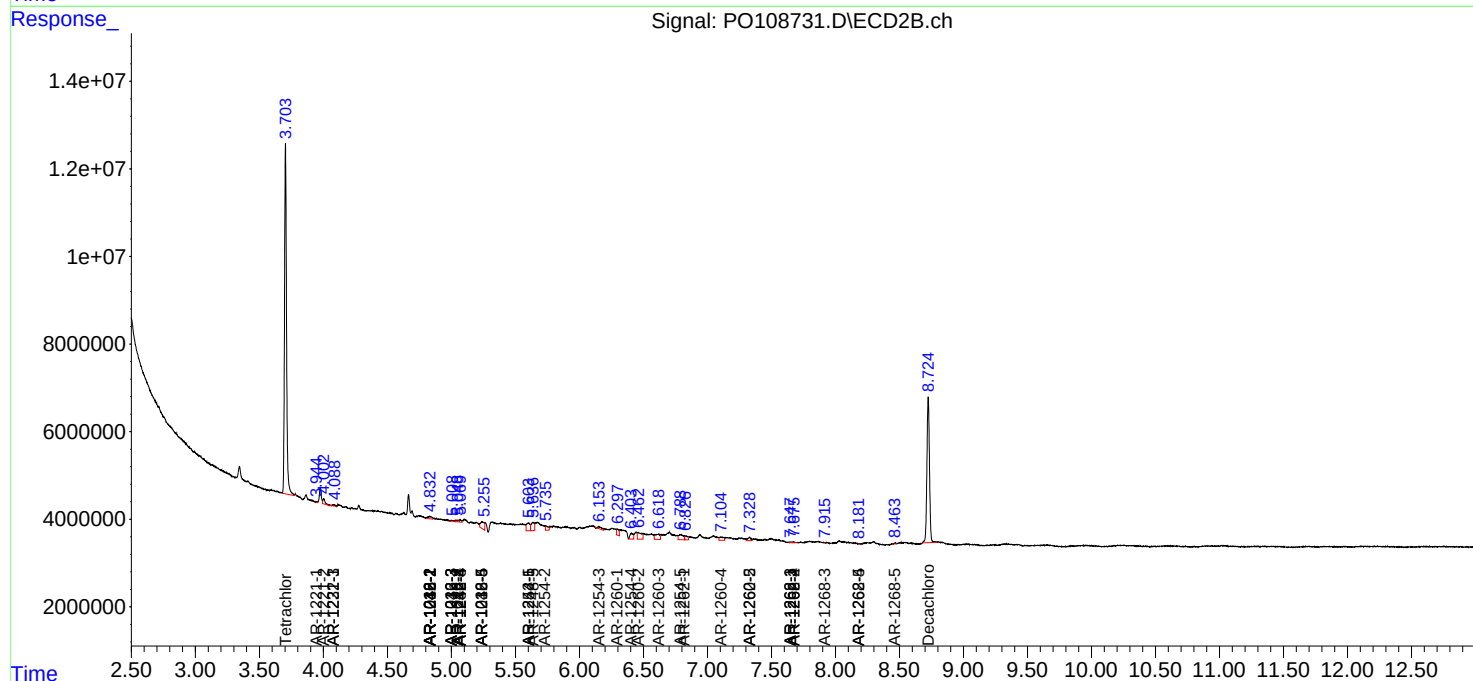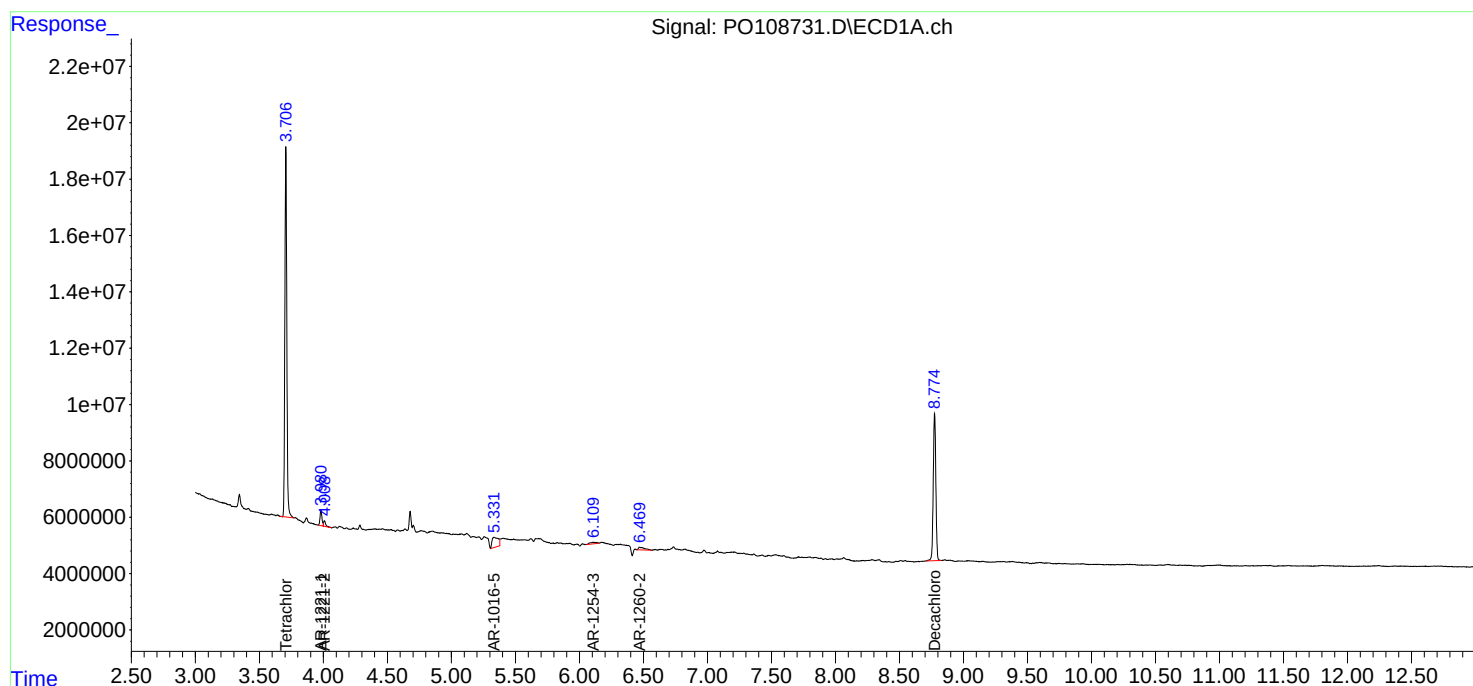


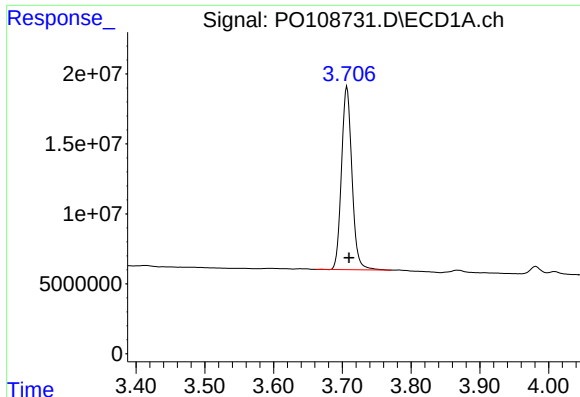

#1 Tetrachloro-m-xylene


R.T.: 3.707 min
Delta R.T.: -0.003 min
Response: 138706455
Conc: 15.94 ng/ml

Instrument :
ECD_O
ClientSampleId :
STAND-PIPE

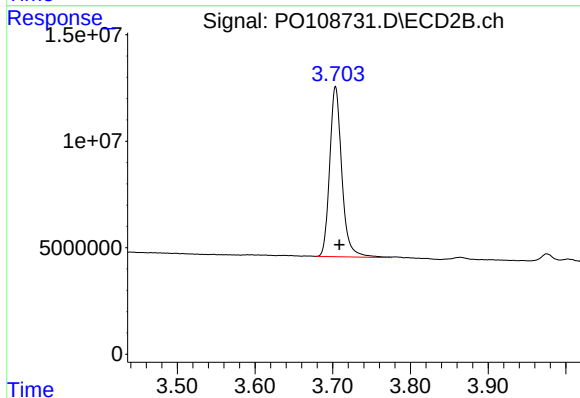


#1 Tetrachloro-m-xylene

R.T.: 3.704 min
Delta R.T.: -0.005 min
Response: 86780903
Conc: 17.12 ng/ml

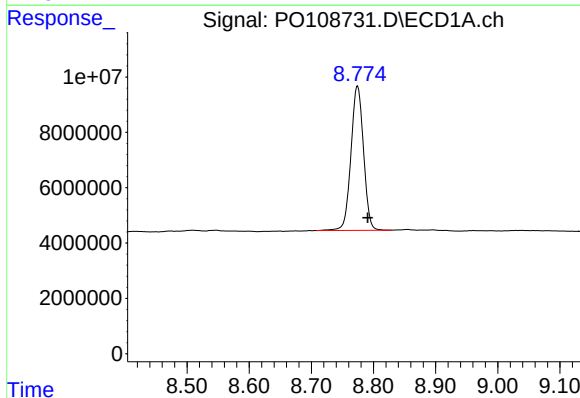


#2 Decachlorobiphenyl

R.T.: 8.775 min
Delta R.T.: -0.016 min
Response: 73232484
Conc: 10.03 ng/ml

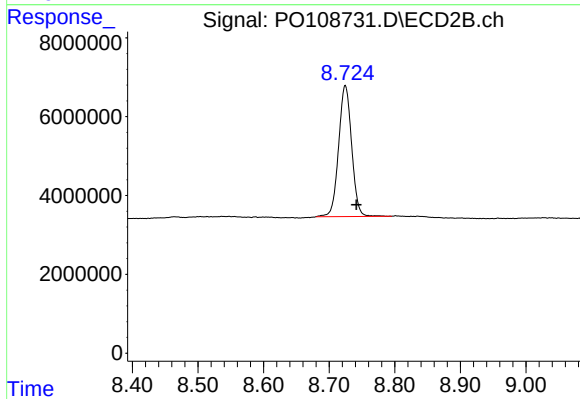

#2 Decachlorobiphenyl


R.T.: 8.725 min
Delta R.T.: -0.017 min
Response: 45869943
Conc: 11.84 ng/ml

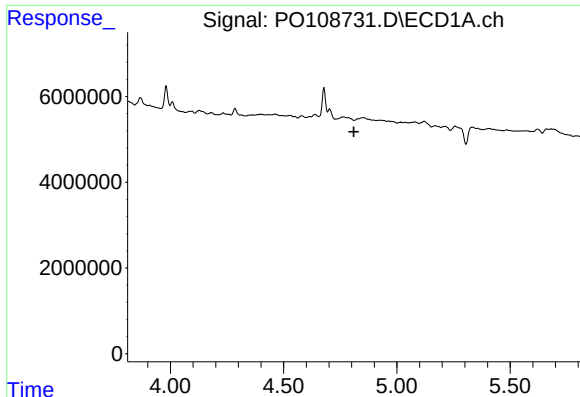

#3 AR-1016-1


R.T.: 0.000 min
Exp R.T.: 4.810 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
STAND-PIPE

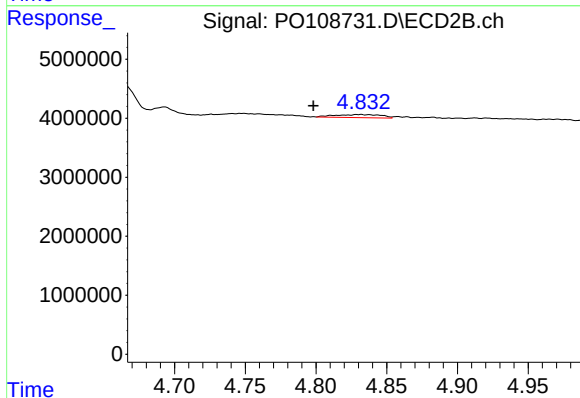


#3 AR-1016-1

R.T.: 4.831 min
Delta R.T.: 0.033 min
Response: 1182334
Conc: 7.37 ng/ml

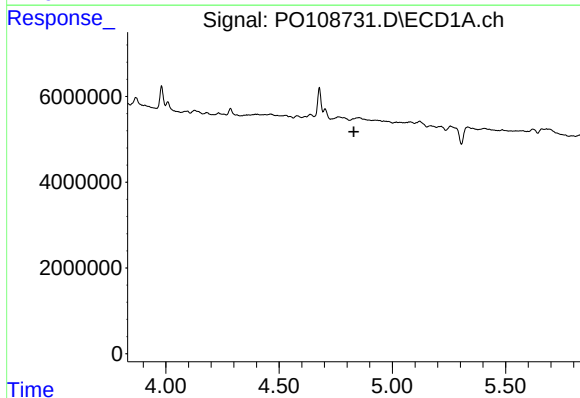


#4 AR-1016-2

R.T.: 0.000 min
Exp R.T.: 4.830 min
Response: 0
Conc: N.D.

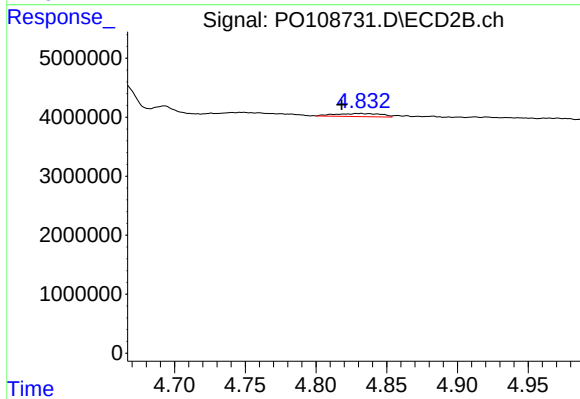

#4 AR-1016-2


R.T.: 4.831 min
Delta R.T.: 0.013 min
Response: 1182334
Conc: 5.32 ng/ml

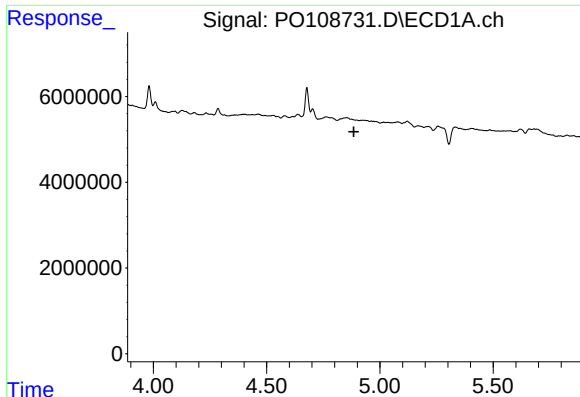

#5 AR-1016-3


R.T.: 0.000 min
Exp R.T.: 4.885 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
STAND-PIPE

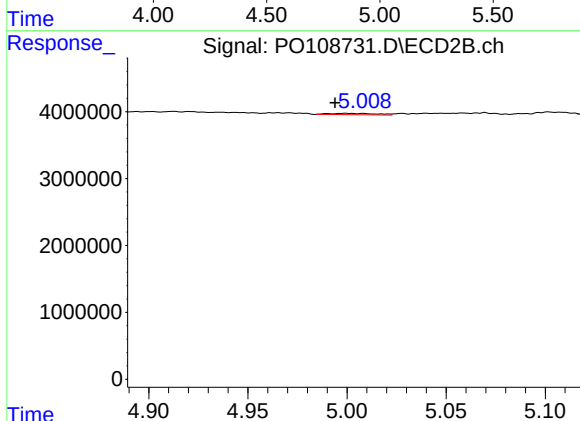


#5 AR-1016-3

R.T.: 5.000 min
Delta R.T.: 0.005 min
Response: 336841
Conc: 2.68 ng/ml

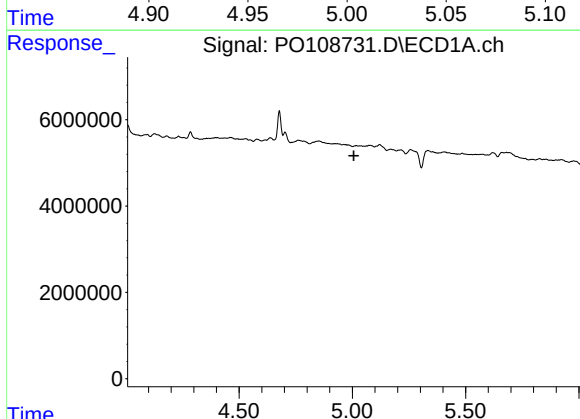


#6 AR-1016-4

R.T.: 0.000 min
Exp R.T.: 5.007 min
Response: 0
Conc: N.D.

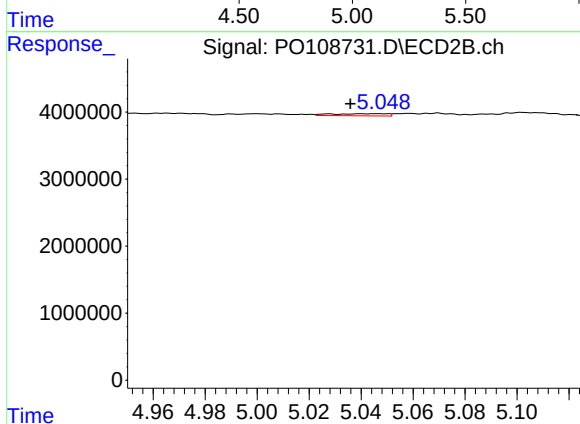

#6 AR-1016-4


R.T.: 5.040 min
Delta R.T.: 0.004 min
Response: 479402
Conc: 4.57 ng/ml

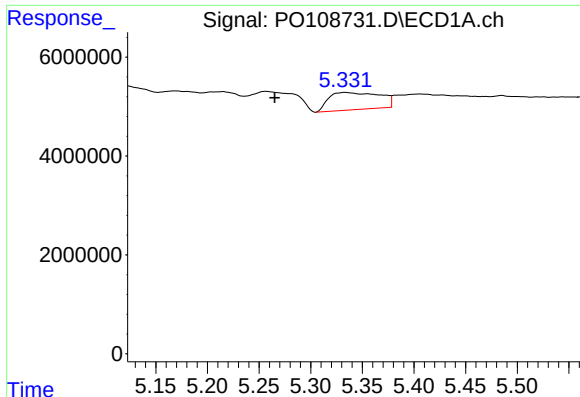

#7 AR-1016-5


R.T.: 5.334 min
Delta R.T.: 0.069 min
Response: 12000197
Conc: 47.68 ng/ml

Instrument :
ECD_O
ClientSampleId :
STAND-PIPE

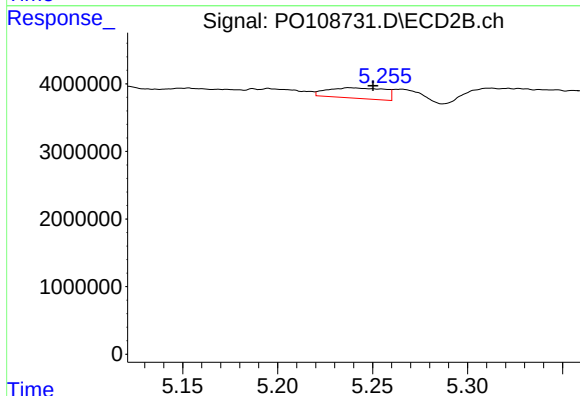


#7 AR-1016-5

R.T.: 5.238 min
Delta R.T.: -0.012 min
Response: 3245618
Conc: 24.00 ng/ml

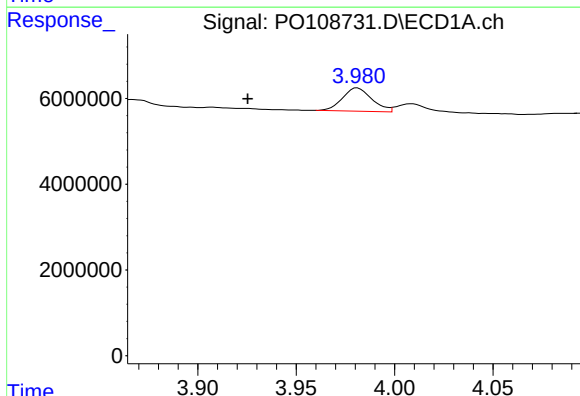


#8 AR-1221-1

R.T.: 3.981 min
Delta R.T.: 0.056 min
Response: 5646246
Conc: 49.90 ng/ml

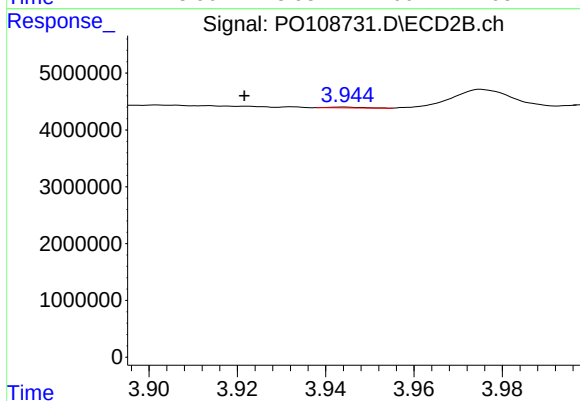

#8 AR-1221-1


R.T.: 3.944 min
Delta R.T.: 0.022 min
Response: 84450
Conc: 1.36 ng/ml

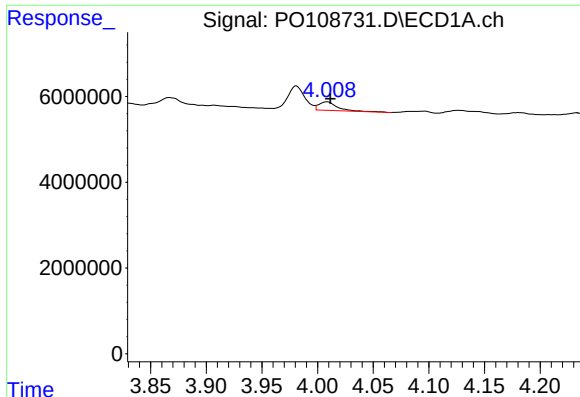

#9 AR-1221-2


R.T.: 4.008 min
Delta R.T.: -0.003 min
Response: 2263997
Conc: 26.11 ng/ml

Instrument :
ECD_O
ClientSampleId :
STAND-PIPE

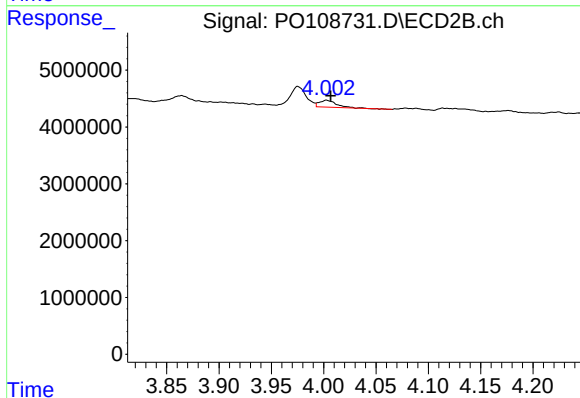


#9 AR-1221-2

R.T.: 4.003 min
Delta R.T.: -0.004 min
Response: 1416688
Conc: 29.86 ng/ml

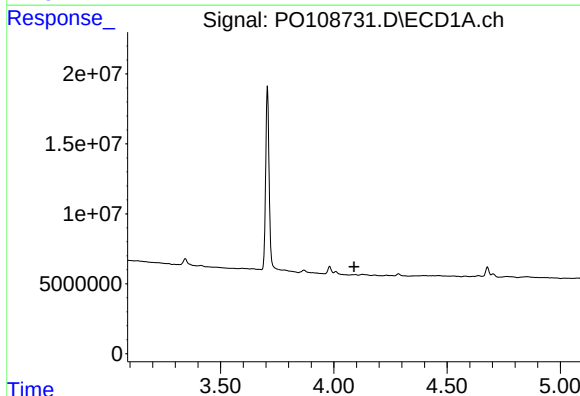


#10 AR-1221-3

R.T.: 0.000 min
Exp R.T. : 4.089 min
Response: 0
Conc: N.D.

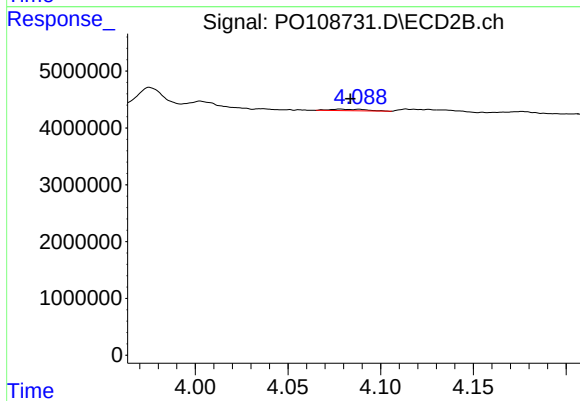

#10 AR-1221-3


R.T.: 4.078 min
Delta R.T.: -0.005 min
Response: 378984
Conc: 2.70 ng/ml

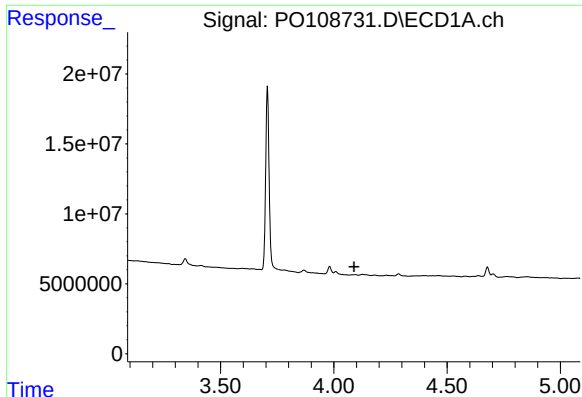

#11 AR-1232-1


R.T.: 0.000 min
Exp R.T.: 4.089 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
STAND-PIPE

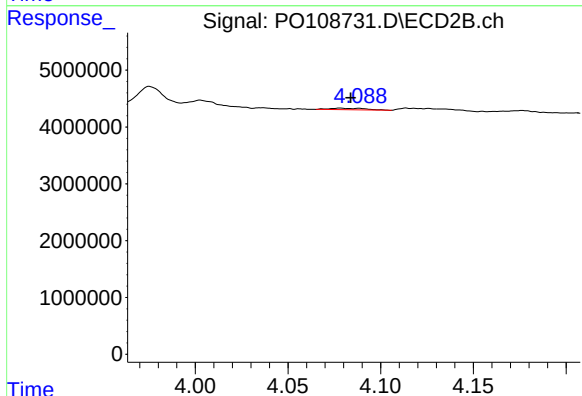


#11 AR-1232-1

R.T.: 4.078 min
Delta R.T.: -0.006 min
Response: 378984
Conc: 3.38 ng/ml

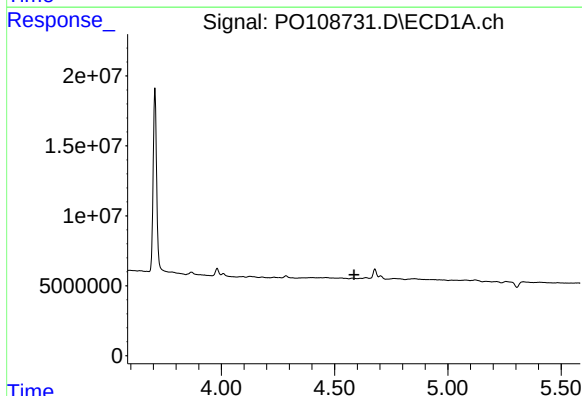


#12 AR-1232-2

R.T.: 0.000 min
Exp R.T.: 4.586 min
Response: 0
Conc: N.D.

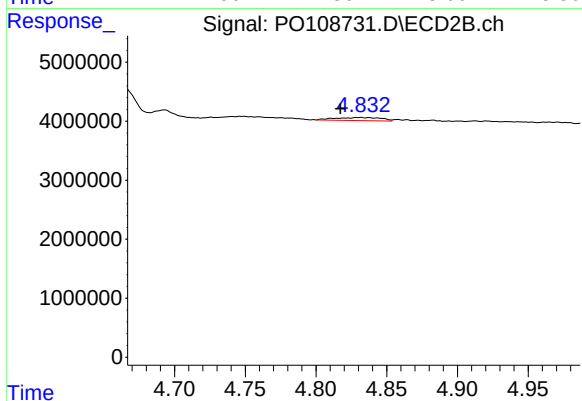

#12 AR-1232-2


R.T.: 4.831 min
Delta R.T.: 0.014 min
Response: 1182334
Conc: 11.18 ng/ml

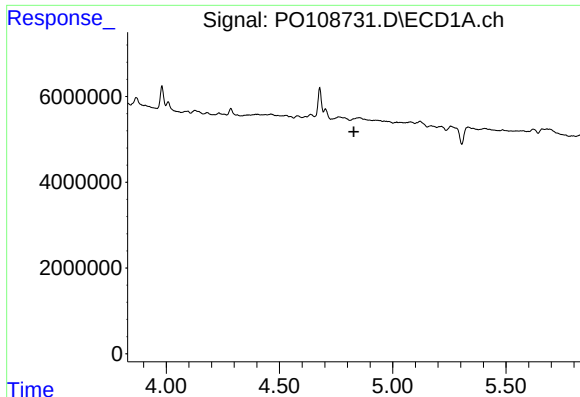

#13 AR-1232-3


R.T.: 0.000 min
Exp R.T.: 4.829 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
STAND-PIPE

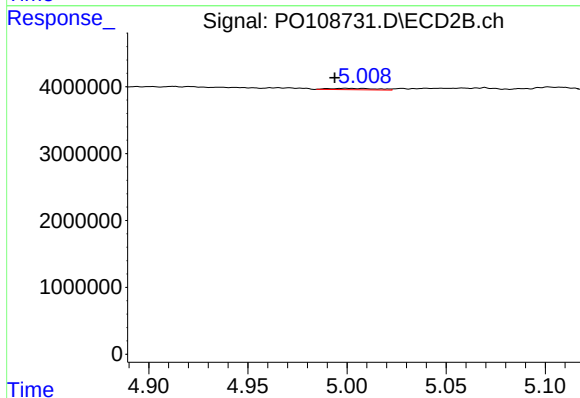


#13 AR-1232-3

R.T.: 5.000 min
Delta R.T.: 0.006 min
Response: 336841
Conc: 5.58 ng/ml

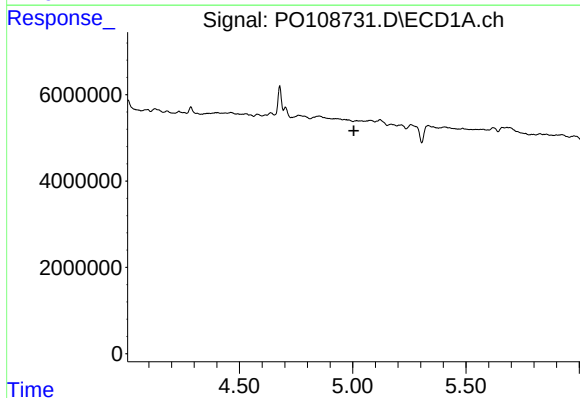


#14 AR-1232-4

R.T.: 0.000 min
Exp R.T.: 5.005 min
Response: 0
Conc: N.D.

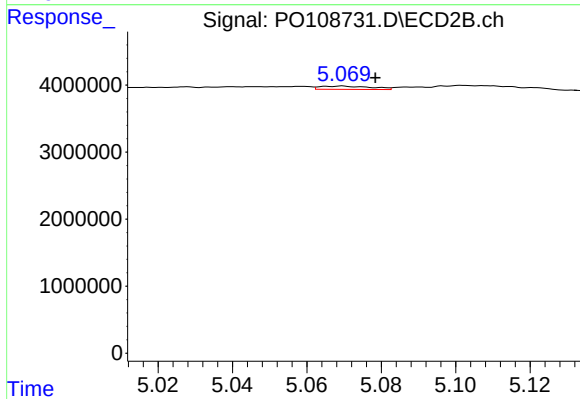

#14 AR-1232-4


R.T.: 5.069 min
Delta R.T.: -0.009 min
Response: 470536
Conc: 8.47 ng/ml

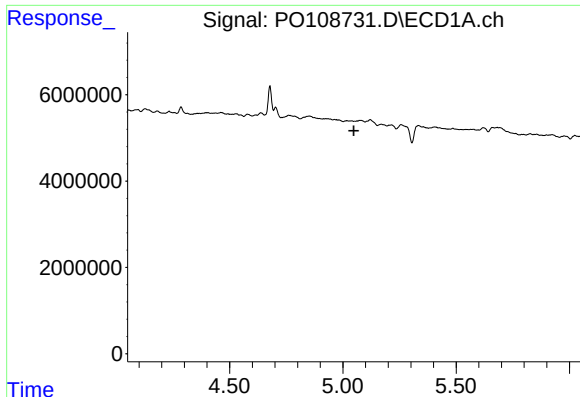

#15 AR-1232-5


R.T.: 0.000 min
Exp R.T.: 5.048 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
STAND-PIPE

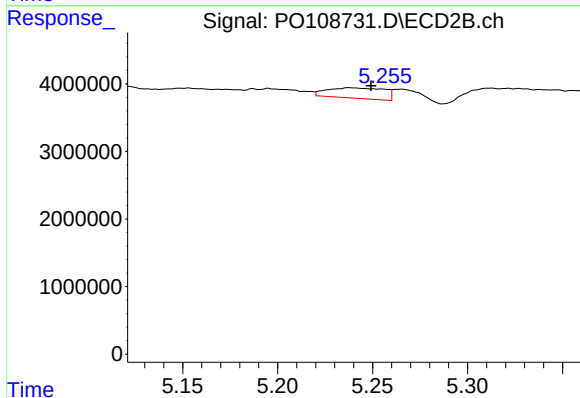


#15 AR-1232-5

R.T.: 5.238 min
Delta R.T.: -0.011 min
Response: 3245618
Conc: 56.37 ng/ml

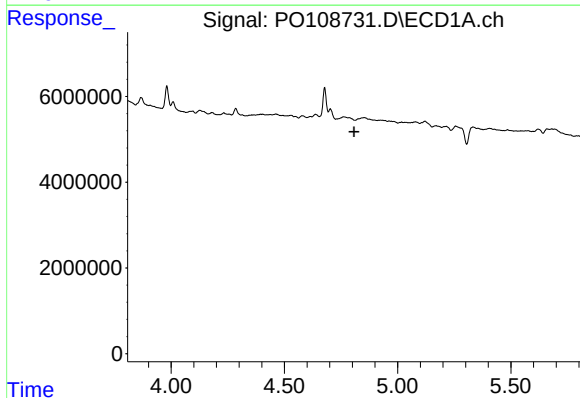


#16 AR-1242-1

R.T.: 0.000 min
Exp R.T.: 4.808 min
Response: 0
Conc: N.D.

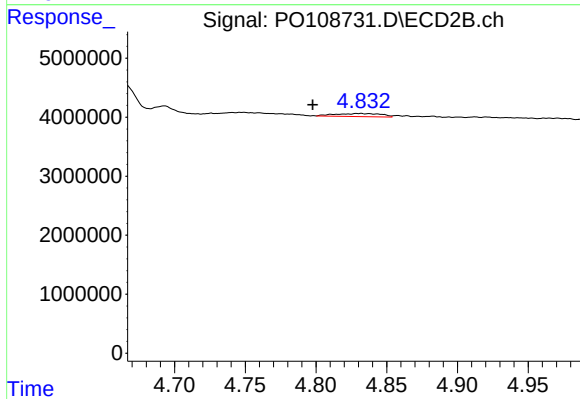

#16 AR-1242-1


R.T.: 4.831 min
Delta R.T.: 0.034 min
Response: 1182334
Conc: 8.71 ng/ml

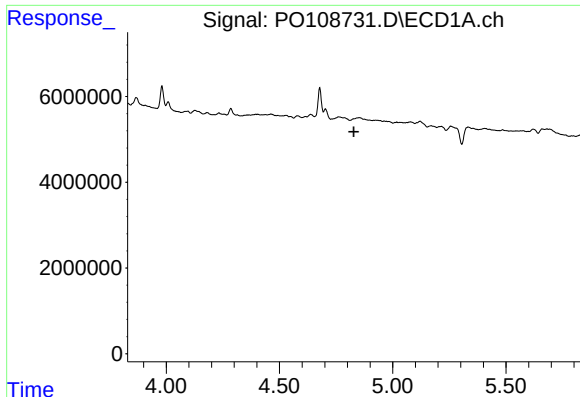

#17 AR-1242-2


R.T.: 0.000 min
Exp R.T.: 4.828 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
STAND-PIPE

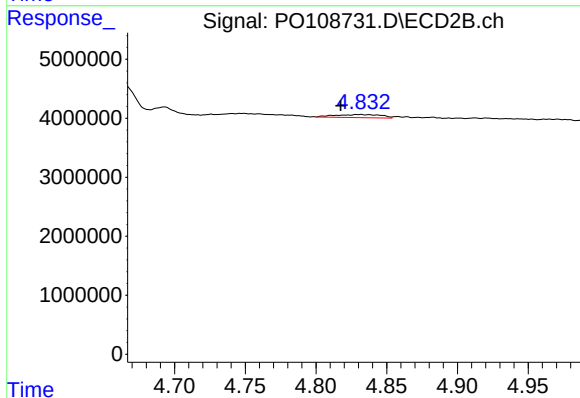


#17 AR-1242-2

R.T.: 4.831 min
Delta R.T.: 0.014 min
Response: 1182334
Conc: 6.38 ng/ml

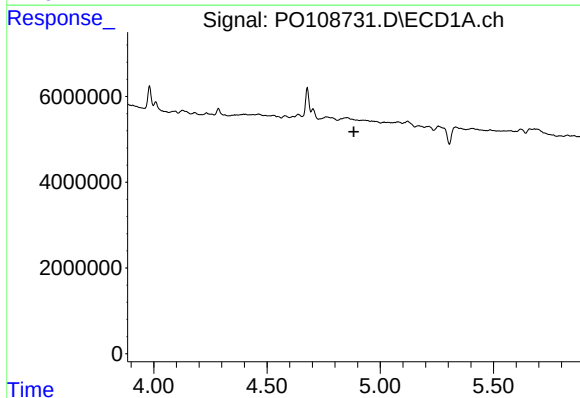


#18 AR-1242-3

R.T.: 0.000 min
Exp R.T.: 4.884 min
Response: 0
Conc: N.D.

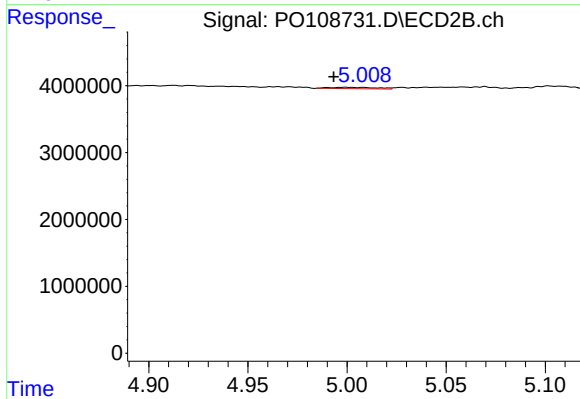

#18 AR-1242-3


R.T.: 5.000 min
Delta R.T.: 0.006 min
Response: 336841
Conc: 3.20 ng/ml

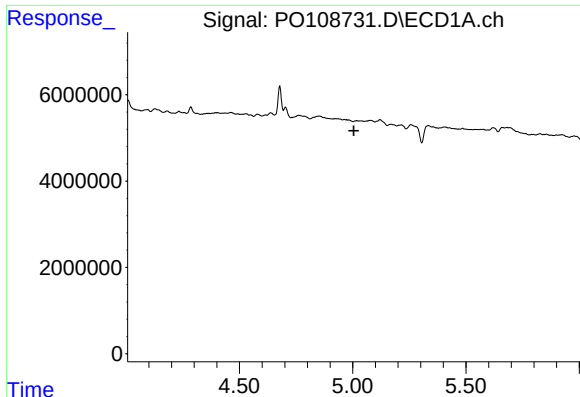

#19 AR-1242-4


R.T.: 0.000 min
Exp R.T.: 5.005 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
STAND-PIPE

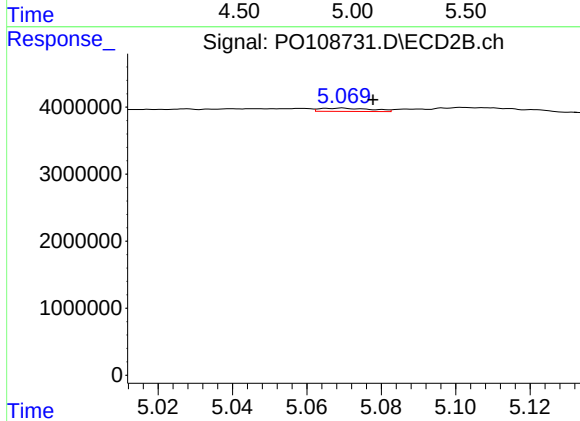


#19 AR-1242-4

R.T.: 5.069 min
Delta R.T.: -0.008 min
Response: 470536
Conc: 4.38 ng/ml

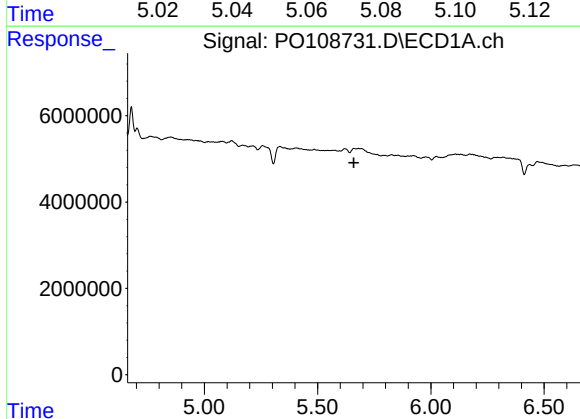


#20 AR-1242-5

R.T.: 0.000 min
Exp R.T.: 5.660 min
Response: 0
Conc: N.D.

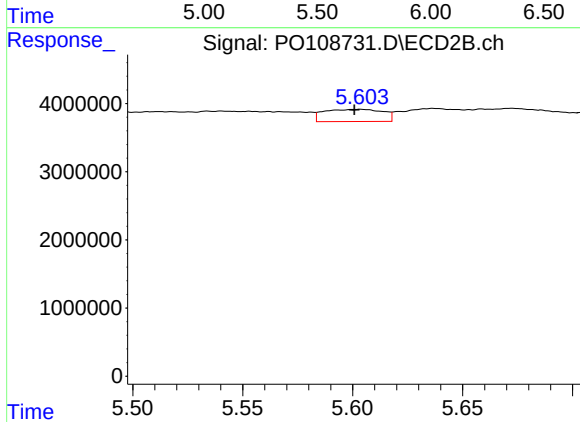

#20 AR-1242-5


R.T.: 5.604 min
Delta R.T.: 0.003 min
Response: 3345208
Conc: 26.47 ng/ml

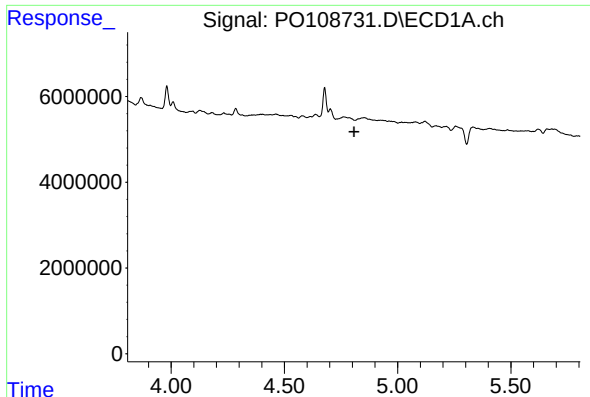

#21 AR-1248-1


R.T.: 0.000 min
Exp R.T.: 4.807 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
STAND-PIPE

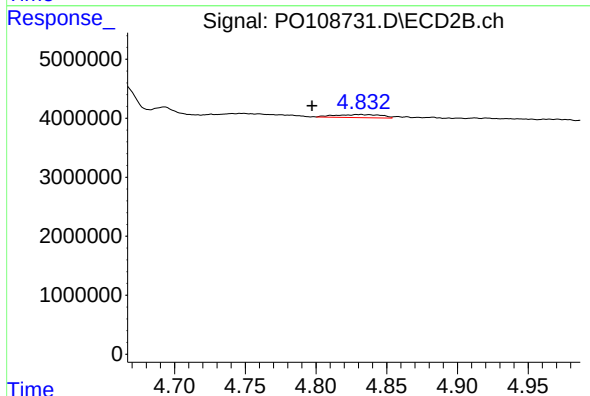


#21 AR-1248-1

R.T.: 4.831 min
Delta R.T.: 0.034 min
Response: 1182334
Conc: 11.25 ng/ml

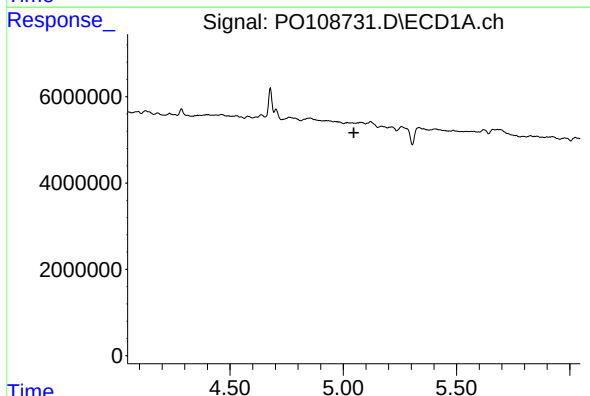


#22 AR-1248-2

R.T.: 0.000 min
Exp R.T.: 5.047 min
Response: 0
Conc: N.D.

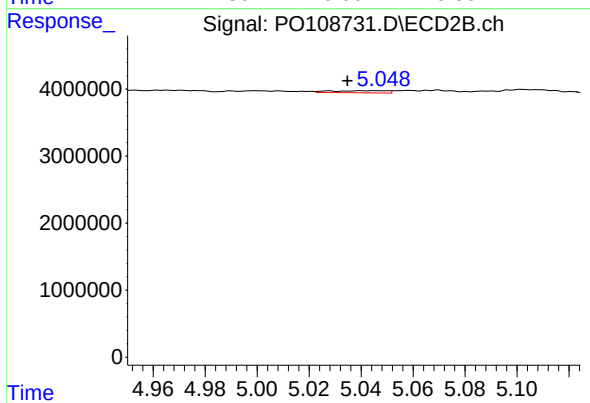

#22 AR-1248-2


R.T.: 5.040 min
Delta R.T.: 0.005 min
Response: 479402
Conc: 3.21 ng/ml

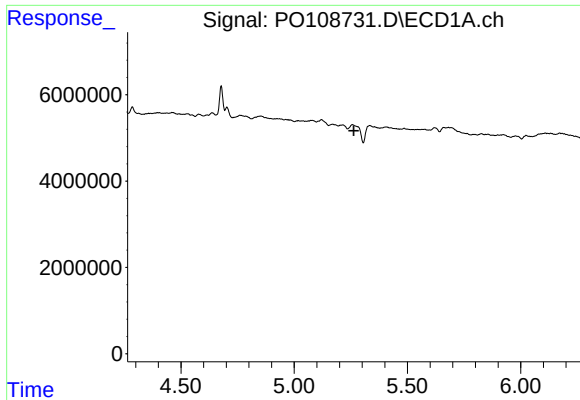

#23 AR-1248-3


R.T.: 0.000 min
Exp R.T.: 5.263 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
STAND-PIPE

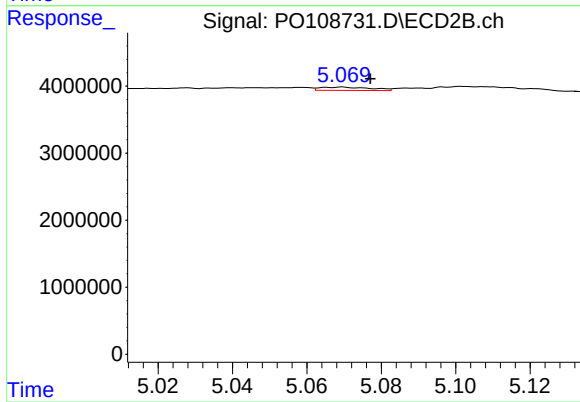


#23 AR-1248-3

R.T.: 5.069 min
Delta R.T.: -0.008 min
Response: 470536
Conc: 2.97 ng/ml

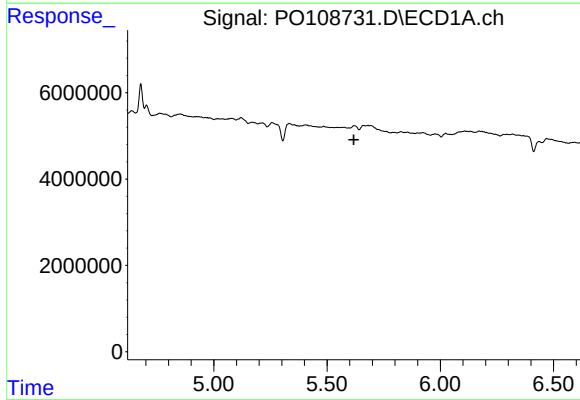


#24 AR-1248-4

R.T.: 0.000 min
Exp R.T.: 5.618 min
Response: 0
Conc: N.D.

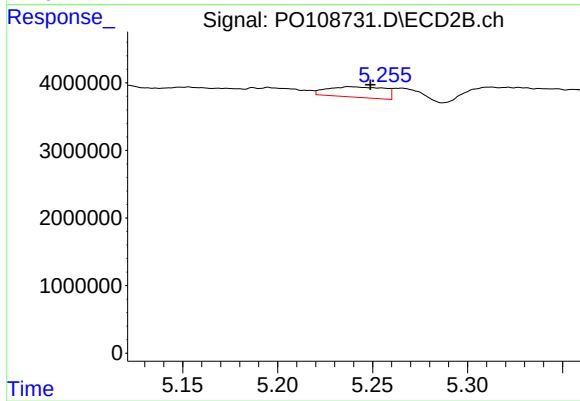

#24 AR-1248-4


R.T.: 5.238 min
Delta R.T.: -0.011 min
Response: 3245618
Conc: 17.78 ng/ml

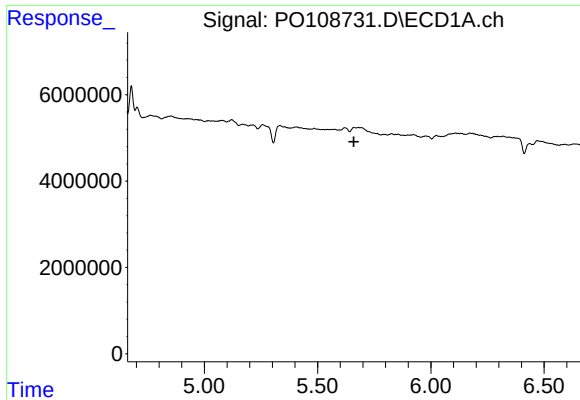

#25 AR-1248-5


R.T.: 0.000 min
Exp R.T.: 5.660 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
STAND-PIPE

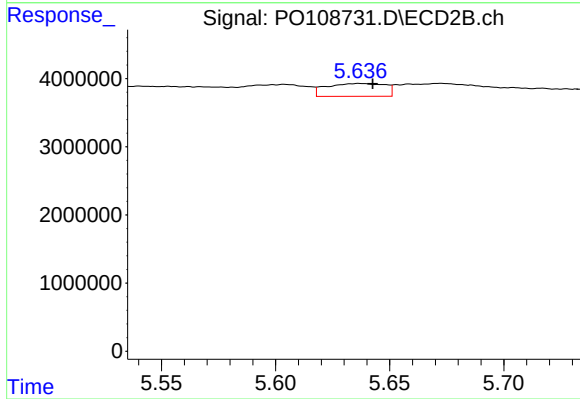


#25 AR-1248-5

R.T.: 5.637 min
Delta R.T.: -0.005 min
Response: 3373776
Conc: 19.21 ng/ml

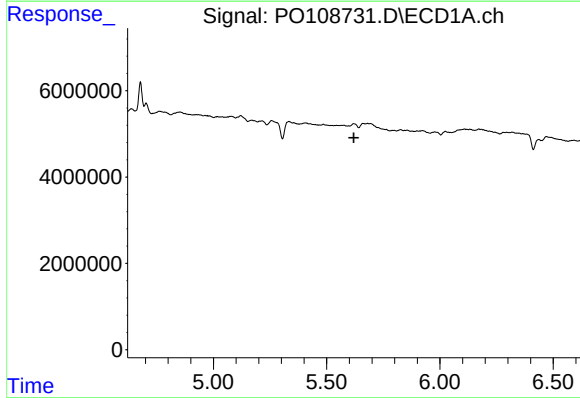


#26 AR-1254-1

R.T.: 0.000 min
Exp R.T.: 5.619 min
Response: 0
Conc: N.D.

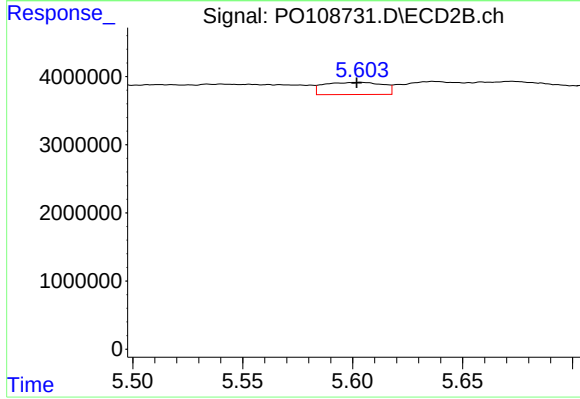

#26 AR-1254-1


R.T.: 5.604 min
Delta R.T.: 0.002 min
Response: 3345208
Conc: 12.35 ng/ml

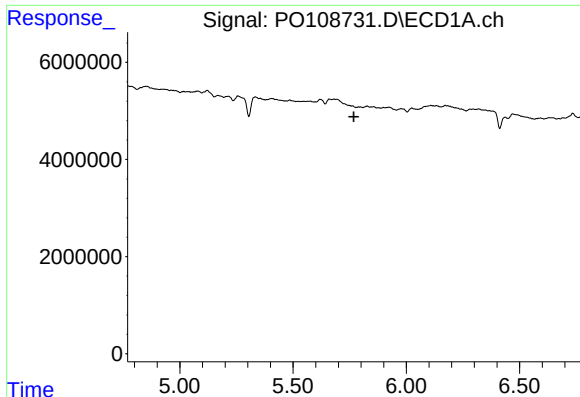

#27 AR-1254-2


R.T.: 0.000 min
Exp R.T.: 5.768 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
STAND-PIPE

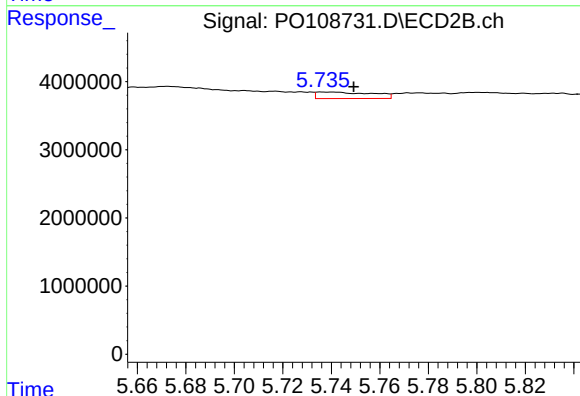


#27 AR-1254-2

R.T.: 5.736 min
Delta R.T.: -0.014 min
Response: 1542326
Conc: 6.43 ng/ml

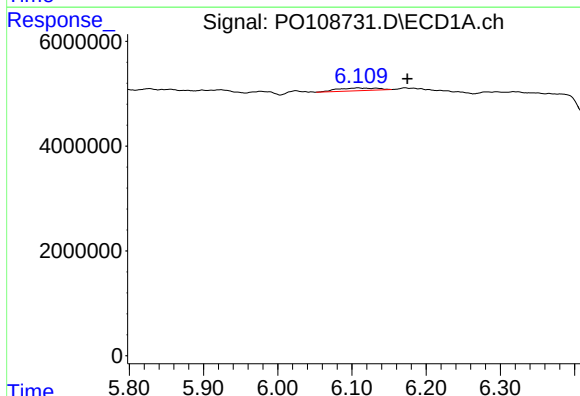


#28 AR-1254-3

R.T.: 6.108 min
Delta R.T.: -0.067 min
Response: 1949804
Conc: 2.71 ng/ml

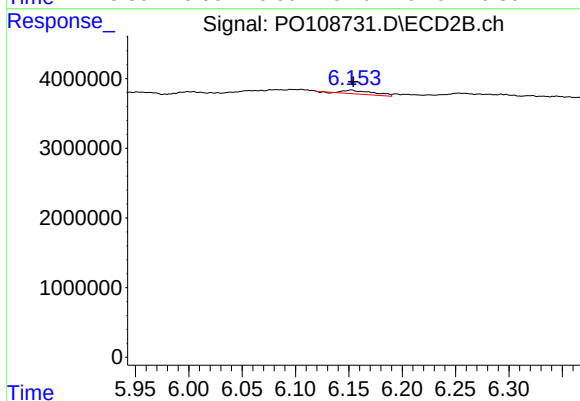

#28 AR-1254-3


R.T.: 6.152 min
Delta R.T.: -0.002 min
Response: 1049546
Conc: 2.79 ng/ml

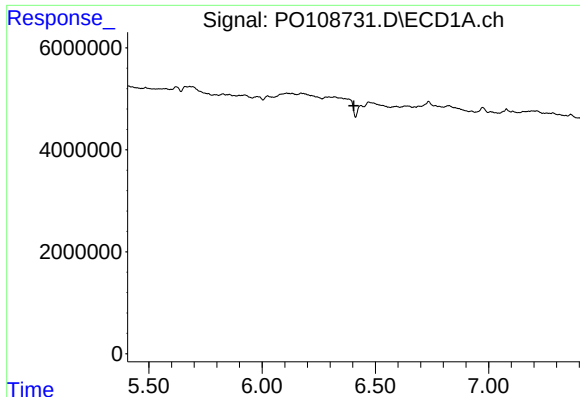

#29 AR-1254-4


R.T.: 6.437 min
Delta R.T.: 0.032 min
Response: -2940577
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
STAND-PIPE

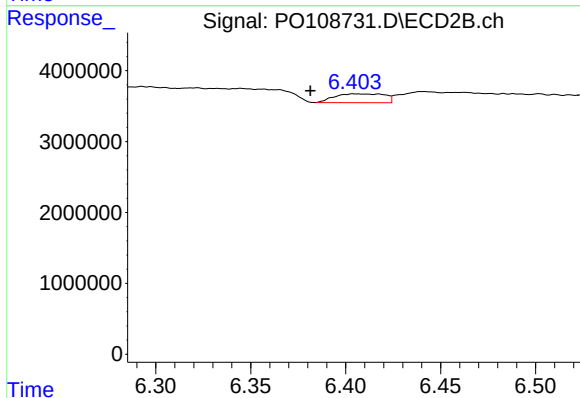


#29 AR-1254-4

R.T.: 6.405 min
Delta R.T.: 0.023 min
Response: 2295517
Conc: 10.55 ng/ml

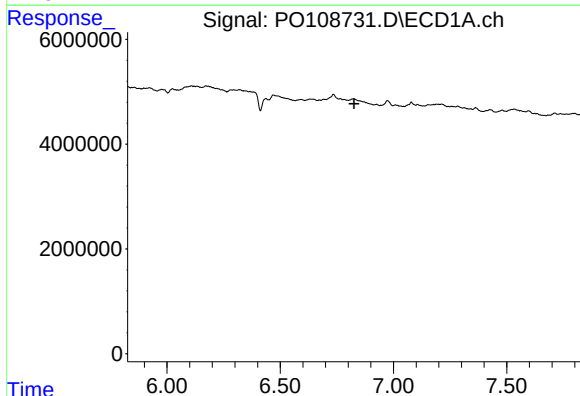


#30 AR-1254-5

R.T.: 0.000 min
Exp R.T. : 6.826 min
Response: 0
Conc: N.D.

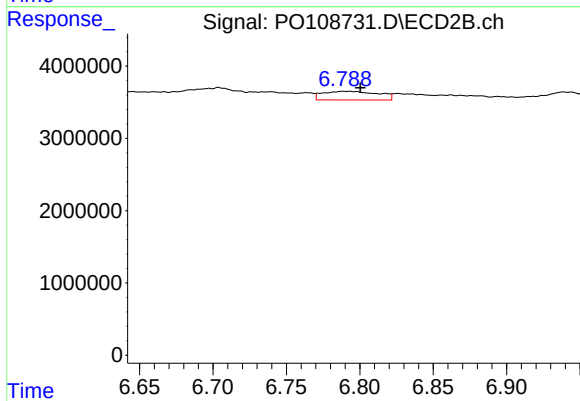

#30 AR-1254-5


R.T.: 6.789 min
Delta R.T.: -0.012 min
Response: 3121994
Conc: 9.67 ng/ml

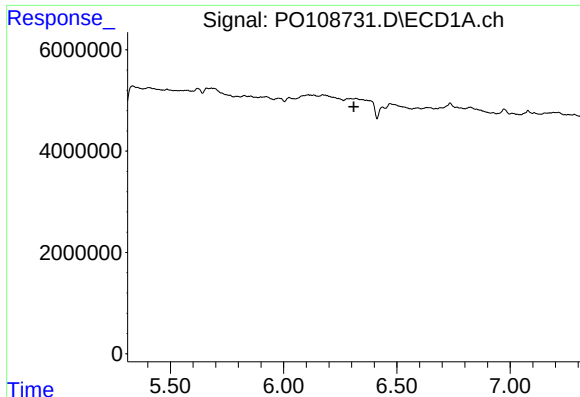

#31 AR-1260-1


R.T.: 0.000 min
Exp R.T.: 6.310 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
STAND-PIPE

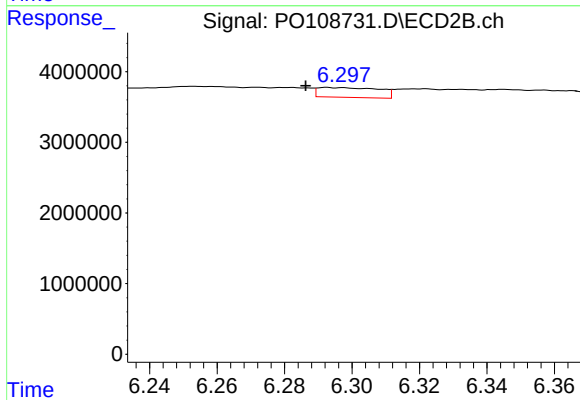


#31 AR-1260-1

R.T.: 6.293 min
Delta R.T.: 0.006 min
Response: 1748756
Conc: 7.47 ng/ml

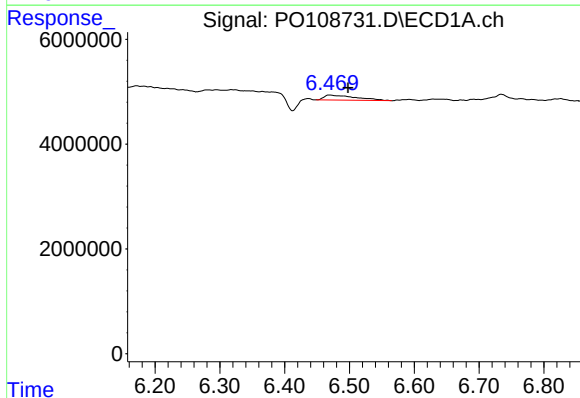


#32 AR-1260-2

R.T.: 6.472 min
Delta R.T.: -0.026 min
Response: 3235515
Conc: 5.82 ng/ml

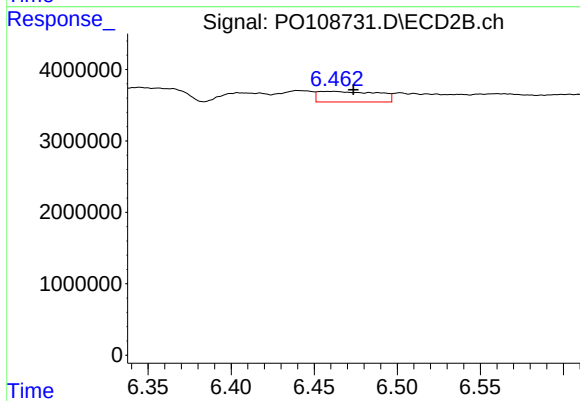

#32 AR-1260-2


R.T.: 6.462 min
Delta R.T.: -0.011 min
Response: 3692095
Conc: 13.16 ng/ml

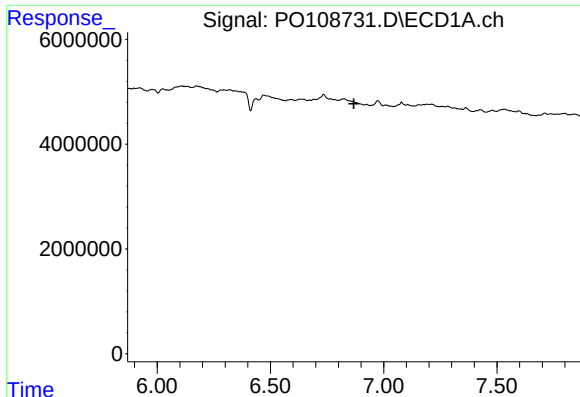

#33 AR-1260-3


R.T.: 0.000 min
Exp R.T.: 6.869 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
STAND-PIPE

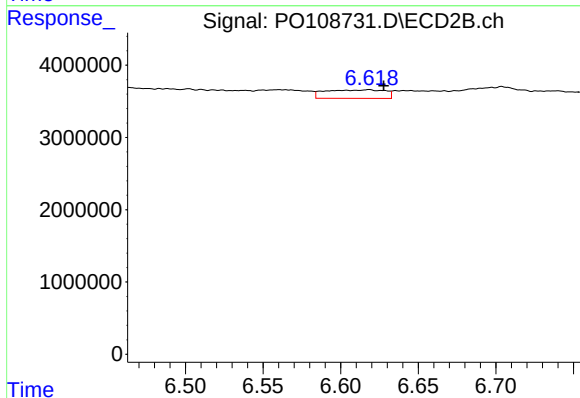


#33 AR-1260-3

R.T.: 6.618 min
Delta R.T.: -0.009 min
Response: 3181632
Conc: 12.07 ng/ml

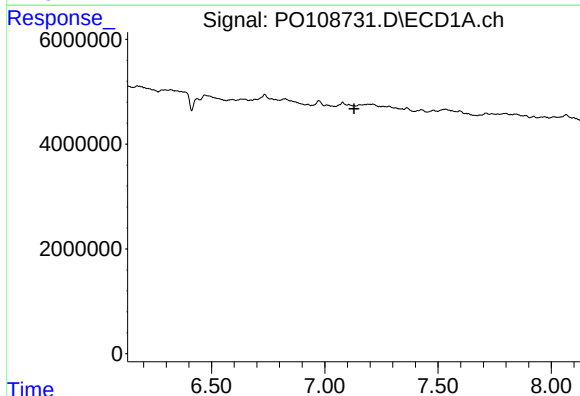


#34 AR-1260-4

R.T.: 0.000 min
Exp R.T.: 7.129 min
Response: 0
Conc: N.D.

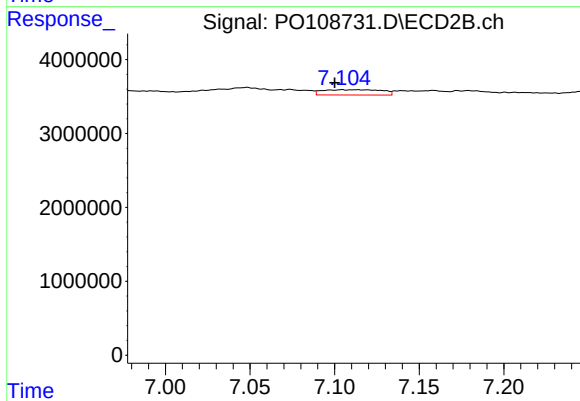

#34 AR-1260-4


R.T.: 7.104 min
Delta R.T.: 0.004 min
Response: 1754150
Conc: 8.25 ng/ml

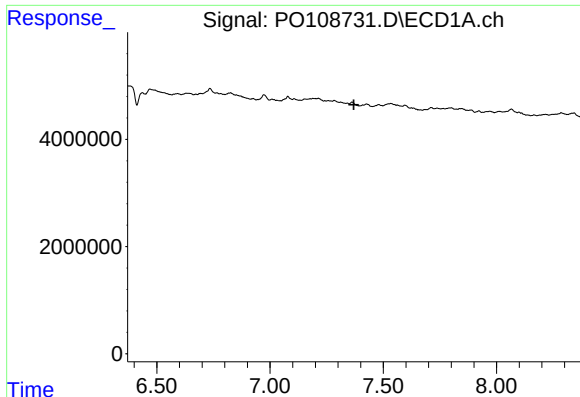

#35 AR-1260-5


R.T.: 0.000 min
Exp R.T.: 7.370 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
STAND-PIPE

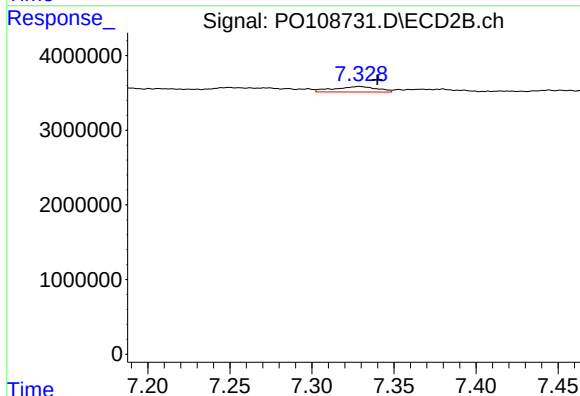


#35 AR-1260-5

R.T.: 7.329 min
Delta R.T.: -0.011 min
Response: 1333601
Conc: 2.76 ng/ml

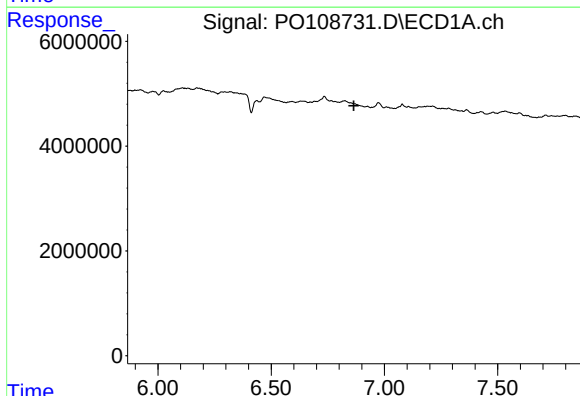


#36 AR-1262-1

R.T.: 0.000 min
Exp R.T.: 6.865 min
Response: 0
Conc: N.D.

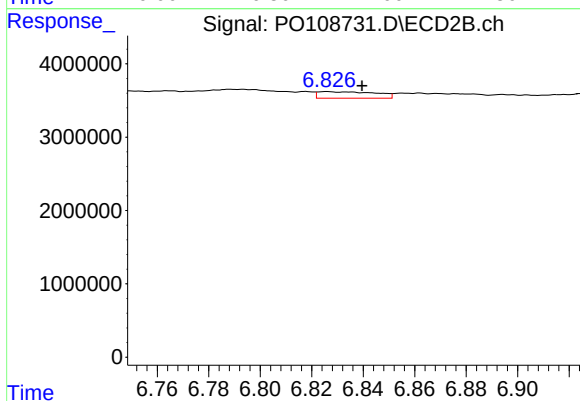

#36 AR-1262-1


R.T.: 6.826 min
Delta R.T.: -0.014 min
Response: 1388147
Conc: 4.11 ng/ml

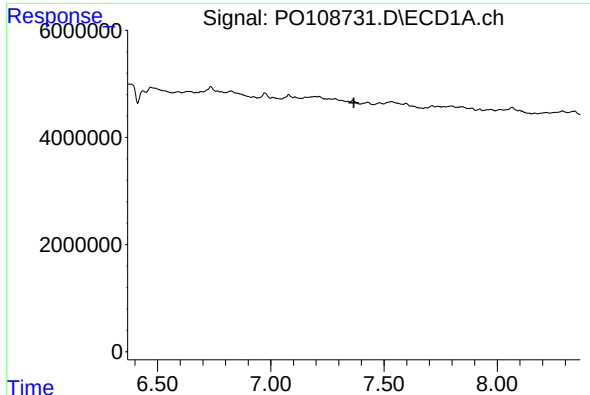

#37 AR-1262-2


R.T.: 0.000 min
Exp R.T.: 7.367 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
STAND-PIPE

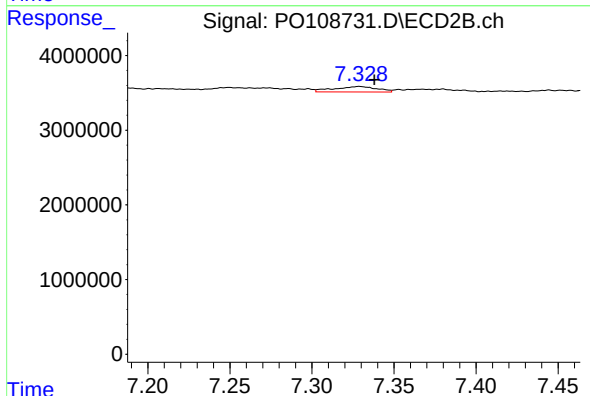


#37 AR-1262-2

R.T.: 7.329 min
Delta R.T.: -0.009 min
Response: 1333601
Conc: 2.33 ng/ml

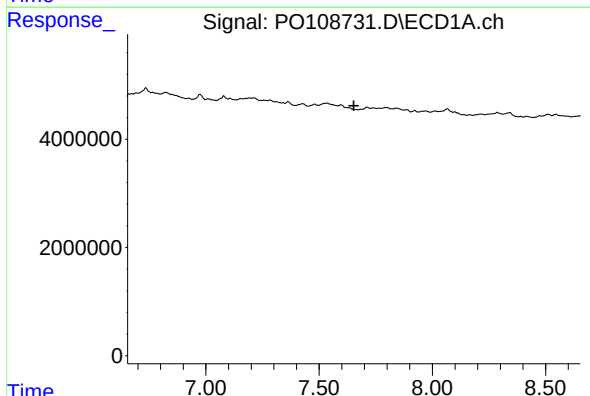


#38 AR-1262-3

R.T.: 0.000 min
Exp R.T.: 7.654 min
Response: 0
Conc: N.D.

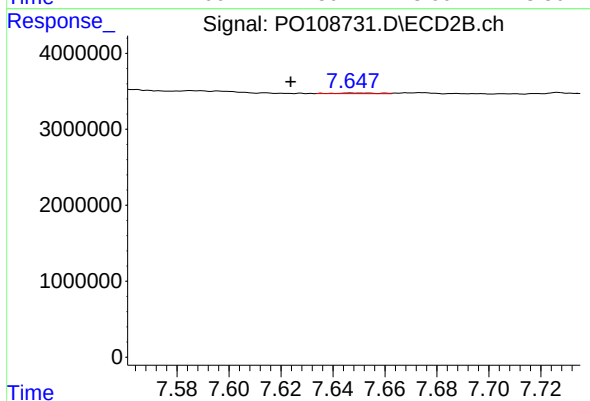

#38 AR-1262-3


R.T.: 7.647 min
Delta R.T.: 0.023 min
Response: 105135
Conc: 0.47 ng/ml

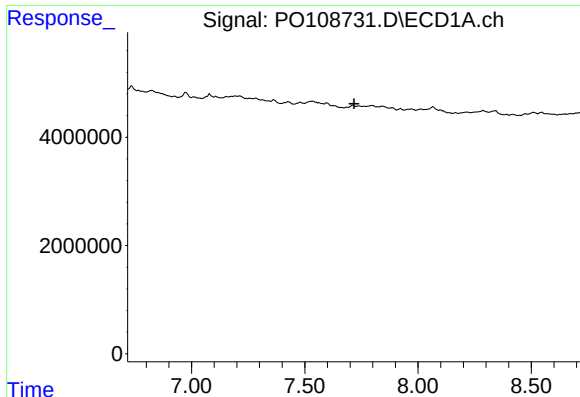

#39 AR-1262-4


R.T.: 0.000 min
Exp R.T.: 7.717 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
STAND-PIPE

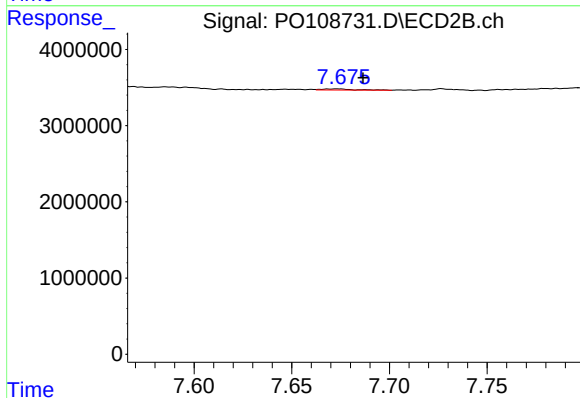


#39 AR-1262-4

R.T.: 7.674 min
Delta R.T.: -0.012 min
Response: 177111
Conc: 0.43 ng/ml

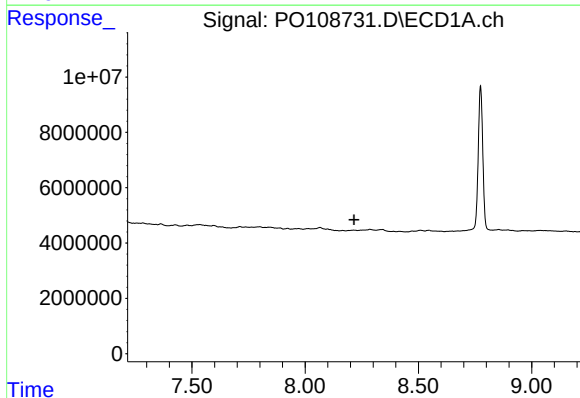


#40 AR-1262-5

R.T.: 0.000 min
Exp R.T.: 8.216 min
Response: 0
Conc: N.D.

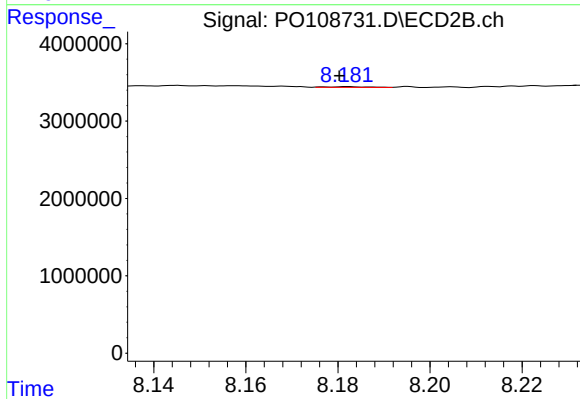

#40 AR-1262-5


R.T.: 8.182 min
Delta R.T.: 0.002 min
Response: 57996
Conc: 0.31 ng/ml

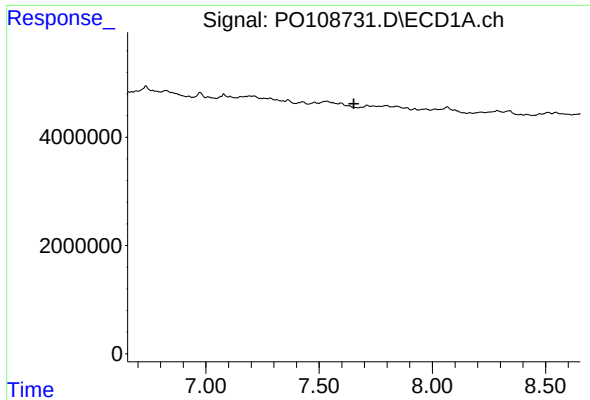

#41 AR-1268-1


R.T.: 0.000 min
Exp R.T.: 7.653 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
STAND-PIPE

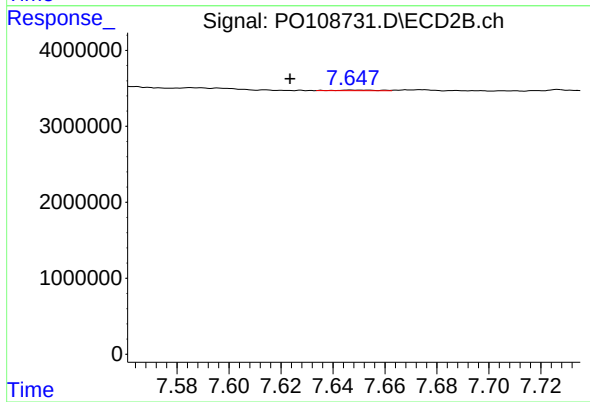


#41 AR-1268-1

R.T.: 7.647 min
Delta R.T.: 0.024 min
Response: 105135
Conc: 0.16 ng/ml

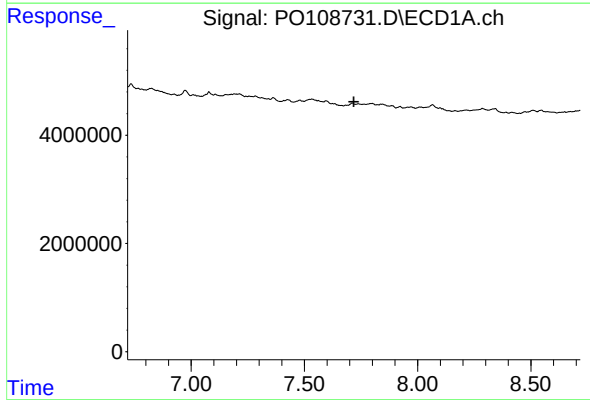


#42 AR-1268-2

R.T.: 0.000 min
Exp R.T.: 7.718 min
Response: 0
Conc: N.D.

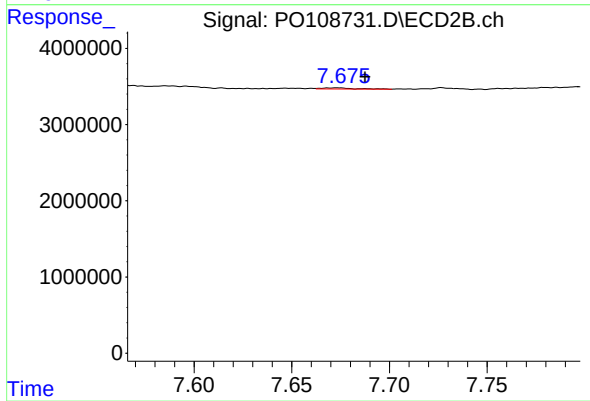

#42 AR-1268-2


R.T.: 7.674 min
Delta R.T.: -0.014 min
Response: 177111
Conc: 0.30 ng/ml

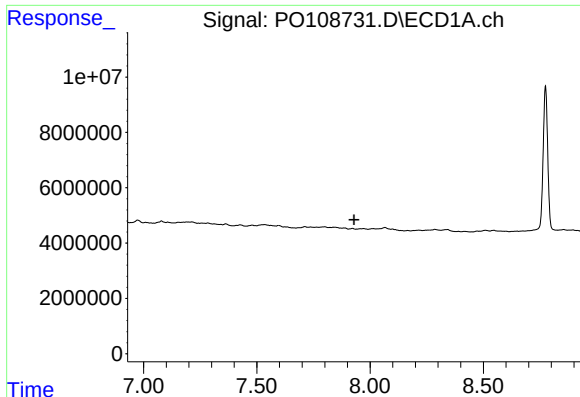

#43 AR-1268-3


R.T.: 0.000 min
Exp R.T.: 7.929 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
STAND-PIPE

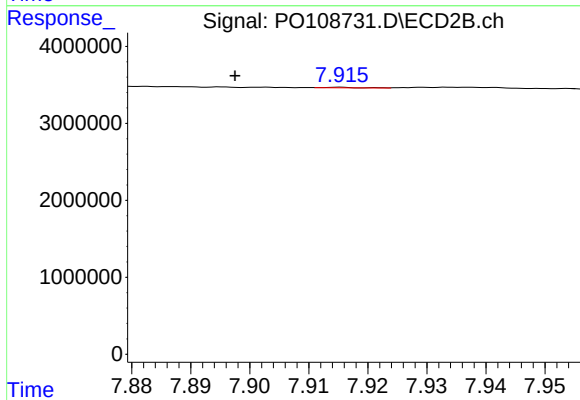


#43 AR-1268-3

R.T.: 7.915 min
Delta R.T.: 0.018 min
Response: 23452
Conc: 0.05 ng/ml

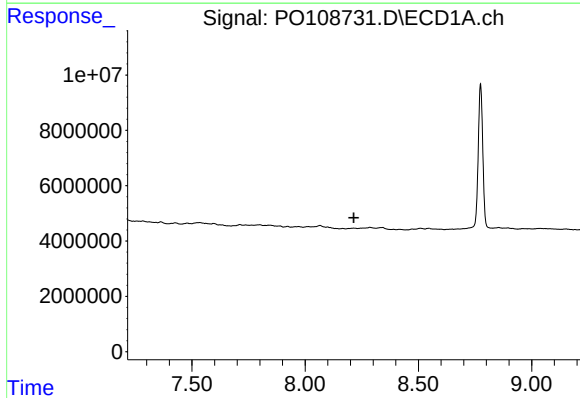


#44 AR-1268-4

R.T.: 0.000 min
Exp R.T.: 8.215 min
Response: 0
Conc: N.D.

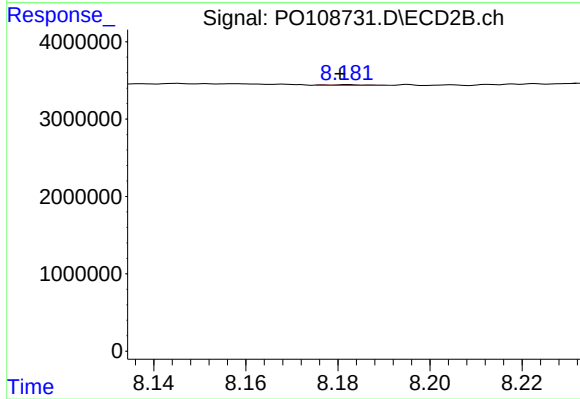

#44 AR-1268-4


R.T.: 8.182 min
Delta R.T.: 0.002 min
Response: 57996
Conc: 0.29 ng/ml

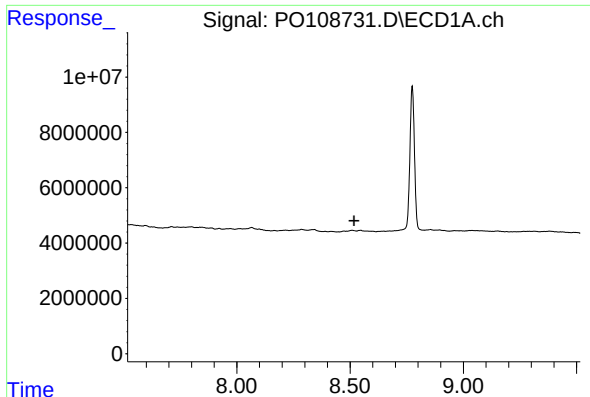

#45 AR-1268-5

R.T.: 0.000 min
Exp R.T.: 8.517 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
STAND-PIPE

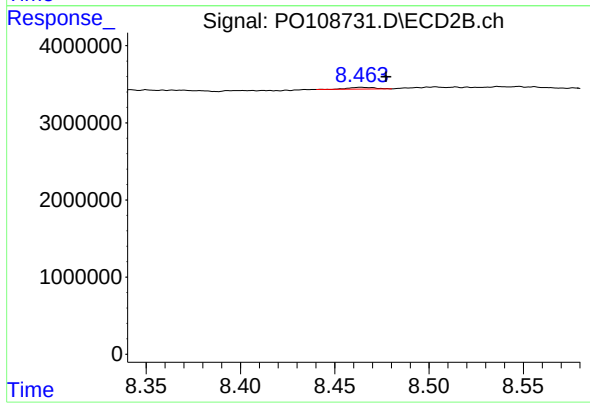

#45 AR-1268-5

R.T.: 8.464 min
Delta R.T.: -0.013 min
Response: 218469
Conc: 0.15 ng/ml