

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0122024\
 Data File : P0108730.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Dec 2024 22:19
 Operator : YP/AJ
 Sample : P5343-06
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 PUMP-WATER-271

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 12/23/2024
 Supervised By :Ankita Jodhani 12/27/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 21 01:27:29 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0120624.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Dec 07 05:58:15 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.706	3.704	79844130	56028814	9.177m	11.052
2) SA Decachlor...	8.774	8.725	92591025	57401276	12.677	14.814

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO122024\
Data File : PO108730.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Dec 2024 22:19
Operator : YP/AJ
Sample : P5343-06
Misc :
ALS Vial : 27 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
PUMP-WATER-271


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 12/23/2024
Supervised By :Ankita Jodhani 12/27/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 21 01:27:29 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO120624.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Dec 07 05:58:15 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

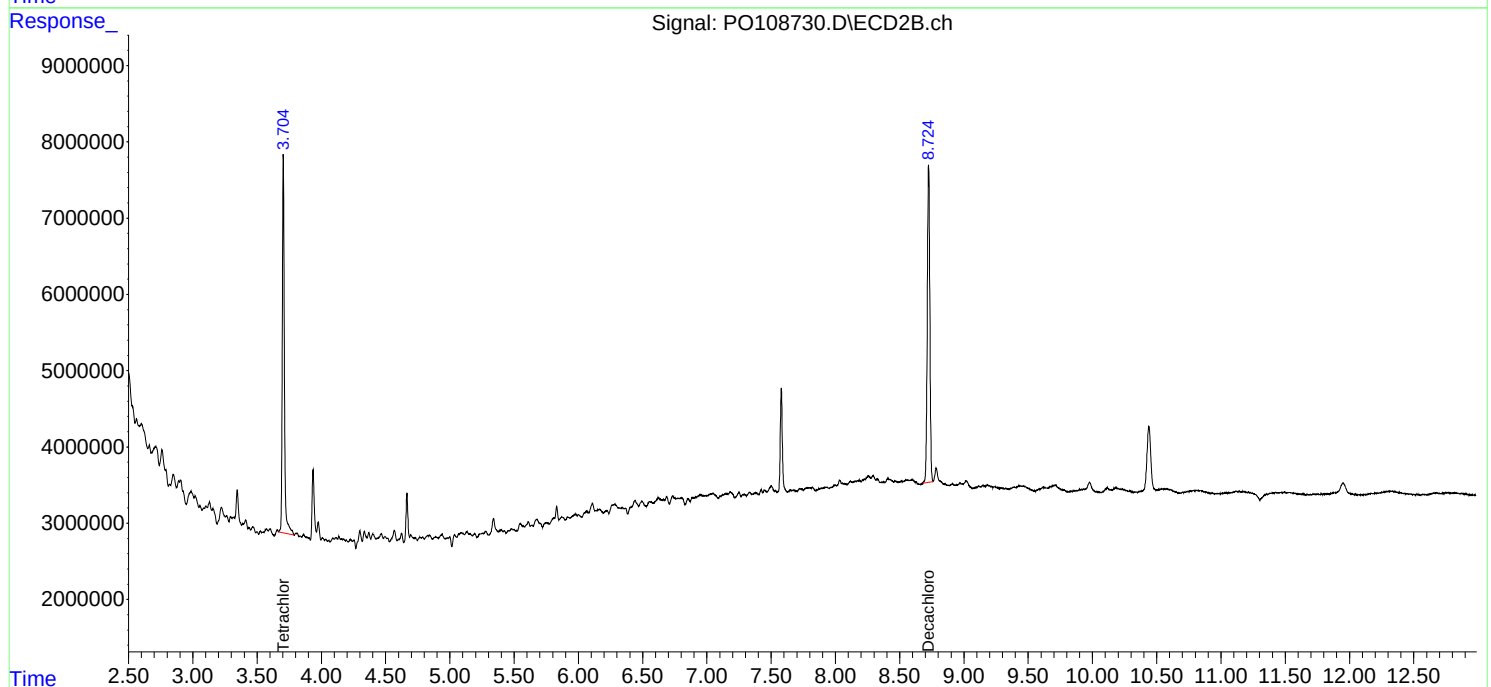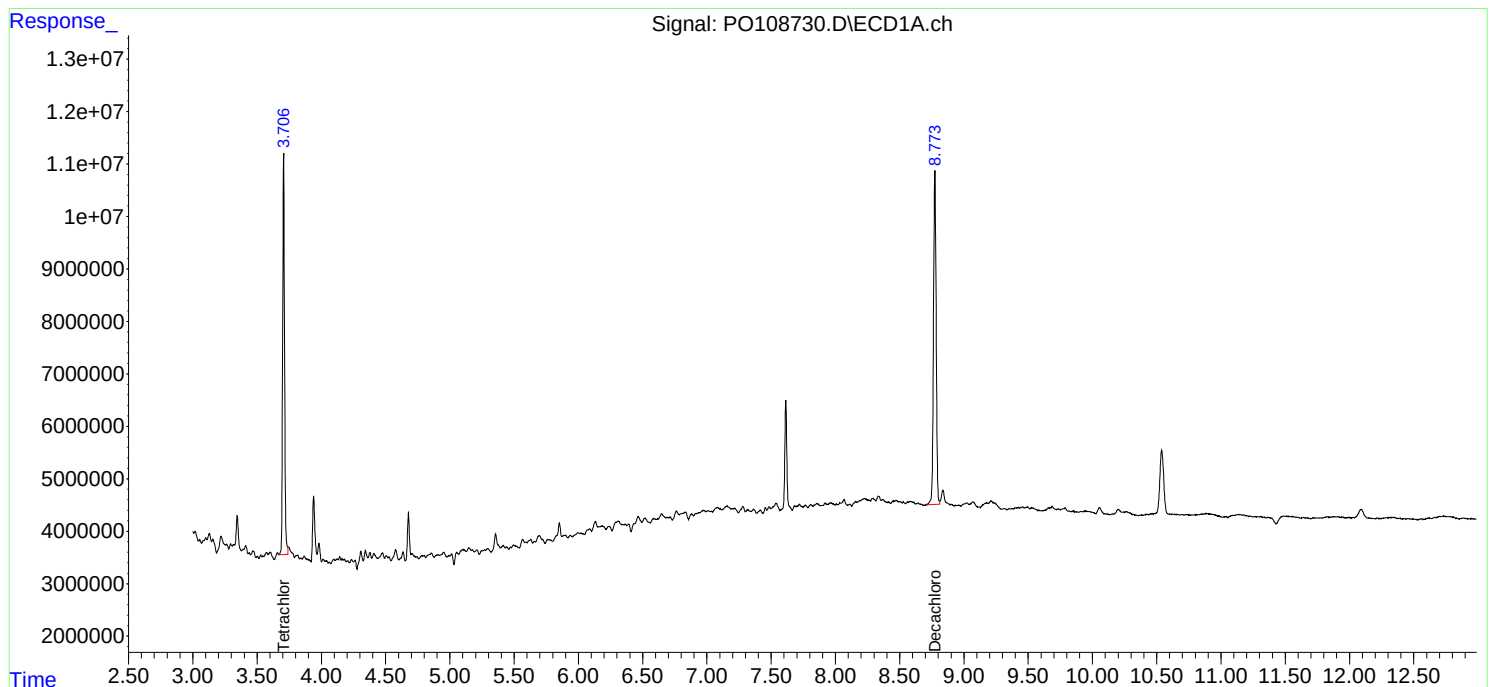

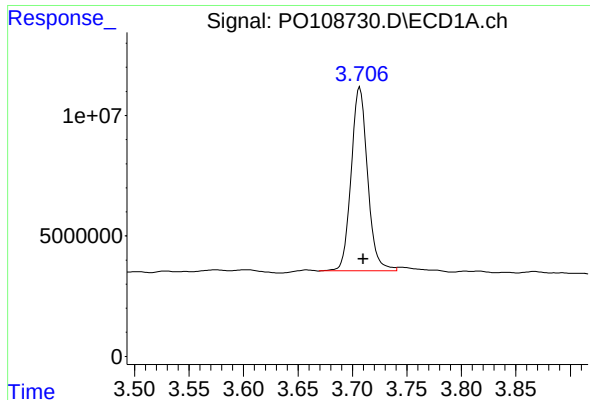


#1 Tetrachloro-m-xylene

R.T.: 3.706 min
Delta R.T.: -0.004 min
Response: 79844130
Conc: 9.18 ng/ml

Instrument :
ECD_O
ClientSampleId :
PUMP-WATER-271


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 12/23/2024
Supervised By :Ankita Jodhani 12/27/2024

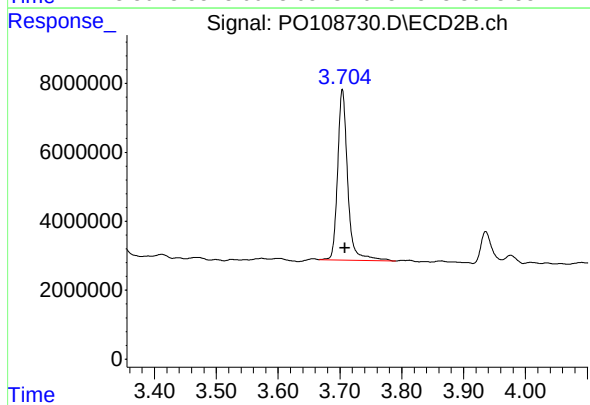


#1 Tetrachloro-m-xylene

R.T.: 3.704 min
Delta R.T.: -0.004 min
Response: 56028814
Conc: 11.05 ng/ml

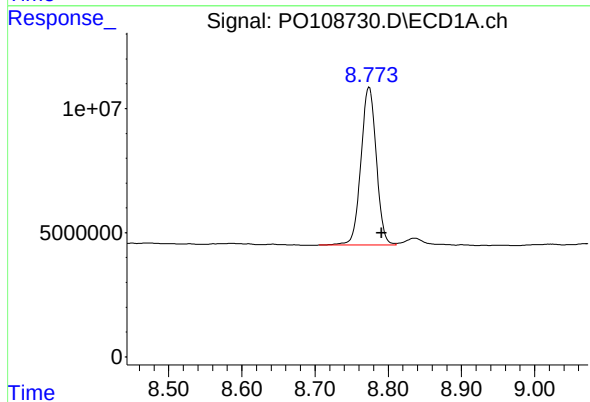

#2 Decachlorobiphenyl

R.T.: 8.774 min
Delta R.T.: -0.017 min
Response: 92591025
Conc: 12.68 ng/ml

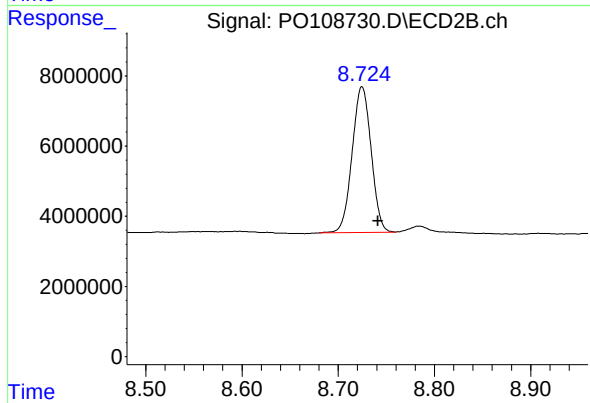

#2 Decachlorobiphenyl

R.T.: 8.725 min
Delta R.T.: -0.017 min
Response: 57401276
Conc: 14.81 ng/ml