

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0122120\
 Data File : P0073999.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 21 Dec 2020 23:13
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 22 02:27:15 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0121020.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Dec 11 03:58:06 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.938	3.997	2010600	1210477	21.991	22.568
2)	SA Decachlor...	10.964	9.261	1779213	990900	21.530	21.177
Target Compounds							
9)	L2 AR-1221-2	5.293	0.000	24428	0	31.099	N.D. #
20)	L4 AR-1242-5	7.253	0.000	1903	0	0.871	N.D. #
24)	L5 AR-1248-4	7.181f	0.000	94900	0	23.730	N.D. #
25)	L5 AR-1248-5	7.253	0.000	1903	0	0.503	N.D. #
26)	L6 AR-1254-1	7.181	0.000	94900	0	25.001	N.D. #
30)	L6 AR-1254-5	8.515	0.000	6757	0	1.312	N.D. #
33)	L7 AR-1260-3	8.597	0.000	6678	0	1.461	N.D. #
36)	L8 AR-1262-1	8.597	0.000	6678	0	0.892	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO122120\
Data File : PO073999.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 21 Dec 2020 23:13
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 22 02:27:15 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO121020.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Dec 11 03:58:06 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

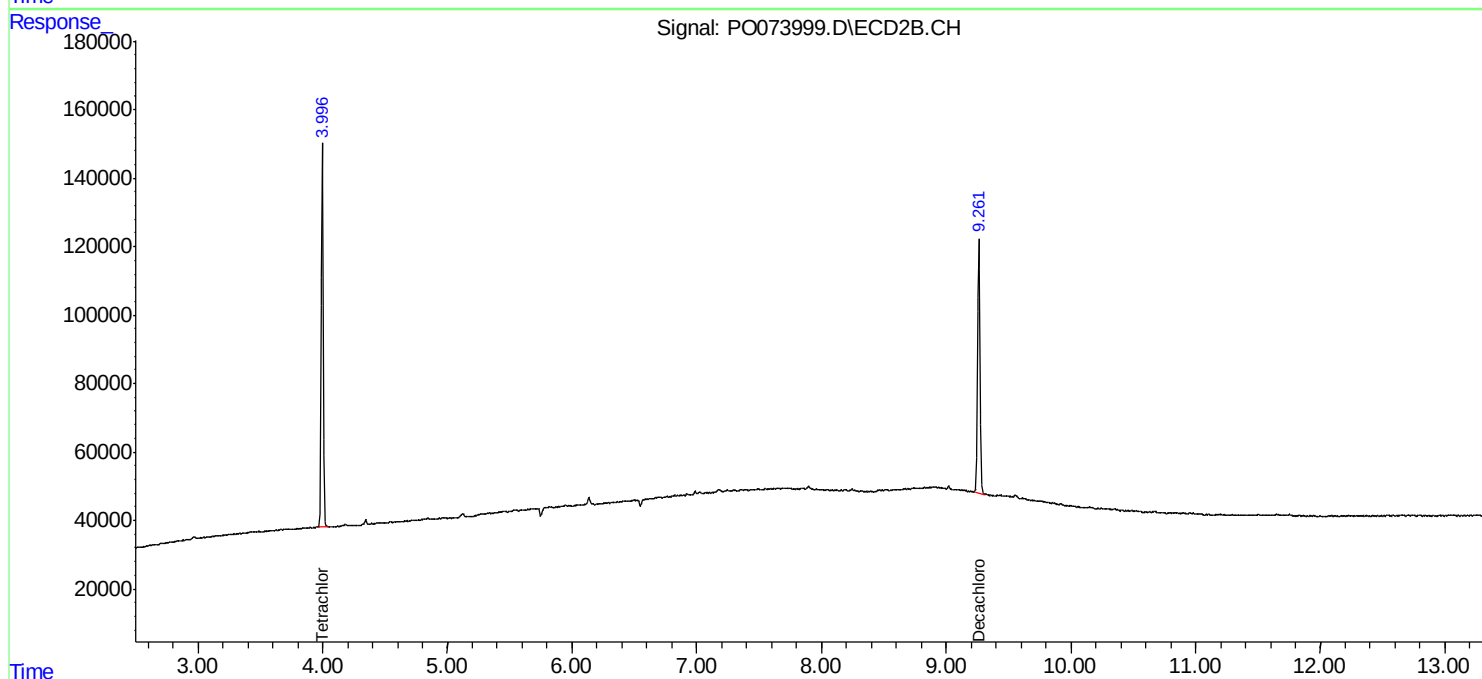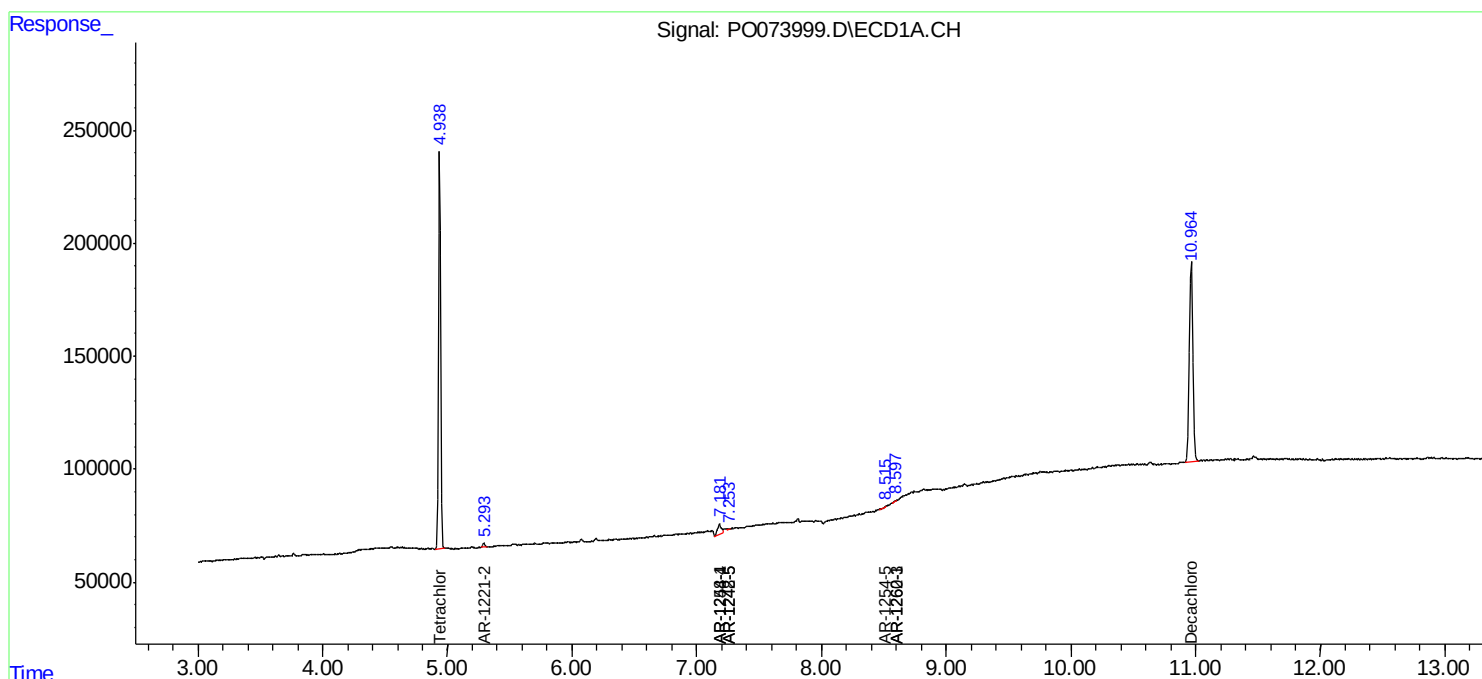


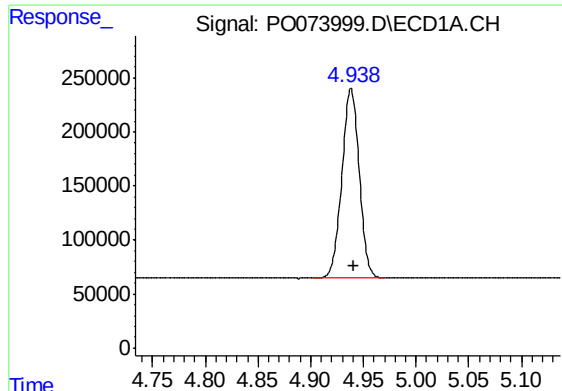

#1 Tetrachloro-m-xylene


R.T.: 4.938 min
Delta R.T.: -0.003 min
Response: 2010600
Conc: 21.99 ng/ml

Instrument :
ECD_O
ClientSampleId :
I.BLK

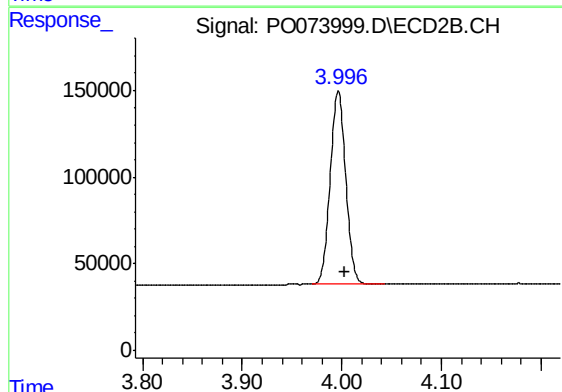


#1 Tetrachloro-m-xylene

R.T.: 3.997 min
Delta R.T.: -0.007 min
Response: 1210477
Conc: 22.57 ng/ml

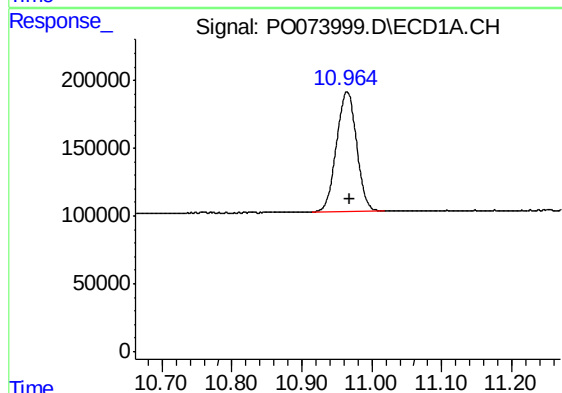


#2 Decachlorobiphenyl

R.T.: 10.964 min
Delta R.T.: -0.004 min
Response: 1779213
Conc: 21.53 ng/ml

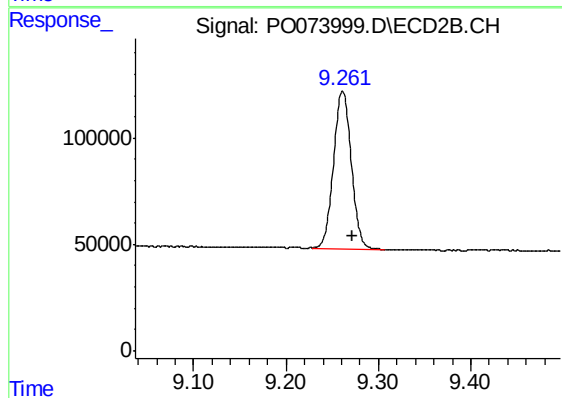

#2 Decachlorobiphenyl


R.T.: 9.261 min
Delta R.T.: -0.010 min
Response: 990900
Conc: 21.18 ng/ml

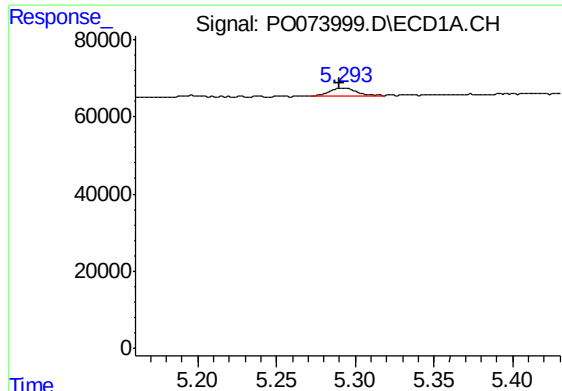

#9 AR-1221-2


R.T.: 5.293 min
Delta R.T.: 0.002 min
Response: 24428
Conc: 31.10 ng/ml

Instrument :
ECD_O
ClientSampleId :
I.BLK

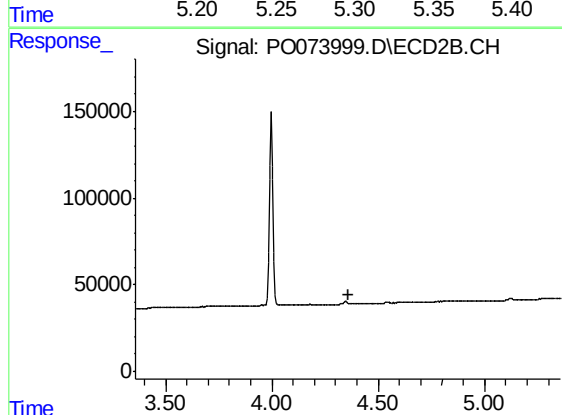


#9 AR-1221-2

R.T.: 0.000 min
Exp R.T. : 4.357 min
Response: 0
Conc: N.D.

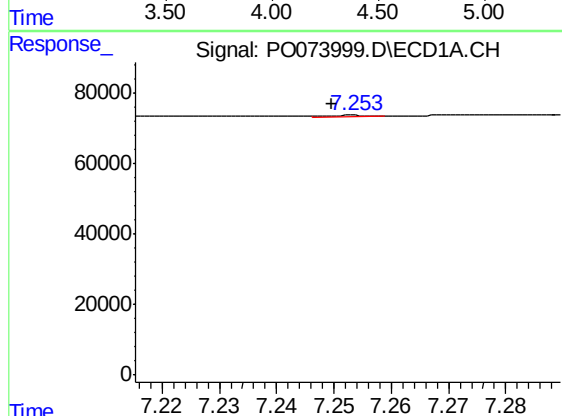


#20 AR-1242-5

R.T.: 7.253 min
Delta R.T.: 0.004 min
Response: 1903
Conc: 0.87 ng/ml

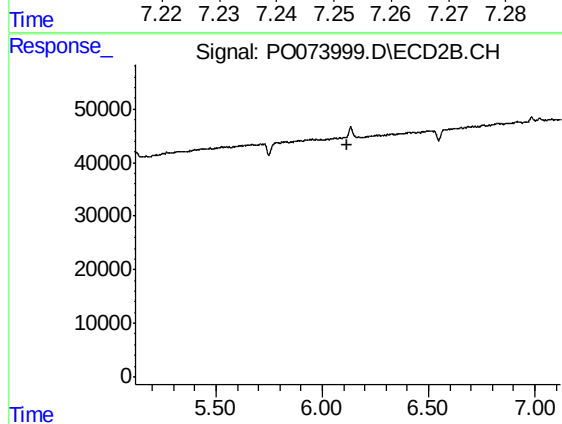

#20 AR-1242-5


R.T.: 0.000 min
Exp R.T. : 6.120 min
Response: 0
Conc: N.D.

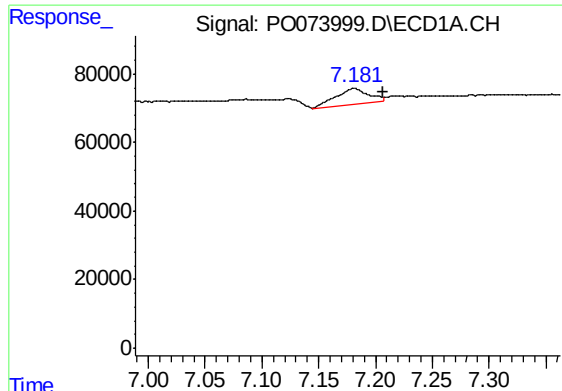

#24 AR-1248-4


R.T.: 7.181 min
Delta R.T.: -0.026 min
Response: 94900
Conc: 23.73 ng/ml

Instrument :
ECD_O
ClientSampleId :
I.BLK

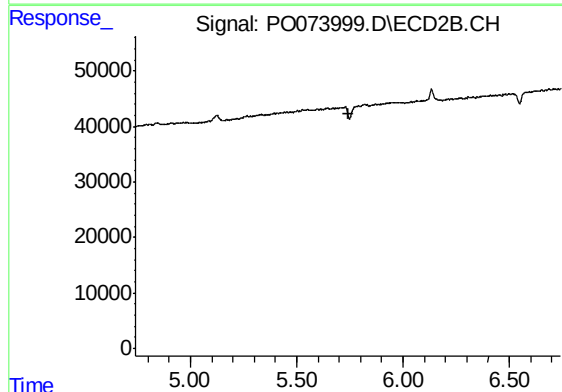


#24 AR-1248-4

R.T.: 0.000 min
Exp R.T. : 5.741 min
Response: 0
Conc: N.D.

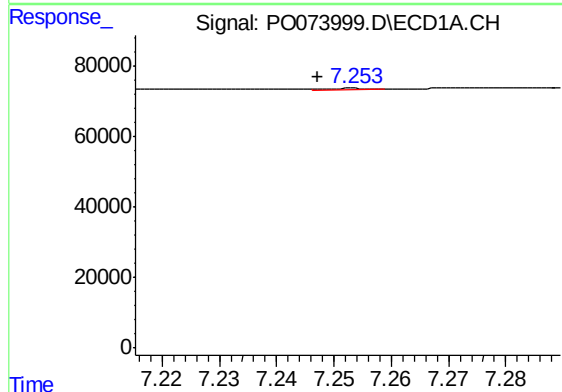


#25 AR-1248-5

R.T.: 7.253 min
Delta R.T.: 0.006 min
Response: 1903
Conc: 0.50 ng/ml

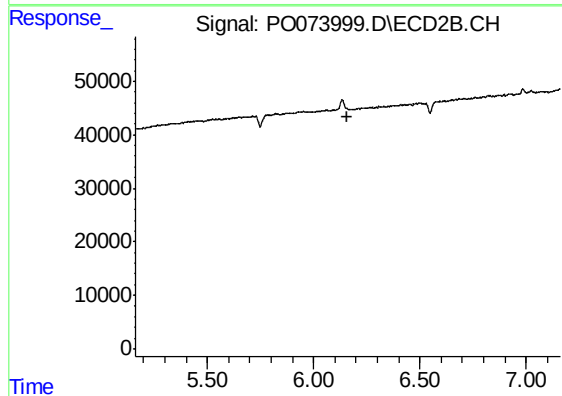

#25 AR-1248-5


R.T.: 0.000 min
Exp R.T. : 6.161 min
Response: 0
Conc: N.D.

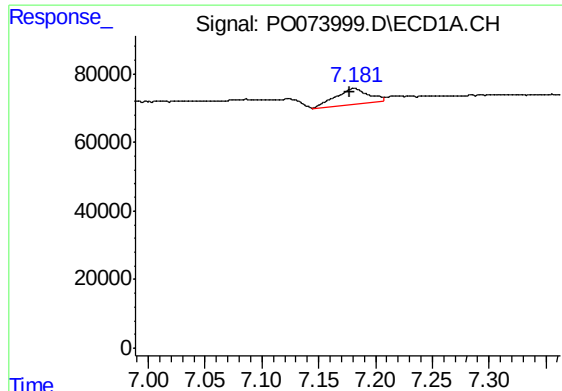

#26 AR-1254-1


R.T.: 7.181 min
Delta R.T.: 0.004 min
Response: 94900
Conc: 25.00 ng/ml

Instrument :
ECD_O
ClientSampleId :
I.BLK

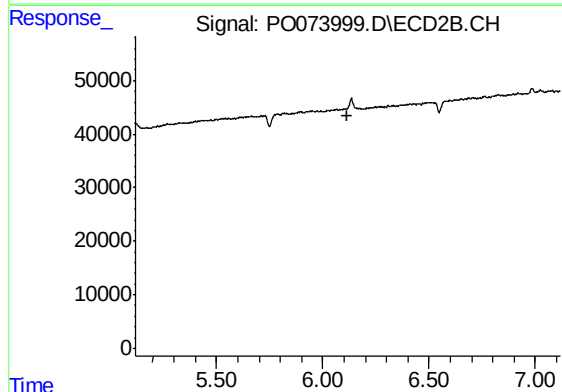


#26 AR-1254-1

R.T.: 0.000 min
Exp R.T. : 6.118 min
Response: 0
Conc: N.D.

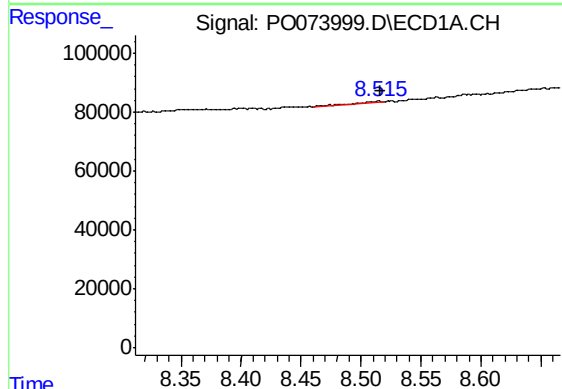


#30 AR-1254-5

R.T.: 8.515 min
Delta R.T.: -0.002 min
Response: 6757
Conc: 1.31 ng/ml

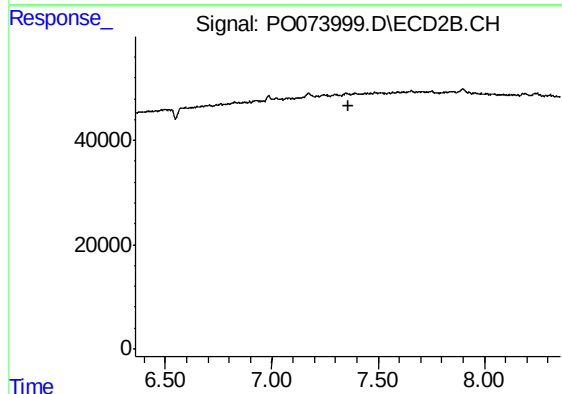

#30 AR-1254-5


R.T.: 0.000 min
Exp R.T. : 7.359 min
Response: 0
Conc: N.D.

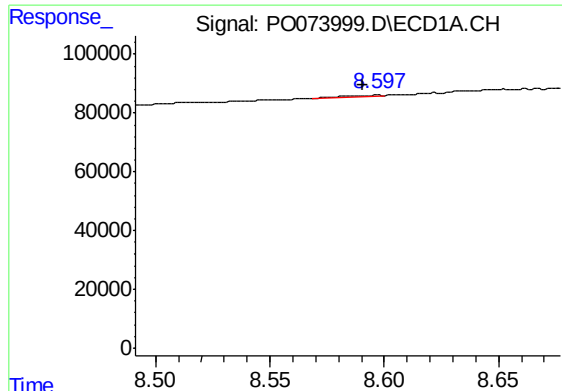

#33 AR-1260-3


R.T.: 8.597 min
Delta R.T.: 0.006 min
Response: 6678
Conc: 1.46 ng/ml

Instrument :
ECD_O
ClientSampleId :
I.BLK

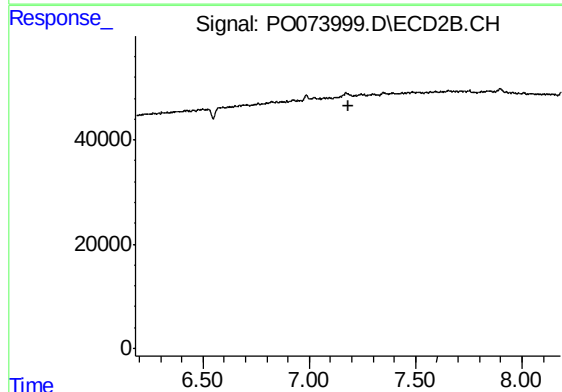


#33 AR-1260-3

R.T.: 0.000 min
Exp R.T. : 7.182 min
Response: 0
Conc: N.D.

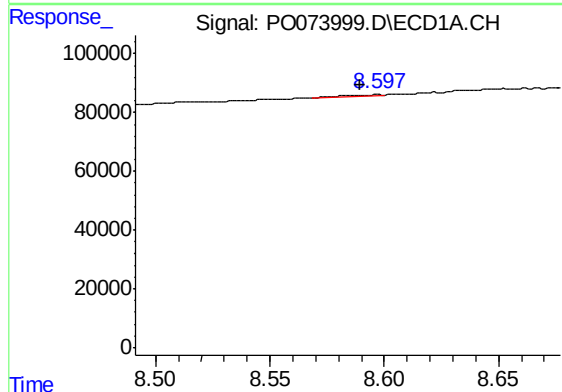

#36 AR-1262-1

R.T.: 8.597 min
Delta R.T.: 0.007 min
Response: 6678
Conc: 0.89 ng/ml

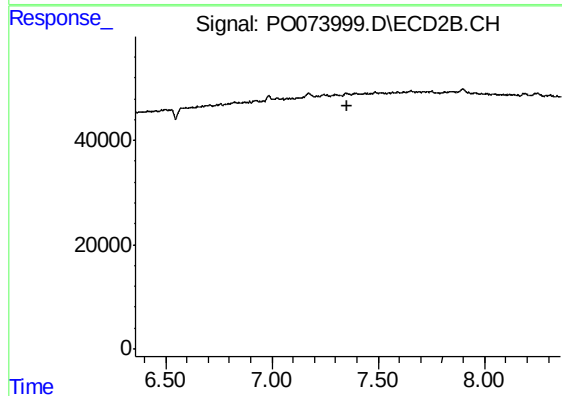

#36 AR-1262-1

R.T.: 0.000 min
Exp R.T. : 7.357 min
Response: 0
Conc: N.D.