

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0122120\
 Data File : P0073970.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 21 Dec 2020 14:06
 Operator : DD\AJ
 Sample : L5155-01
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 TR-04-12-18-20

Manual Integrations
 APPROVED

Ankita
 12/22/2020 1:13:30 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 21 14:41:35 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0121020.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Dec 11 03:58:06 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.937	3.996	1834718	1142120	20.067	21.294
2) SA Decachlor...	10.965	9.260	1699262	983900	20.562	21.028

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO122120\
Data File : PO073970.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 21 Dec 2020 14:06
Operator : DD\AJ
Sample : L5155-01
Misc :
ALS Vial : 12 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
TR-04-12-18-20


Manual Integrations
APPROVED

Ankita
12/22/2020 1:13:30 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 21 14:41:35 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO121020.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Dec 11 03:58:06 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

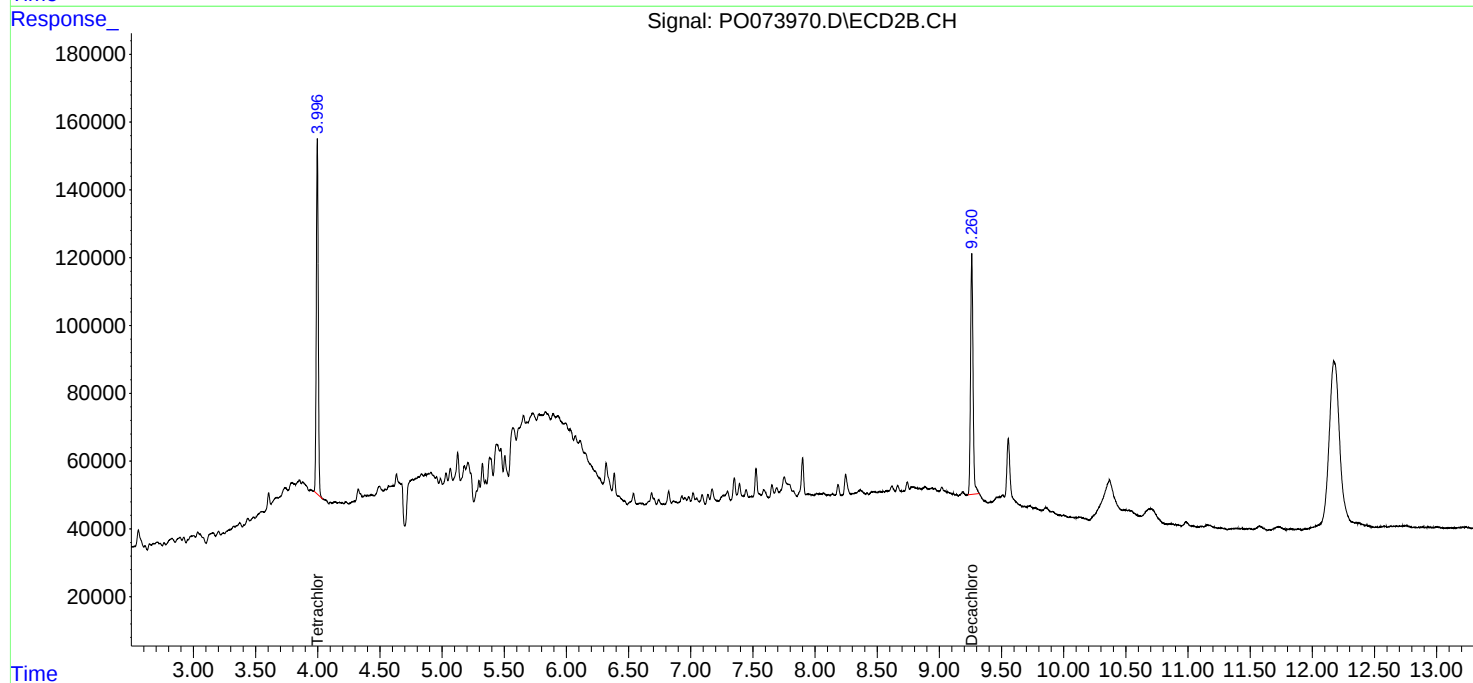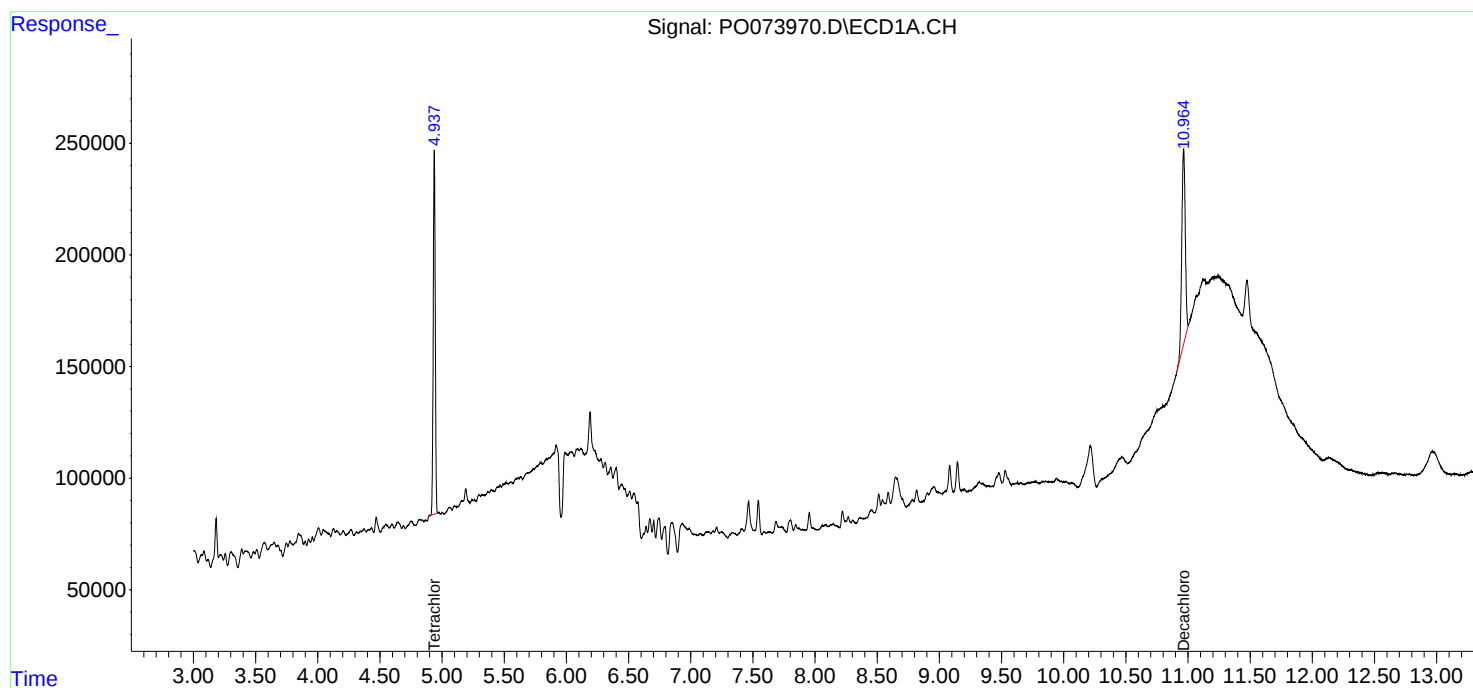

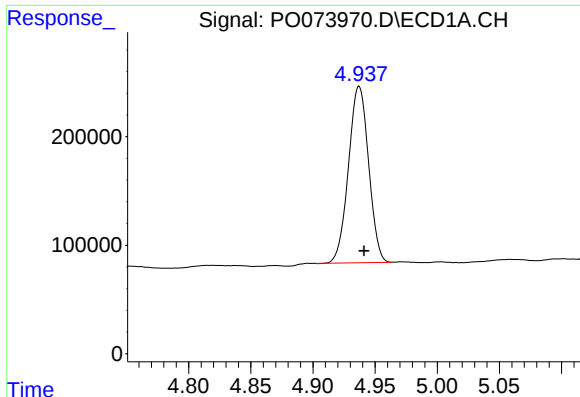


#1 Tetrachloro-m-xylene

R.T.: 4.937 min
Delta R.T.: -0.004 min
Response: 1834718
Conc: 20.07 ng/ml

Instrument :
ECD_O
ClientSampleId :
TR-04-12-18-20


Manual Integrations
APPROVED

Ankita
12/22/2020 1:13:30 PM

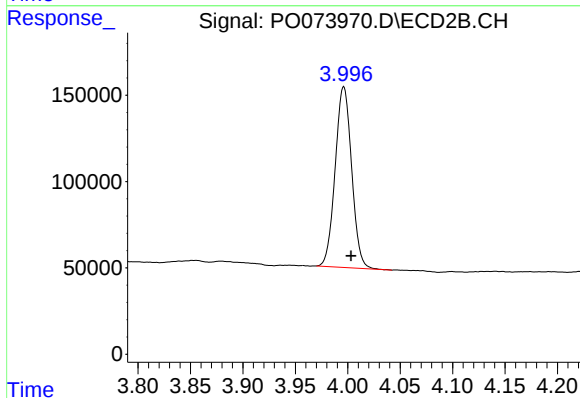


#1 Tetrachloro-m-xylene

R.T.: 3.996 min
Delta R.T.: -0.007 min
Response: 1142120
Conc: 21.29 ng/ml

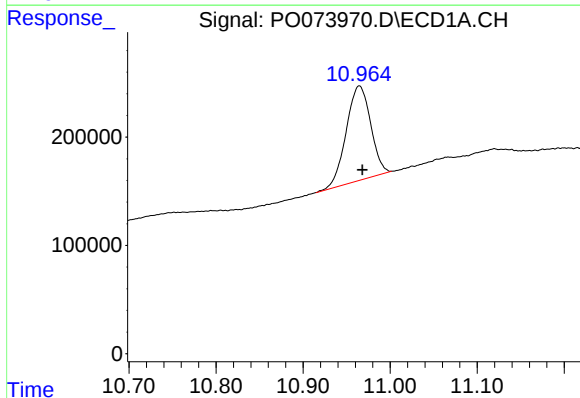

#2 Decachlorobiphenyl

R.T.: 10.965 min
Delta R.T.: -0.004 min
Response: 1699262
Conc: 20.56 ng/ml

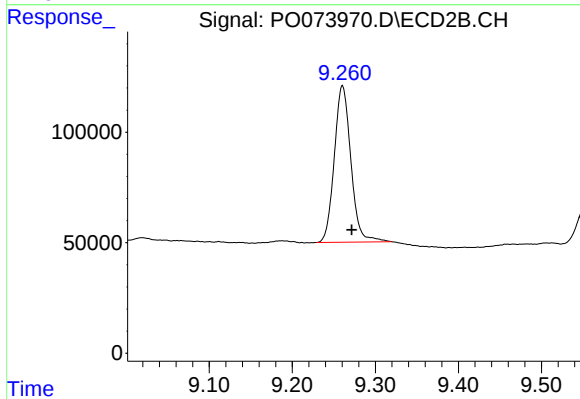

#2 Decachlorobiphenyl

R.T.: 9.260 min
Delta R.T.: -0.011 min
Response: 983900
Conc: 21.03 ng/ml