

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD122222\
 Data File : PD073417.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Dec 2022 19:25
 Operator : AR\AJ
 Sample : INDA301
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 22 02:35:50 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD122222CLP-TCLP.M
 Quant Title : GC Extractables
 QLast Update : Thu Dec 22 02:34:05 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	2.694	3.455	43291746	1581.7E6	20.000	20.000
27)	SA Decachlor...	7.818	8.900	103.0E6	800.3E6	40.000	40.000
Target Compounds							
2)	A alpha-BHC	3.196	3.918	67564452	2243.3E6	20.000	20.000
3)	MA gamma-BHC...	3.526	4.251	62939756	1769.3E6	20.000	20.000
4)	MA Heptachlor	3.857	4.817	65914056	1229.0E6	20.000	20.000
9)	A Endosulfan I	5.009	5.972	55507001	823.0E6	20.000	20.000
13)	MA Dieldrin	5.275	6.248	122.0E6	1734.0E6	40.000	40.000
14)	MA Endrin	5.552	6.480	107.1E6	1397.8E6	40.000	40.000
16)	A 4,4'-DDD	5.699	6.615	96952096	1299.6E6	40.000	40.000
17)	MA 4,4'-DDT	5.947	6.922	97126962	1235.6E6	40.000	40.000
20)	A Methoxychlor	6.530	7.402	275.2E6	2616.5E6	200.000	200.000

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD122222\
Data File : PD073417.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Dec 2022 19:25
Operator : AR\AJ
Sample : INDA301
Misc :
ALS Vial : 14 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 22 02:35:50 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD122222CLP-TCLP.M
Quant Title : GC Extractables
QLast Update : Thu Dec 22 02:34:05 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

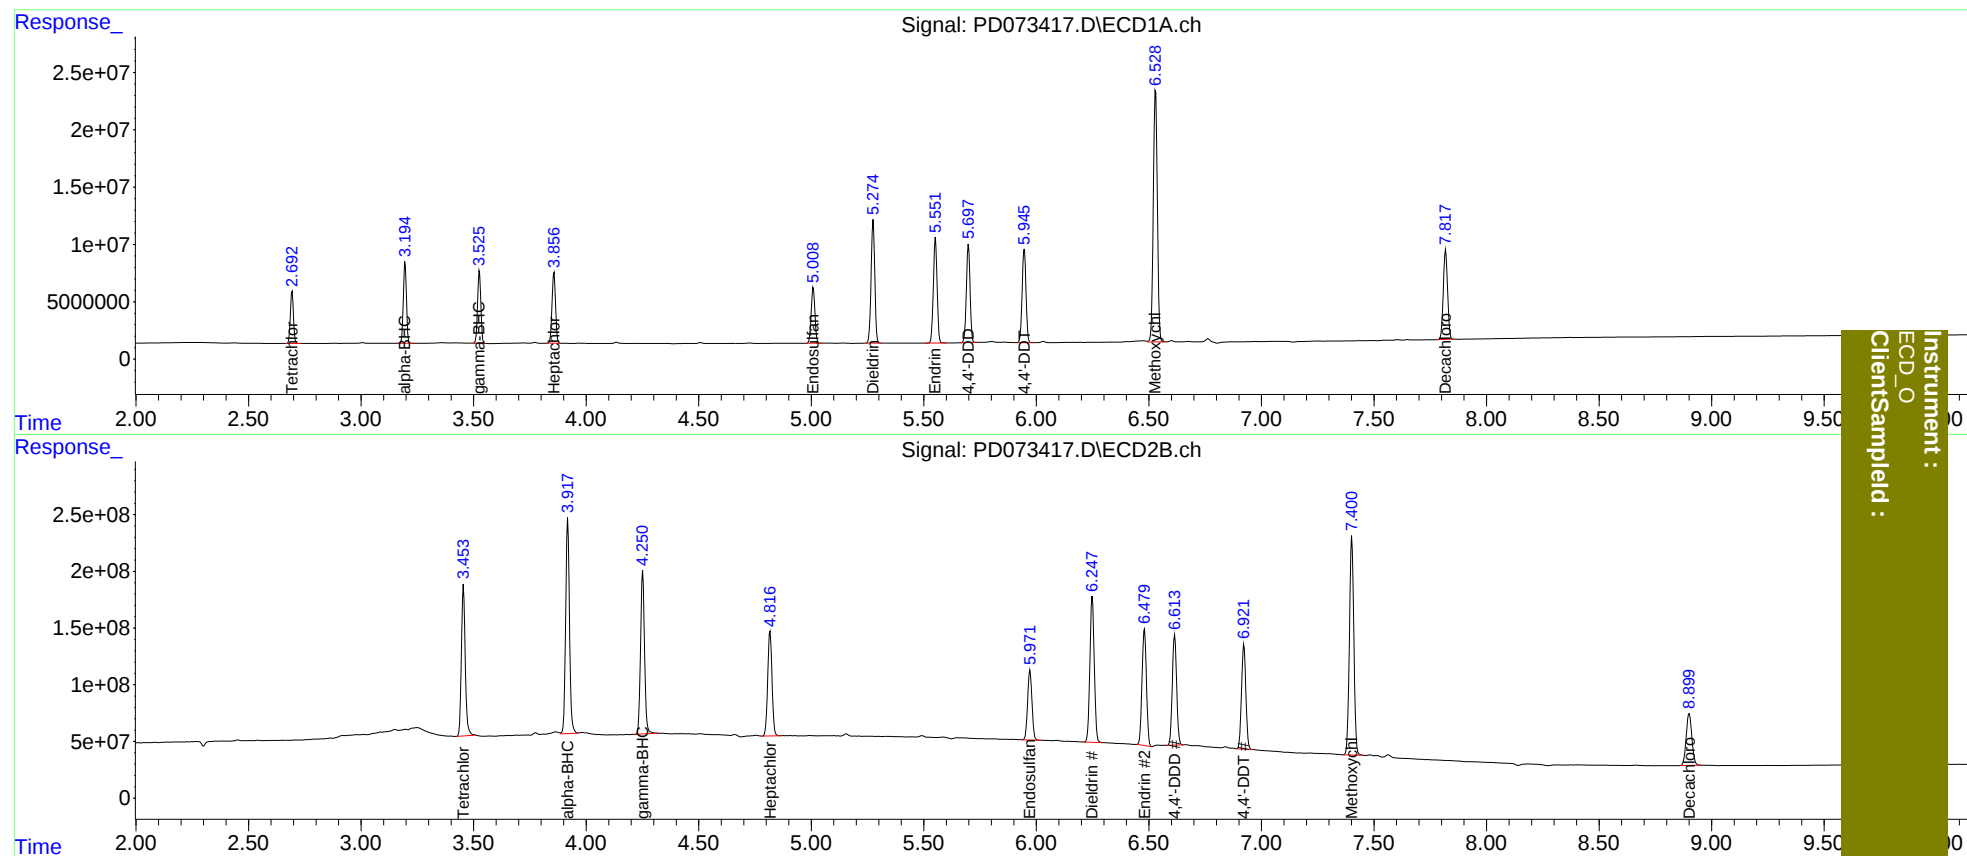

Instrument :
ECD_O
ClientSampled :
INDA301