

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD122222\
 Data File : PD073420.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Dec 2022 20:06
 Operator : AR\AJ
 Sample : INDB401
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 22 04:01:32 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD122222CLP-TCLP.M
 Quant Title : GC Extractables
 QLast Update : Thu Dec 22 04:01:21 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	2.694	3.455	79972965	2786.2E6	39.888	38.046
27)	SA Decachlor...	7.818	8.902	195.6E6	1524.3E6	80.208	80.760
Target Compounds							
5)	MB Aldrin	4.137	5.156	127.7E6	1884.4E6	39.516	39.886
6)	B beta-BHC	3.828	4.467	56037242	1153.3E6	40.098	40.581
7)	B delta-BHC	4.057	4.711	138.1E6	2504.4E6	39.090	38.405
8)	B Heptachlo...	4.641	5.587	115.7E6	1651.4E6	39.636	39.765
10)	B trans-Chl...	4.889	5.841	114.5E6	1589.2E6	39.267	39.631
11)	B cis-Chlor...	4.952	5.916	115.7E6	1593.5E6	39.442	39.797
12)	B 4,4'-DDE	5.141	6.090	233.4E6	3098.6E6	78.898	77.406
15)	B Endosulfa...	5.850	6.709	208.4E6	2507.2E6	79.764	80.361
18)	B Endrin al...	6.031	6.841	165.0E6	1961.1E6	80.278	81.302
19)	B Endosulfa...	6.255	7.074	195.3E6	1850.1E6	79.950	71.327
21)	B Endrin ke...	6.764	7.563	234.1E6	2253.6E6	80.429	80.356


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD122222\
Data File : PD073420.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Dec 2022 20:06
Operator : AR\AJ
Sample : INDB401
Misc :
ALS Vial : 17 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 22 04:01:32 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD122222CLP-TCLP.M
Quant Title : GC Extractables
QLast Update : Thu Dec 22 04:01:21 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

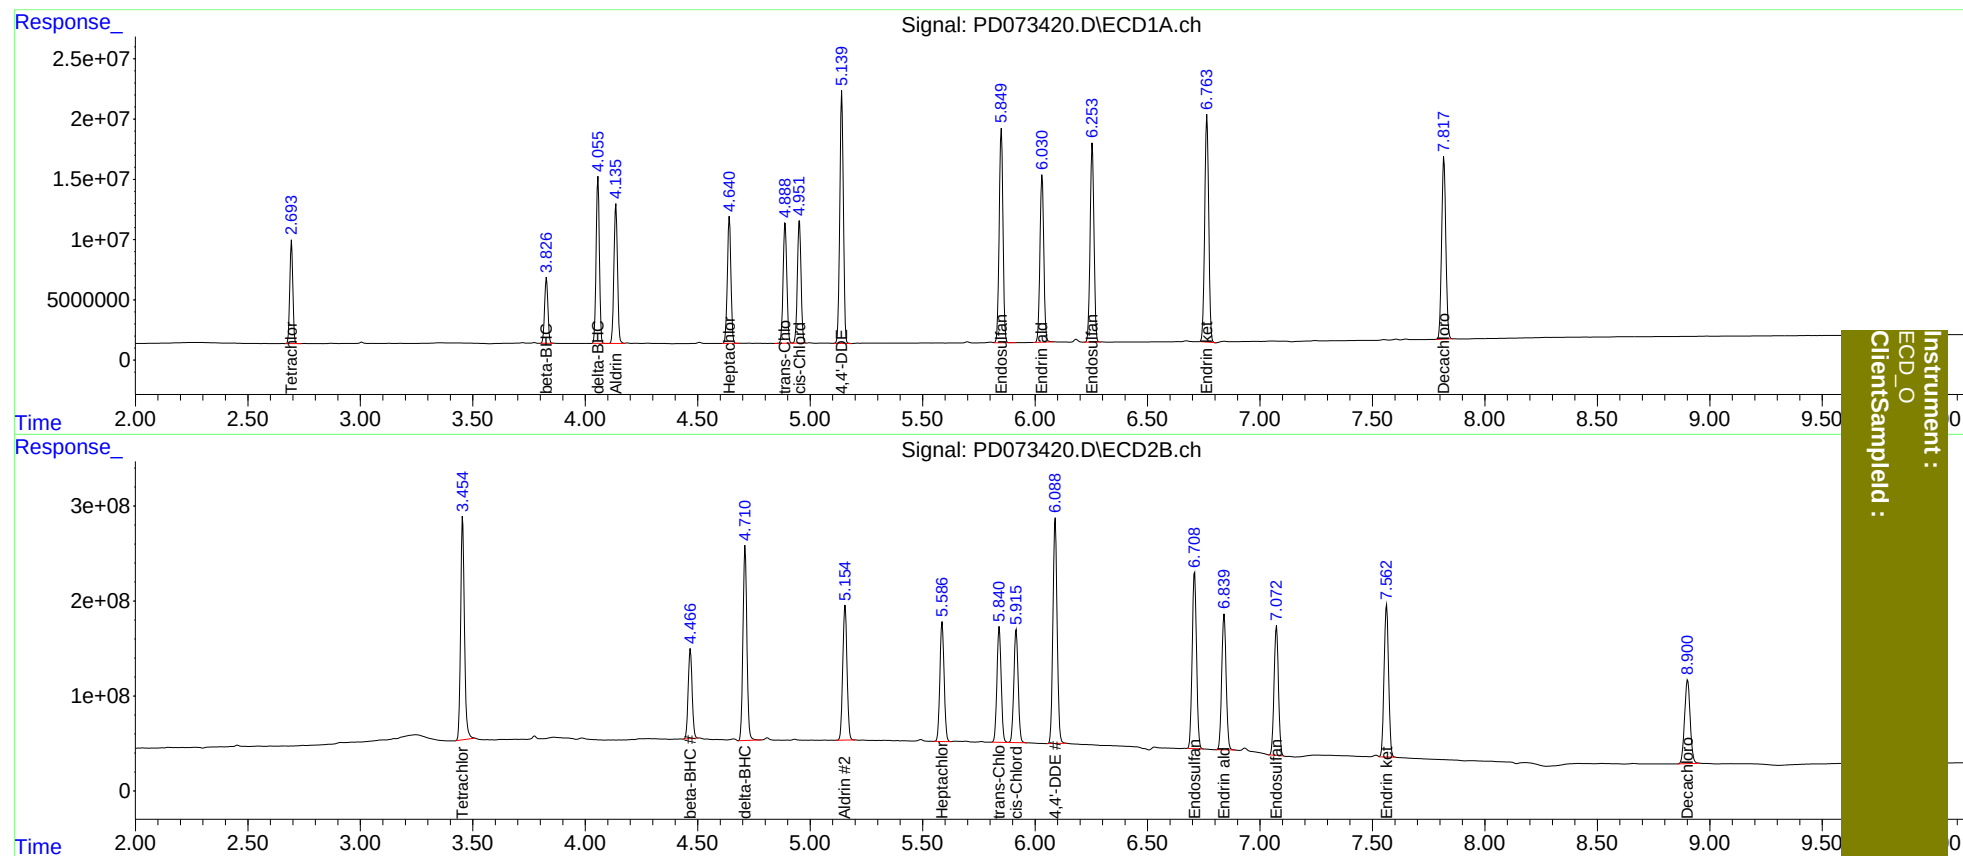


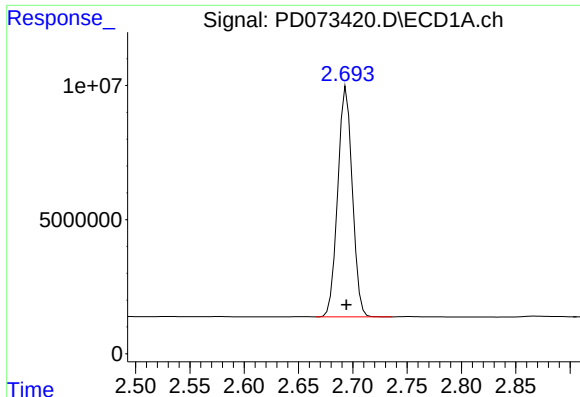

#1 Tetrachloro-m-xylene


R.T.: 2.694 min
Delta R.T.: 0.000 min
Response: 79972965
Conc: 39.89 ng/ml

Instrument :
ECD_O
ClientSampleId :

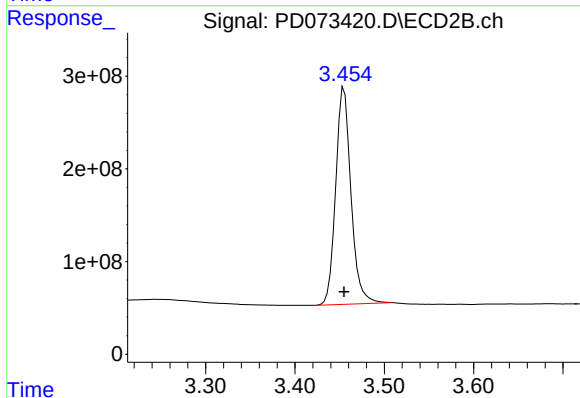


#1 Tetrachloro-m-xylene

R.T.: 3.455 min
Delta R.T.: 0.000 min
Response: 2786201347
Conc: 38.05 ng/ml

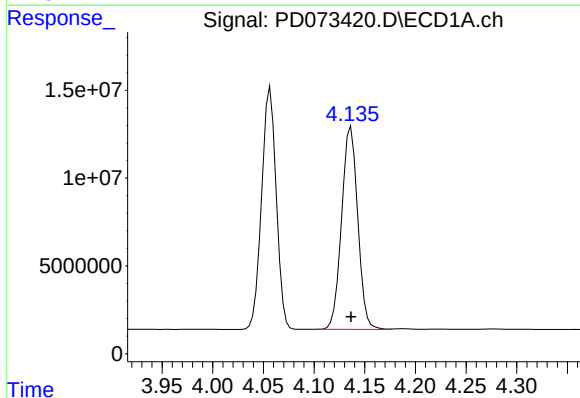


#5 Aldrin

R.T.: 4.137 min
Delta R.T.: 0.000 min
Response: 127698009
Conc: 39.52 ng/ml

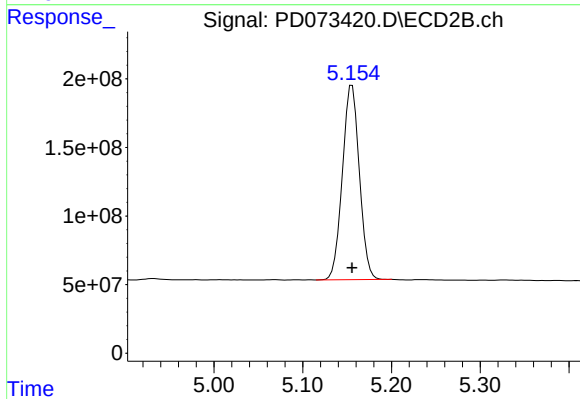

#5 Aldrin


R.T.: 5.156 min
Delta R.T.: 0.000 min
Response: 1884408591
Conc: 39.89 ng/ml

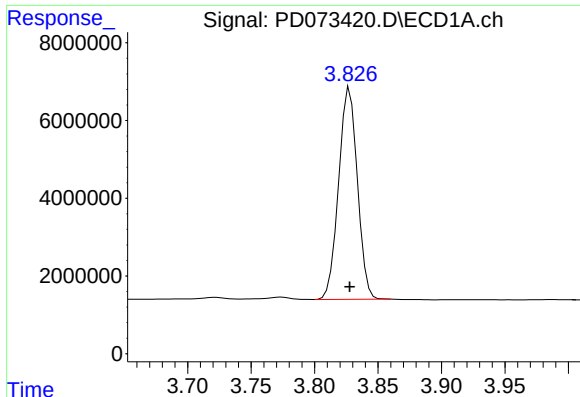

#6 beta-BHC


R.T.: 3.828 min
Delta R.T.: 0.000 min
Response: 56037242
Conc: 40.10 ng/ml

Instrument :
ECD_O
ClientSampleId :

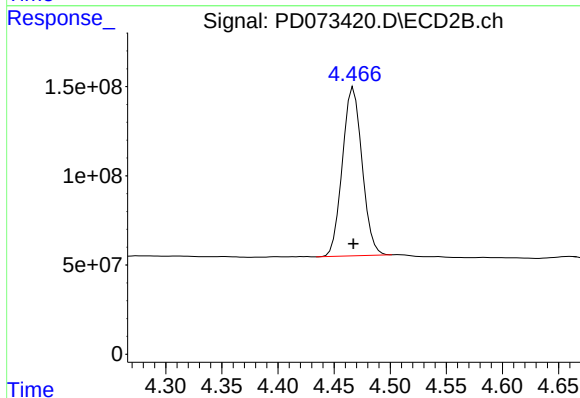


#6 beta-BHC

R.T.: 4.467 min
Delta R.T.: 0.000 min
Response: 1153313492
Conc: 40.58 ng/ml

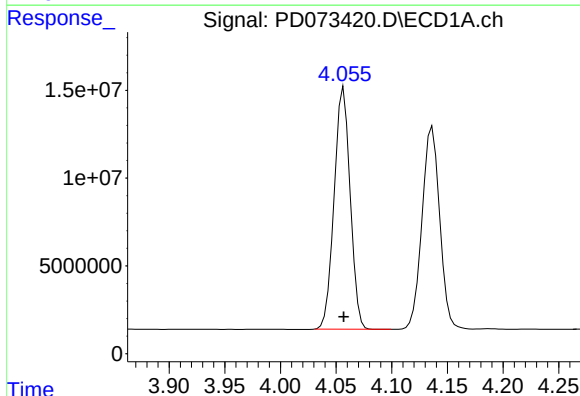


#7 delta-BHC

R.T.: 4.057 min
Delta R.T.: 0.000 min
Response: 138092272
Conc: 39.09 ng/ml

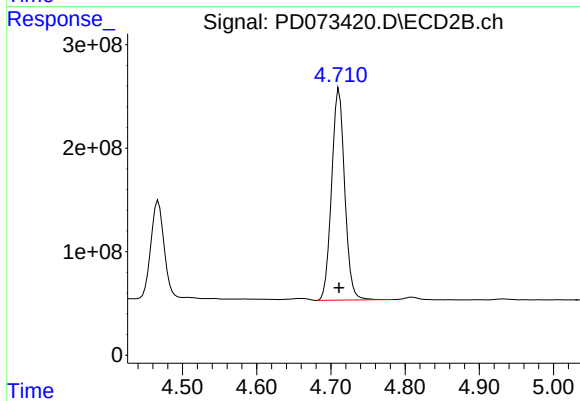

#7 delta-BHC


R.T.: 4.711 min
Delta R.T.: 0.000 min
Response: 2504401215
Conc: 38.40 ng/ml

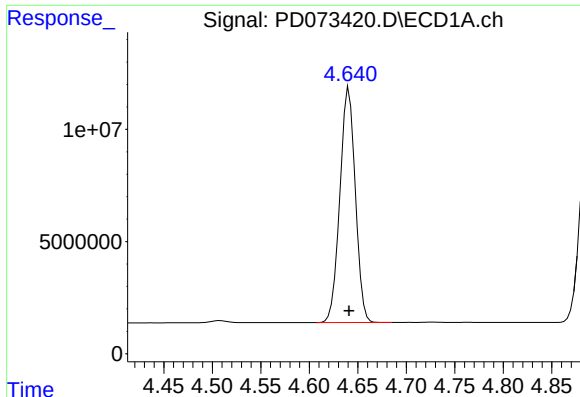

#8 Heptachlor epoxide


R.T.: 4.641 min
Delta R.T.: 0.000 min
Response: 115741786
Conc: 39.64 ng/ml

Instrument :
ECD_O
ClientSampleId :

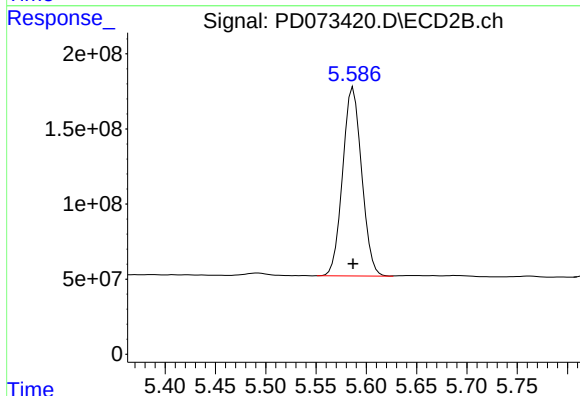


#8 Heptachlor epoxide

R.T.: 5.587 min
Delta R.T.: 0.000 min
Response: 1651440504
Conc: 39.77 ng/ml

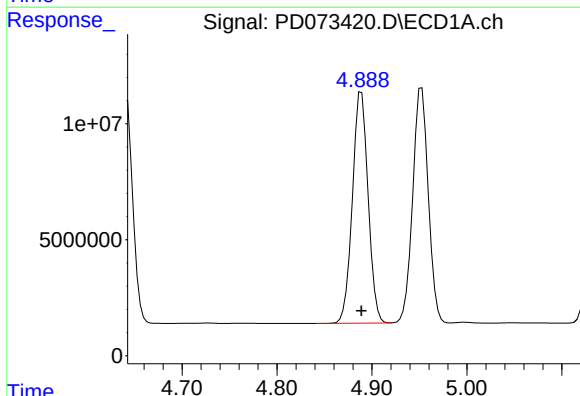


#10 trans-Chlordane

R.T.: 4.889 min
Delta R.T.: 0.000 min
Response: 114531597
Conc: 39.27 ng/ml

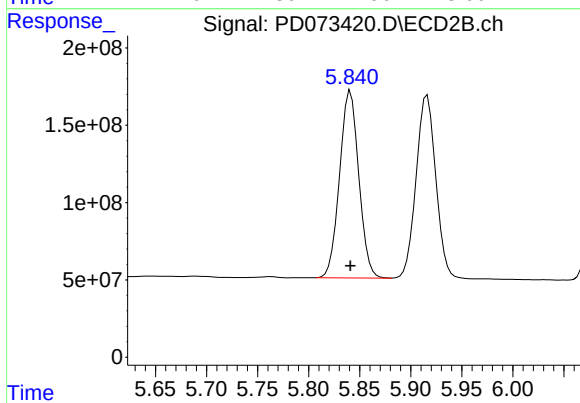

#10 trans-Chlordane


R.T.: 5.841 min
Delta R.T.: 0.000 min
Response: 1589200779
Conc: 39.63 ng/ml

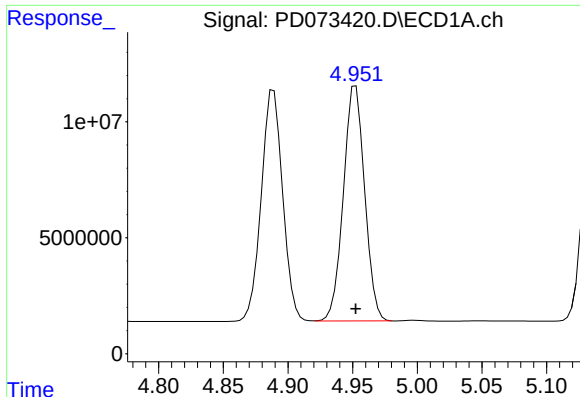

#11 cis-Chlordane


R.T.: 4.952 min
Delta R.T.: 0.000 min
Response: 115744494
Conc: 39.44 ng/ml

Instrument :
ECD_O
ClientSampleId :

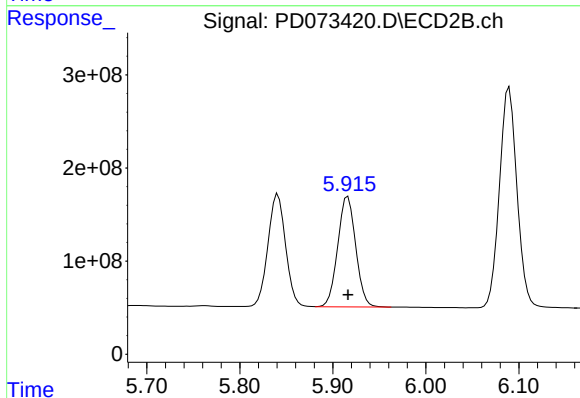


#11 cis-Chlordane

R.T.: 5.916 min
Delta R.T.: 0.000 min
Response: 1593527644
Conc: 39.80 ng/ml

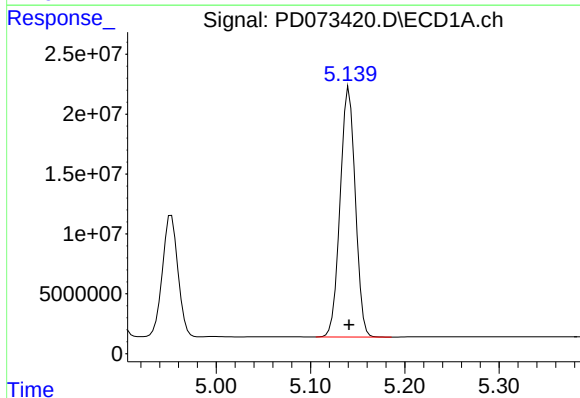


#12 4,4'-DDE

R.T.: 5.141 min
Delta R.T.: 0.000 min
Response: 233353204
Conc: 78.90 ng/ml

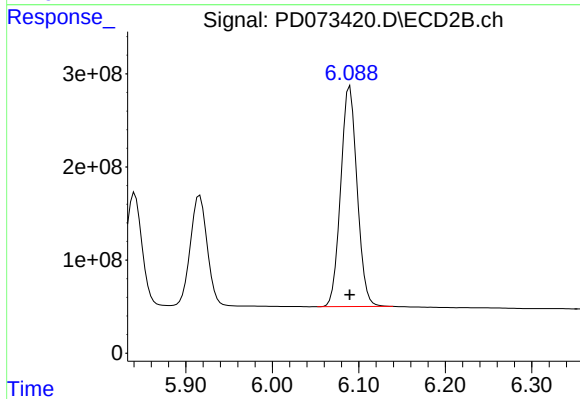

#12 4,4'-DDE


R.T.: 6.090 min
Delta R.T.: 0.000 min
Response: 3098582937
Conc: 77.41 ng/ml

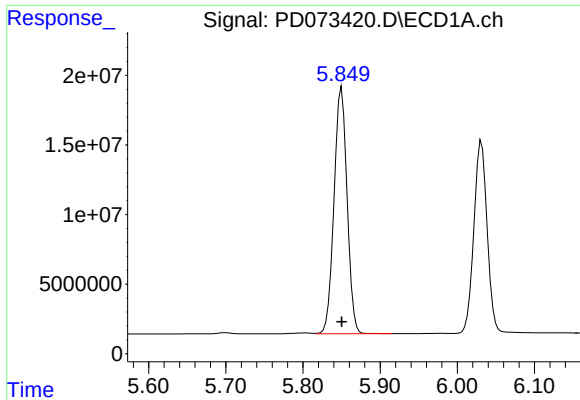

#15 Endosulfan II


R.T.: 5.850 min
Delta R.T.: 0.000 min
Response: 208350829
Conc: 79.76 ng/ml

Instrument :
ECD_O
ClientSampleId :

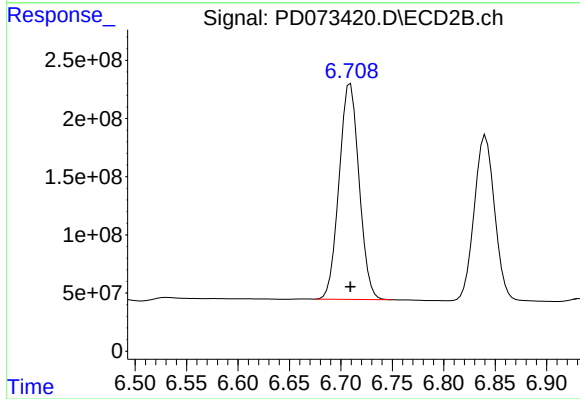


#15 Endosulfan II

R.T.: 6.709 min
Delta R.T.: 0.000 min
Response: 2507190259
Conc: 80.36 ng/ml

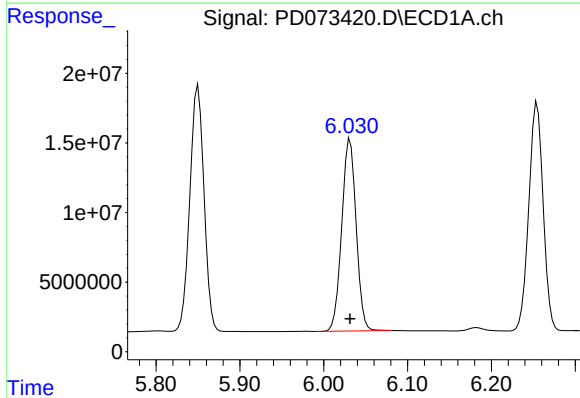


#18 Endrin aldehyde

R.T.: 6.031 min
Delta R.T.: 0.000 min
Response: 165000823
Conc: 80.28 ng/ml

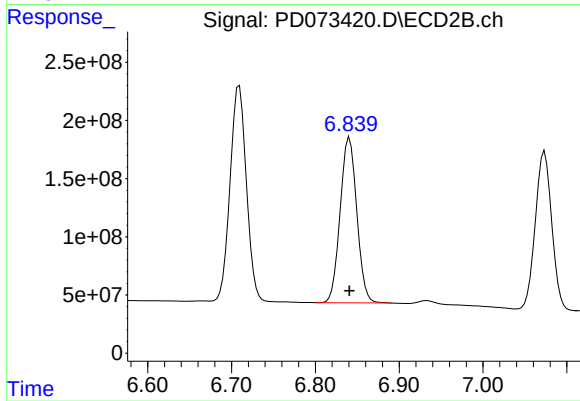

#18 Endrin aldehyde


R.T.: 6.841 min
Delta R.T.: 0.000 min
Response: 1961059184
Conc: 81.30 ng/ml

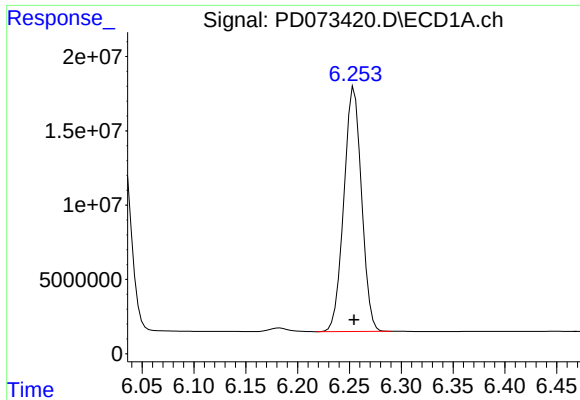

#19 Endosulfan Sulfate


R.T.: 6.255 min
Delta R.T.: 0.000 min
Response: 195323749
Conc: 79.95 ng/ml

Instrument :
ECD_O
ClientSampleId :

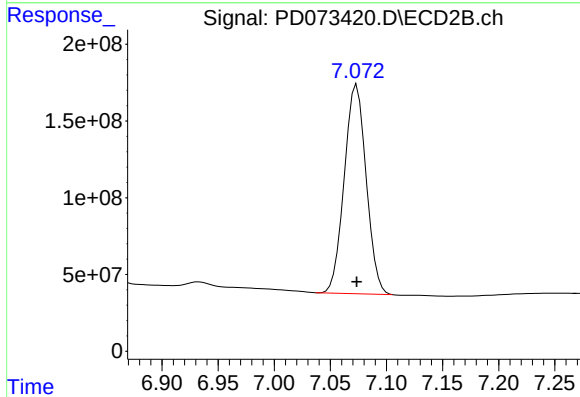


#19 Endosulfan Sulfate

R.T.: 7.074 min
Delta R.T.: 0.000 min
Response: 1850125916
Conc: 71.33 ng/ml

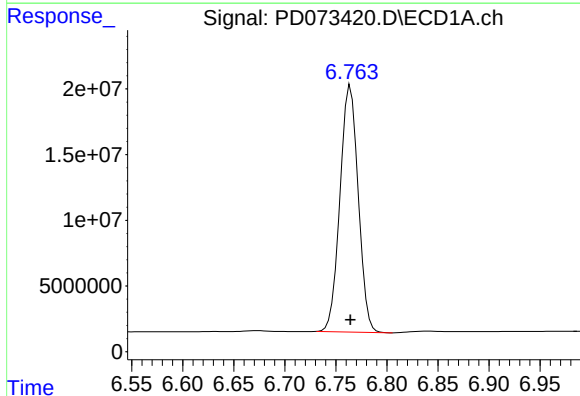


#21 Endrin ketone

R.T.: 6.764 min
Delta R.T.: 0.000 min
Response: 234131081
Conc: 80.43 ng/ml

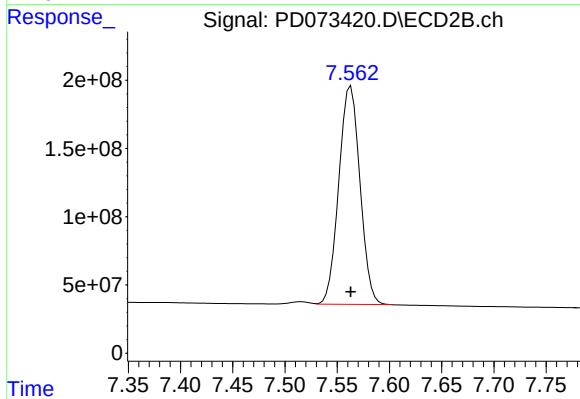

#21 Endrin ketone


R.T.: 7.563 min
Delta R.T.: 0.000 min
Response: 2253563042
Conc: 80.36 ng/ml

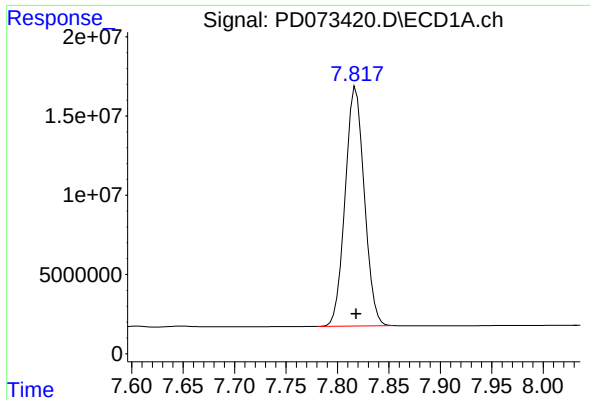

#27 Decachlorobiphenyl

R.T.: 7.818 min
Delta R.T.: 0.000 min
Response: 195595681
Conc: 80.21 ng/ml

Instrument :
ECD_O
ClientSampleId :

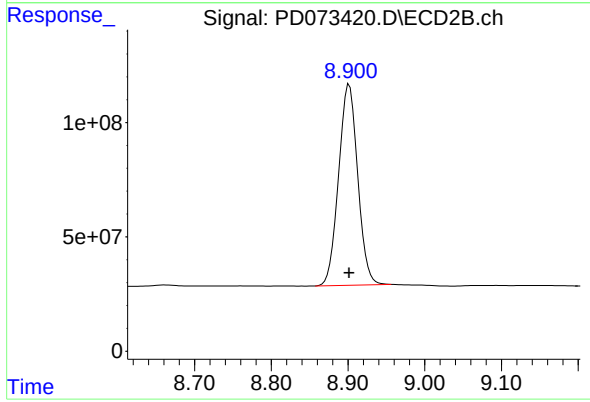

#27 Decachlorobiphenyl

R.T.: 8.902 min
Delta R.T.: 0.000 min
Response: 1524257316
Conc: 80.76 ng/ml