

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD122222\
 Data File : PD073421.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Dec 2022 20:19
 Operator : AR\AJ
 Sample : INDA501
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 22 03:04:34 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD122222CLP-TCLP.M
 Quant Title : GC Extractables
 QLast Update : Thu Dec 22 03:04:23 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	2.694	3.455	167.7E6	5667.1E6	79.387	74.463
27)	SA Decachlor...	7.820	8.901	384.3E6	2954.1E6	157.542	156.961
Target Compounds							
2)	A alpha-BHC	3.196	3.919	293.3E6	8575.5E6	81.463	68.346
3)	MA gamma-BHC...	3.526	4.252	271.1E6	6361.6E6	81.351	72.771
4)	MA Heptachlor	3.858	4.818	273.7E6	4203.7E6	81.056	76.463
9)	A Endosulfan I	5.010	5.972	223.7E6	2910.5E6	80.470	77.508
13)	MA Dieldrin	5.276	6.249	512.1E6	6536.1E6	163.540	170.321
14)	MA Endrin	5.552	6.481	430.8E6	4993.8E6	161.115	155.085
16)	A 4,4'-DDD	5.699	6.615	402.0E6	4818.7E6	162.741	156.815
17)	MA 4,4'-DDT	5.948	6.922	412.9E6	4618.8E6	162.911	155.830
20)	A Methoxychlor	6.530	7.402	1030.7E6	8875.4E6	794.870	780.507

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD122222\
Data File : PD073421.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Dec 2022 20:19
Operator : AR\AJ
Sample : INDA501
Misc :
ALS Vial : 18 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 22 03:04:34 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD122222CLP-TCLP.M
Quant Title : GC Extractables
QLast Update : Thu Dec 22 03:04:23 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

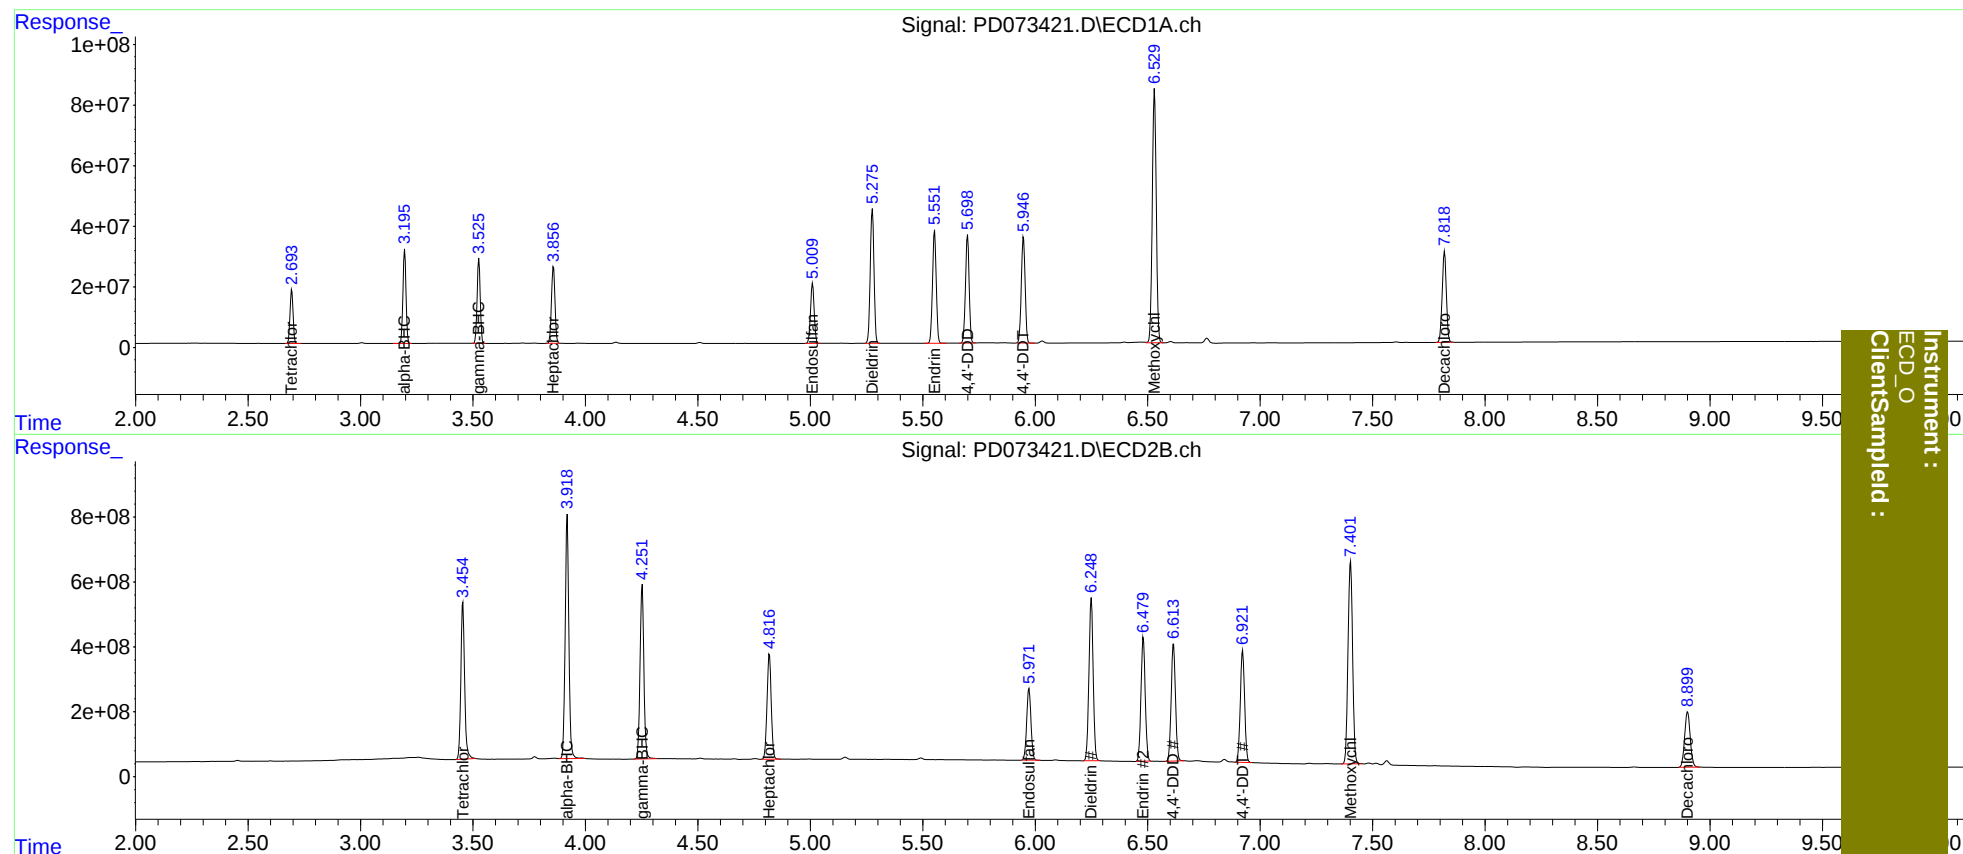

Instrument :
ECD_O
ClientSampled :
0