

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD122222\
 Data File : PD073423.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Dec 2022 20:45
 Operator : AR\AJ
 Sample : INDA601
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 22 03:02:06 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD122222CLP-TCLP.M
 Quant Title : GC Extractables
 QLast Update : Thu Dec 22 03:01:53 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	2.694	3.456	332.4E6	12542.9E6	156.723	159.297
27)	SA Decachlor...	7.819	8.901	749.5E6	5757.5E6	304.927	303.038
Target Compounds							
2)	A alpha-BHC	3.196	3.926	600.9E6	25128.9E6	168.469	186.680
3)	MA gamma-BHC...	3.526	4.254	553.9E6	15084.2E6	167.620	165.089
4)	MA Heptachlor	3.858	4.818	546.2E6	8149.7E6	162.812	145.033
9)	A Endosulfan I	5.010	5.972	443.0E6	5619.1E6	159.817	147.344
13)	MA Dieldrin	5.275	6.255	1005.9E6	9895.8E6	324.803	266.466
14)	MA Endrin	5.552	6.481	848.7E6	9742.5E6	318.557	297.983
16)	A 4,4'-DDD	5.698	6.615	791.9E6	9465.3E6	323.334	304.996
17)	MA 4,4'-DDT	5.947	6.922	830.4E6	9331.8E6	330.620	310.785
20)	A Methoxychlor	6.530	7.402	1961.2E6	15899.8E6	1507.665	1381.405

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD122222\
Data File : PD073423.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Dec 2022 20:45
Operator : AR\AJ
Sample : INDA601
Misc :
ALS Vial : 20 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 22 03:02:06 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD122222CLP-TCLP.M
Quant Title : GC Extractables
QLast Update : Thu Dec 22 03:01:53 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

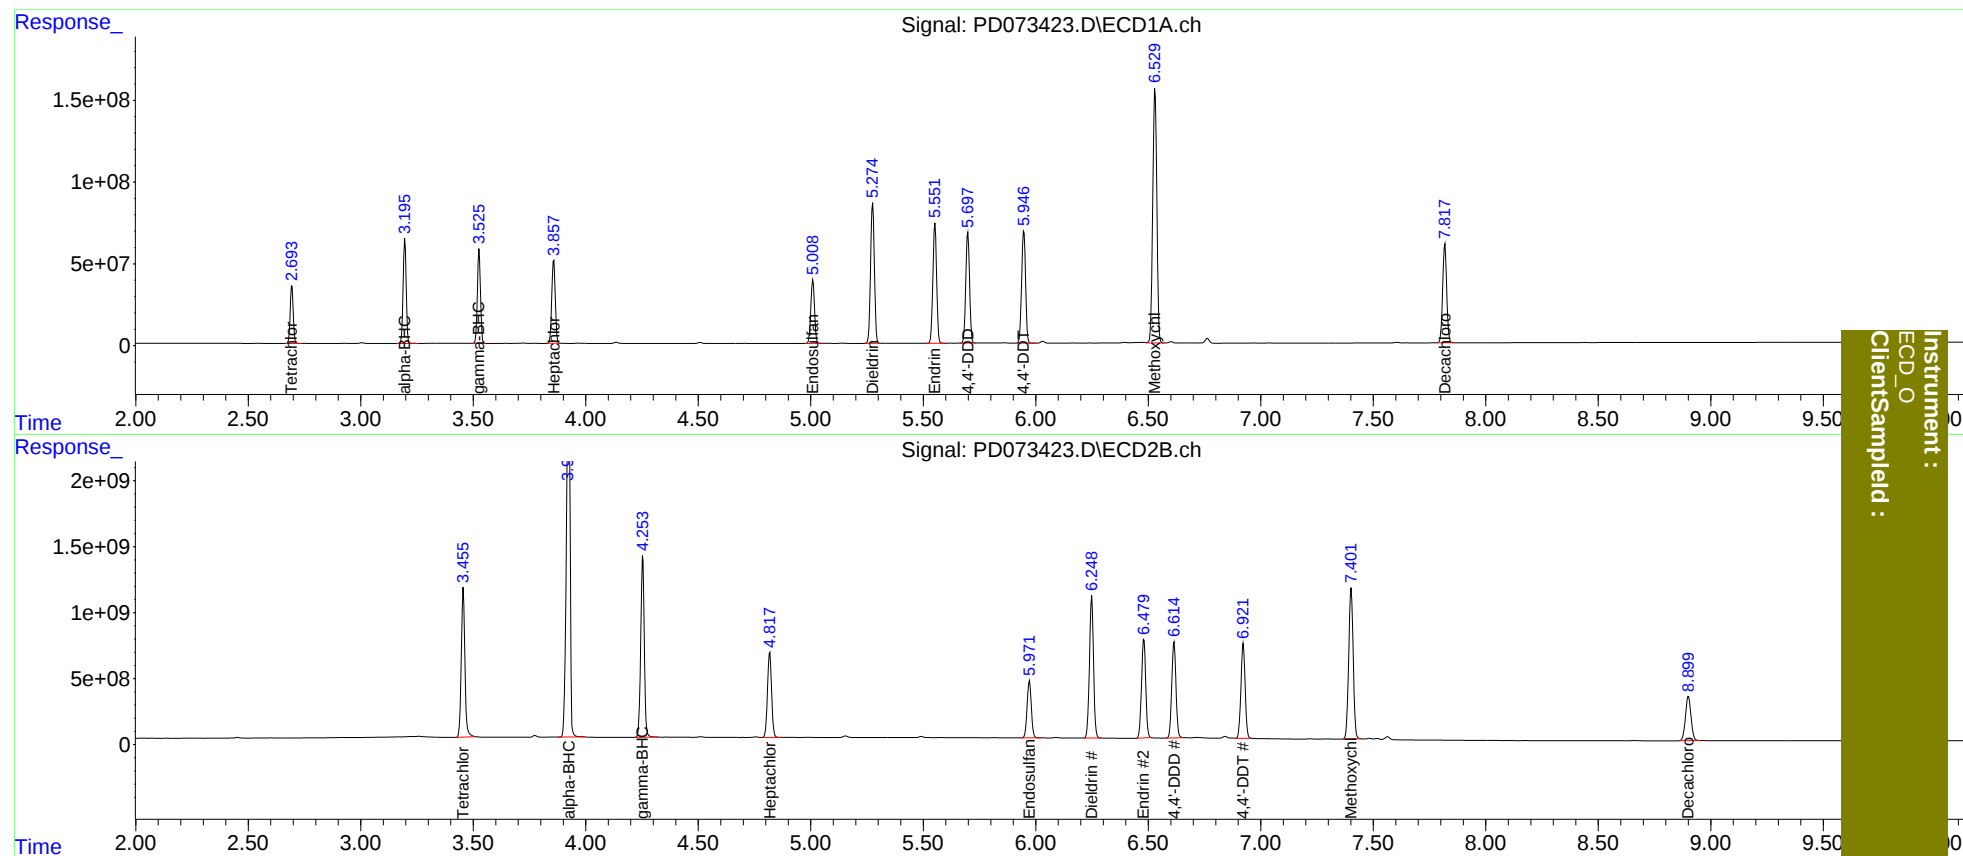

Instrument :
ECD_O
ClientSampled :
0