

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO122123\
 Data File : PO100627.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Dec 2023 14:38
 Operator : YP/AJ
 Sample : 05968-03 10X
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 KZZ246M-END-1-1

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 12/22/2023
 Supervised By :Ankita Jodhani 12/22/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 21 15:12:21 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO122023.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Dec 21 04:28:19 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.349	3.646	3925509	3129112	1.258m	1.531
2) SA Decachlor...	10.090	8.706	3913916	2187753	1.873	1.449m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO122123\
Data File : PO100627.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Dec 2023 14:38
Operator : YP/AJ
Sample : 05968-03 10X
Misc :
ALS Vial : 11 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
KZZ246M-END-1-1


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 12/22/2023
Supervised By :Ankita Jodhani 12/22/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 21 15:12:21 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO122023.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Dec 21 04:28:19 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

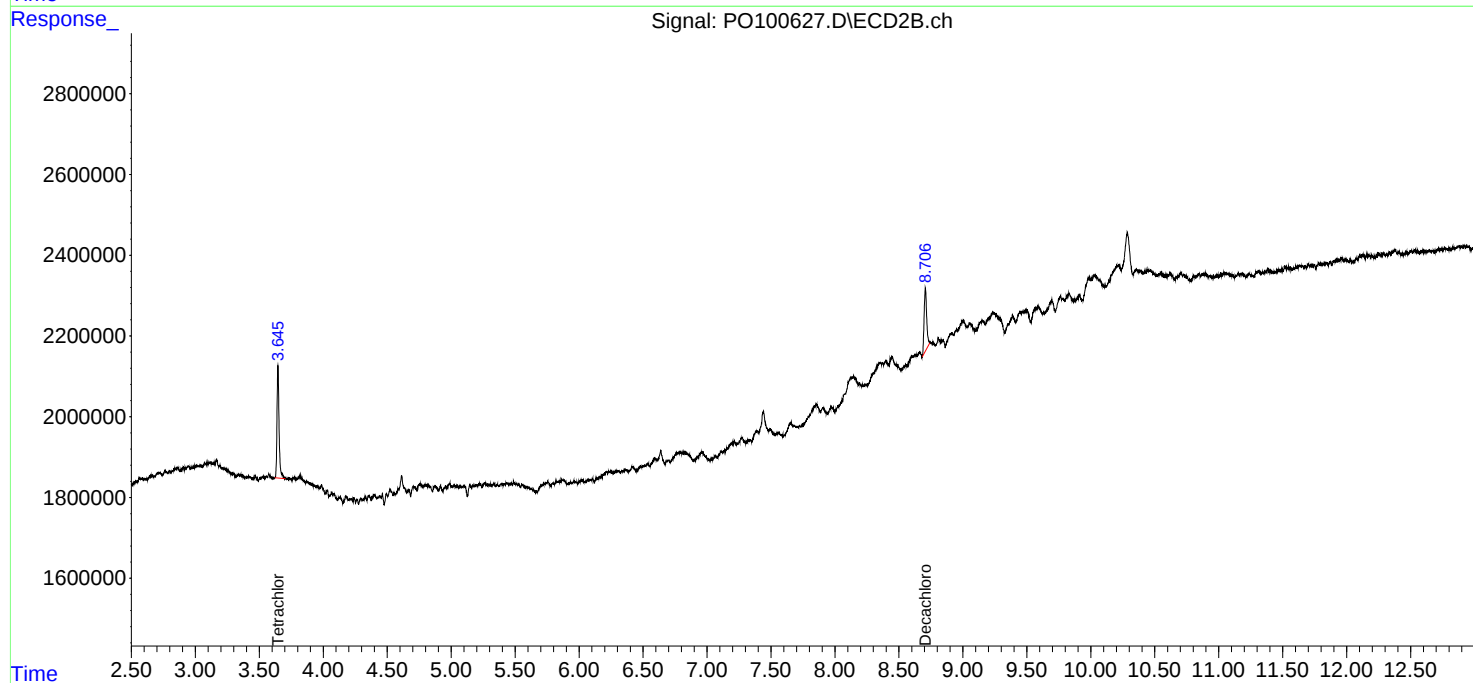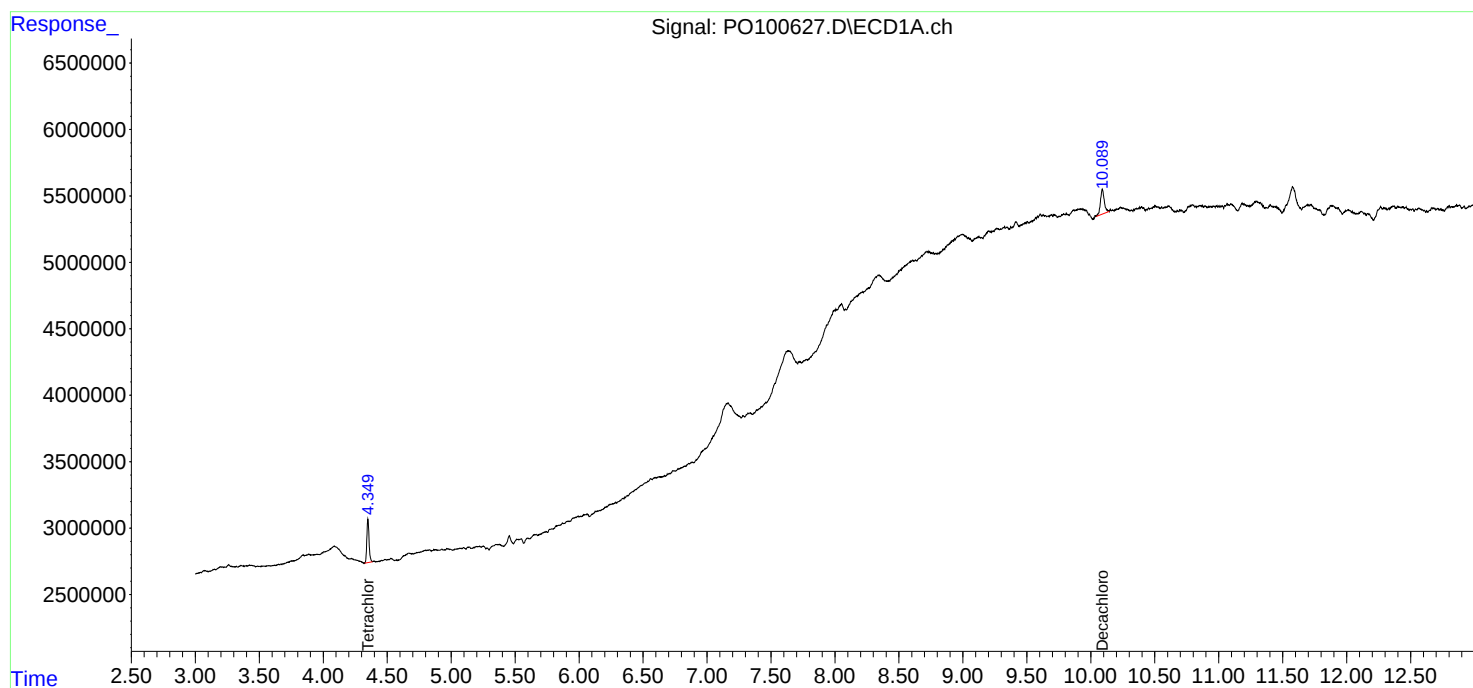

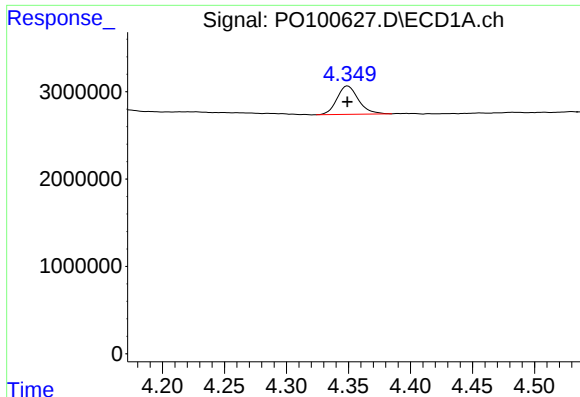


#1 Tetrachloro-m-xylene

R.T.: 4.349 min
Delta R.T.: 0.000 min
Response: 3925509
Conc: 1.26 ng/ml

Instrument :
ECD_O
ClientSampleId :
KZZ246M-END-1-1


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 12/22/2023
Supervised By :Ankita Jodhani 12/22/2023

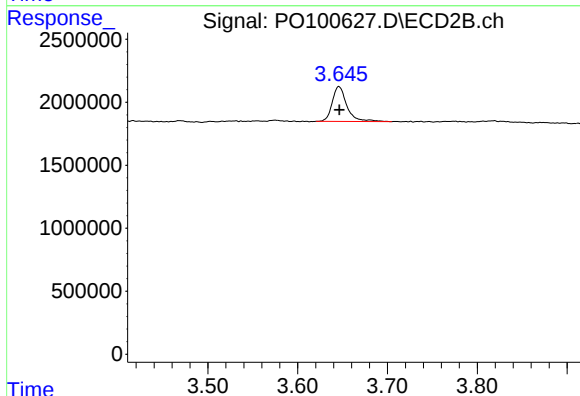


#1 Tetrachloro-m-xylene

R.T.: 3.646 min
Delta R.T.: 0.000 min
Response: 3129112
Conc: 1.53 ng/ml

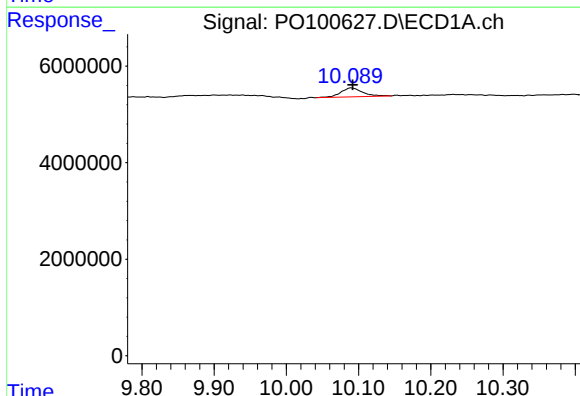

#2 Decachlorobiphenyl

R.T.: 10.090 min
Delta R.T.: -0.002 min
Response: 3913916
Conc: 1.87 ng/ml

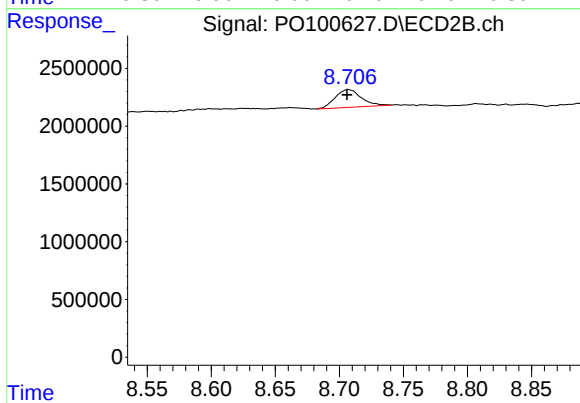

#2 Decachlorobiphenyl

R.T.: 8.706 min
Delta R.T.: 0.000 min
Response: 2187753
Conc: 1.45 ng/ml m