

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO122218\
 Data File : PO052916.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 24 Dec 2018 5:56
 Operator : SM/SJ
 Sample : J6505-09
 Misc :
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 SB-61(0-23)-COMP

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 24 06:47:30 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO122118.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Dec 24 02:43:03 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.240	3.267	22545231	4948938	16.383	16.722
2) SA Decachlor...	9.773	7.942	9455190	3971418	13.487	14.111

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO122218\
Data File : PO052916.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 24 Dec 2018 5:56
Operator : SM/SJ
Sample : J6505-09
Misc :
ALS Vial : 42 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
SB-61(0-23)-COMP

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 24 06:47:30 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO122118.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Dec 24 02:43:03 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

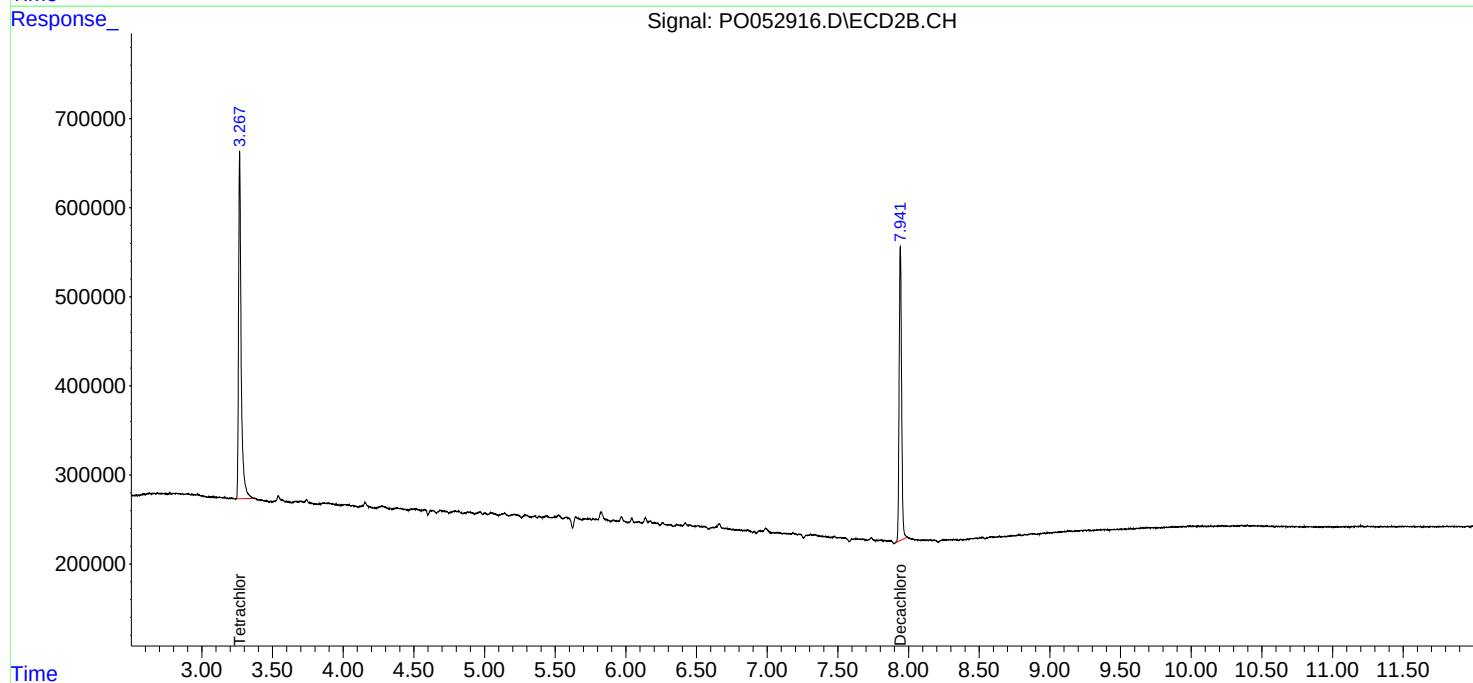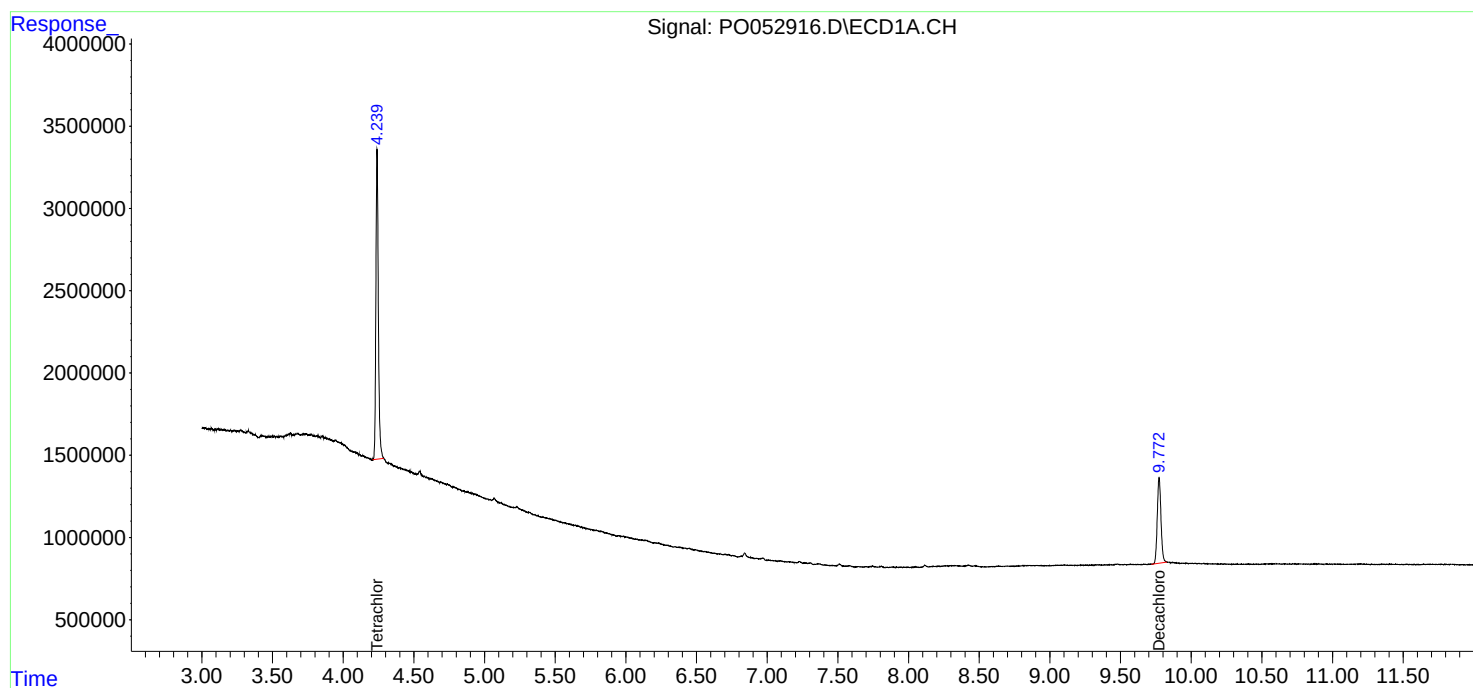


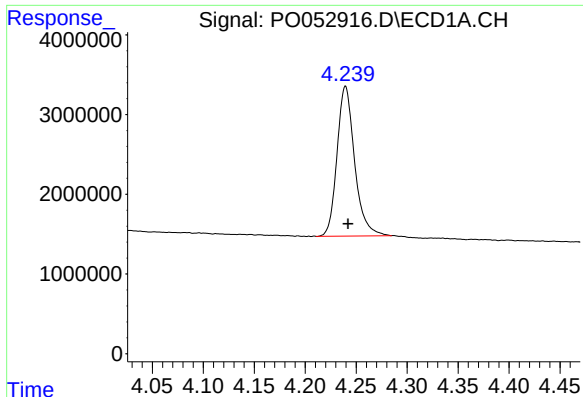

#1 Tetrachloro-m-xylene


R.T.: 4.240 min
Delta R.T.: -0.002 min
Response: 22545231
Conc: 16.38 ng/ml

Instrument :
ECD_O
ClientSampleId :
SB-61(0-23)-COMP

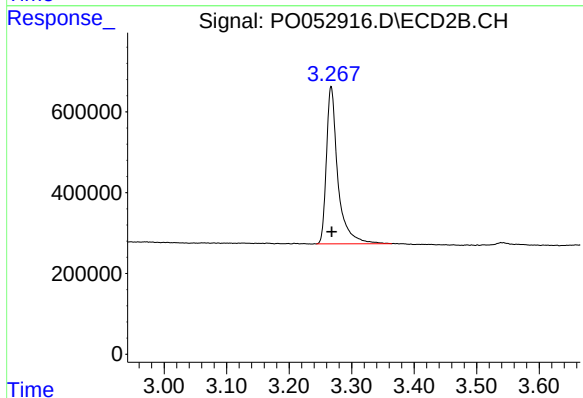


#1 Tetrachloro-m-xylene

R.T.: 3.267 min
Delta R.T.: 0.000 min
Response: 4948938
Conc: 16.72 ng/ml

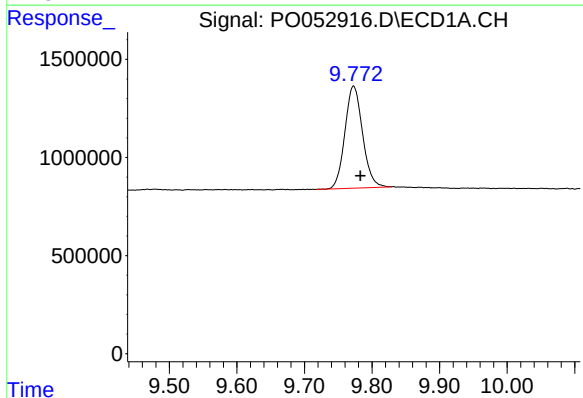

#2 Decachlorobiphenyl

R.T.: 9.773 min
Delta R.T.: -0.010 min
Response: 9455190
Conc: 13.49 ng/ml

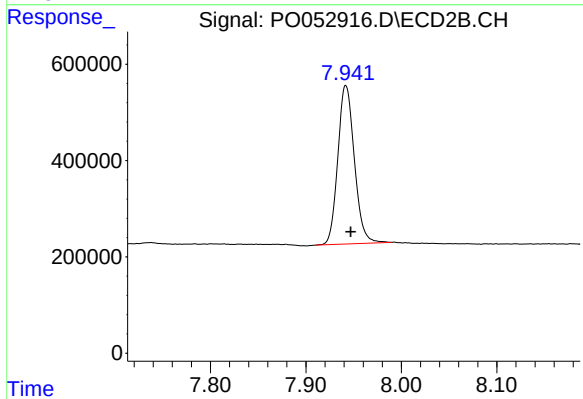

#2 Decachlorobiphenyl

R.T.: 7.942 min
Delta R.T.: -0.005 min
Response: 3971418
Conc: 14.11 ng/ml