

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0122220\
 Data File : P0074040.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 22 Dec 2020 18:25
 Operator : DD\AJ
 Sample : L5193-04
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 LLEXSITUTV-022-001-SO

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 23 08:09:34 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0121020.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Dec 11 03:58:06 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.934	3.993	2191729	1272978	23.972	23.733
2)	SA Decachlor...	10.957	9.256	1958092	1099747	23.694	23.504
Target Compounds							
8)	L2 AR-1221-1	5.190	0.000	115315	0	108.836	N.D. #
9)	L2 AR-1221-2	5.289	0.000	26396	0	33.604	N.D. #
29)	L6 AR-1254-4	8.080	0.000	7266	0	1.385	N.D. #
30)	L6 AR-1254-5	8.515	0.000	12243	0	2.377	N.D. #
32)	L7 AR-1260-2	8.216	0.000	3364	0	0.599	N.D. #
34)	L7 AR-1260-4	8.849f	0.000	13736	0	2.901	N.D. #
39)	L8 AR-1262-4	9.522f	0.000	27340	0	8.174	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO122220\
Data File : PO074040.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 22 Dec 2020 18:25
Operator : DD\AJ
Sample : L5193-04
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
LLEXSITUTV-022-001-SO

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 23 08:09:34 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO121020.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Dec 11 03:58:06 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

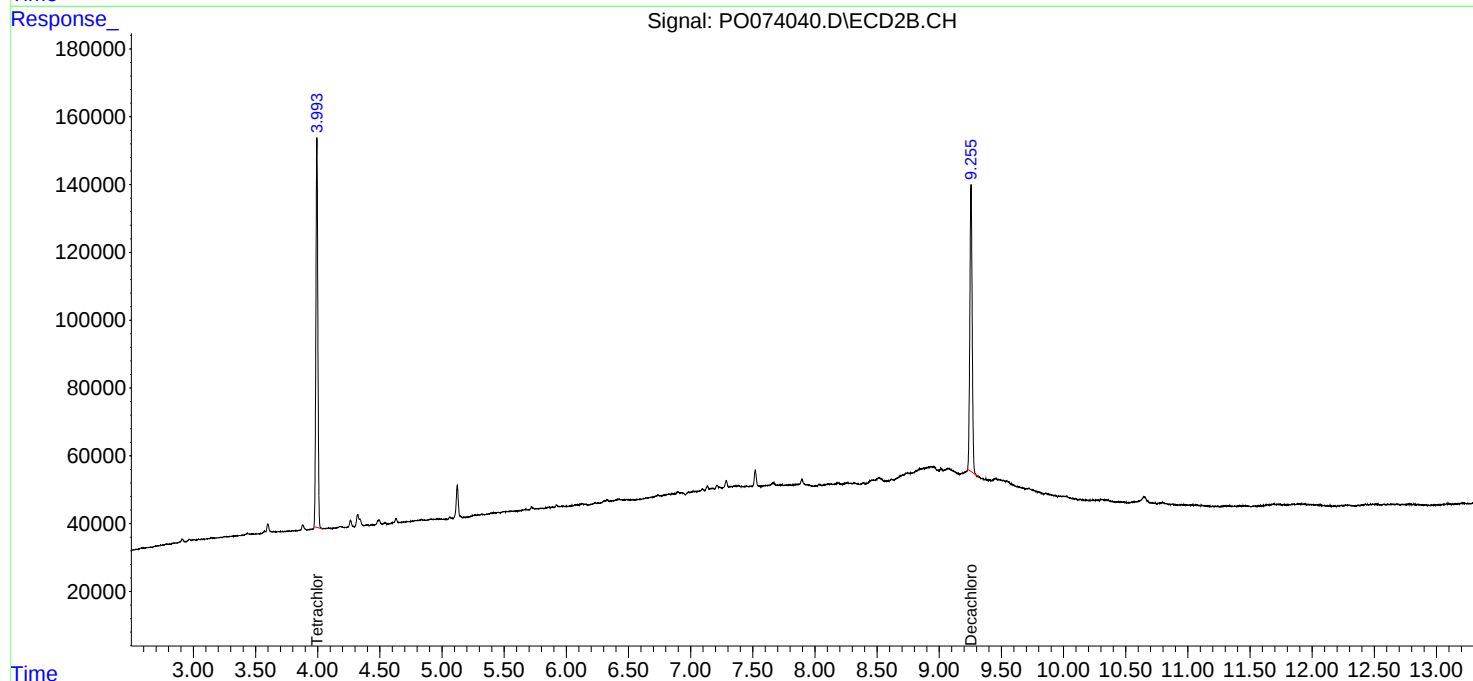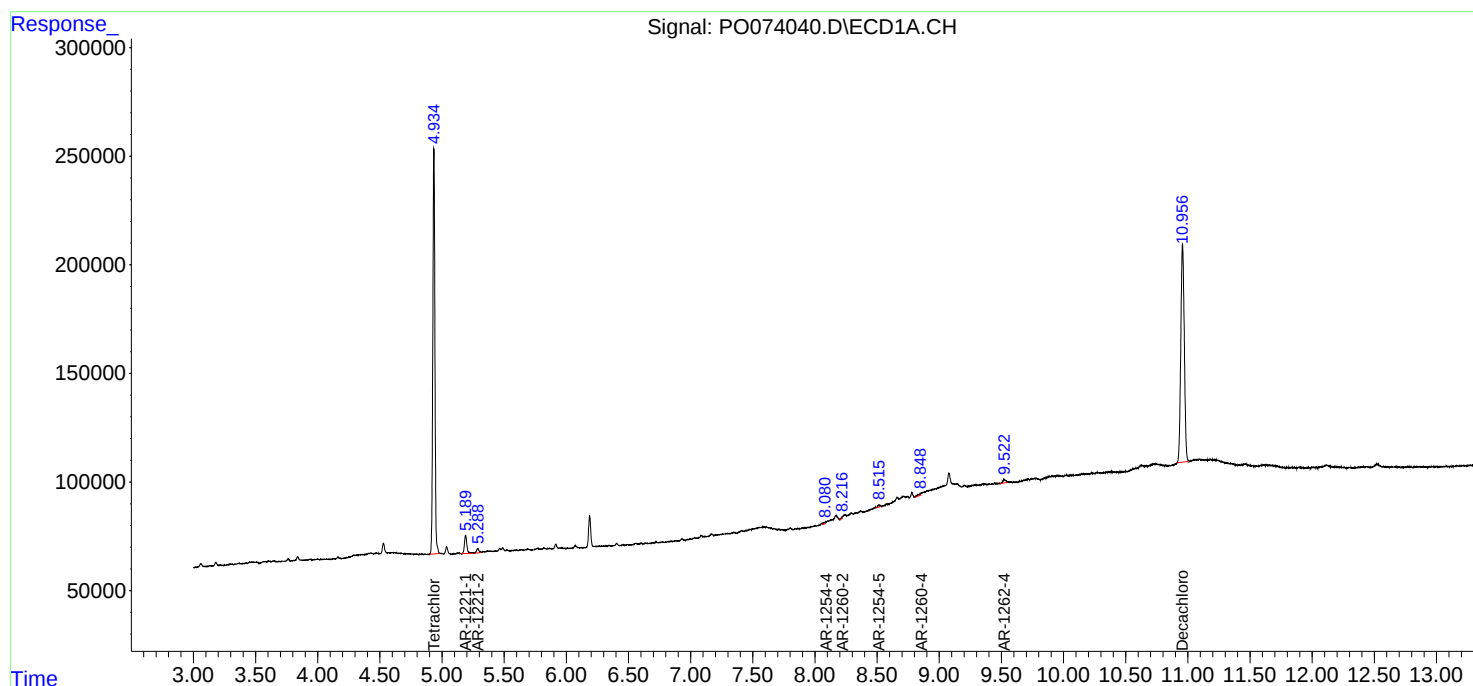


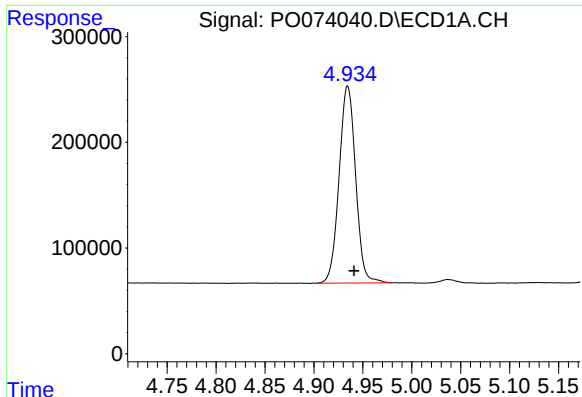

#1 Tetrachloro-m-xylene


R.T.: 4.934 min
Delta R.T.: -0.007 min
Response: 2191729
Conc: 23.97 ng/ml

Instrument :
ECD_O
ClientSampleId :
LLEXSITUTV-022-001-SO

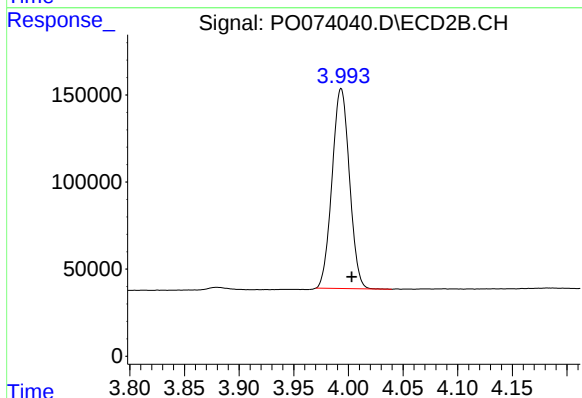


#1 Tetrachloro-m-xylene

R.T.: 3.993 min
Delta R.T.: -0.010 min
Response: 1272978
Conc: 23.73 ng/ml

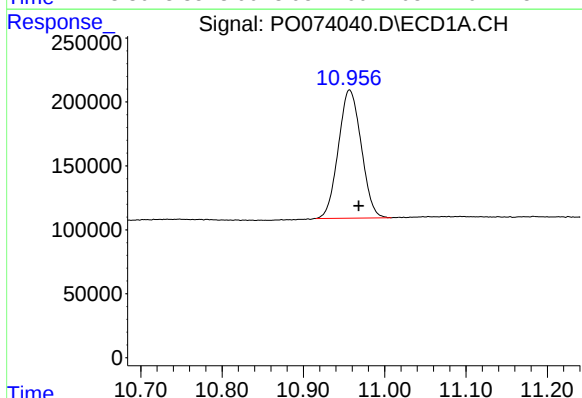


#2 Decachlorobiphenyl

R.T.: 10.957 min
Delta R.T.: -0.011 min
Response: 1958092
Conc: 23.69 ng/ml

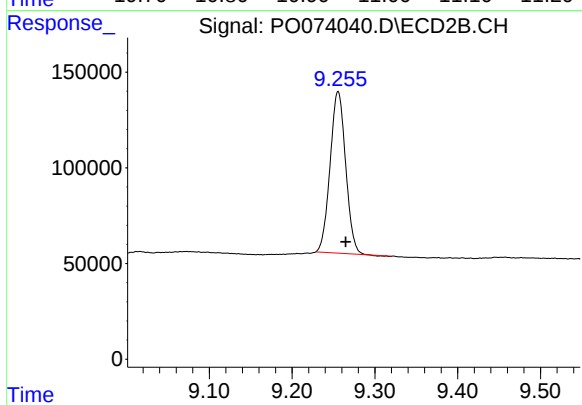

#2 Decachlorobiphenyl


R.T.: 9.256 min
Delta R.T.: -0.009 min
Response: 1099747
Conc: 23.50 ng/ml

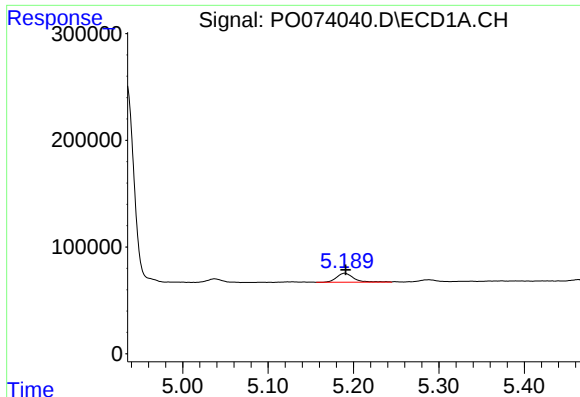

#8 AR-1221-1


R.T.: 5.190 min
Delta R.T.: -0.001 min
Response: 115315
Conc: 108.84 ng/ml

Instrument :
ECD_O
ClientSampleId :
LLEXSITUTV-022-001-SO

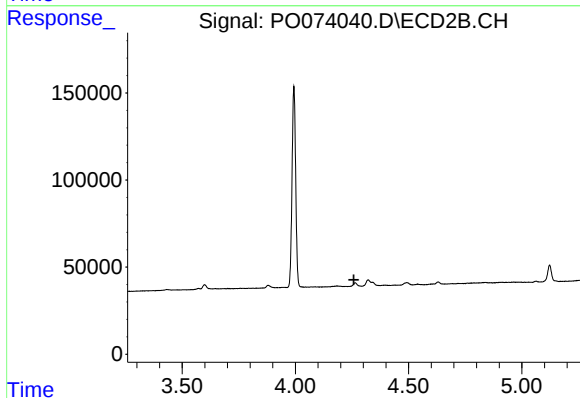


#8 AR-1221-1

R.T.: 0.000 min
Exp R.T. : 4.259 min
Response: 0
Conc: N.D.

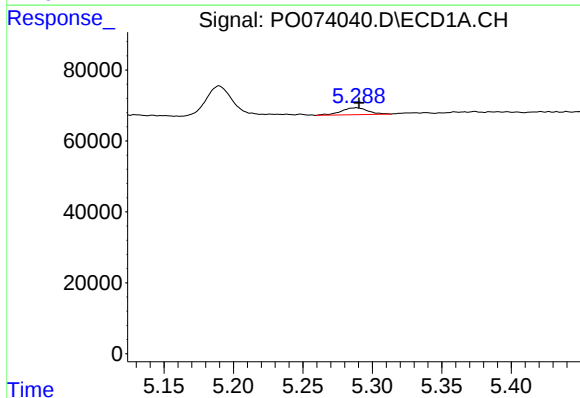


#9 AR-1221-2

R.T.: 5.289 min
Delta R.T.: -0.002 min
Response: 26396
Conc: 33.60 ng/ml

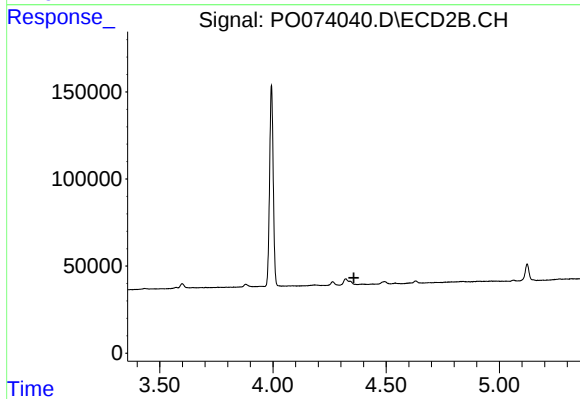

#9 AR-1221-2


R.T.: 0.000 min
Exp R.T. : 4.357 min
Response: 0
Conc: N.D.

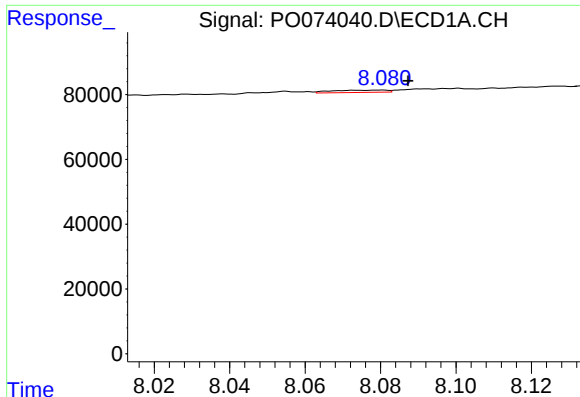

#29 AR-1254-4


R.T.: 8.080 min
Delta R.T.: -0.007 min
Response: 7266
Conc: 1.39 ng/ml

Instrument :
ECD_O
ClientSampleId :
LLEXSITUTV-022-001-SO

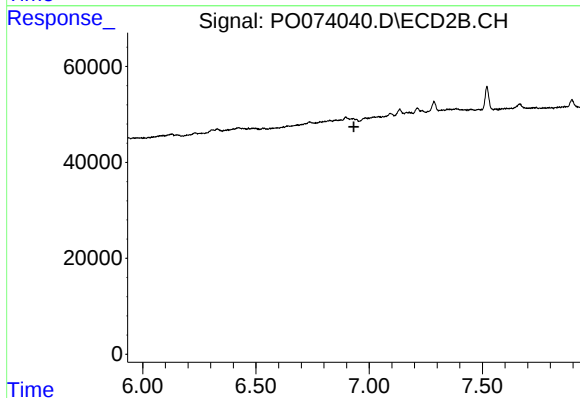


#29 AR-1254-4

R.T.: 0.000 min
Exp R.T. : 6.932 min
Response: 0
Conc: N.D.

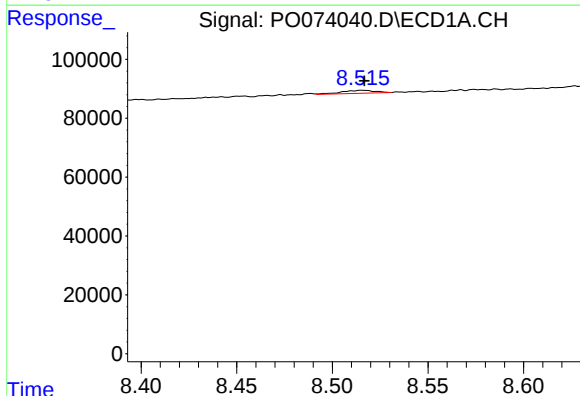


#30 AR-1254-5

R.T.: 8.515 min
Delta R.T.: -0.001 min
Response: 12243
Conc: 2.38 ng/ml

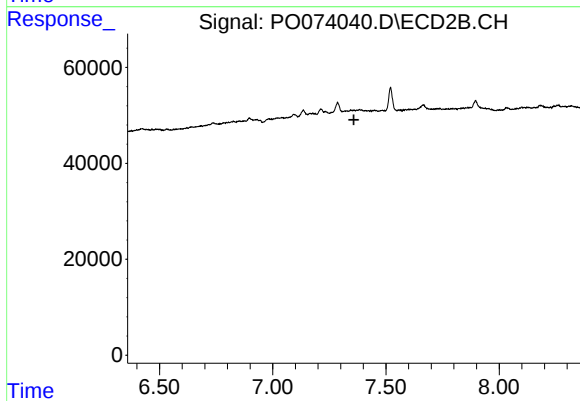

#30 AR-1254-5


R.T.: 0.000 min
Exp R.T. : 7.359 min
Response: 0
Conc: N.D.

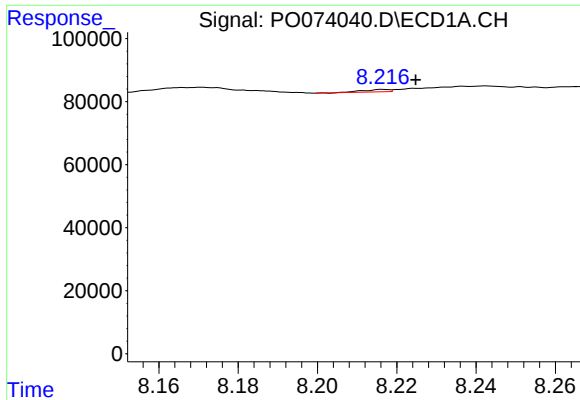

#32 AR-1260-2


R.T.: 8.216 min
Delta R.T.: -0.008 min
Response: 3364
Conc: 0.60 ng/ml

Instrument :
ECD_O
ClientSampleId :
LLEXSITUTV-022-001-SO

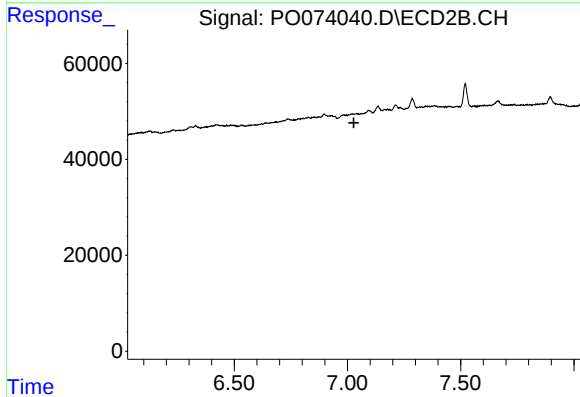


#32 AR-1260-2

R.T.: 0.000 min
Exp R.T. : 7.028 min
Response: 0
Conc: N.D.

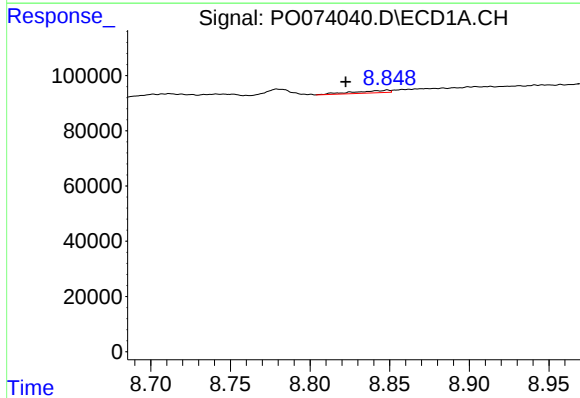


#34 AR-1260-4

R.T.: 8.849 min
Delta R.T.: 0.026 min
Response: 13736
Conc: 2.90 ng/ml

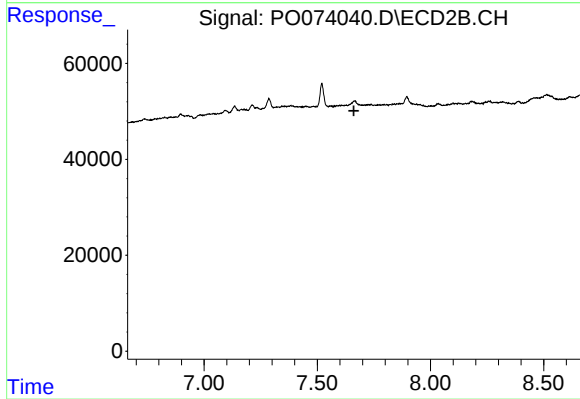

#34 AR-1260-4


R.T.: 0.000 min
Exp R.T. : 7.662 min
Response: 0
Conc: N.D.

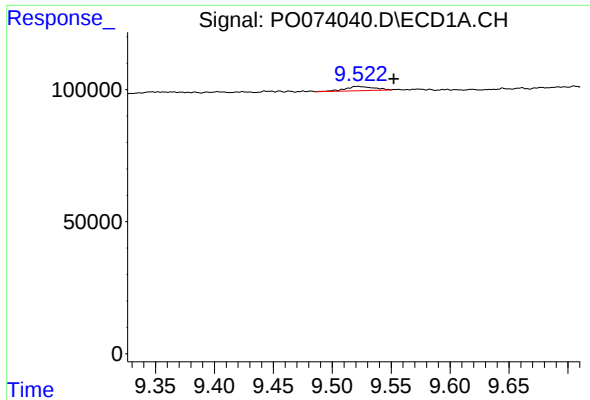

#39 AR-1262-4

R.T.: 9.522 min
Delta R.T.: -0.030 min
Response: 27340
Conc: 8.17 ng/ml

Instrument :
ECD_O
ClientSampleId :
LLEXSITUTV-022-001-SO

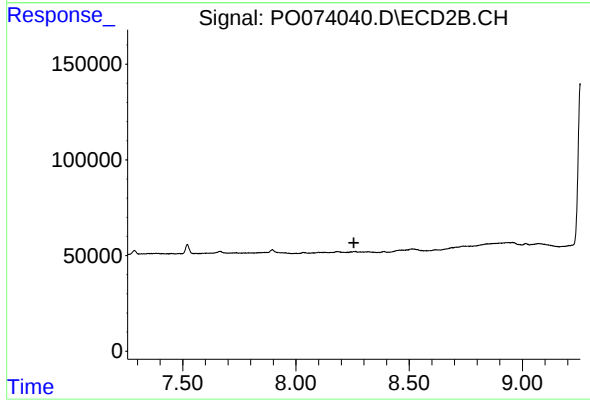

#39 AR-1262-4

R.T.: 0.000 min
Exp R.T. : 8.256 min
Response: 0
Conc: N.D.