

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO122220\
 Data File : PO074021.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 22 Dec 2020 12:42
 Operator : DD\AJ
 Sample : L5165-09
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 S4-09-A

Manual Integrations
 APPROVED

Ankita
 1/4/2021 8:38:55 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 29 10:24:37 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO121020.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Dec 11 03:58:06 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.936	3.996	1960163	1199304	21.439	22.360
2) SA Decachlor...	10.961	9.260	1438969	789113	17.413	16.865
Target Compounds						
41) L9 AR-1268-1	9.455	8.184	317714	189529	22.306	19.694
42) L9 AR-1268-2	9.552	8.248	297353	130471	24.122	15.837 #
43) L9 AR-1268-3	9.777	8.456	193878	92318	17.864	13.075 #
44) L9 AR-1268-4	10.216	8.741	54044	33773	11.537	11.410m
45) L9 AR-1268-5	10.629	9.020	495609	255651	15.144	12.725

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\PO122220\
Data File : PO074021.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 22 Dec 2020 12:42
Operator : DD\AJ
Sample : L5165-09
Misc :
ALS Vial : 14 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampled :
S4-09-A


Manual Integrations
APPROVED

Ankita
1/4/2021 8:38:55 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 29 10:24:37 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\PO121020.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Dec 11 03:58:06 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

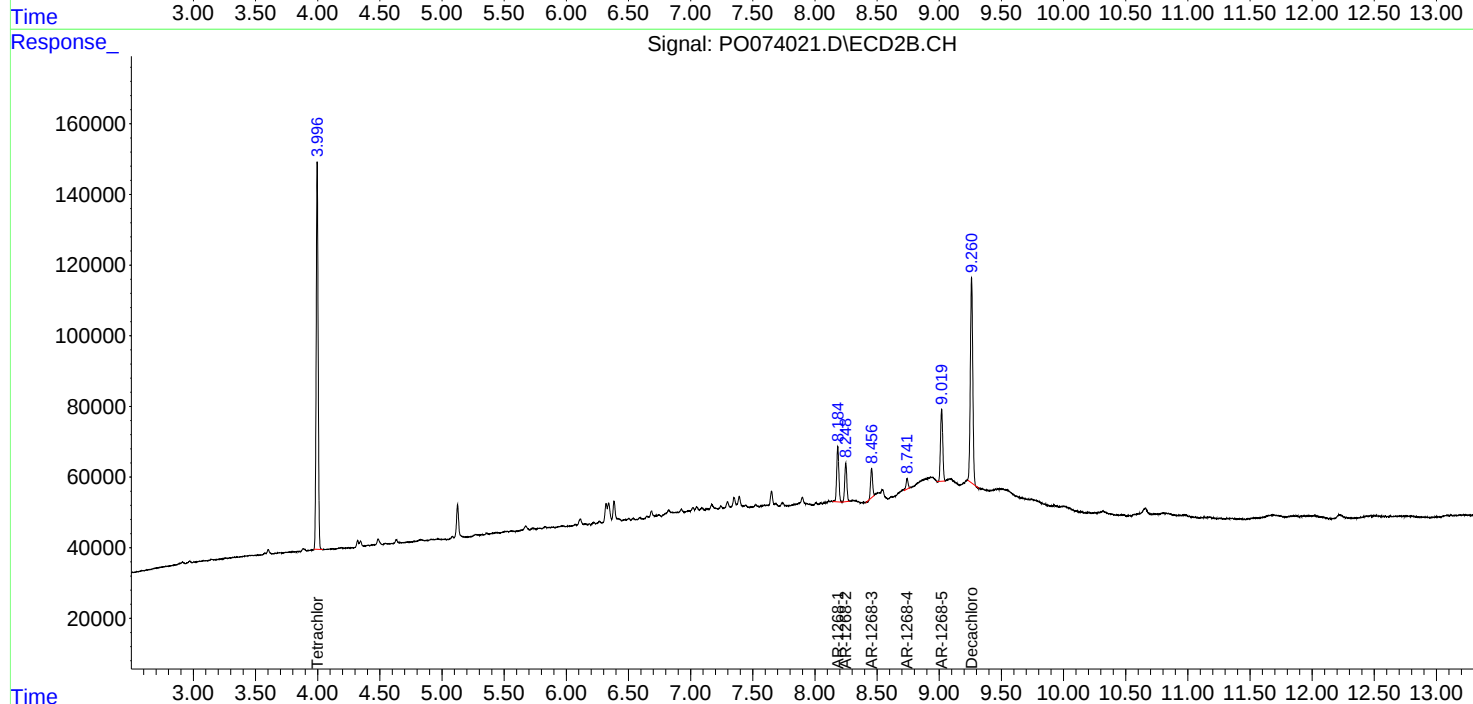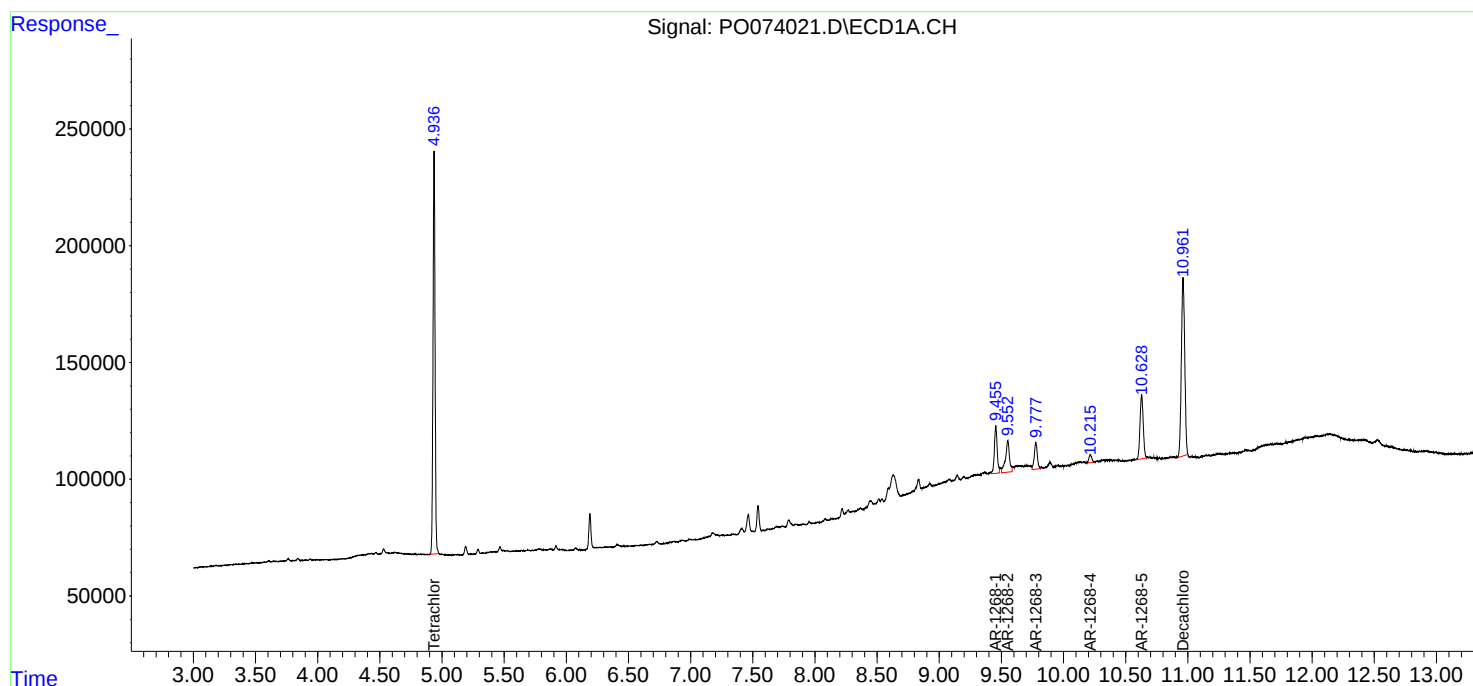

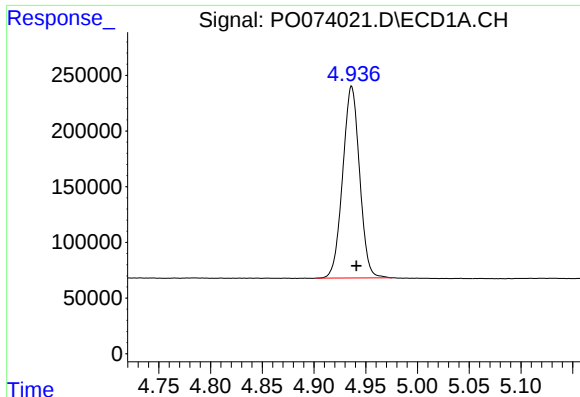


#1 Tetrachloro-m-xylene

R.T.: 4.936 min
Delta R.T.: -0.005 min
Response: 1960163
Conc: 21.44 ng/ml

Instrument :
ECD_O
ClientSampleId :
S4-09-A


Manual Integrations
APPROVED

Ankita
1/4/2021 8:38:55 AM

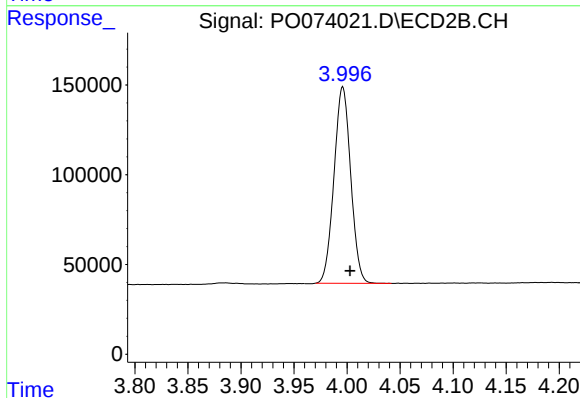


#1 Tetrachloro-m-xylene

R.T.: 3.996 min
Delta R.T.: -0.007 min
Response: 1199304
Conc: 22.36 ng/ml

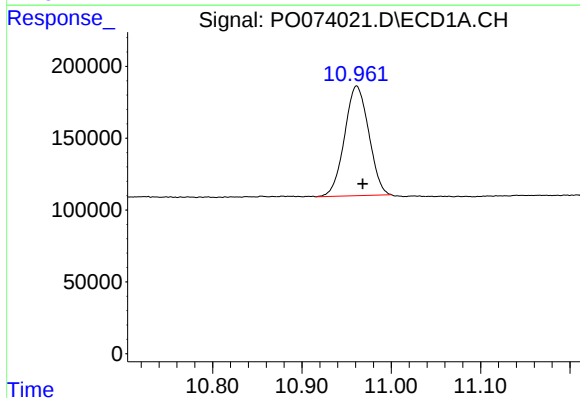


#2 Decachlorobiphenyl

R.T.: 10.961 min
Delta R.T.: -0.007 min
Response: 1438969
Conc: 17.41 ng/ml

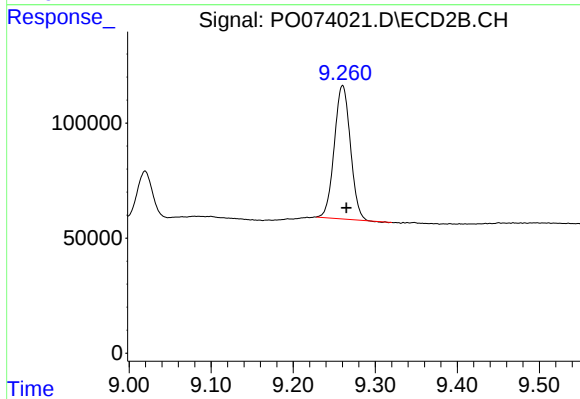

#2 Decachlorobiphenyl

R.T.: 9.260 min
Delta R.T.: -0.005 min
Response: 789113
Conc: 16.86 ng/ml

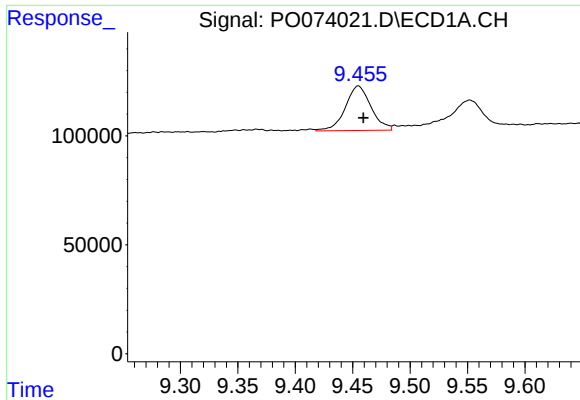


#41 AR-1268-1

R.T.: 9.455 min
Delta R.T.: -0.004 min
Response: 317714
Conc: 22.31 ng/ml

Instrument :
ECD_O
ClientSampleId :
S4-09-A


Manual Integrations
APPROVED

Ankita
1/4/2021 8:38:55 AM

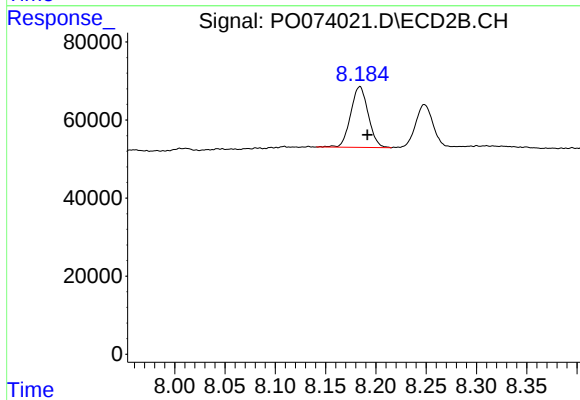


#41 AR-1268-1

R.T.: 8.184 min
Delta R.T.: -0.007 min
Response: 189529
Conc: 19.69 ng/ml

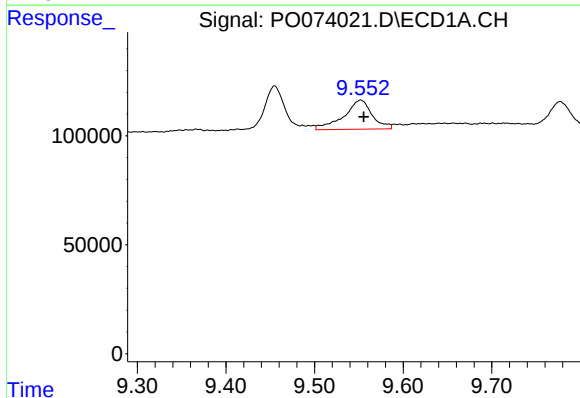


#42 AR-1268-2

R.T.: 9.552 min
Delta R.T.: -0.004 min
Response: 297353
Conc: 24.12 ng/ml

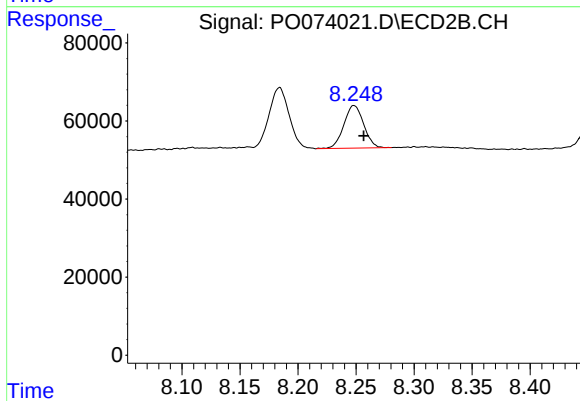

#42 AR-1268-2

R.T.: 8.248 min
Delta R.T.: -0.009 min
Response: 130471
Conc: 15.84 ng/ml

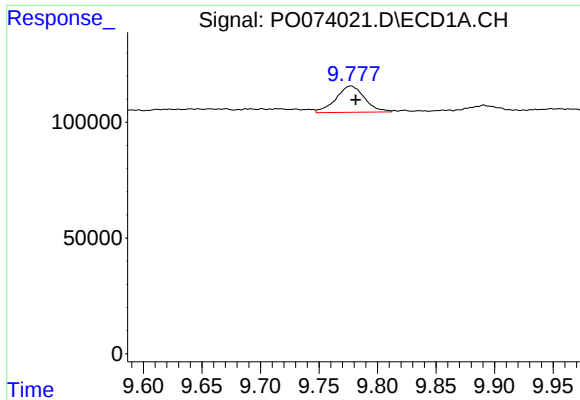


#43 AR-1268-3

R.T.: 9.777 min
Delta R.T.: -0.004 min
Response: 193878
Conc: 17.86 ng/ml

Instrument :
ECD_O
ClientSampleId :
S4-09-A


Manual Integrations
APPROVED

Ankita
1/4/2021 8:38:55 AM

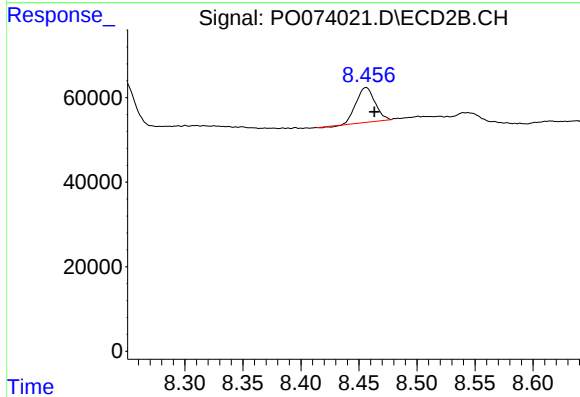


#43 AR-1268-3

R.T.: 8.456 min
Delta R.T.: -0.007 min
Response: 92318
Conc: 13.07 ng/ml

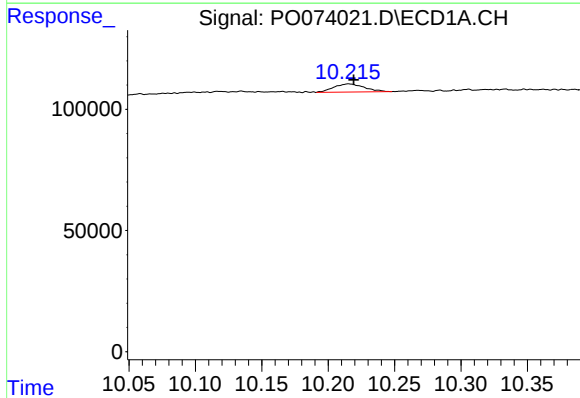


#44 AR-1268-4

R.T.: 10.216 min
Delta R.T.: -0.004 min
Response: 54044
Conc: 11.54 ng/ml

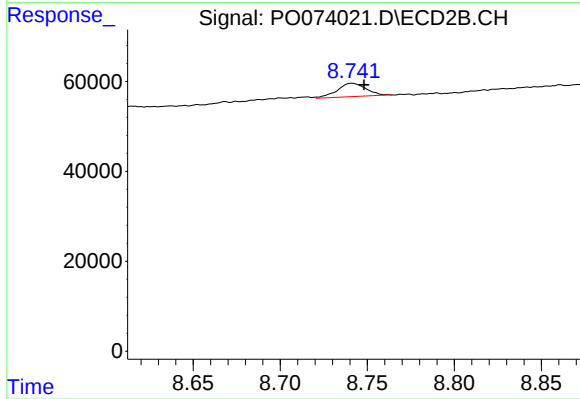

#44 AR-1268-4

R.T.: 8.741 min
Delta R.T.: -0.007 min
Response: 33773
Conc: 11.41 ng/ml m

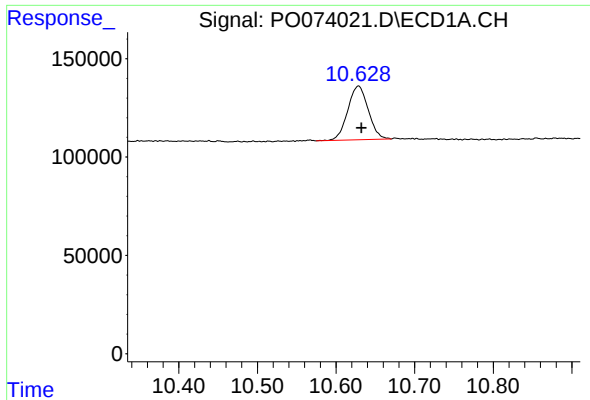


#45 AR-1268-5

R.T.: 10.629 min
Delta R.T.: -0.003 min
Response: 495609
Conc: 15.14 ng/ml

Instrument :
ECD_O
ClientSampleId :
S4-09-A

Manual Integrations
APPROVED

Ankita
1/4/2021 8:38:55 AM

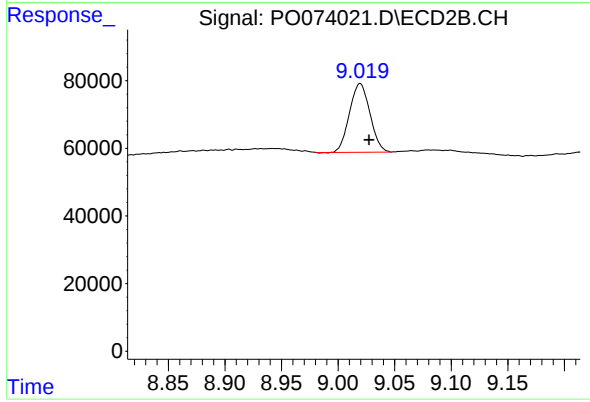

#45 AR-1268-5

R.T.: 9.020 min
Delta R.T.: -0.008 min
Response: 255651
Conc: 12.73 ng/ml