

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0122220\
 Data File : P0074069.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 23 Dec 2020 3:32
 Operator : DD\AJ
 Sample : PB133751BL
 Misc :
 ALS Vial : 53 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 PB133751BL

Manual Integrations
 APPROVED

Ankita
 12/23/2020 2:55:12 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 23 08:18:22 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0121020.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Dec 11 03:58:06 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.934	3.992	2119215	1183337	23.179	22.062
2) SA Decachlor...	10.954	9.253	2134161	1241187	25.825	26.526m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO122220\
Data File : PO074069.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 23 Dec 2020 3:32
Operator : DD\AJ
Sample : PB133751BL
Misc :
ALS Vial : 53 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
PB133751BL


Manual Integrations
APPROVED

Ankita
12/23/2020 2:55:12 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 23 08:18:22 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO121020.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Dec 11 03:58:06 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

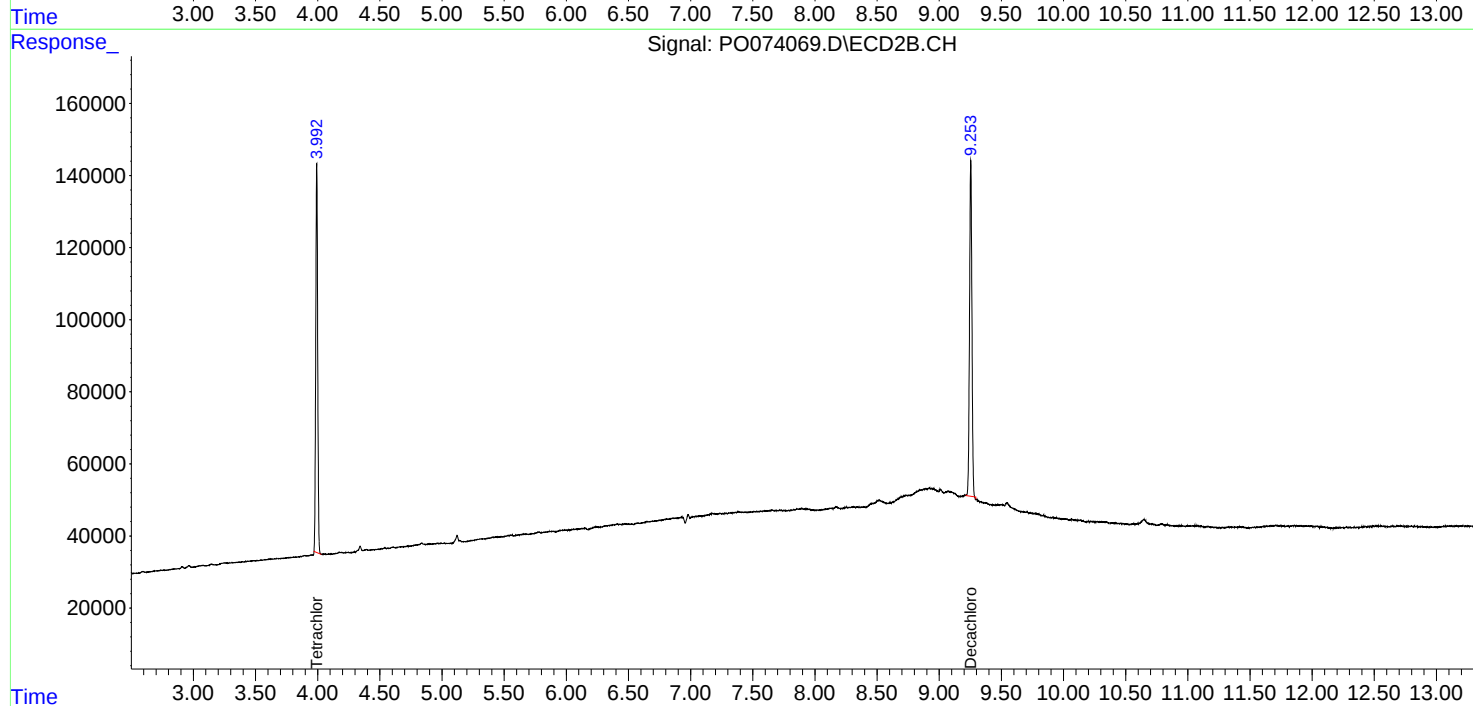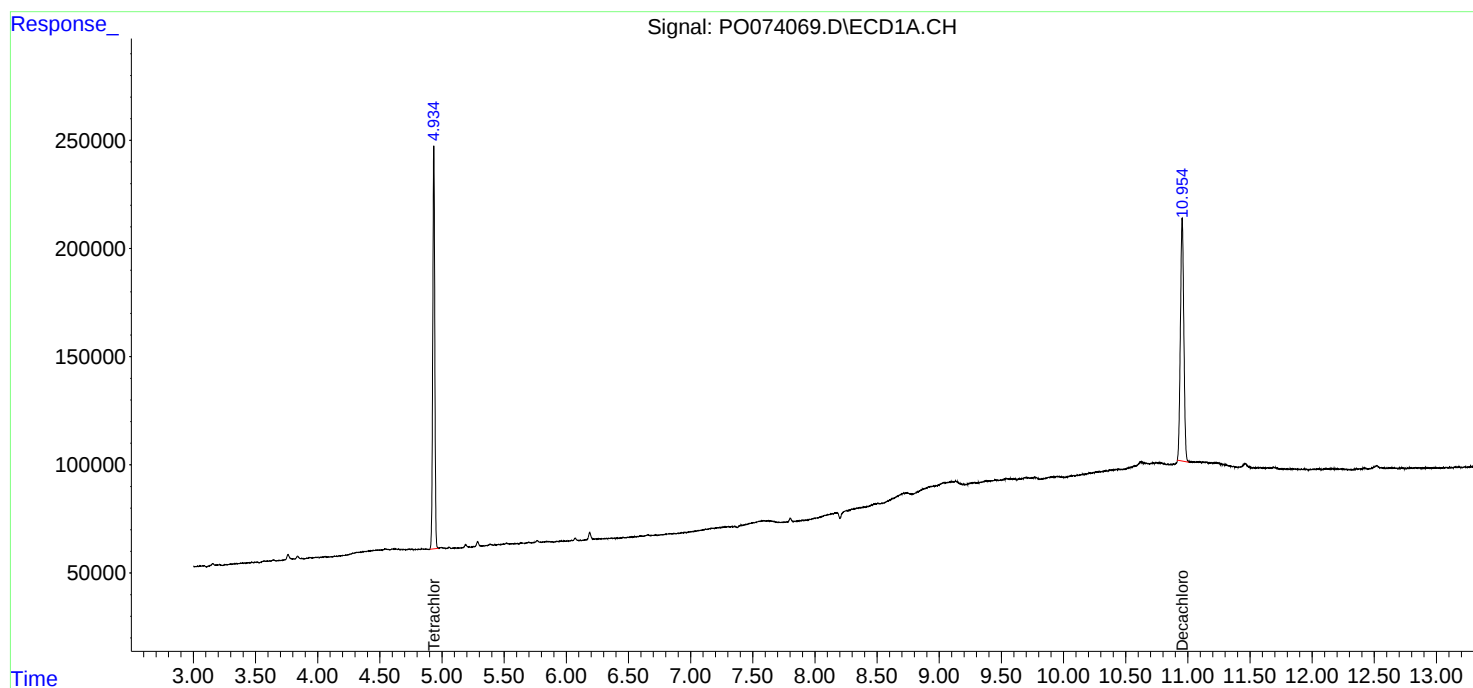

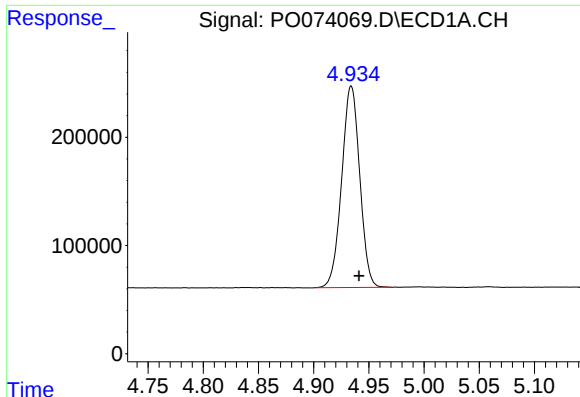


#1 Tetrachloro-m-xylene

R.T.: 4.934 min
Delta R.T.: -0.007 min
Response: 2119215
Conc: 23.18 ng/ml

Instrument :
ECD_O
ClientSampleId :
PB133751BL


Manual Integrations
APPROVED

Ankita
12/23/2020 2:55:12 PM

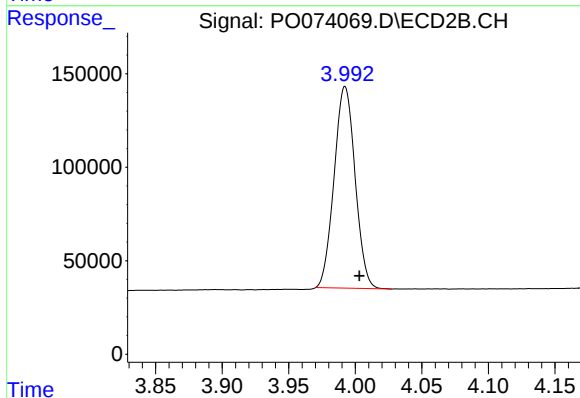


#1 Tetrachloro-m-xylene

R.T.: 3.992 min
Delta R.T.: -0.011 min
Response: 1183337
Conc: 22.06 ng/ml

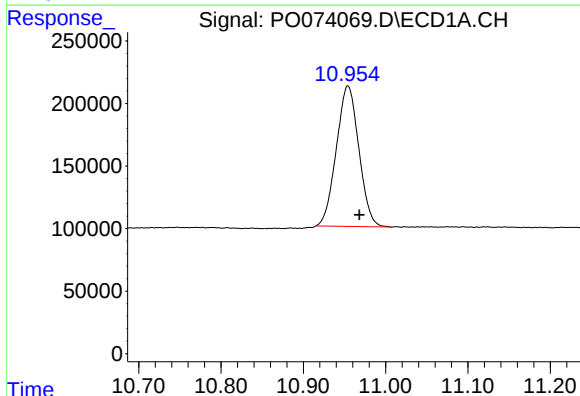

#2 Decachlorobiphenyl

R.T.: 10.954 min
Delta R.T.: -0.014 min
Response: 2134161
Conc: 25.82 ng/ml

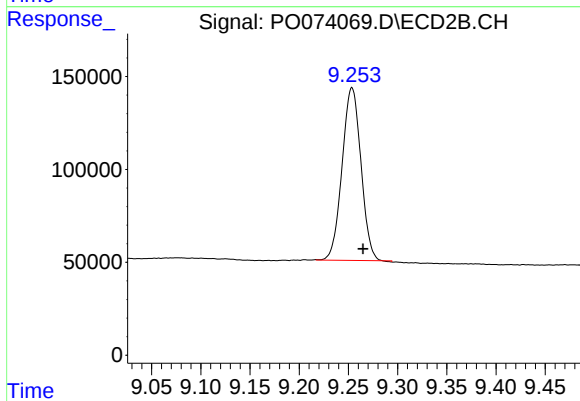

#2 Decachlorobiphenyl

R.T.: 9.253 min
Delta R.T.: -0.012 min
Response: 1241187
Conc: 26.53 ng/ml m